
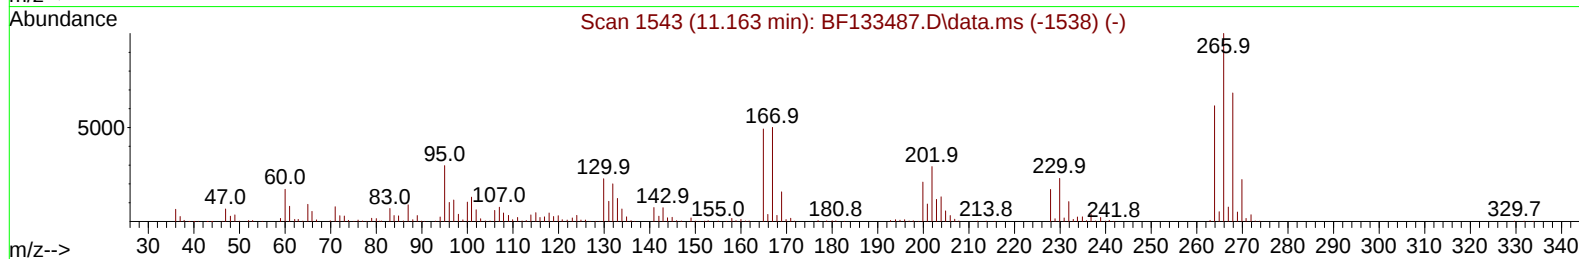
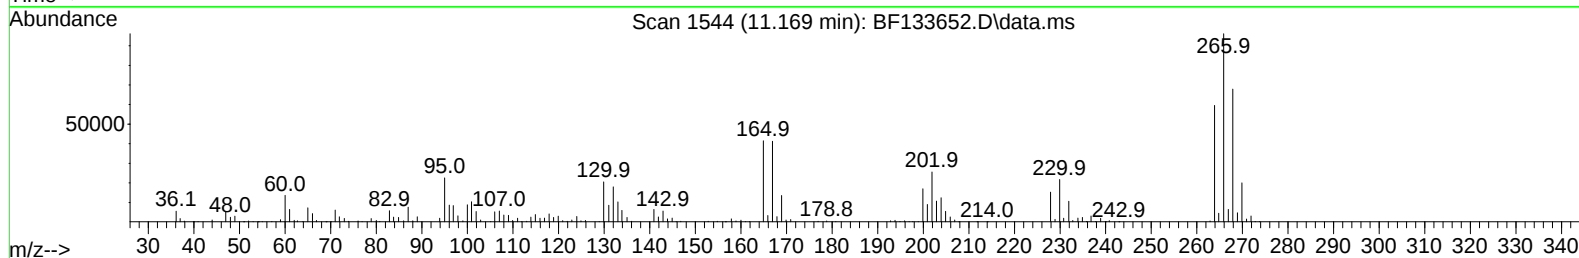


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060823\
Data File : BF133652.D
Acq On : 08 Jun 2023 21:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 05:41:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 11:43:32 2023
Response via : Initial Calibration

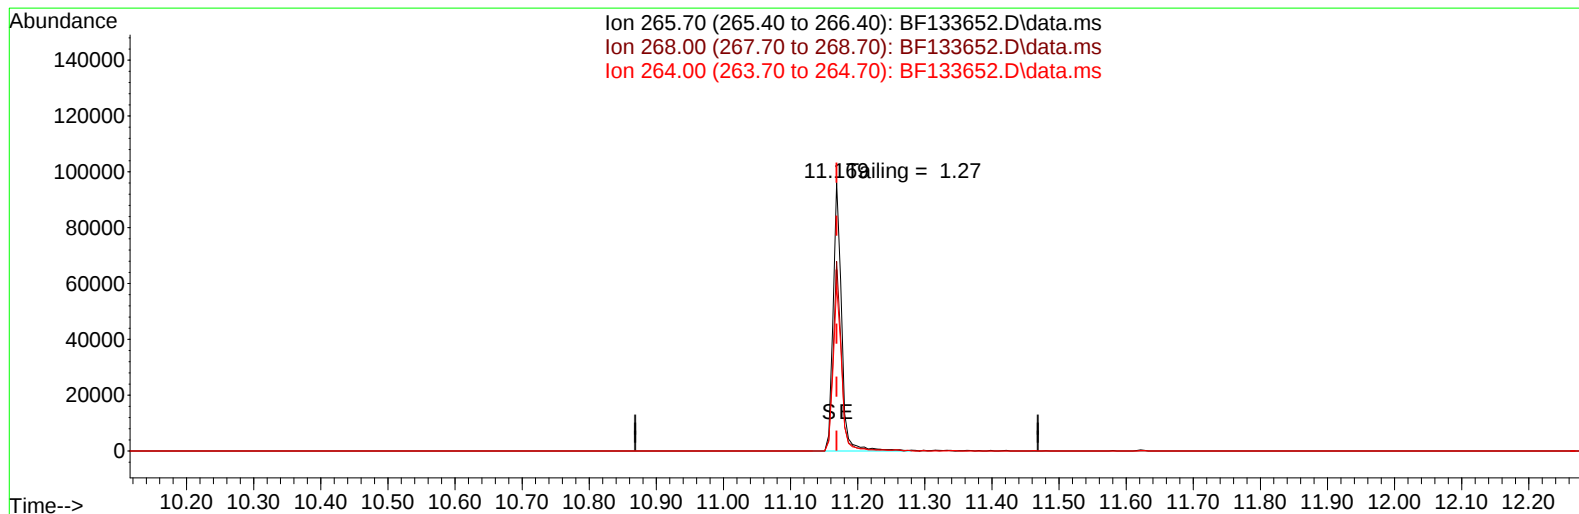

TIC: BF133652.D\data.ms

(70) Pentachlorophenol (C)




11.169min (+ 0.000) 23181.62 ng

response 83896

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.30	70.58
264.00	61.50	61.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060823\
 Data File : BF133652.D
 Acq On : 08 Jun 2023 21:23
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 05:41:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 08 11:43:32 2023
 Response via : Initial Calibration

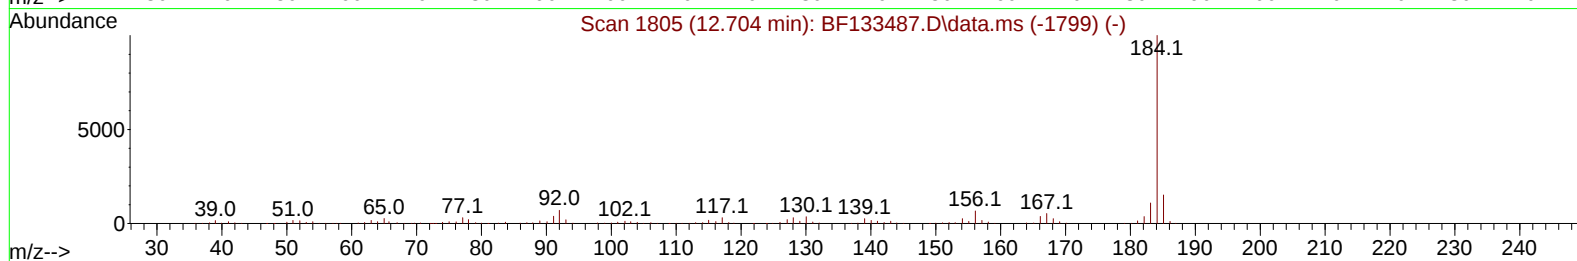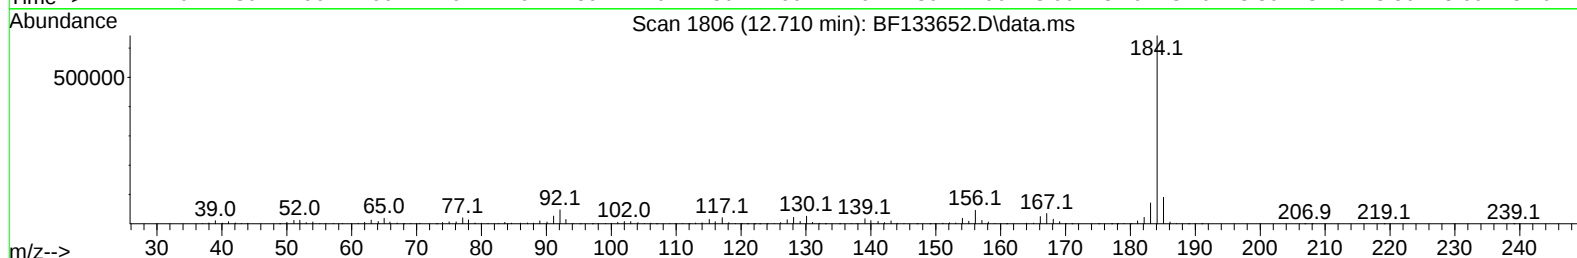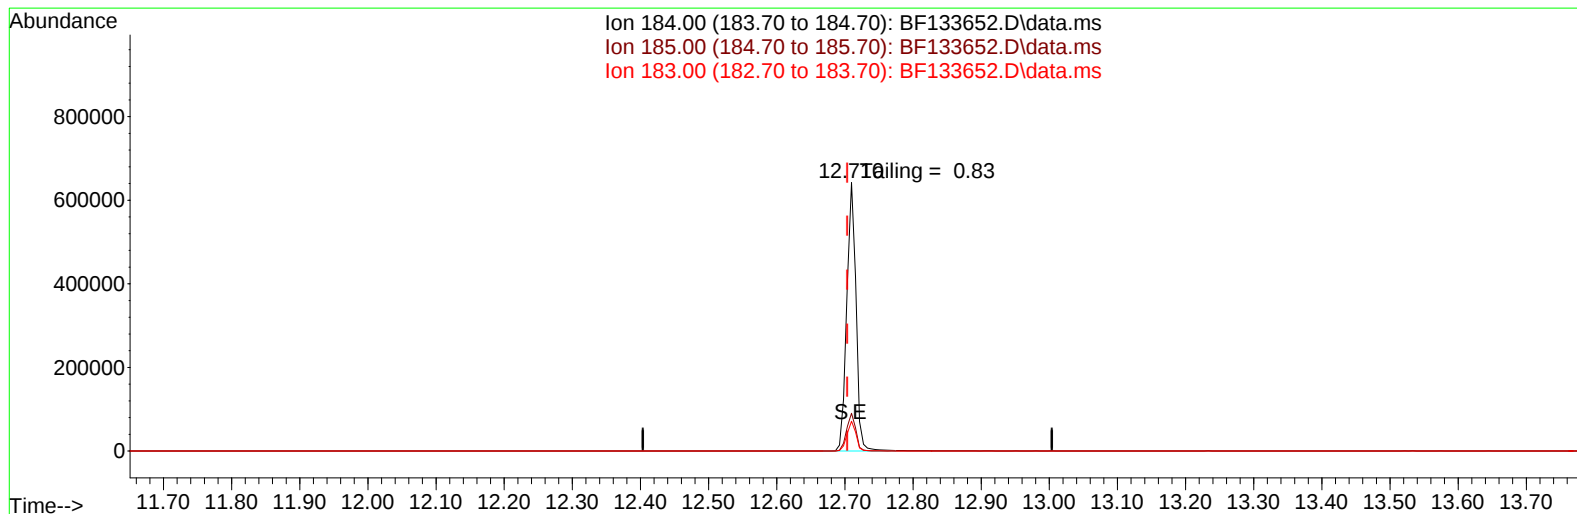

TIC: BF133652.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 40004.97 ng

response 607256

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.08
183.00	10.90	11.11
0.00	0.00	0.00