

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060823\
 Data File : BF133634.D
 Acq On : 08 Jun 2023 10:23
 Operator : CG\JU
 Sample : PB153261BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB153261BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133634.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.075	505	508	517	rVB	39904	54582	1.19%	0.205%
2	5.457	567	573	576	rBV	3305060	3417880	74.54%	12.844%
3	6.463	738	744	747	rBV	2836400	3497040	76.27%	13.141%
4	6.834	803	807	810	rBV	913156	715420	15.60%	2.688%
5	7.398	897	903	906	rBV	2201398	2301316	50.19%	8.648%
6	8.116	1021	1025	1028	rBV	1207156	941764	20.54%	3.539%
7	9.198	1203	1209	1212	rBV	4471931	4013651	87.53%	15.082%
8	9.875	1320	1324	1327	rBV	1379638	1049556	22.89%	3.944%
9	10.669	1454	1459	1462	rBV	2862900	2727306	59.48%	10.249%
10	11.363	1573	1577	1580	rBV	1483494	1190746	25.97%	4.475%
11	12.957	1843	1848	1851	rBV	4333367	4585346	100.00%	17.231%
12	14.010	2022	2027	2030	rBV	1202243	1077919	23.51%	4.051%
13	15.474	2270	2276	2281	rBV	847145	1039107	22.66%	3.905%




Sum of corrected areas: 26611633

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060823\
Data File : BF133634.D
Acq On : 08 Jun 2023 10:23
Operator : CG\JU
Sample : PB153261BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153261BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

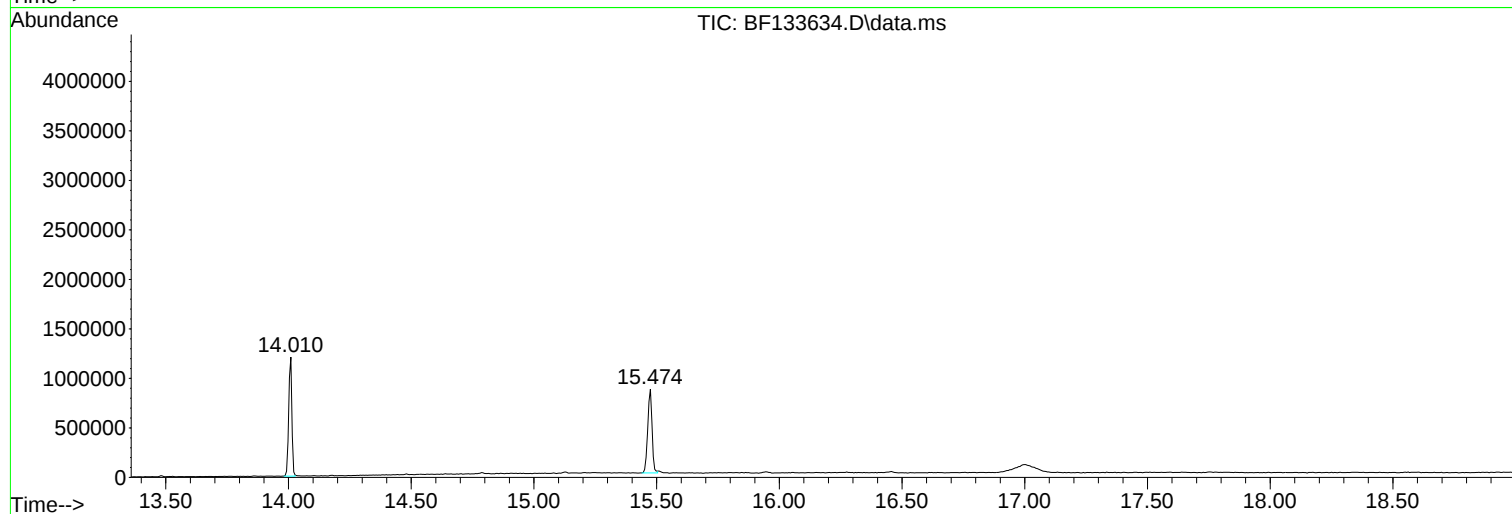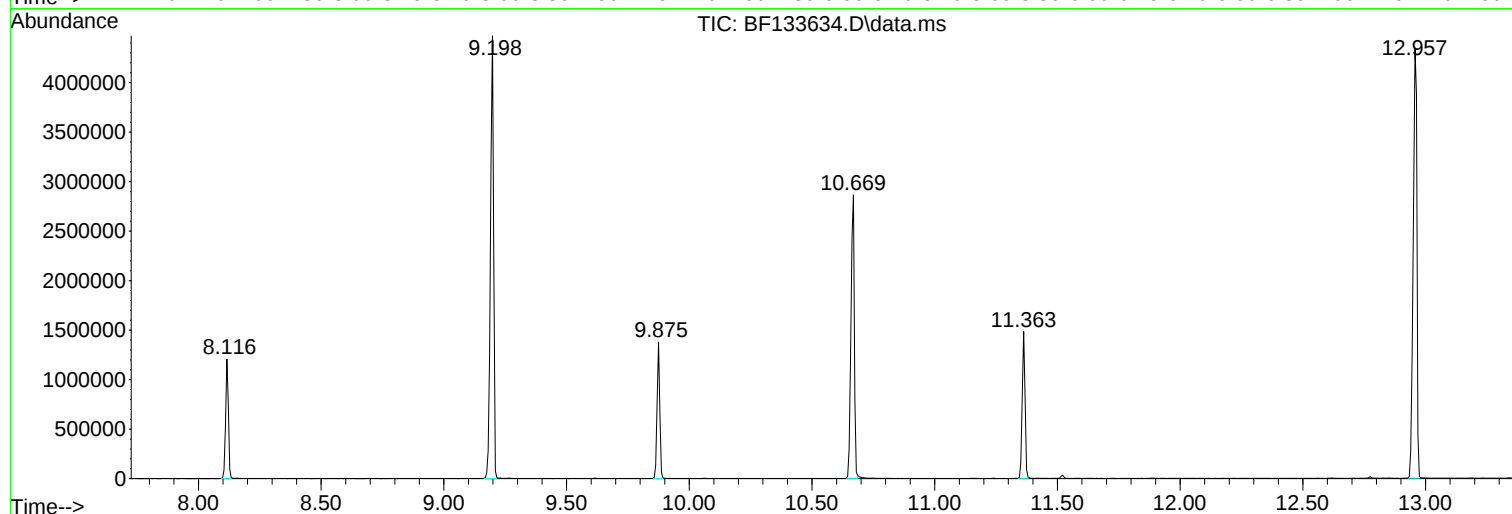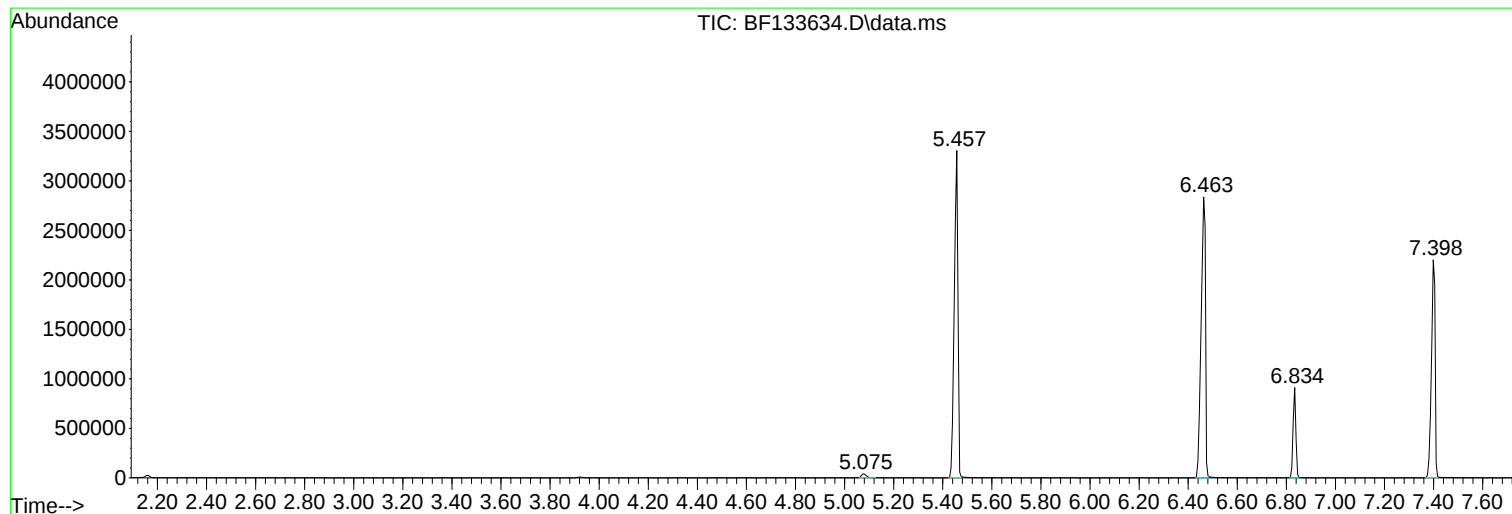

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060823\
Data File : BF133634.D
Acq On : 08 Jun 2023 10:23
Operator : CG\JU
Sample : PB153261BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153261BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060823\
Data File : BF133634.D
Acq On : 08 Jun 2023 10:23
Operator : CG\JU
Sample : PB153261BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153261BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------