
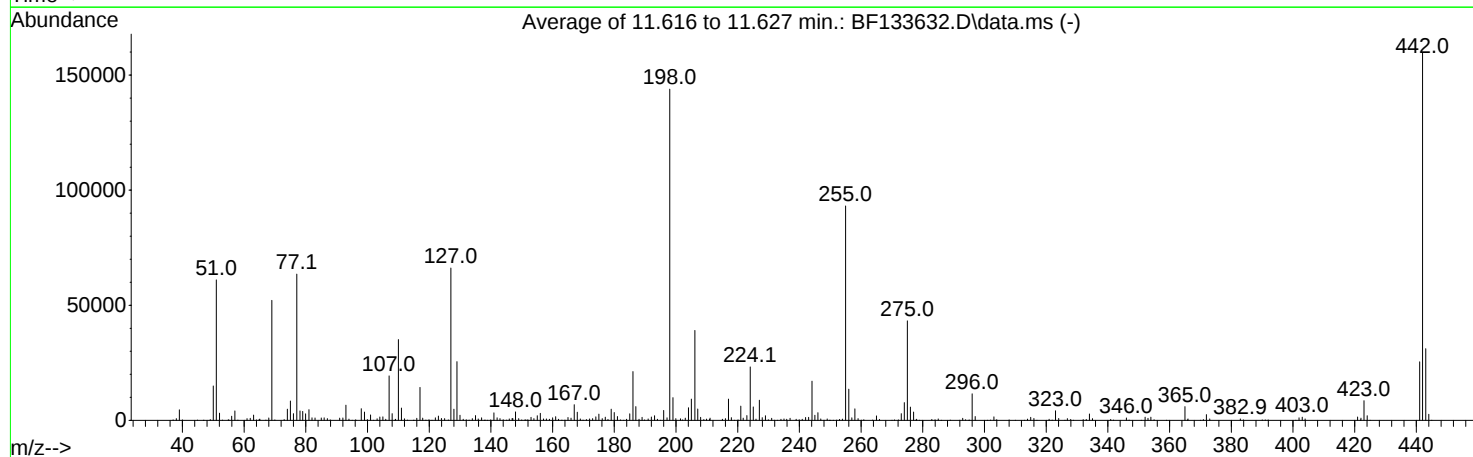


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060823\
Data File : BF133632.D
Acq On : 08 Jun 2023 08:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 08 11:43:32 2023

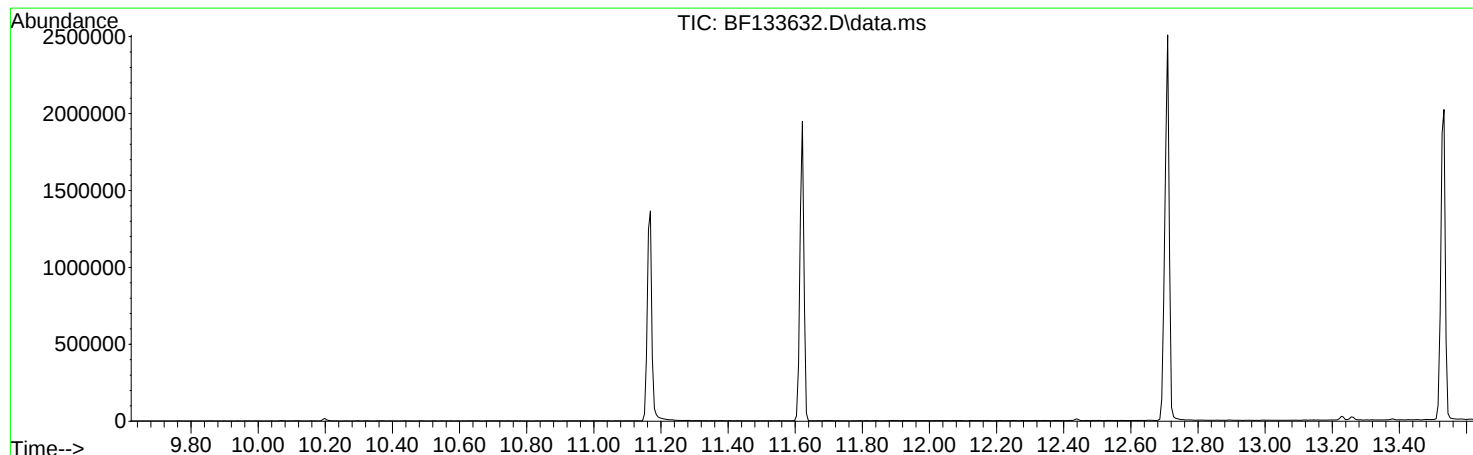

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	61048	PASS
68	69	0.00	2	2.0	1018	PASS
69	198	0.00	100	36.3	52173	PASS
70	69	0.00	2	0.4	225	PASS
127	198	10	80	46.0	66187	PASS
197	198	0.00	2	0.8	1117	PASS
198	198	100	100	100.0	143899	PASS
199	198	5	9	6.9	9881	PASS
275	198	10	60	30.1	43251	PASS
365	198	1	100	4.2	6005	PASS
441	198	0.01	100	17.7	25455	PASS
442	442	50	100	100.0	159813	PASS
443	442	15	24	19.5	31115	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/8/2023	BNA_F	<u>BF133632.D</u>
Compound Name	Response	Retention Time
DDT	357395	13.533
DDD	7765	13.227
DDE	429	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8194	365589	2.24

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060823\
Data File : BF133632.D
Acq On : 08 Jun 2023 08:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 08 09:23:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 07 11:27:15 2023
Response via : Initial Calibration

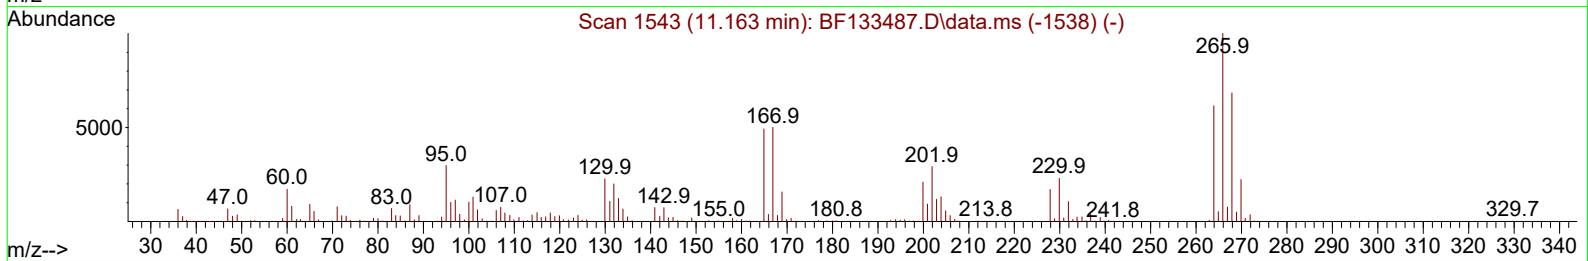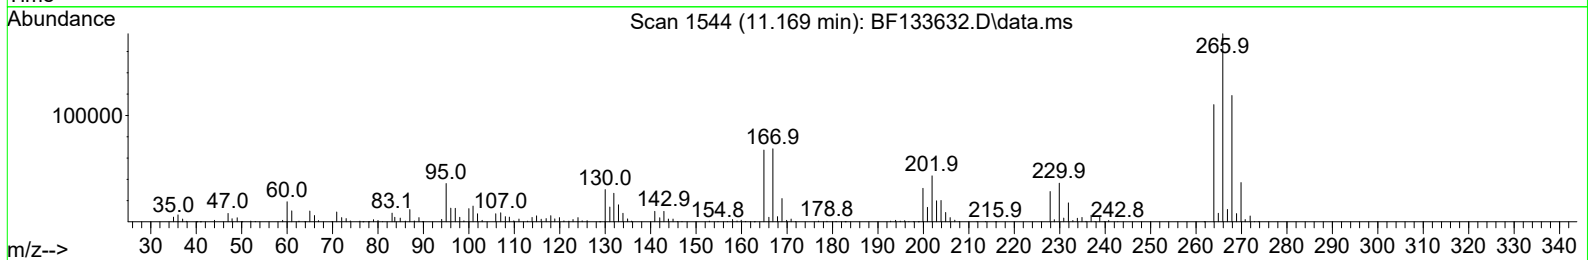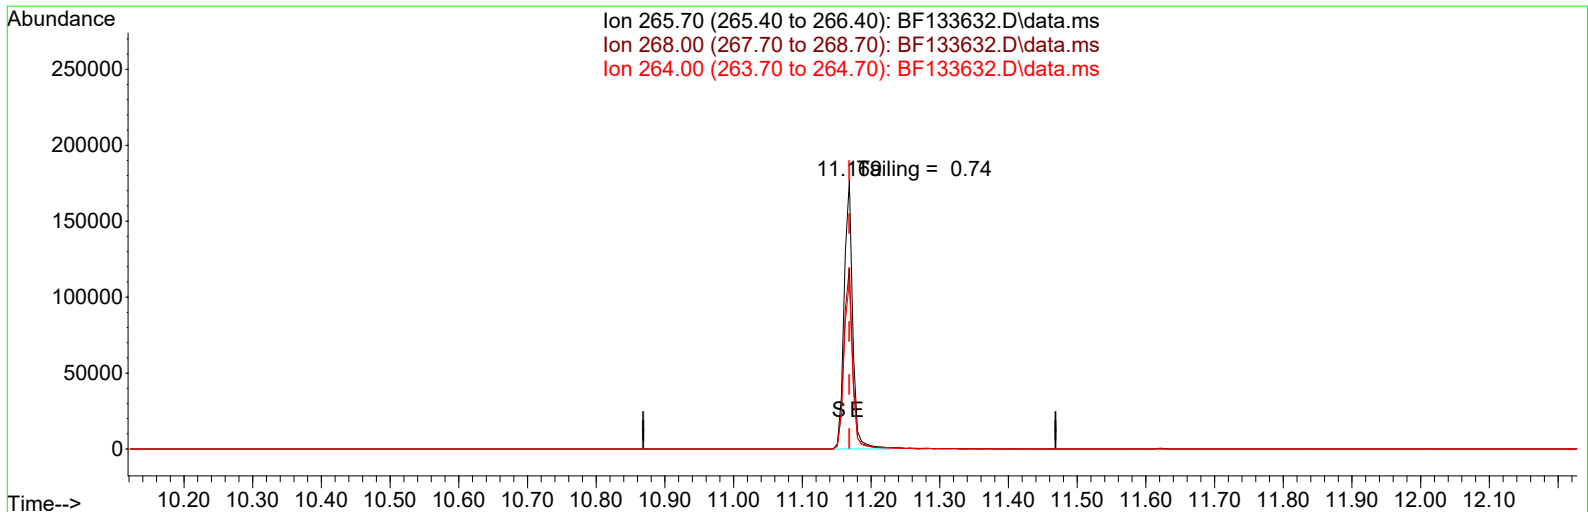

TIC: BF133632.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.000) 41512.83 ng




response 153546

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.30	67.21
264.00	61.50	62.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060823\
Data File : BF133632.D
Acq On : 08 Jun 2023 08:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 08 09:23:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 07 11:27:15 2023
Response via : Initial Calibration

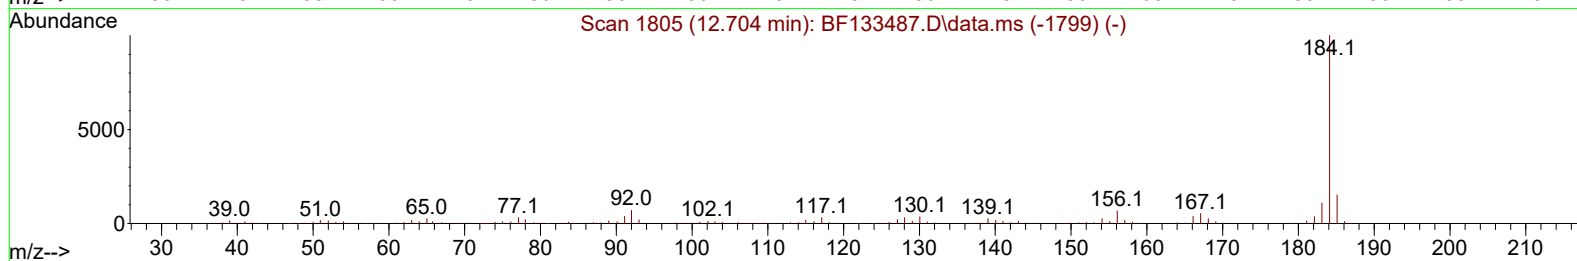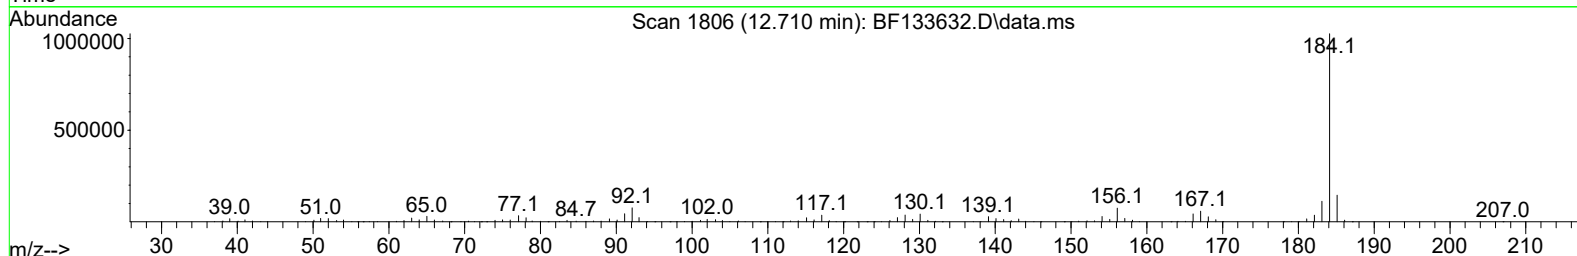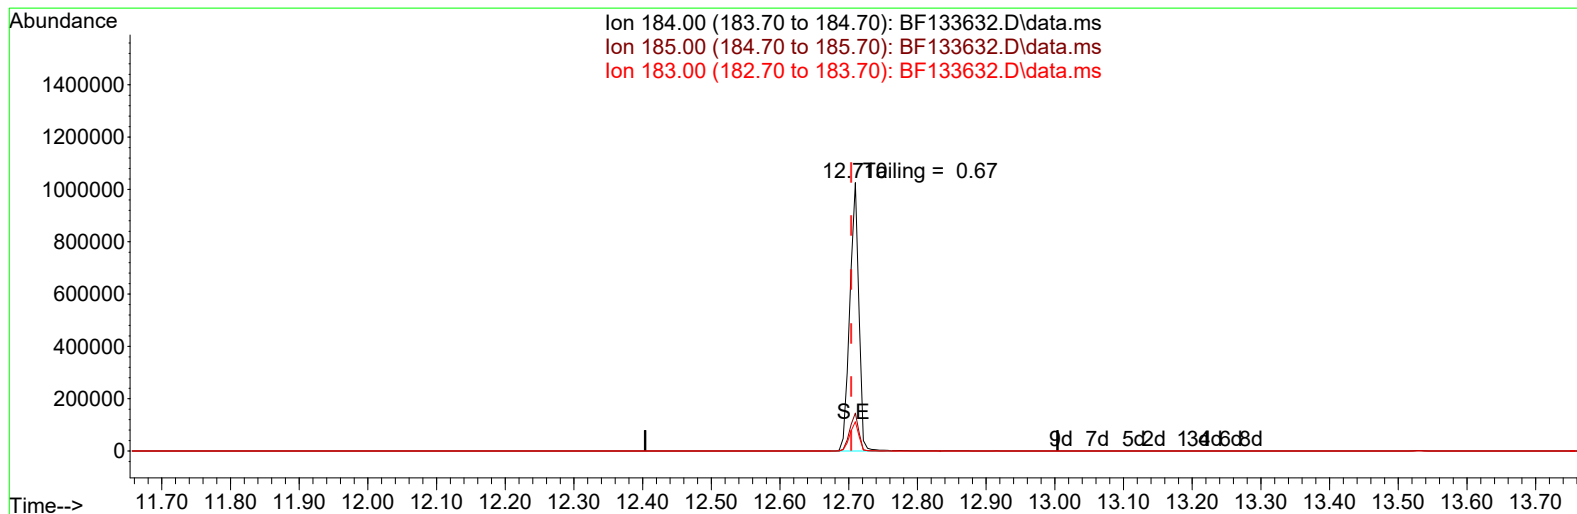

TIC: BF133632.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 450537.25 ng

response 935577

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.12
183.00	10.90	10.90
0.00	0.00	0.00