


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060823\
Data File : BF133652.D
Acq On : 08 Jun 2023 21:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 08 11:43:32 2023

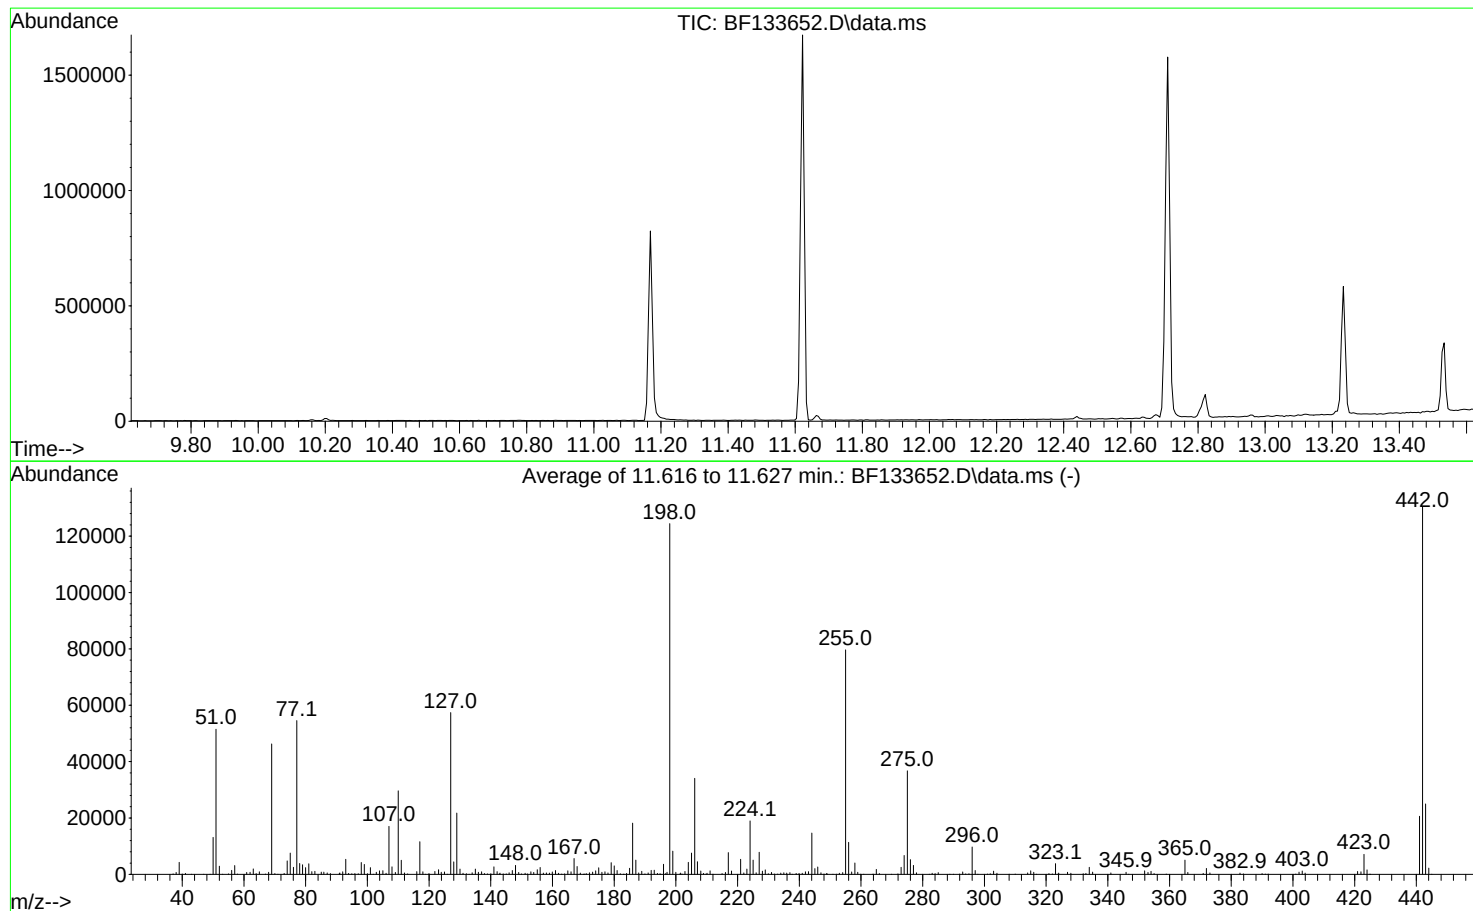

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	51518	PASS
68	69	0.00	2	1.6	743	PASS
69	198	0.00	100	37.2	46262	PASS
70	69	0.00	2	0.7	313	PASS
127	198	10	80	46.1	57379	PASS
197	198	0.00	2	0.6	774	PASS
198	198	100	100	100.0	124437	PASS
199	198	5	9	6.6	8212	PASS
275	198	10	60	29.5	36763	PASS
365	198	1	100	4.1	5069	PASS
441	198	0.01	100	16.6	20618	PASS
442	442	50	100	100.0	130525	PASS
443	442	15	24	19.1	24985	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/8/2023	BNA_F	<u>BF133652.D</u>
Compound Name	Response	Retention Time
DDT	49749	13.533
DDD	95114	13.233
DDE	187	12.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
95301	145050	65.70

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060823\
 Data File : BF133652.D
 Acq On : 08 Jun 2023 21:23
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 09 05:41:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 08 11:43:32 2023
 Response via : Initial Calibration

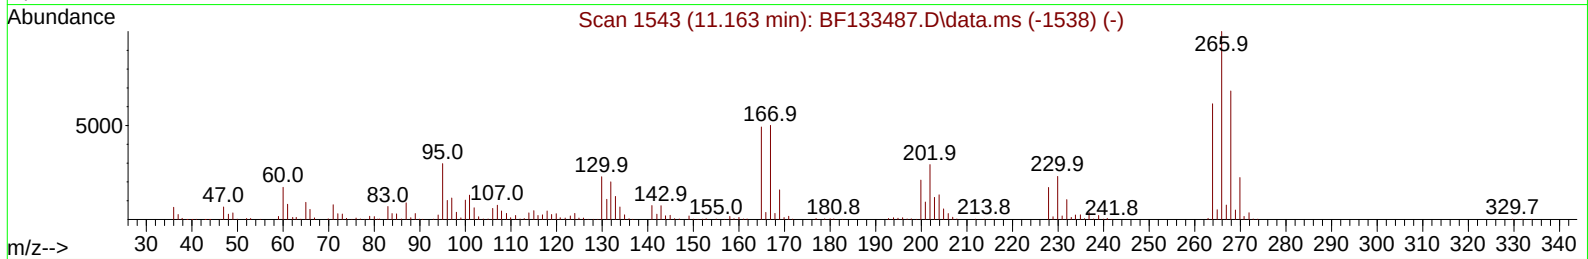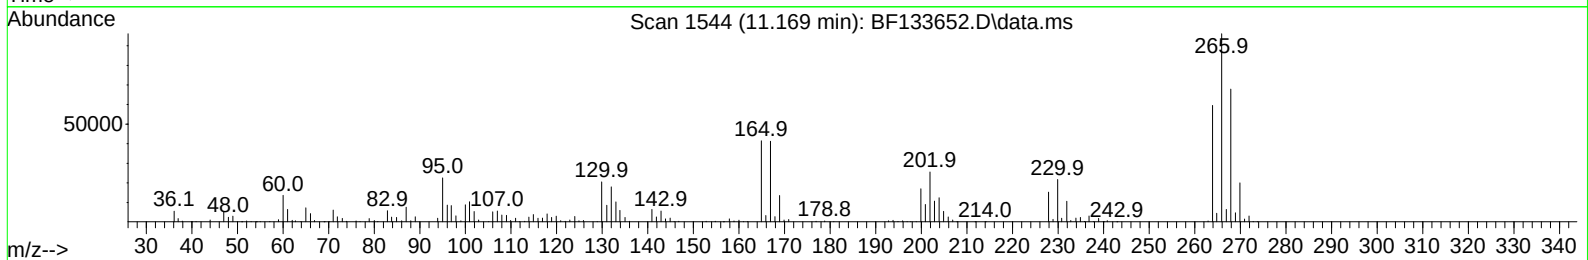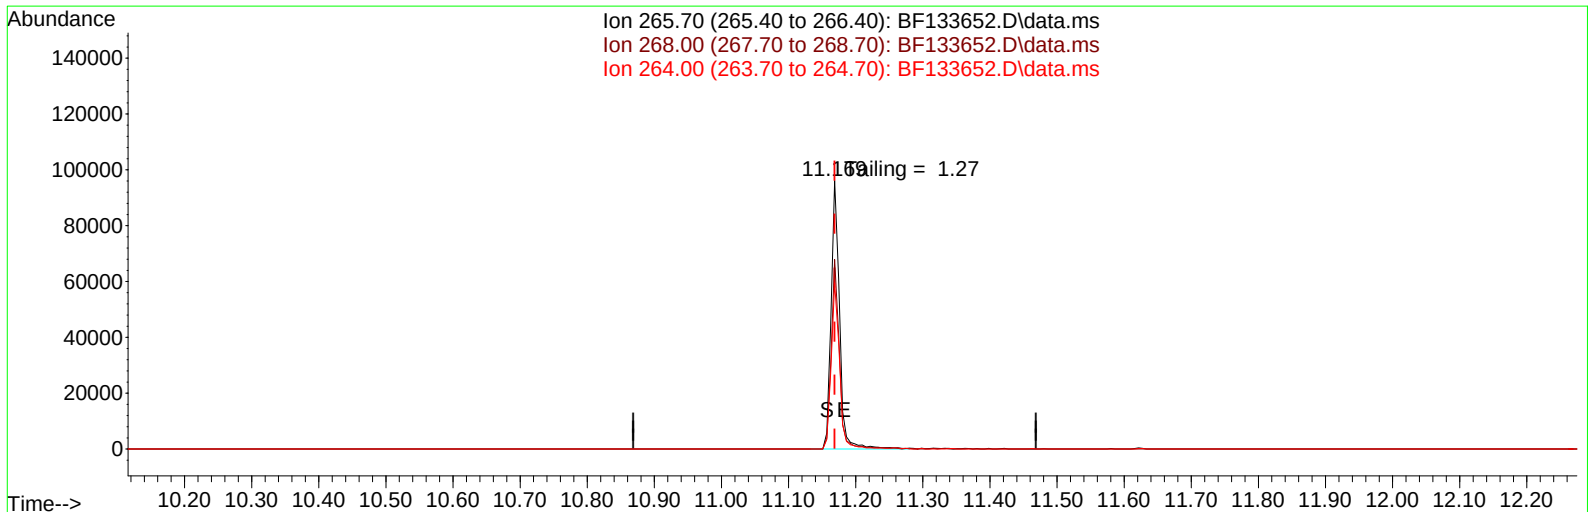

TIC: BF133652.D\data.ms

(70) Pentachlorophenol (C)

11.169min (+ 0.000) 23181.62 ng




response 83896

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.30	70.58
264.00	61.50	61.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060823\
Data File : BF133652.D
Acq On : 08 Jun 2023 21:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 09 05:41:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 11:43:32 2023
Response via : Initial Calibration

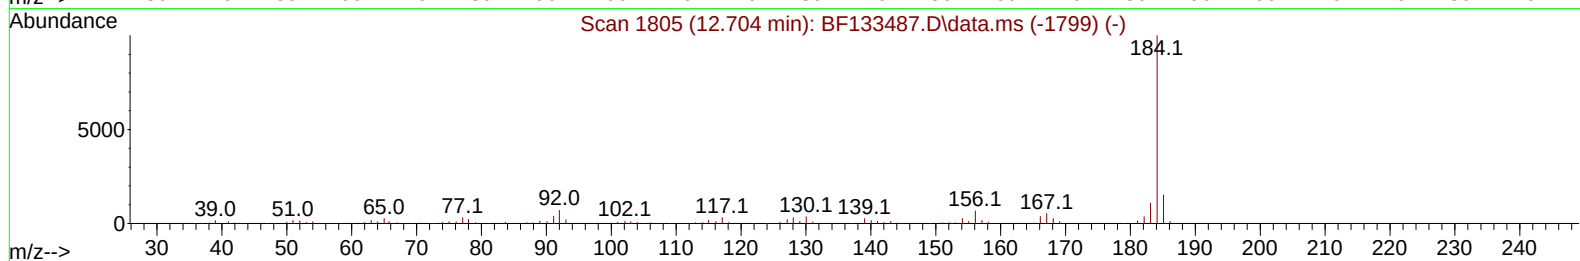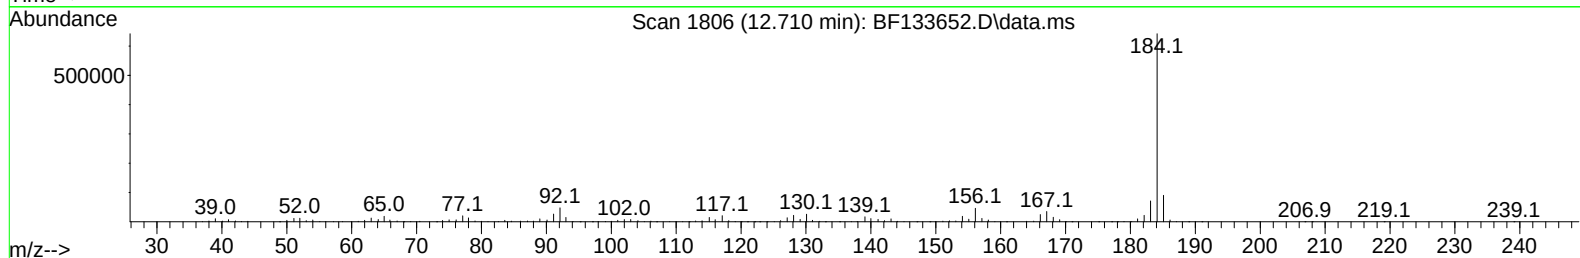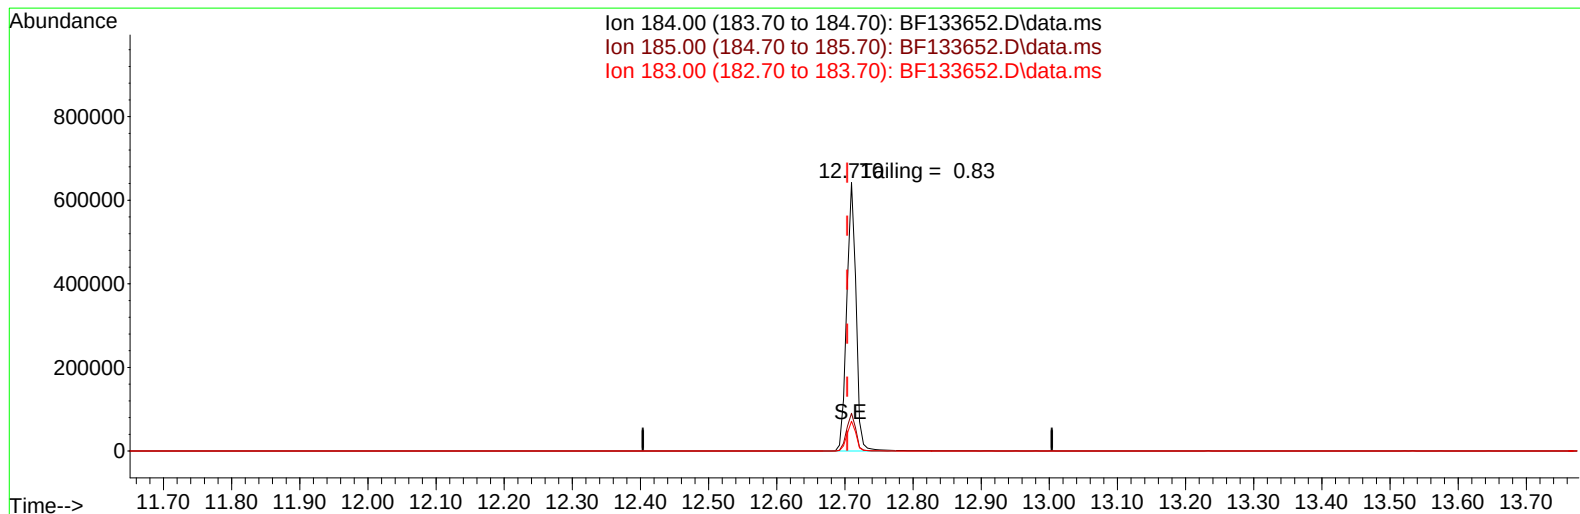

TIC: BF133652.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 40004.97 ng

response 607256

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.08
183.00	10.90	11.11
0.00	0.00	0.00