
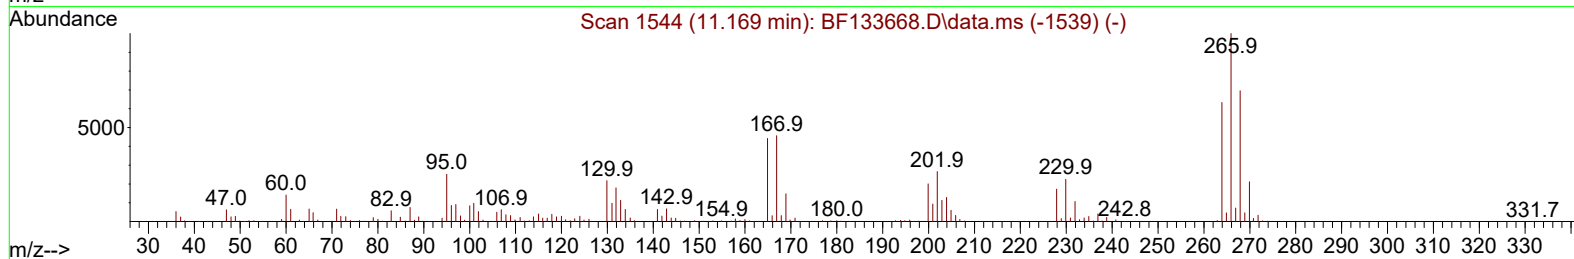
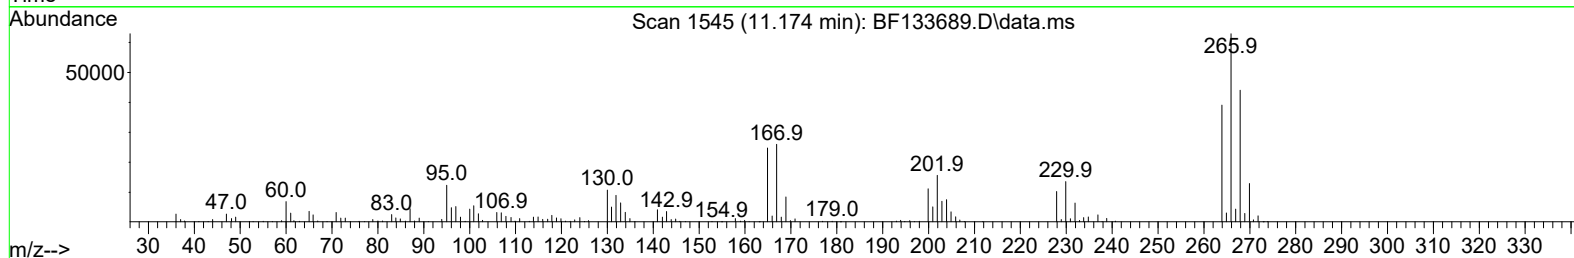


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060923\
Data File : BF133689.D
Acq On : 09 Jun 2023 22:12
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 03:23:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 09 15:37:41 2023
Response via : Initial Calibration

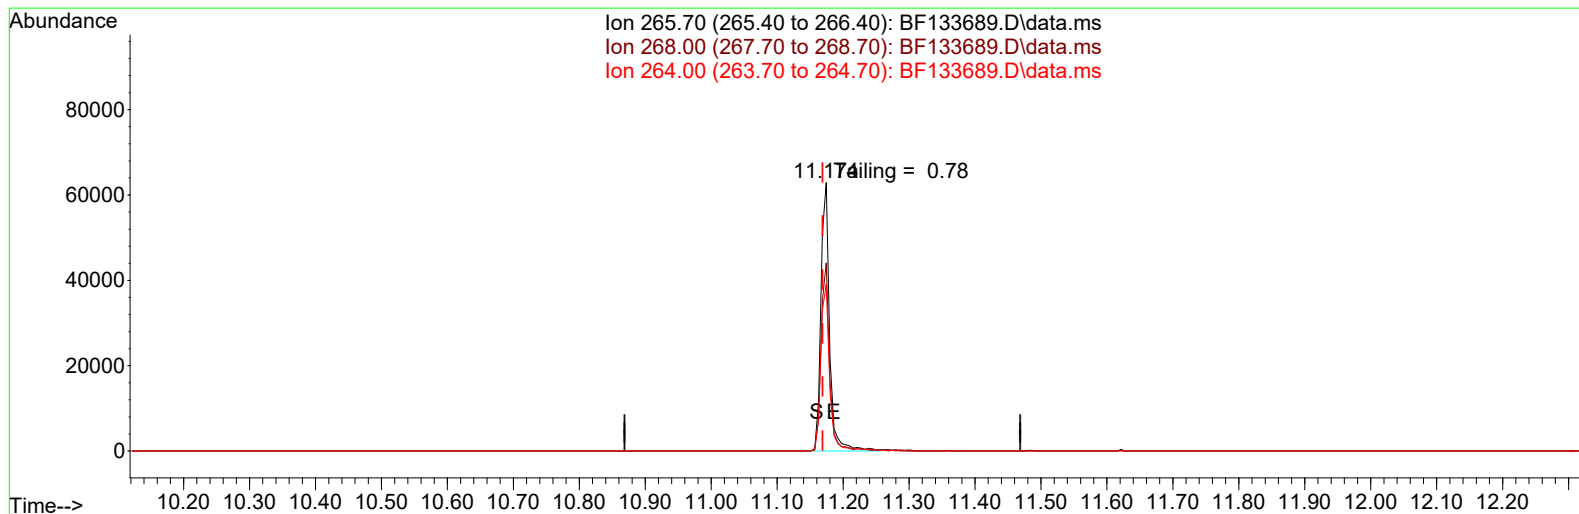

TIC: BF133689.D\data.ms

(70) Pentachlorophenol (C)




11.174min (+ 0.006) 16790.67 ng

response 58650

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.60	70.06
264.00	63.40	62.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060923\
Data File : BF133689.D
Acq On : 09 Jun 2023 22:12
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 10 03:23:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 09 15:37:41 2023
Response via : Initial Calibration

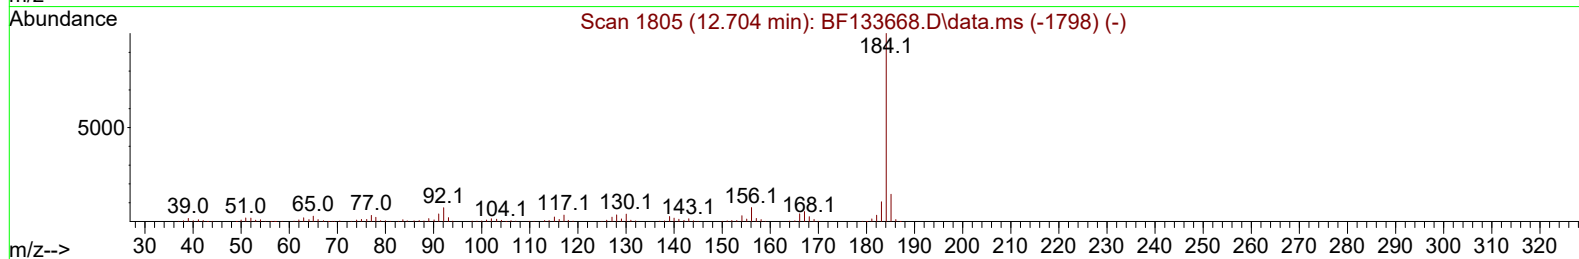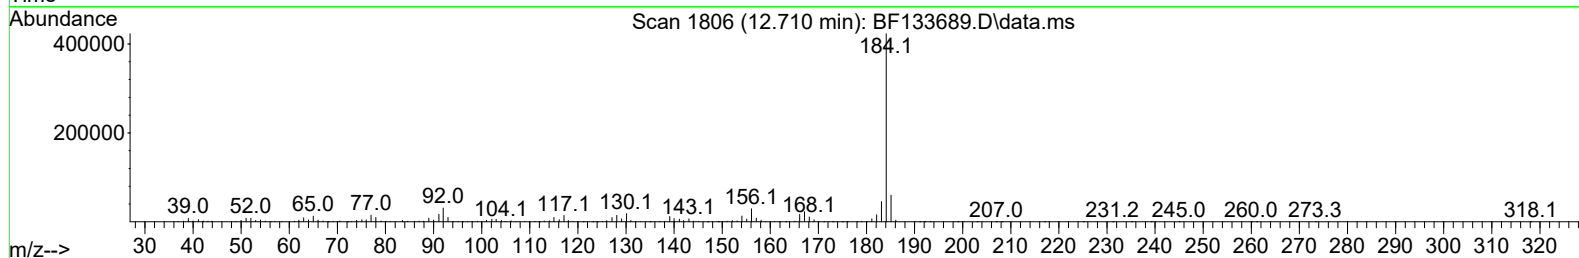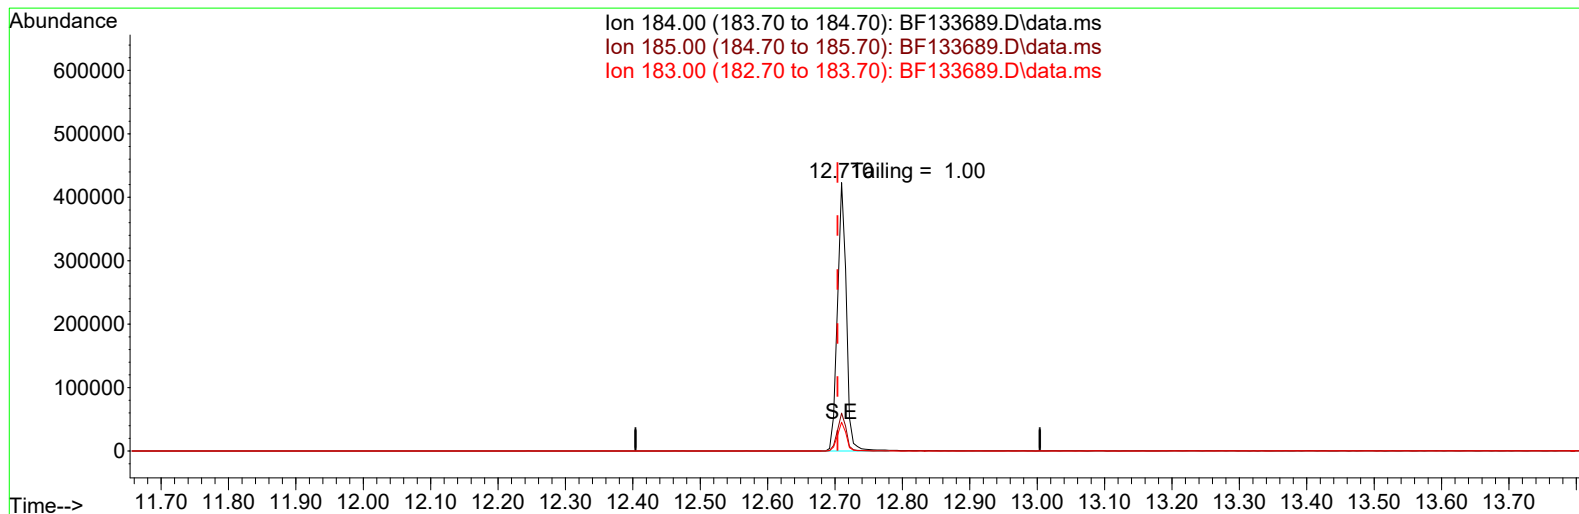

TIC: BF133689.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 50379.87 ng

response 278940

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.15
183.00	10.50	10.73
0.00	0.00	0.00