

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060923\
 Data File : BF133675.D
 Acq On : 09 Jun 2023 14:42
 Operator : CG\JU
 Sample : PB153207BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB153207BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133675.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.081	505	509	517	rBV	28071	40342	1.30%	0.212%
2	5.463	568	574	577	rBV	2515094	2670444	85.95%	14.050%
3	6.469	738	745	748	rBV	2393320	2690809	86.60%	14.157%
4	6.834	803	807	810	rBV	696102	532849	17.15%	2.804%
5	7.404	897	904	907	rBV	1824108	1762339	56.72%	9.272%
6	8.116	1021	1025	1029	rBV	787657	680632	21.91%	3.581%
7	9.198	1203	1209	1212	rBV	3661922	3107110	100.00%	16.348%
8	9.875	1320	1324	1327	rBV	942583	729584	23.48%	3.839%
9	10.669	1454	1459	1462	rBV	2138824	1966220	63.28%	10.345%
10	11.363	1573	1577	1581	rBV	923667	760059	24.46%	3.999%
11	12.957	1843	1848	1851	rBV	3220693	3068837	98.77%	16.146%
12	14.010	2023	2027	2030	rBV	636263	564253	18.16%	2.969%
13	15.474	2270	2276	2288	rVB	339936	432990	13.94%	2.278%




Sum of corrected areas: 19006468

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060923\
Data File : BF133675.D
Acq On : 09 Jun 2023 14:42
Operator : CG\JU
Sample : PB153207BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153207BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

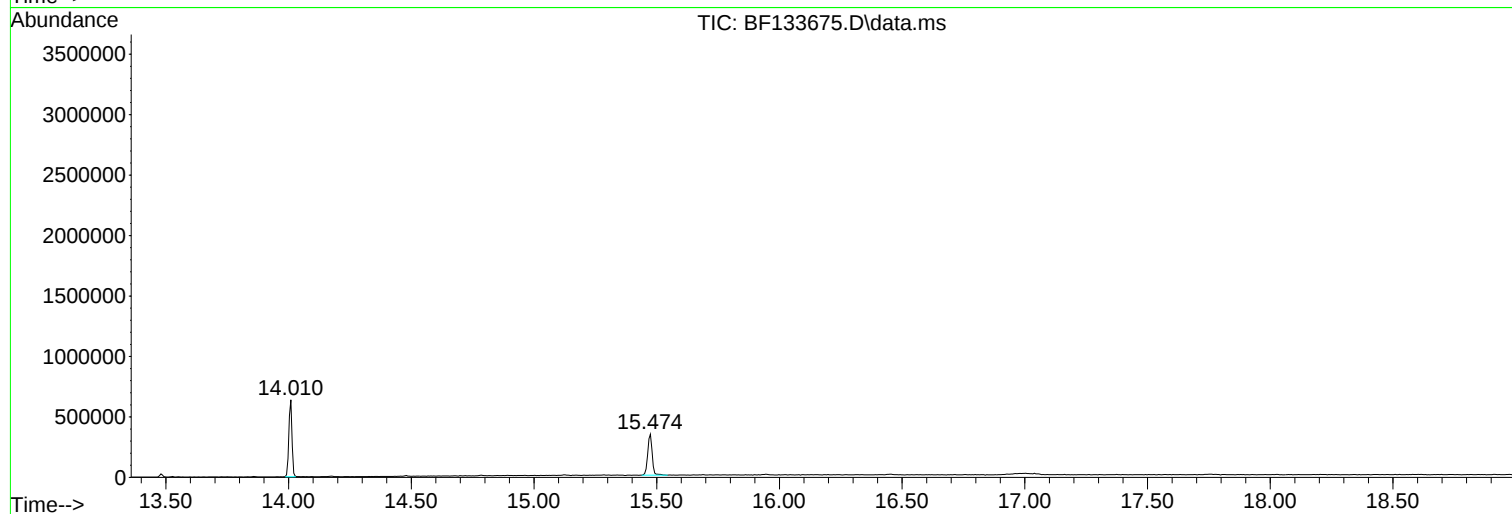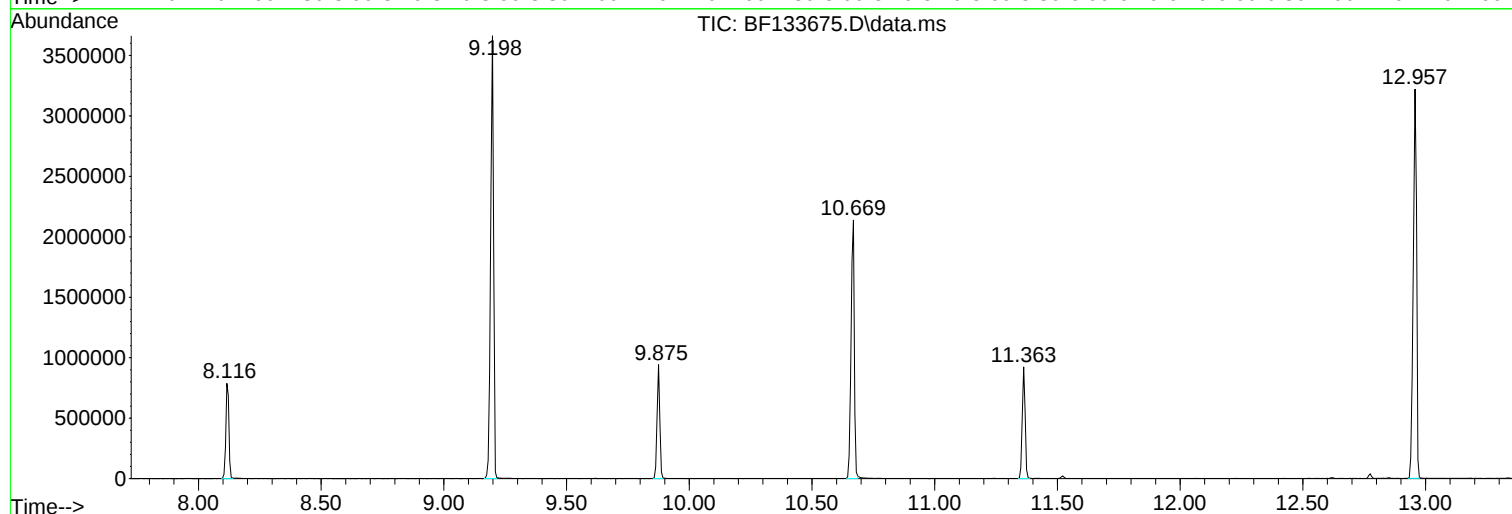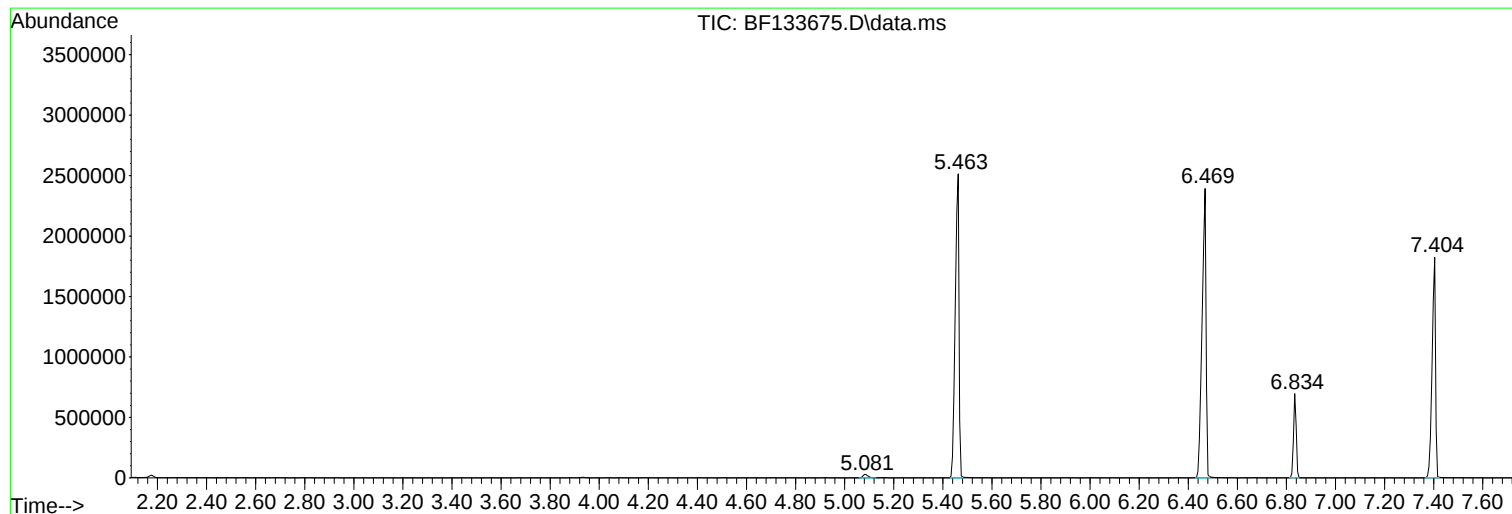

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060923\
Data File : BF133675.D
Acq On : 09 Jun 2023 14:42
Operator : CG\JU
Sample : PB153207BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153207BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060923\
Data File : BF133675.D
Acq On : 09 Jun 2023 14:42
Operator : CG\JU
Sample : PB153207BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153207BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------