


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060923\
Data File : BF133663.D
Acq On : 09 Jun 2023 08:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 09 15:37:41 2023

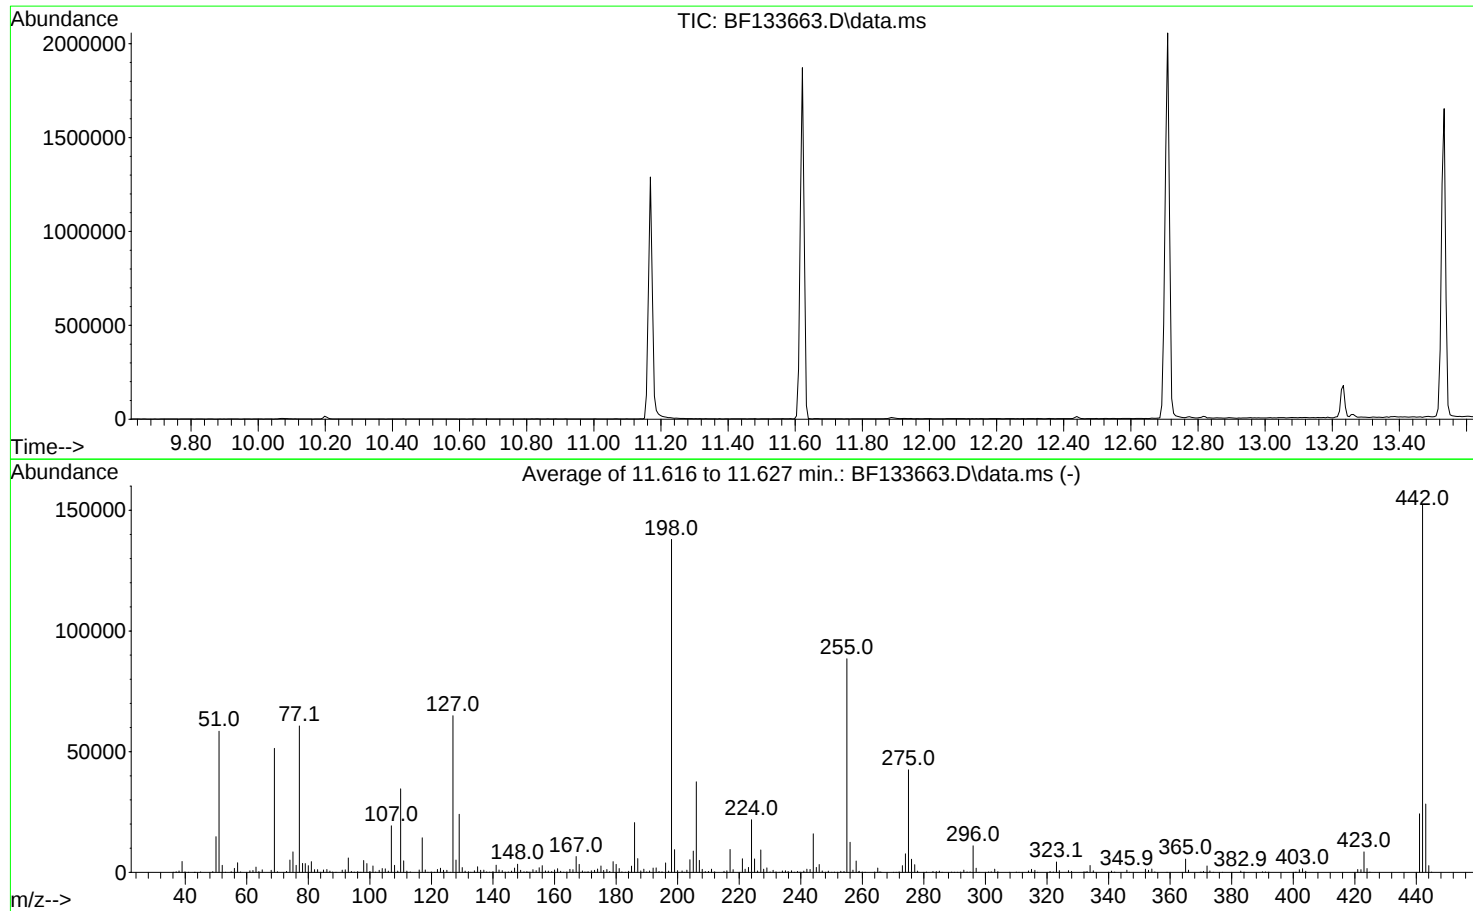




AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	58485	PASS
68	69	0.00	2	1.7	860	PASS
69	198	0.00	100	37.2	51357	PASS
70	69	0.00	2	0.5	254	PASS
127	198	10	80	47.1	64907	PASS
197	198	0.00	2	0.4	513	PASS
198	198	100	100	100.0	137944	PASS
199	198	5	9	6.8	9396	PASS
275	198	10	60	30.8	42464	PASS
365	198	1	100	4.0	5541	PASS
441	198	0.01	100	17.6	24244	PASS
442	442	50	100	100.0	152408	PASS
443	442	15	24	18.6	28309	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060923\
 Data File : BF133663.D
 Acq On : 09 Jun 2023 08:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 09 10:30:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 08 11:43:32 2023
 Response via : Initial Calibration

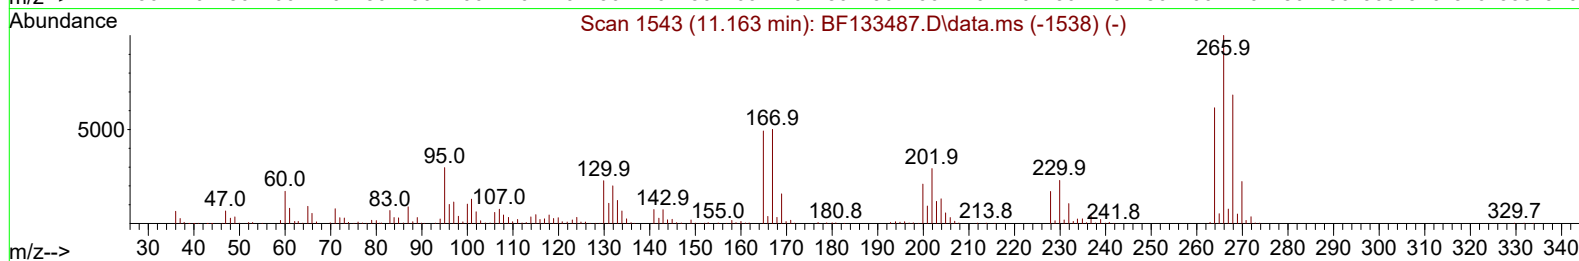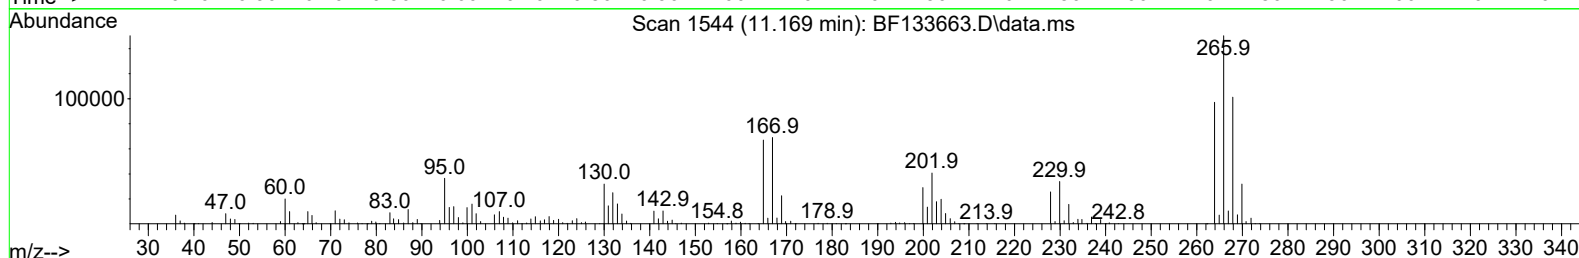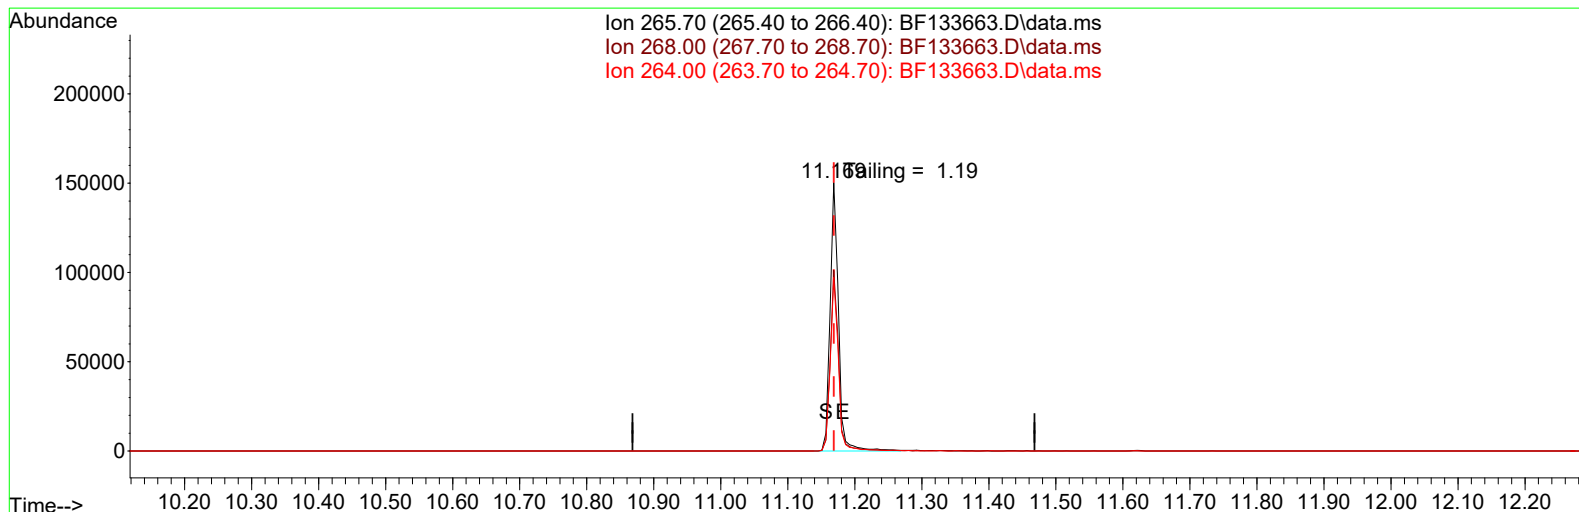

TIC: BF133663.D\data.ms

(70) Pentachlorophenol (C)

11.169min (0.000) 28970.25 ng




response 130624

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.30	67.33
264.00	61.50	64.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060923\
Data File : BF133663.D
Acq On : 09 Jun 2023 08:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 09 10:30:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 08 11:43:32 2023
Response via : Initial Calibration

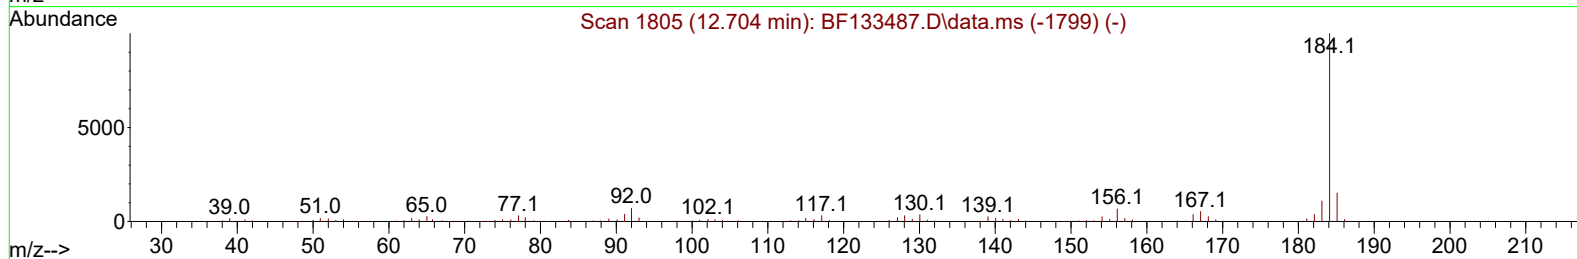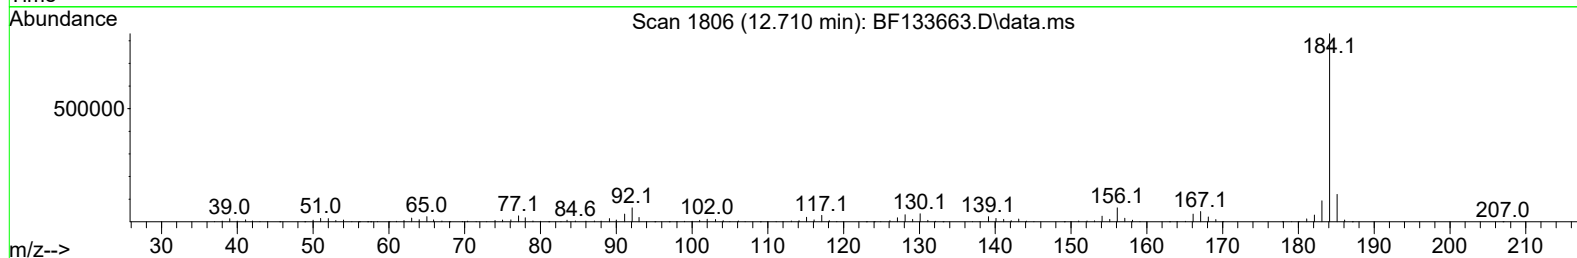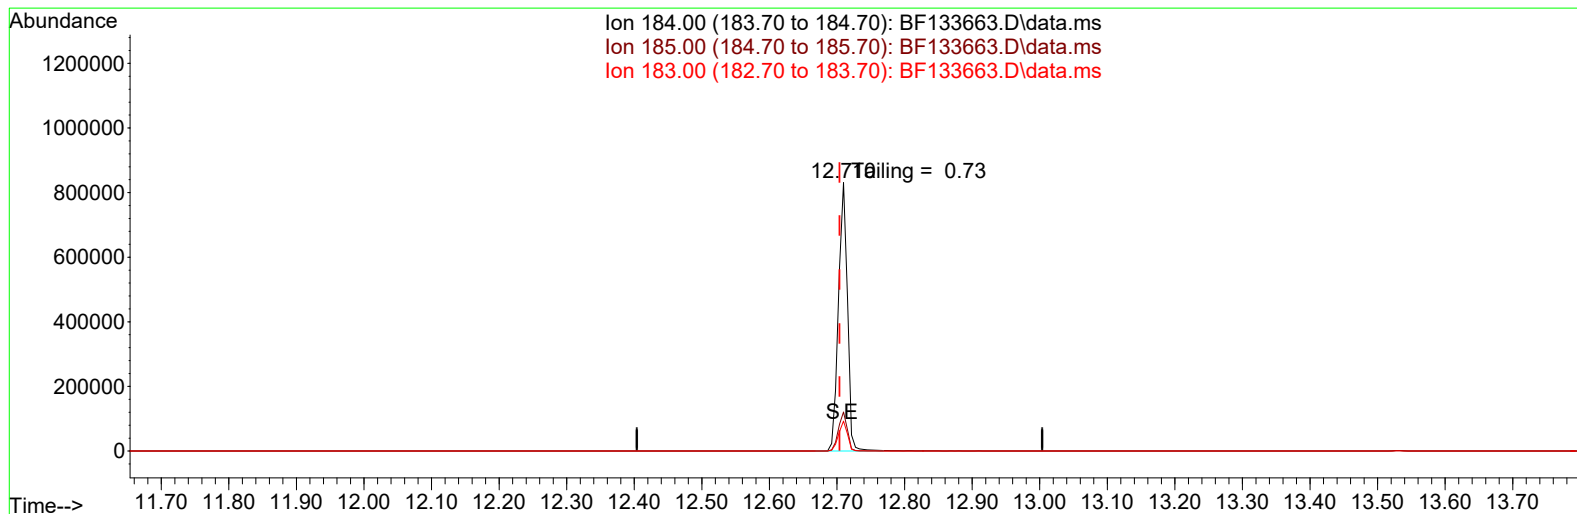

TIC: BF133663.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 486021.22 ng

response 753393

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.56
183.00	10.90	11.16
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/9/2023	BNA_F	<u>BF133663.D</u>
Compound Name	Response	Retention Time
DDT	275247	13.533
DDD	32549	13.233
DDE	458	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33007	308254	10.71

Instrument :
BNA_F
ClientSampleId :
DFTPP