
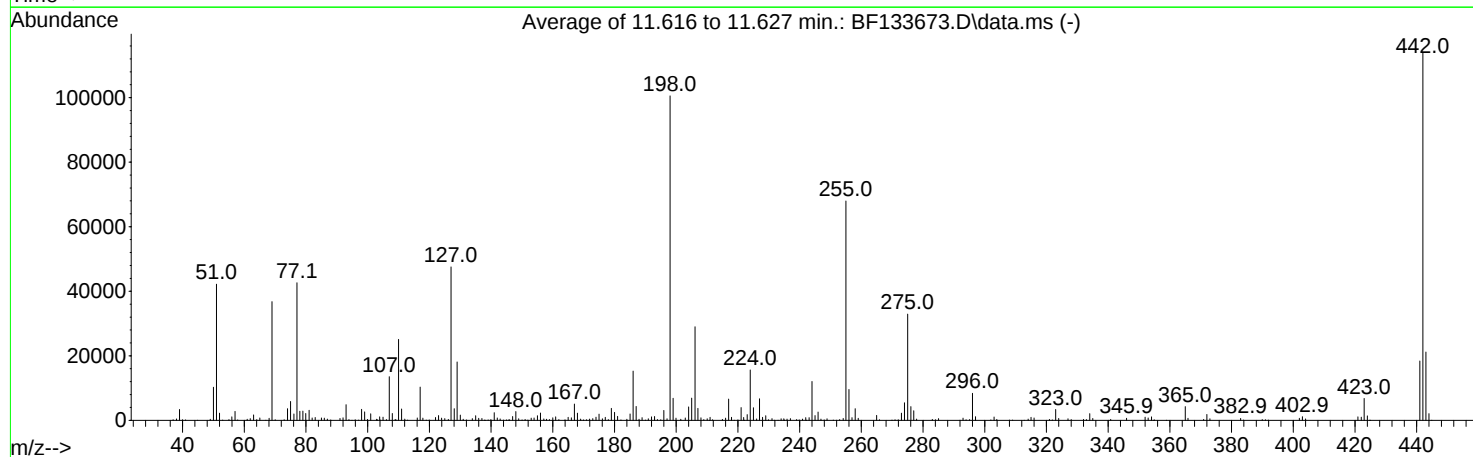


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060923\
 Data File : BF133673.D
 Acq On : 09 Jun 2023 13:38
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 09 15:37:41 2023

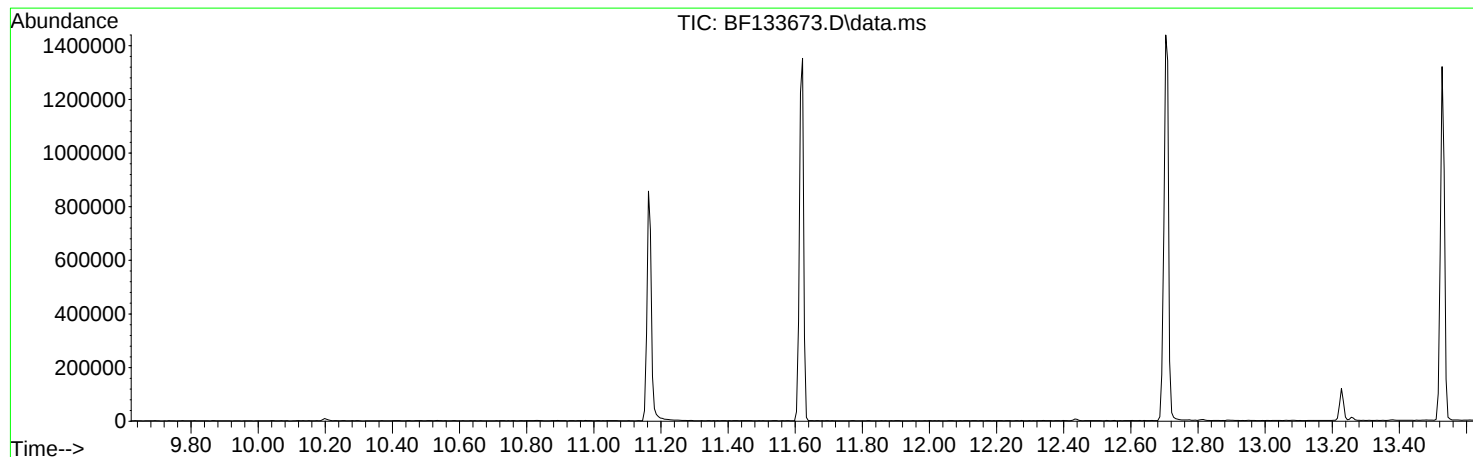

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	42198	PASS
68	69	0.00	2	1.7	643	PASS
69	198	0.00	100	36.6	36787	PASS
70	69	0.00	2	0.5	188	PASS
127	198	10	80	47.3	47554	PASS
197	198	0.00	2	0.5	522	PASS
198	198	100	100	100.0	100555	PASS
199	198	5	9	6.8	6853	PASS
275	198	10	60	32.7	32913	PASS
365	198	1	100	4.2	4255	PASS
441	198	0.01	100	18.3	18386	PASS
442	442	50	100	100.0	113984	PASS
443	442	15	24	18.6	21160	PASS

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/9/2023	BNA_F	<u>BF133673.D</u>
Compound Name	Response	Retention Time
DDT	217062	13.527
DDD	21842	13.227
DDE	398	12.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22240	239302	9.29

Instrument :
BNA_F
ClientSampleId :
DFTPP