


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060923\
 Data File : BF133689.D
 Acq On : 09 Jun 2023 22:12
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 09 15:37:41 2023

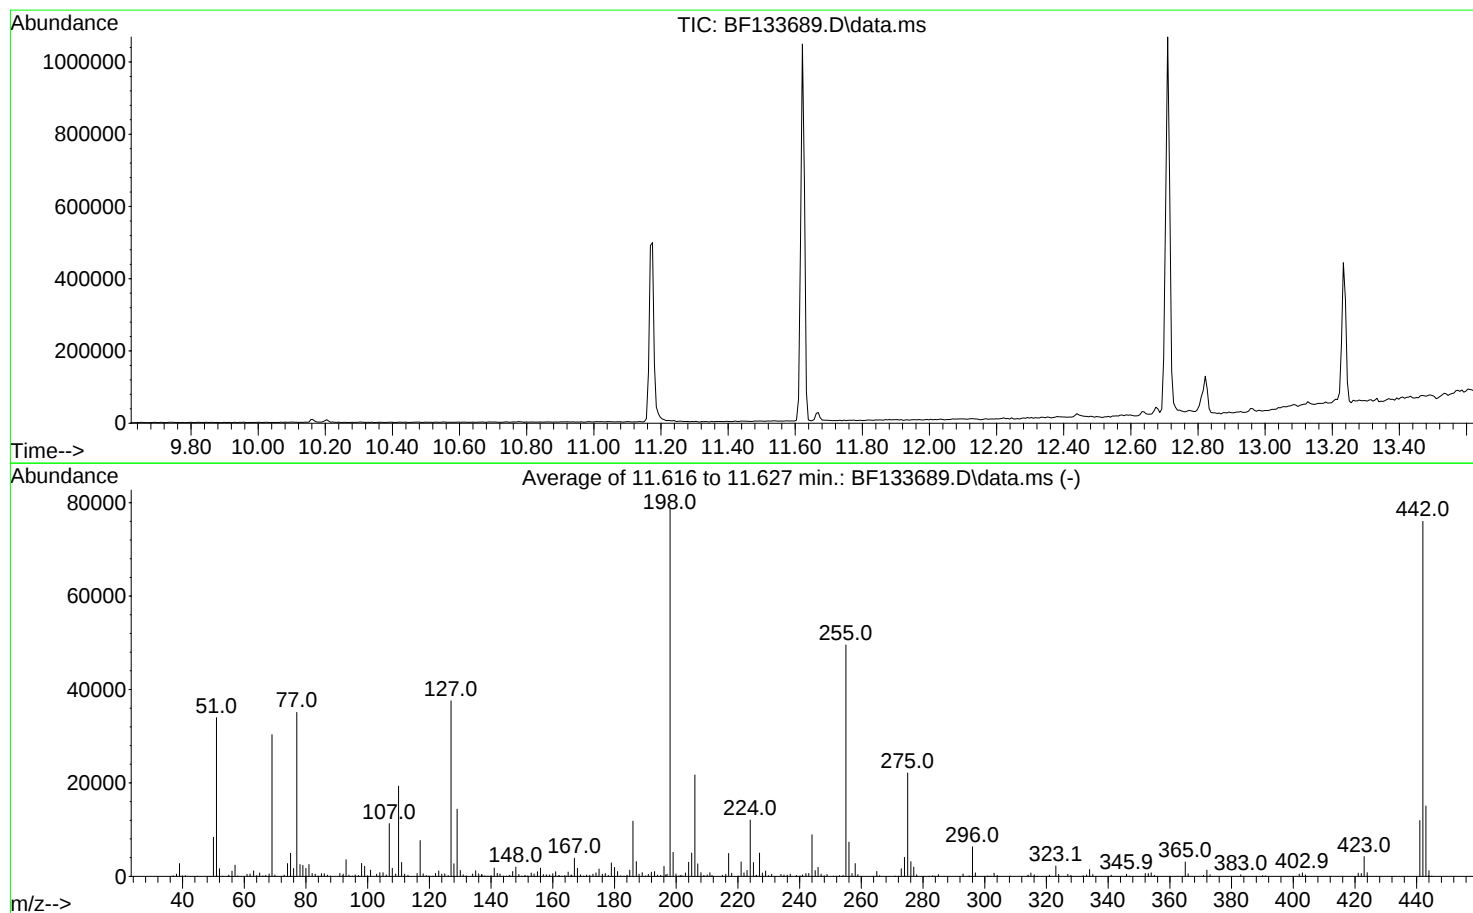

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	33973	PASS
68	69	0.00	2	1.7	514	PASS
69	198	0.00	100	38.5	30339	PASS
70	69	0.00	2	1.0	291	PASS
127	198	10	80	47.7	37579	PASS
197	198	0.00	2	0.6	472	PASS
198	198	100	100	100.0	78752	PASS
199	198	5	9	6.5	5129	PASS
275	198	10	60	28.1	22138	PASS
365	198	1	100	3.9	3098	PASS
441	198	0.01	100	15.2	11971	PASS
442	442	50	100	100.0	76024	PASS
443	442	15	24	19.8	15079	PASS

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/9/2023	BNA_F	<u>BF133689.D</u>
Compound Name	Response	Retention Time
DDT	65313	13.233
DDD	15828	12.821
DDE	65	12.433
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15893	81206	19.57

Instrument :
BNA_F
ClientSampleId :
DFTPP