


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061019\
 Data File : BF114924.D
 Acq On : 10 Jun 2019 10:04
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 10 16:44:00 2019

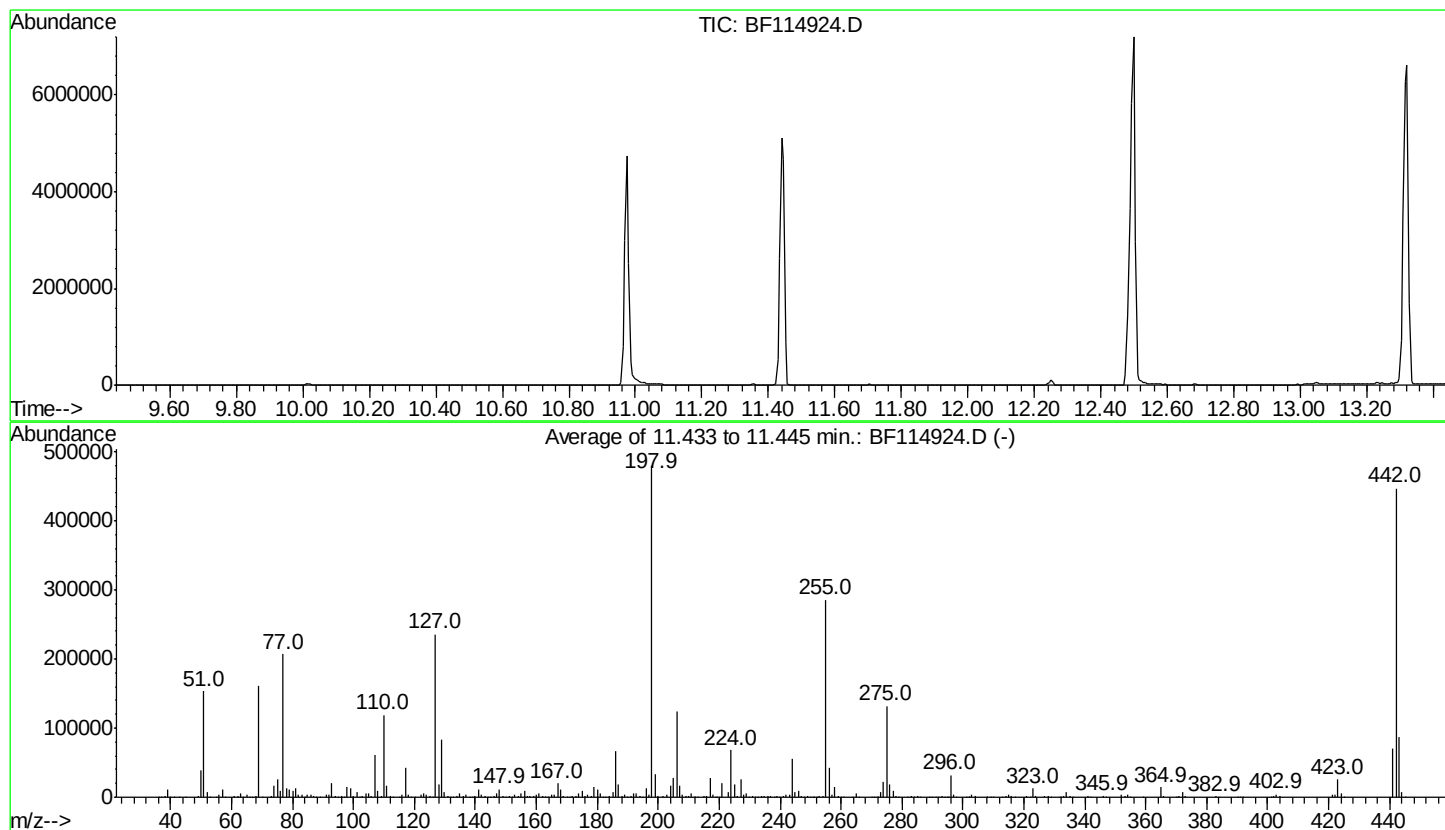

AutoFind: Scans 1589, 1590, 1591; Background Corrected with Scan 1584

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	153037	PASS
68	69	0.00	2	1.7	2670	PASS
69	198	0.00	100	33.5	160640	PASS
70	69	0.00	2	0.5	826	PASS
127	198	10	80	49.0	235072	PASS
197	198	0.00	2	0.7	3117	PASS
198	198	100	100	100.0	479445	PASS
199	198	5	9	6.8	32530	PASS
275	198	10	60	27.6	132237	PASS
365	198	1	100	3.1	14705	PASS
441	198	0.01	100	14.6	70000	PASS
442	198	50	100	93.1	446186	PASS
443	442	15	24	19.3	86325	PASS