

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061118\
 Data File : BF106313.D
 Acq On : 11 Jun 2018 23:36
 Operator : JU/SJ
 Sample : J3422-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SP-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.201	483	487	494	rVB	313345	378621	9.48%	1.008%
2	5.590	548	553	556	rBV	3860151	3915248	98.05%	10.428%
3	6.590	717	723	726	rBV	3817667	3992917	100.00%	10.634%
4	6.737	744	748	752	rBV	3808927	3952364	98.98%	10.526%
5	6.972	784	788	791	rVB	1546984	1235656	30.95%	3.291%
6	7.125	810	814	818	rVB	3204662	3080309	77.14%	8.204%
7	7.531	878	883	886	rBV	2794703	2600148	65.12%	6.925%
8	8.254	1002	1006	1009	rBV	1870590	1501530	37.60%	3.999%
9	9.325	1184	1188	1192	rBV	4144262	3899192	97.65%	10.385%
10	9.719	1251	1255	1258	rBV	572421	486086	12.17%	1.295%
11	9.925	1288	1290	1293	rVB	70856	56048	1.40%	0.149%
12	10.013	1301	1305	1308	rBV	1784162	1494469	37.43%	3.980%
13	10.431	1373	1376	1378	rVB	129813	108215	2.71%	0.288%
14	10.648	1408	1413	1415	rBV	36129	41691	1.04%	0.111%
15	10.801	1435	1439	1442	rBV	2442675	2259354	56.58%	6.017%
16	10.901	1453	1456	1466	rVB	138687	138475	3.47%	0.369%
17	11.348	1529	1532	1535	rBV	67713	52416	1.31%	0.140%
18	11.501	1554	1558	1561	rBV	1591844	1293758	32.40%	3.446%
19	12.007	1641	1644	1650	rBV	206033	227275	5.69%	0.605%
20	12.795	1775	1778	1784	rBV4	45284	45930	1.15%	0.122%
21	13.083	1823	1827	1831	rBV	3638726	3282415	82.21%	8.742%
22	13.613	1914	1917	1921	rBV	58701	54719	1.37%	0.146%
23	13.966	1973	1977	1985	rBV	427248	418595	10.48%	1.115%
24	14.142	2003	2007	2011	rBV	1539491	1394560	34.93%	3.714%
25	14.607	2083	2086	2095	rBV	257346	293355	7.35%	0.781%
26	15.007	2150	2154	2159	rVB	195724	206361	5.17%	0.550%
27	15.283	2198	2201	2203	rBV	40843	42050	1.05%	0.112%
28	15.671	2262	2267	2273	rBV	827756	1045271	26.18%	2.784%
29	16.148	2346	2348	2352	rVB2	44155	49996	1.25%	0.133%


Sum of corrected areas: 37547024

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061118\
Data File : BF106313.D
Acq On : 11 Jun 2018 23:36
Operator : JU/SJ
Sample : J3422-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

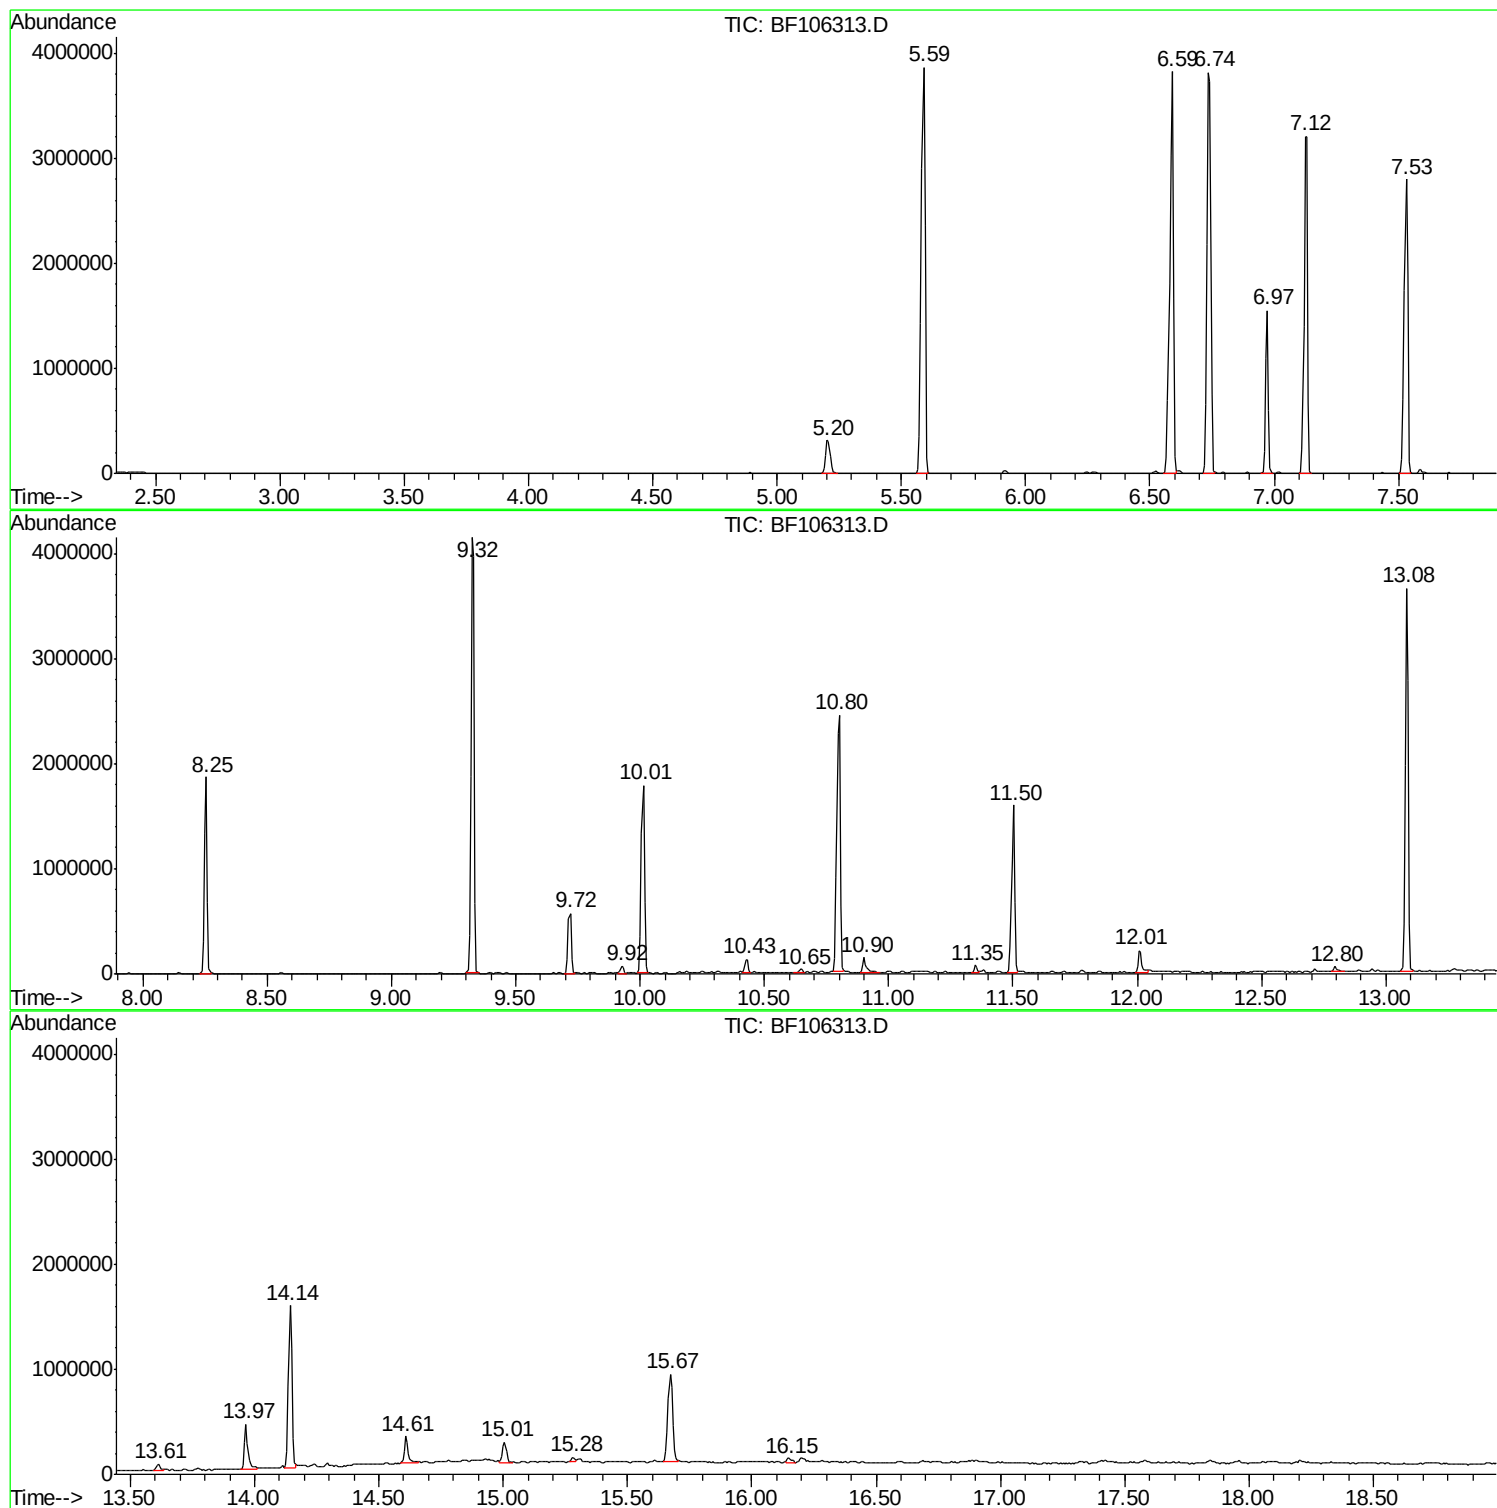

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061118\
Data_File : BF106313.D
Acq_On : 11-Jun-2018 23:366
Operator : JU/SJJ
Sample : J3422-011
Misc :
ALS_Vial : 20 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SP-1

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
