


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061118\
 Data File : BF106285.D
 Acq On : 11 Jun 2018 10:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 11 15:00:22 2018

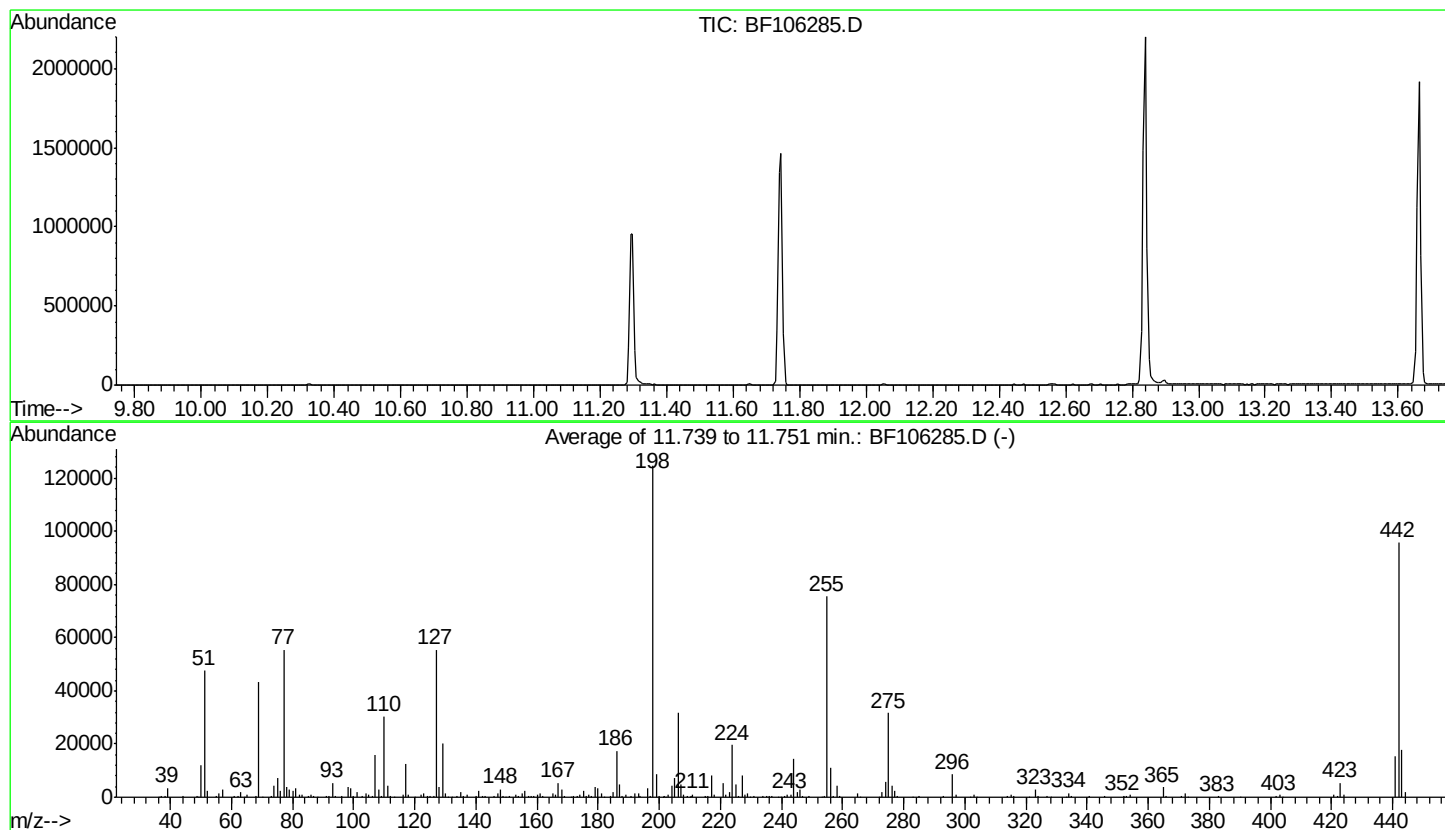

AutoFind: Scans 1641, 1642, 1643; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	47572	PASS
68	69	0.00	2	1.6	692	PASS
69	198	0.00	100	34.6	43081	PASS
70	69	0.00	2	0.3	125	PASS
127	198	10	80	44.5	55517	PASS
197	198	0.00	2	0.5	604	PASS
198	198	100	100	100.0	124640	PASS
199	198	5	9	7.1	8796	PASS
275	198	10	60	25.4	31704	PASS
365	198	1	100	2.9	3671	PASS
441	443	0.01	100	87.1	15371	PASS
442	198	50	100	76.8	95709	PASS
443	442	15	24	18.4	17657	PASS