


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061118\
Data File : BF106294.D
Acq On : 11 Jun 2018 15:04
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 11 15:00:22 2018

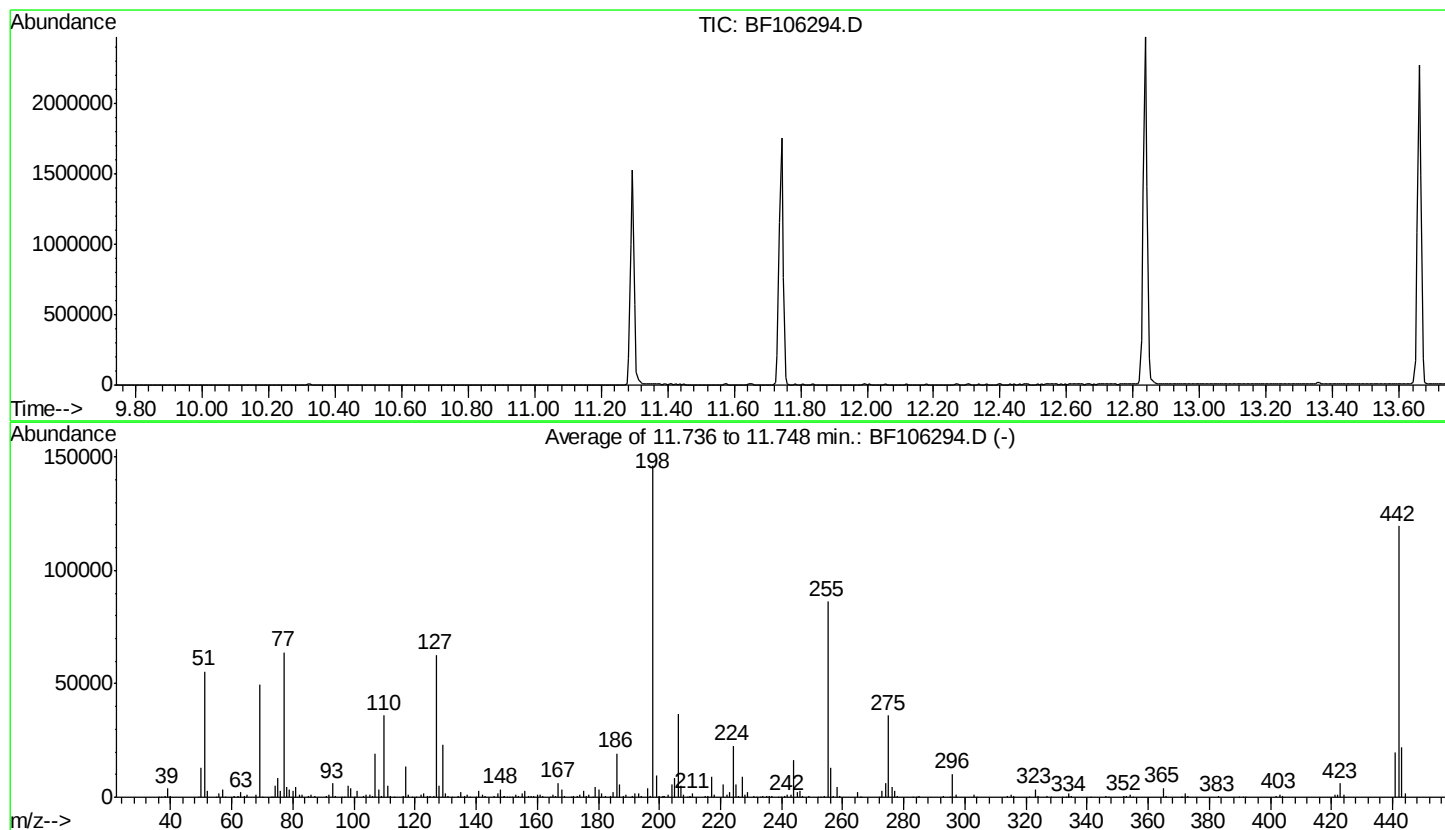

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	55536	PASS
68	69	0.00	2	1.9	929	PASS
69	198	0.00	100	34.1	49936	PASS
70	69	0.00	2	0.5	271	PASS
127	198	10	80	42.9	62690	PASS
197	198	0.00	2	0.4	603	PASS
198	198	100	100	100.0	146266	PASS
199	198	5	9	6.7	9781	PASS
275	198	10	60	24.7	36093	PASS
365	198	1	100	2.8	4083	PASS
441	443	0.01	100	88.8	19559	PASS
442	198	50	100	81.8	119602	PASS
443	442	15	24	18.4	22033	PASS