


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061118\
 Data File : BF106322.D
 Acq On : 12 Jun 2018 4:01
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 11 15:00:22 2018

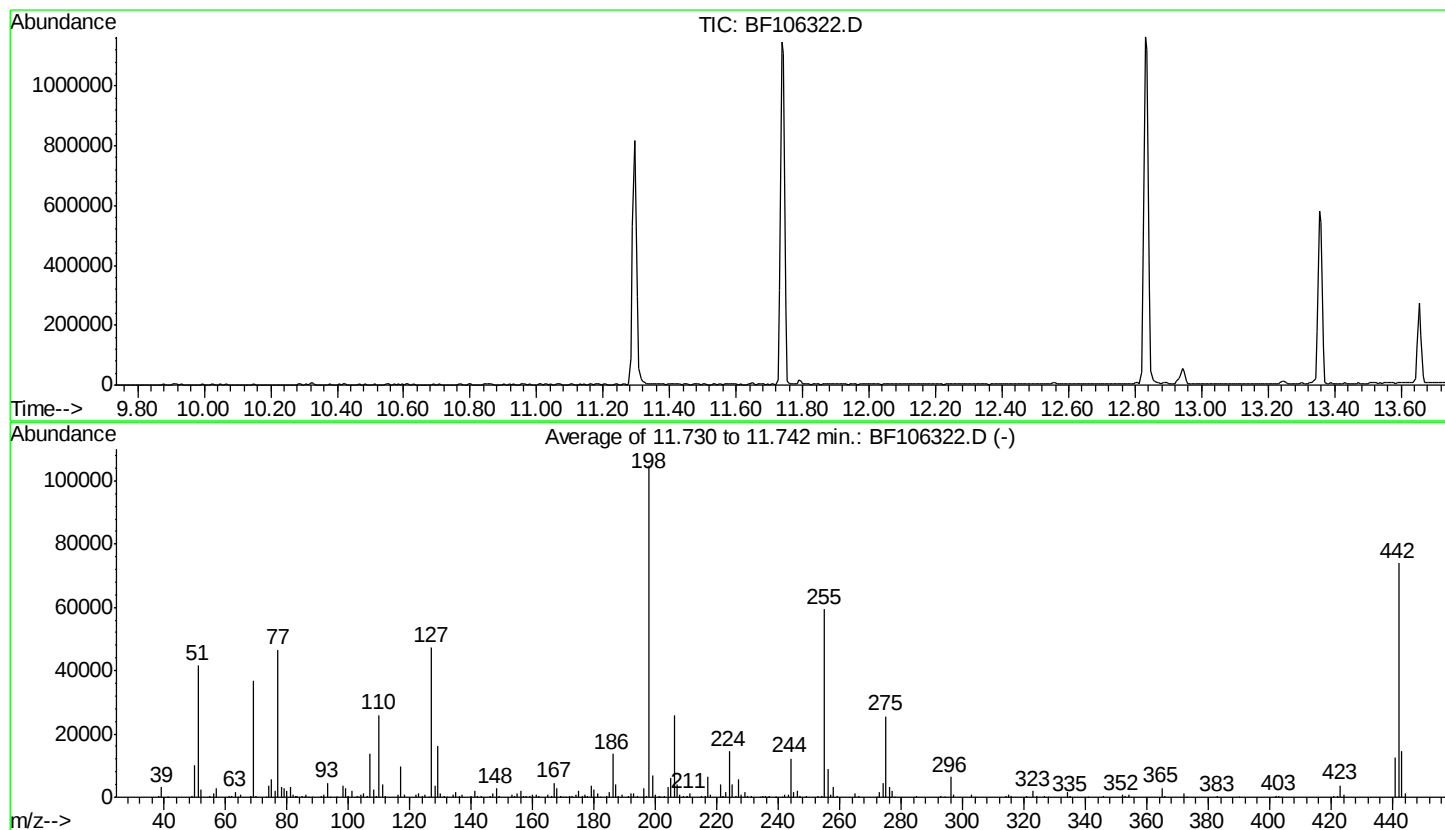

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	41653	PASS
68	69	0.00	2	1.4	506	PASS
69	198	0.00	100	35.1	36813	PASS
70	69	0.00	2	0.7	275	PASS
127	198	10	80	45.0	47194	PASS
197	198	0.00	2	0.5	552	PASS
198	198	100	100	100.0	104802	PASS
199	198	5	9	6.5	6789	PASS
275	198	10	60	24.4	25541	PASS
365	198	1	100	2.8	2929	PASS
441	443	0.01	100	86.8	12656	PASS
442	198	50	100	70.5	73916	PASS
443	442	15	24	19.7	14581	PASS