

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061119\
 Data File : BF114965.D
 Acq On : 12 Jun 2019 1:06
 Operator : HP/JU
 Sample : K3214-01DL 2X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-1ADL

Quant Time: Jun 12 04:35:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 10 16:44:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.67	152	217490	20.00	ng	0.00
21) Naphthalene-d8	7.99	136	688557	20.00	ng	0.05
39) Acenaphthene-d10	9.77	164	19857	20.00	ng	0.08
64) Phenanthrene-d10	11.17	188	612649	20.00	ng	0.01
76) Chrysene-d12	13.79	240	531394	20.00	ng	0.00
87) Perylene-d12	15.17	264	423786	20.00	ng	0.00

System Monitoring Compounds

5) 2-Fluorophenol	5.23	112	36945	2.87	ng	-0.04
7) Phenol-d6	6.33	99	18138	1.17	ng	0.02
23) Nitrobenzene-d5	7.25	82	565821	50.49	ng	0.02
42) 2,4,6-Tribromophenol	10.49	330	239867	1110.46	ng	0.01
45) 2-Fluorobiphenyl	9.06	172	1213750	970.09	ng	0.04
79) Terphenyl-d14	12.75	244	1185997	44.39	ng	0.00

Target Compounds

						Qvalue
3) Pyridine	2.99	79	65756	3.874	ng	99
6) Aniline	6.34	93	1643453	78.272	ng	# 78
9) Benzaldehyde	6.22	77	123007	12.399	ng	# 1
10) Phenol	6.39	94	194305	11.242	ng	82
11) bis(2-Chloroethyl)ether	6.34	93	1643453	119.303	ng	# 28
15) Benzyl Alcohol	6.80	79	72790	6.508	ng	# 52
17) 2-Methylphenol	6.98	107	1806914	147.137	ng	93
18) Hexachloroethane	7.21	117	158618	25.215	ng	# 29
20) 3+4-Methylphenols	6.98	107	1806914	131.410	ng	87
24) Nitrobenzene	7.30	77	106253	9.114	ng	# 29
26) 2-Nitrophenol	7.58	139	16110	2.487	ng	# 1
27) 2,4-Dimethylphenol	7.68	122	5514594	581.859	ng	93
28) bis(2-Chloroethoxy)methane	7.73	93	426158	30.357	ng	# 1
31) Naphthalene	8.06	128	23894882	753.136	ng	# 92
32) Benzoic acid	7.74	122	4819139	680.726	ng	# 22
33) 4-Chloroaniline	8.06	127	4031293	269.252	ng	# 37
36) 4-Chloro-3-methylphenol	8.54	107	823581	81.697	ng	# 18
37) 2-Methylnaphthalene	8.72	142	5813127	269.628	ng	# 94
38) 1-Methylnaphthalene	8.82	142	4347266	213.198	ng	# 98
46) 1,1'-Biphenyl	9.15	154	1069722	720.072	ng	96
47) 2-Chloronaphthalene	9.23	162	134030	106.876	ng	# 1
48) 2-Nitroaniline	9.32	65	297952	780.530	ng	# 15
49) Acenaphthylene	9.58	152	157102	85.010	ng	# 84
50) Dimethylphthalate	9.51	163	105202	70.490	ng	# 1
51) 2,6-Dinitrotoluene	9.56	165	2447	7.139	ng	# 1
52) Acenaphthene	9.75	154	1309259	1169.412	ng	99
53) 3-Nitroaniline	9.75	138	1599	3.885	ng	# 1
54) 2,4-Dinitrophenol	9.87	184	71490	421.373	ng	# 1
55) Dibenzofuran	9.92	168	1496526	936.384	ng	98
56) 4-Nitrophenol	9.92	139	594210	2025.488	ng	# 20
57) 2,4-Dinitrotoluene	9.87	165	30895	71.303	ng	# 1
58) Fluorene	10.25	166	721584	585.714	ng	99
60) Diethylphthalate	10.17	149	41333	28.495	ng	# 71
61) 4-Chlorophenyl-phenylether	10.30	204	1613	2.615	ng	# 1


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061119\
 Data File : BF114965.D
 Acq On : 12 Jun 2019 1:06
 Operator : HP/JU
 Sample : K3214-01DL 2X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-1ADL

Quant Time: Jun 12 04:35:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 10 16:44:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
62) 4-Nitroaniline	10.53	138	4396	10.421	nq	85
63) Azobenzene	10.47	77	190372	150.787	nq #	67
65) 4,6-Dinitro-2-methylphenol	10.32	198	25742	7.492	nq #	70
66) n-Nitrosodiphenylamine	10.12	169	57279	3.147	nq	90
67) 4-Bromophenyl-phenylether	10.49	248	15450	2.328	nq #	1
71) Phenanthrene	11.20	178	518936	17.458	nq	97
72) Anthracene	11.20	178	518936	17.201	nq	99
73) Carbazole	11.42	167	463433	16.872	nq	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

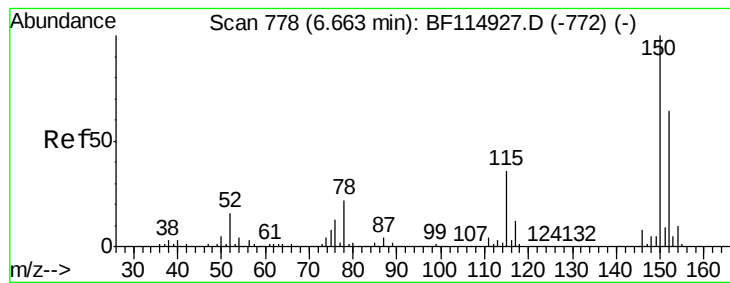

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 6.67 min Scan# 779

Delta R.T. 0.01 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06

Instrument :

BNA_F

ClientSampleId :

MW-1ADL


Tot Ion:152 Resp: 217490

Ion Ratio Lower Upper

152 100

150 152.9 125.2 187.8




115 59.1 45.0 67.4



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

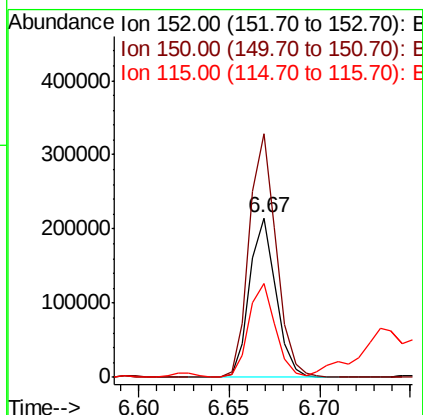

#3

Pyridine

Concen: 3.874 ng

RT: 2.99 min Scan# 154

Delta R.T. 0.02 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06


Tgt Ion: 79 Resp: 65756

Ion Ratio Lower Upper

79 100

52 62.2 50.2 75.2



51 29.3 24.6 37.0




Abundance Ion 79.00 (78.70 to 79.70): BF1

Ion 52.00 (51.70 to 52.70): BF1

Ion 51.00 (50.70 to 51.70): BF1

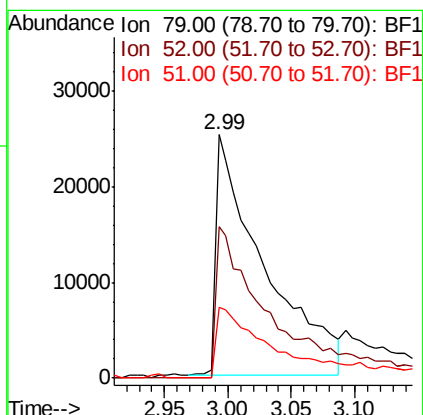

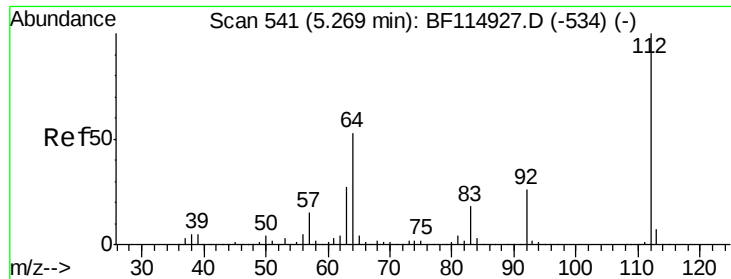

#5

2-Fluorophenol

Concen: 2.875 ng

RT: 5.23 min Scan# 535

Delta R.T. -0.04 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06

Instrument :

BNA_F

ClientSampleId :

MW-1ADL


Tot Ion: 112 Resp: 36945

Ion Ratio Lower Upper

112 100

64 110.1 42.1 63.1#




63 544.6 21.8 32.8#

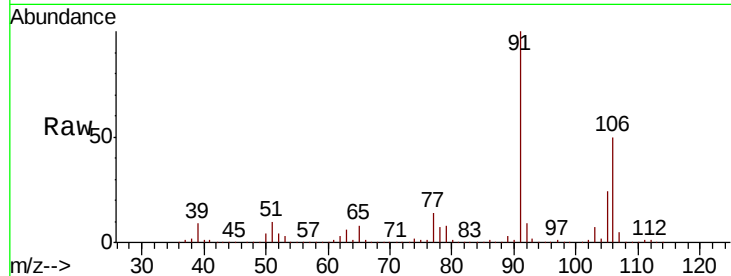

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

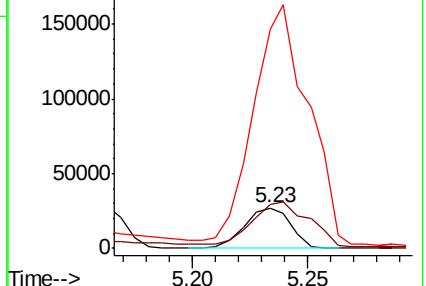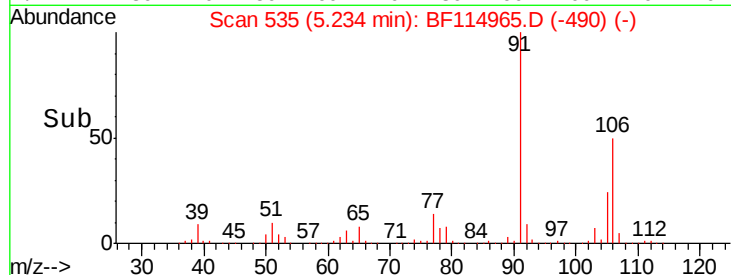

#6

Aniline

Concen: 78.272 ng

RT: 6.34 min Scan# 723

Delta R.T. 0.01 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06


Tgt Ion: 93 Resp: 1643453

Ion Ratio Lower Upper

93 100

66 38.1 43.6 65.4#



65 20.6 25.7 38.5#




Abundance Ion 93.00 (92.70 to 93.70): BF1

Ion 66.00 (65.70 to 66.70): BF1

Ion 65.00 (64.70 to 65.70): BF1

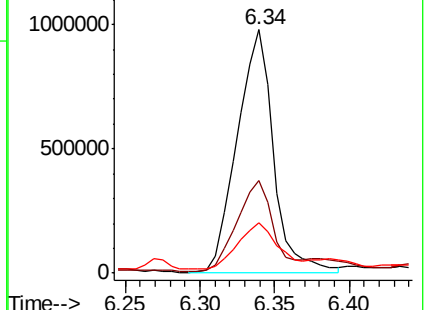



#7

Phenol-d6

Concen: 1.170 ng

RT: 6.33 min Scan# 721

Delta R.T. 0.02 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06

Instrument :

BNA_F

ClientSampleId :

MW-1ADL


Tot Ion: 99 Resp: 18138

Ion Ratio Lower Upper

99 100

42 77.3 13.1 19.7#




71 44.3 26.8 40.2#



Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

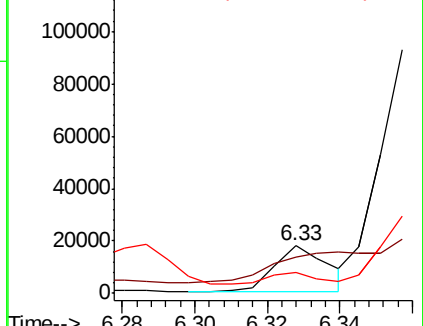

#9

Benzaldehyde

Concen: 12.399 ng

RT: 6.22 min Scan# 703

Delta R.T. 0.02 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06


Tgt Ion: 77 Resp: 123007

Ion Ratio Lower Upper

77 100

105 724.2 84.5 124.5#



106 100.2 79.2 119.2




Abundance Ion 77.00 (76.70 to 77.70): BF1

Ion 105.00 (104.70 to 105.70): E

Ion 106.00 (105.70 to 106.70): E

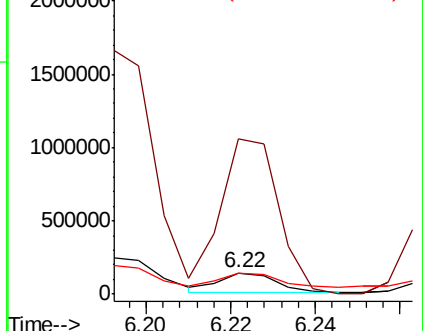



#10

Phenol

Concen: 11.242 ng

RT: 6.39 min Scan# 731

Delta R.T. 0.06 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06

Instrument :

BNA_F

ClientSampleId :

MW-1ADL


Tot Ion: 94 Resp: 194305

Ion Ratio Lower Upper




94 100

65 56.7 19.6 59.6

66 53.5 42.6 82.6



Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

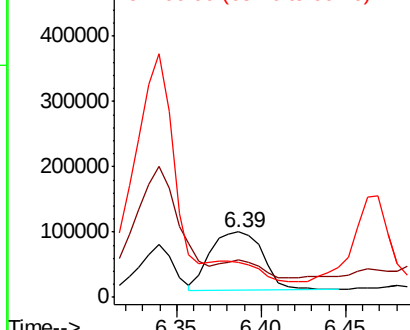

#11

bis(2-Chloroethyl)ether

Concen: 119.303 ng

RT: 6.34 min Scan# 723

Delta R.T. -0.06 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06


Tgt Ion: 93 Resp: 1643453

Ion Ratio Lower Upper



93 100




63 5.7 50.5 90.5#

95 0.3 13.6 53.6#



Abundance Ion 93.00 (92.70 to 93.70): BF1
Ion 63.00 (62.70 to 63.70): BF1
Ion 95.00 (94.70 to 95.70): BF1

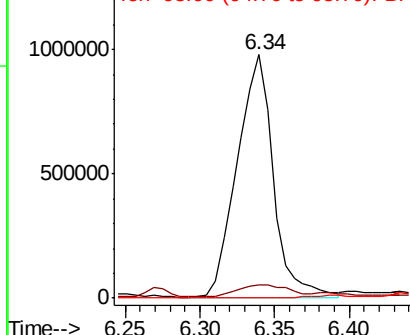

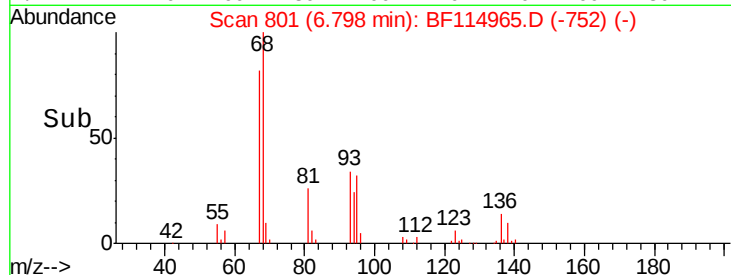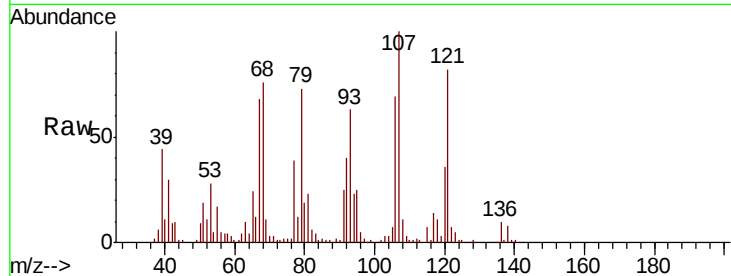

#15

Benzyl Alcohol

Concen: 6.508 ng

RT: 6.80 min Scan# 801

Delta R.T. -0.01 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06

Instrument :

BNA_F

ClientSampleId :

MW-1ADL





Tot Ion: 79 Resp: 72790

Ion Ratio Lower Upper

79 100

108 14.7 65.5 98.3#

77 54.1 51.3 76.9

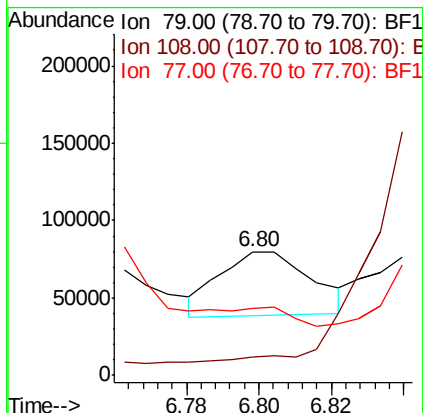

#17

2-Methylphenol

Concen: 147.137 ng

RT: 6.98 min Scan# 832

Delta R.T. 0.05 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06

Tgt Ion: 107 Resp: 1806914


Ion Ratio Lower Upper


107 100

108 101.6 90.2 135.2

77 43.8 35.4 53.0

79 45.8 34.6 52.0




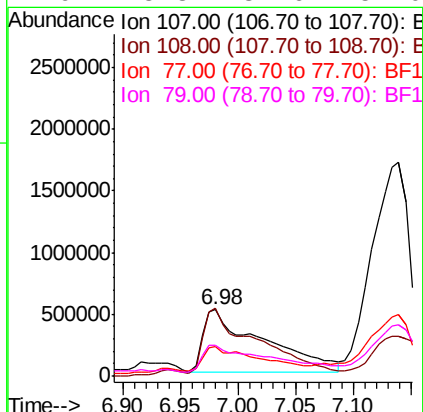




#18
Hexachloroethane
Concen: 25.215 ng
RT: 7.21 min Scan# 871
Delta R.T. 0.04 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06




Instrument :
BNA_F
ClientSampleId :
MW-1ADL


Tot Ion:117 Resp: 158618
Ion Ratio Lower Upper
117 100
119 137.1 76.6 114.8#
201 0.0 77.0 115.6#

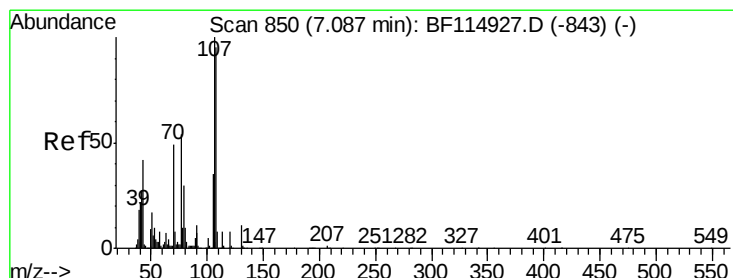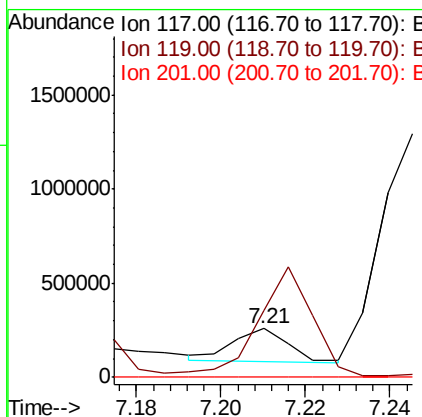

#20
3+4-Methylphenols
Concen: 131.410 ng
RT: 6.98 min Scan# 832
Delta R.T. -0.11 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06

Tgt Ion:107 Resp: 1806914
Ion Ratio Lower Upper
107 100
108 101.6 74.7 114.7
77 43.8 33.7 73.7
79 45.8 10.2 50.2

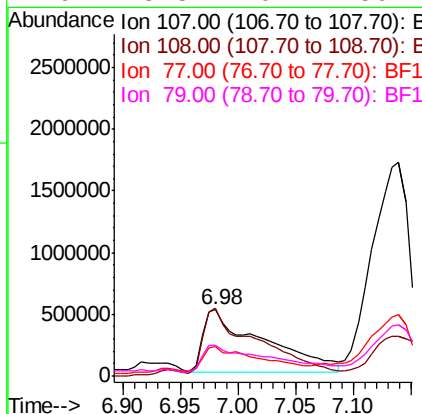



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.99 min Scan# 1004

Delta R.T. 0.05 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06

Instrument :

BNA_F

ClientSampleId :

MW-1ADL

Tot Ion:136 Resp: 688557





Ion Ratio Lower Upper

136 100

137 10.9 9.0 13.6

54 4.2 5.2 7.8#

68 2.6 4.6 7.0#

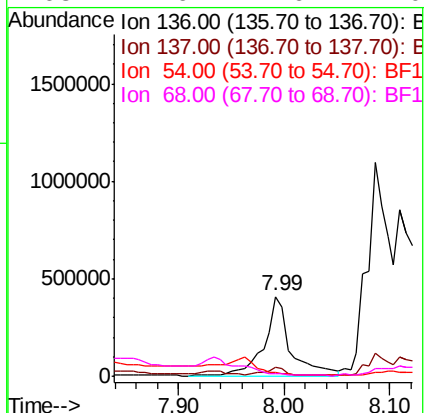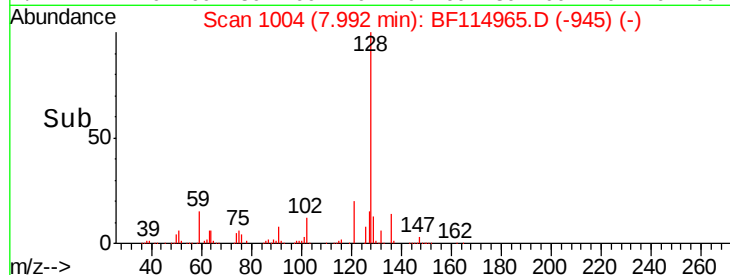

#23

Nitrobenzene-d5

Concen: 50.490 ng

RT: 7.25 min Scan# 877

Delta R.T. 0.02 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06




Tgt Ion: 82 Resp: 565821


Ion Ratio Lower Upper

82 100

128 64.9 40.9 61.3#

54 48.8 37.4 56.0

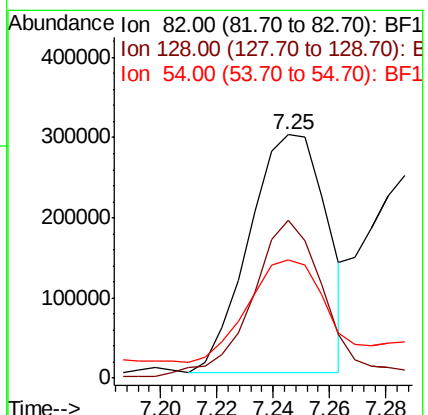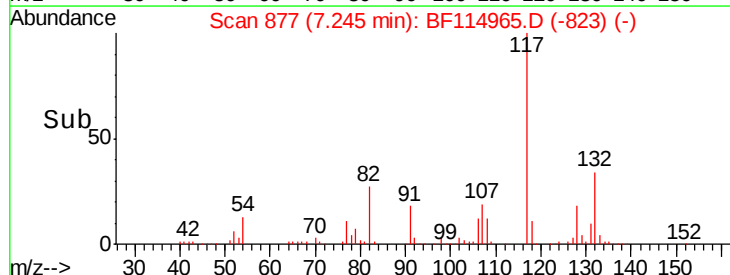



#24

Nitrobenzene

Concen: 9.114 ng

RT: 7.30 min Scan# 886

Delta R.T. 0.05 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06

Instrument :

BNA_F

ClientSampleId :

MW-1ADL


Tot Ion: 77 Resp: 106253

Ion Ratio Lower Upper

77 100

123 10.9 39.8 59.6#




65 62.6 10.7 16.1#



Abundance Ion 77.00 (76.70 to 77.70): BF1

Ion 123.00 (122.70 to 123.70): BF1

Ion 65.00 (64.70 to 65.70): BF1

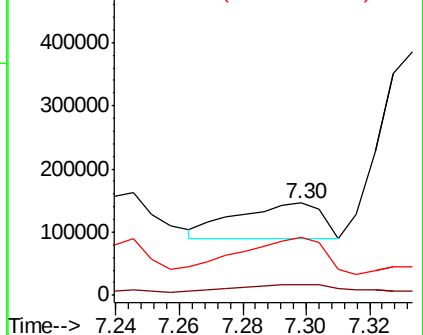

#26

2-Nitrophenol

Concen: 2.487 ng

RT: 7.58 min Scan# 934

Delta R.T. 0.02 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06


Tgt Ion: 139 Resp: 16110

Ion Ratio Lower Upper

139 100

109 169.1 20.6 30.8#



65 357.1 32.2 48.2#




Abundance Ion 139.00 (138.70 to 139.70): BF1

Ion 109.00 (108.70 to 109.70): BF1

Ion 65.00 (64.70 to 65.70): BF1

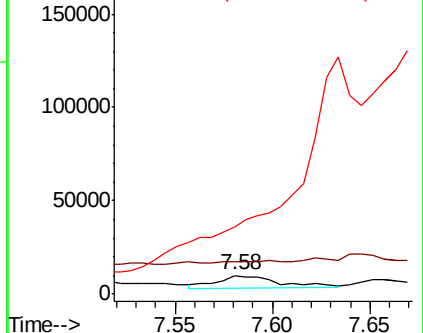


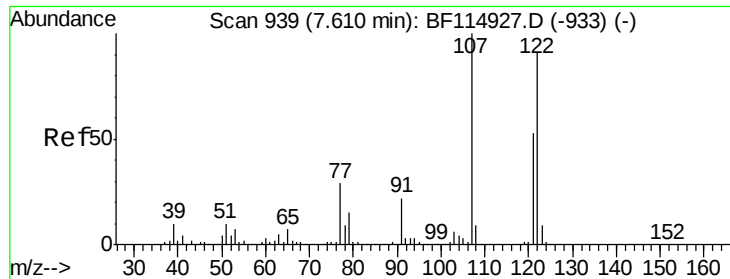




#27
2,4-Dimethylphenol
Concen: 581.859 ng
RT: 7.68 min Scan# 951
Delta R.T. 0.07 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06

Instrument :
BNA_F
ClientSampleId :
MW-1ADL

Tot Ion:122 Resp: 5514594
Ion Ratio Lower Upper
122 100
107 120.2 88.0 132.0
121 57.2 47.0 70.6




Abundance Ion 122.00 (121.70 to 122.70): E
Ion 107.00 (106.70 to 107.70): E
Ion 121.00 (120.70 to 121.70): E


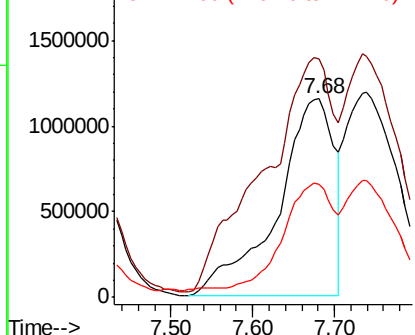



#28
bis(2-Chloroethoxy)methane
Concen: 30.357 ng
RT: 7.73 min Scan# 959
Delta R.T. 0.02 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06

Tgt Ion: 93 Resp: 426158
Ion Ratio Lower Upper
93 100
95 321.8 27.0 40.4#
123 140.3 10.3 15.5#



Abundance Ion 93.00 (92.70 to 93.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 123.00 (122.70 to 123.70): E

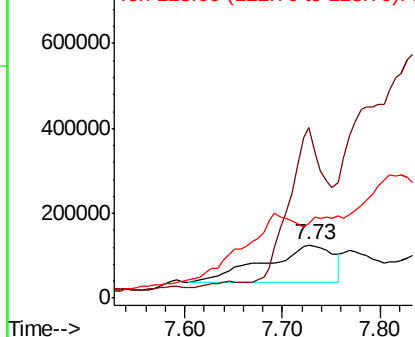

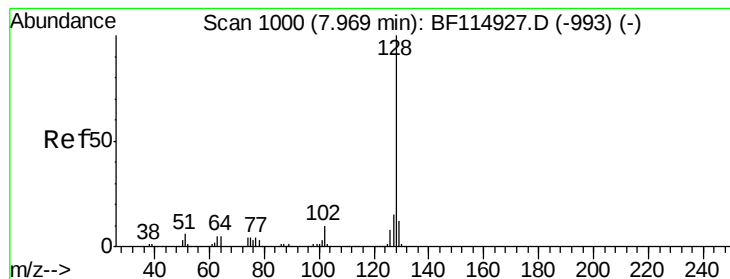

#31

Naphthalene

Concen: 753.136 ng

RT: 8.06 min Scan# 1016

Delta R.T. 0.09 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06

Instrument :

BNA_F

ClientSampleId :

MW-1ADL


Tot Ion:128 Resp:23894882

Ion Ratio Lower Upper

128 100

129 15.1 9.8 14.8#




127 18.3 11.8 17.6#



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

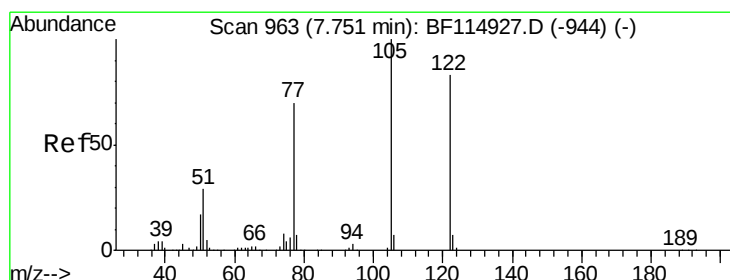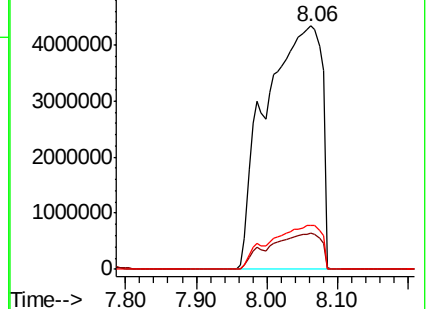

#32

Benzoic acid

Concen: 680.726 ng

RT: 7.74 min Scan# 961

Delta R.T. -0.01 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06


Tgt Ion:122 Resp: 4819139

Ion Ratio Lower Upper

122 100

105 5.1 97.7 137.7#



77 43.4 63.0 103.0#




Abundance Ion 122.00 (121.70 to 122.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BF1




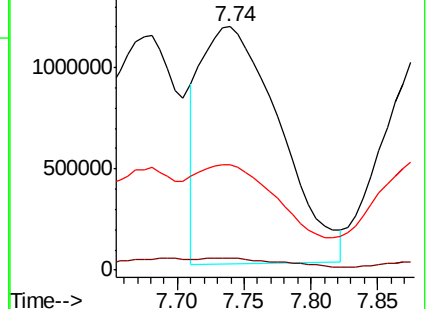




#33
4-Chloroaniline
Concen: 269.252 ng
RT: 8.06 min Scan# 1016
Delta R.T. 0.05 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06




Instrument :
BNA_F
ClientSampleId :
MW-1ADL


Tot Ion:127 Resp: 4031293
Ion Ratio Lower Upper
127 100
129 82.3 26.6 40.0#
65 0.0 21.5 32.3#
92 1.8 14.7 22.1#

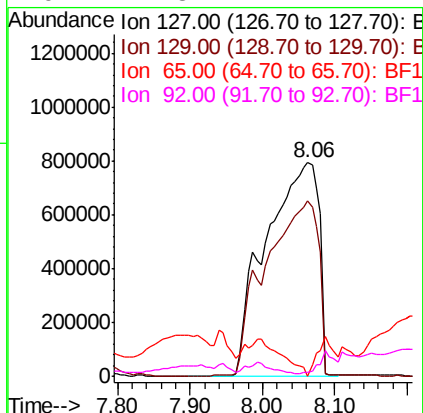

#36
4-Chloro-3-methylphenol
Concen: 81.697 ng
RT: 8.54 min Scan# 1097
Delta R.T. 0.04 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06

Tgt Ion:107 Resp: 823581
Ion Ratio Lower Upper
107 100
144 0.3 21.6 32.4#
142 0.1 66.1 99.1#


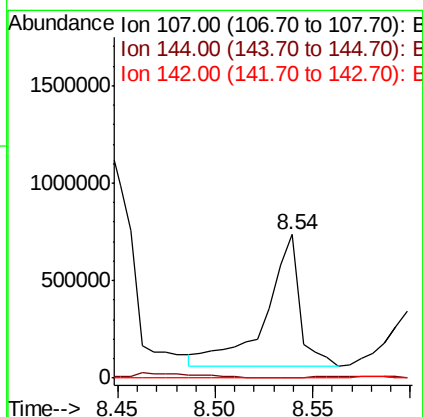




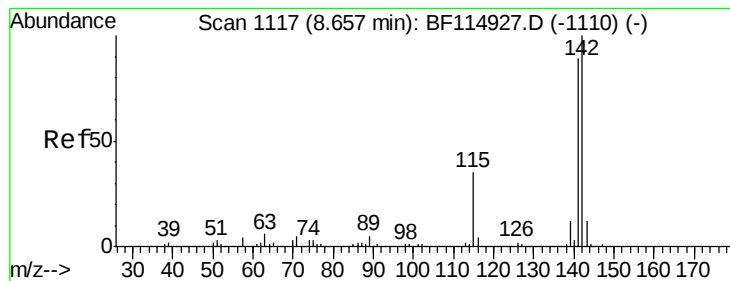

#37
2-Methylnaphthalene
Concen: 269.628 ng
RT: 8.72 min Scan# 1128
Delta R.T. 0.06 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06




Instrument :
BNA_F
ClientSampled :
MW-1ADL


Tot Ion:142 Resp: 5813127
Ion Ratio Lower Upper
142 100
141 90.2 71.1 106.7
115 44.5 27.8 41.6#

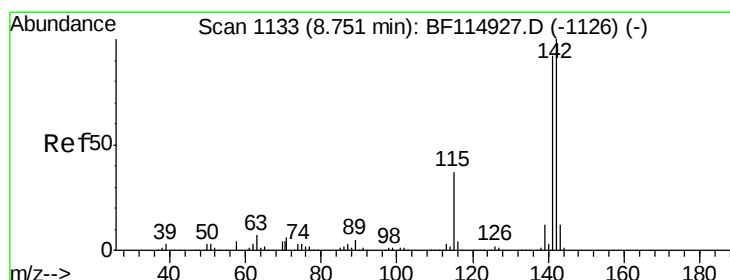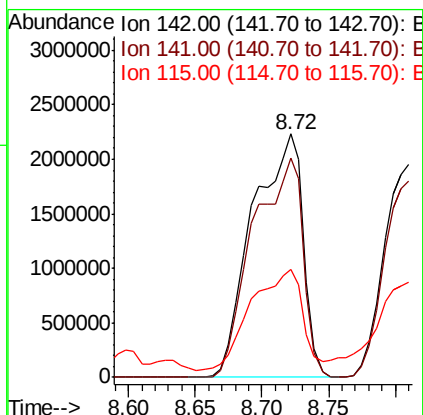

#38
1-Methylnaphthalene
Concen: 213.198 ng
RT: 8.82 min Scan# 1144
Delta R.T. 0.06 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06

Tgt Ion:142 Resp: 4347266
Ion Ratio Lower Upper
142 100
141 93.6 73.7 110.5
116 4.9 3.1 4.7#

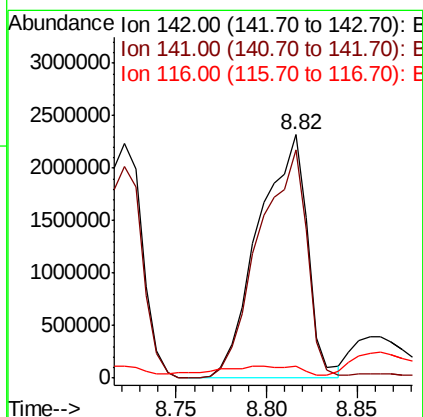



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.77 min Scan# 1306

Delta R.T. 0.08 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06

Instrument :

BNA_F

ClientSampleId :

MW-1ADL


Tot Ion:164 Resp: 19857

Ion Ratio Lower Upper




164 100

162 1253.6 82.4 123.6#

160 36.9 37.5 56.3#



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

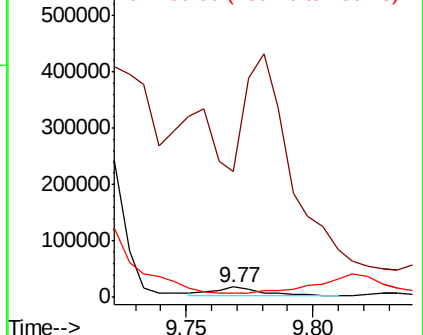

#42

2,4,6-Tribromophenol

Concen: 1110.462 ng

RT: 10.49 min Scan# 1429

Delta R.T. 0.01 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06


Tgt Ion:330 Resp: 239867

Ion Ratio Lower Upper



330 100


332 96.8 76.4 114.6

141 80.1 26.8 40.2#



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

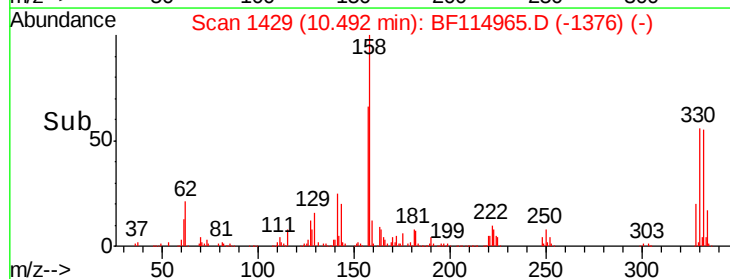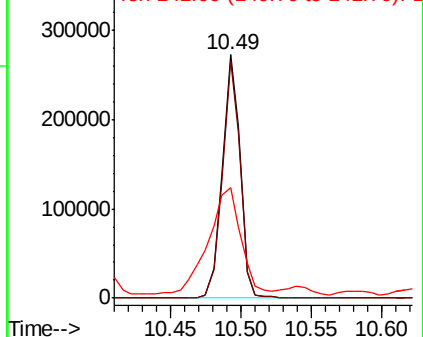


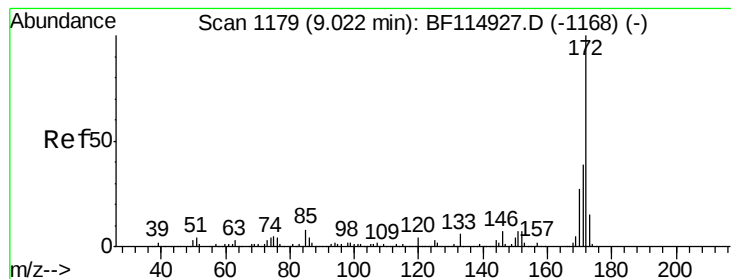




#45
2-Fluorobiphenyl
Concen: 970.087 ng
RT: 9.06 min Scan# 1185
Delta R.T. 0.04 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06

Instrument :
BNA_F
ClientSampleId :
MW-1ADL

Tot Ion:172 Resp: 1213750
Ion Ratio Lower Upper
172 100
171 35.5 31.3 46.9
170 23.8 21.4 32.0




Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

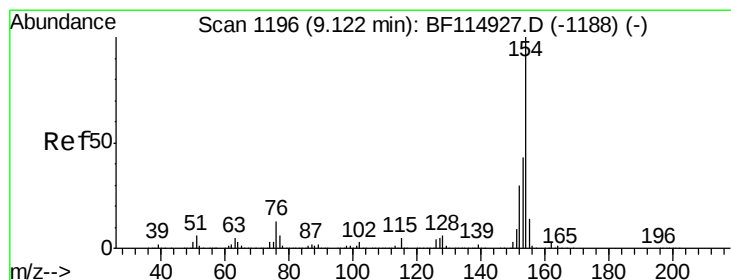
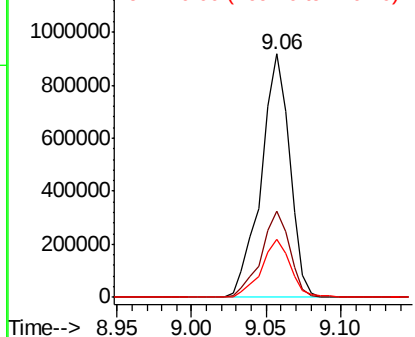



#46
1,1'-Biphenyl
Concen: 720.072 ng
RT: 9.15 min Scan# 1201
Delta R.T. 0.03 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06

Tgt Ion:154 Resp: 1069722
Ion Ratio Lower Upper
154 100
153 40.6 22.8 62.8
76 15.5 0.0 33.0



Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 76.00 (75.70 to 76.70): BF1



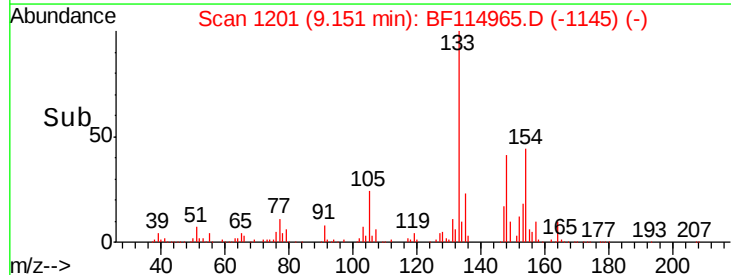
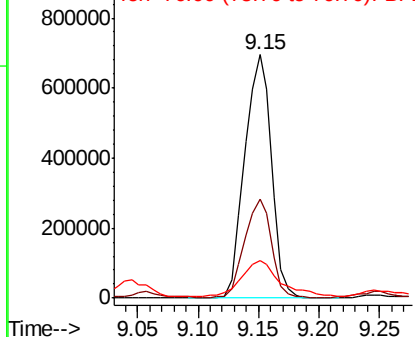




#47
 2-Chloronaphthalene
 Concen: 106.876 ng
 RT: 9.23 min Scan# 1214
 Delta R.T. 0.09 min
 Lab File: BF114965.D
 Acq: 12 Jun 2019 1:06




Instrument :
 BNA_F
 ClientSampleId :
 MW-1ADL


Tot Ion: 162 Resp: 134030
 Ion Ratio Lower Upper
 162 100
 127 20.9 34.6 51.8#
 164 146.2 27.5 41.3#

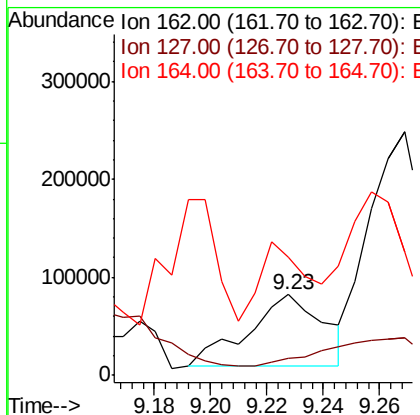

#48
 2-Nitroaniline
 Concen: 780.530 ng
 RT: 9.32 min Scan# 1230
 Delta R.T. 0.08 min
 Lab File: BF114965.D
 Acq: 12 Jun 2019 1:06

Tgt Ion: 65 Resp: 297952
 Ion Ratio Lower Upper
 65 100
 92 45.3 61.9 92.9#
 138 1.8 108.6 162.8#

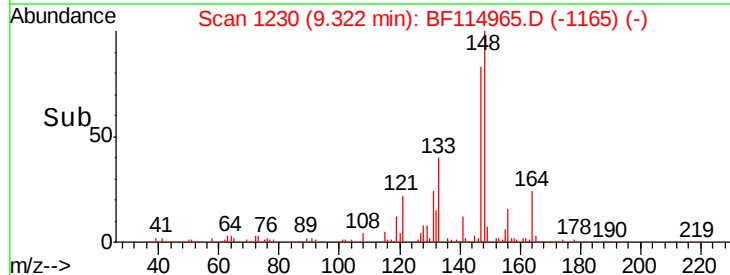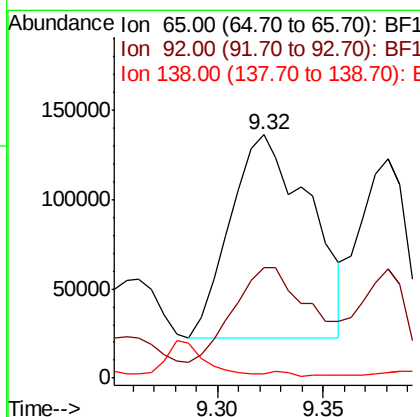

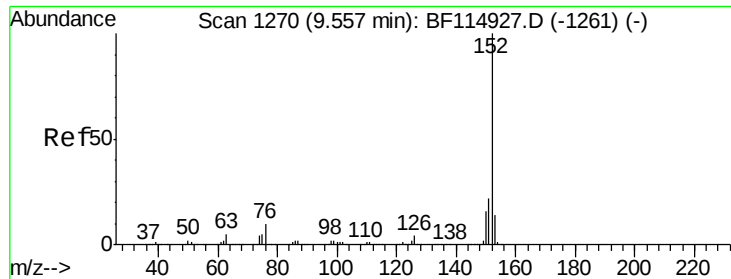

#49

Acenaphthylene

Concen: 85.010 ng

RT: 9.58 min Scan# 1274

Delta R.T. 0.02 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06

Instrument :

BNA_F

ClientSampleId :

MW-1ADL


Tot Ion:152 Resp: 157102

Ion Ratio Lower Upper

152 100

151 23.0 17.6 26.4




153 30.0 11.4 17.0#



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

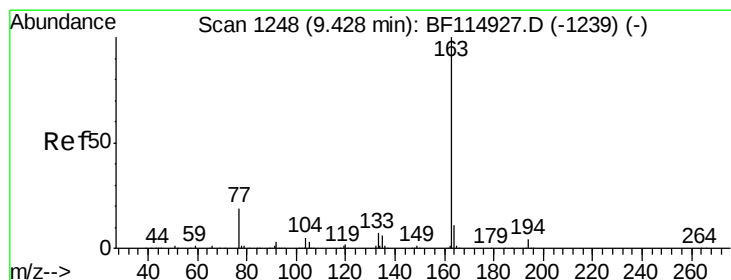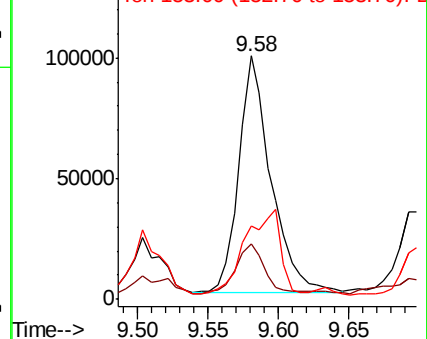

#50

Dimethylphthalate

Concen: 70.490 ng

RT: 9.51 min Scan# 1262

Delta R.T. 0.08 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06


Tgt Ion:163 Resp: 105202

Ion Ratio Lower Upper

163 100

194 0.6 3.4 5.0#



164 75.3 8.7 13.1#




Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E




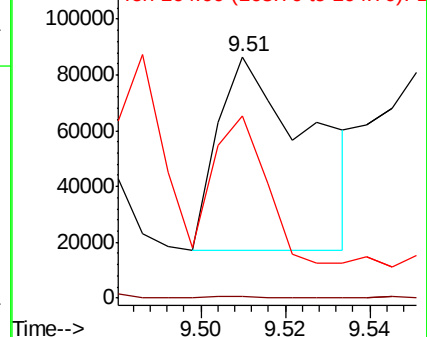




#51
2,6-Dinitrotoluene
Concen: 7.139 ng
RT: 9.56 min Scan# 1270
Delta R.T. 0.08 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06




Instrument :
BNA_F
ClientSampleId :
MW-1ADL


Tot Ion:165 Resp: 2447
Ion Ratio Lower Upper
165 100
63 827.2 38.3 57.5#
89 538.0 40.8 61.2#

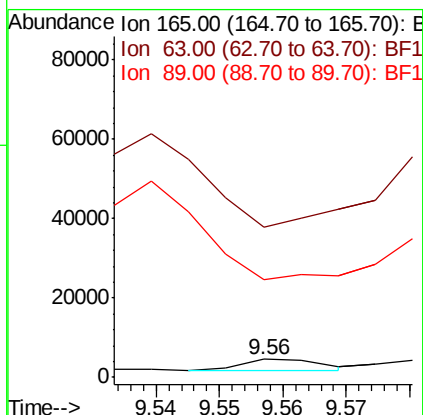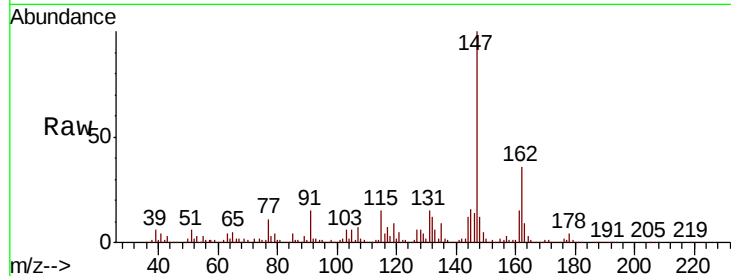

#52
Acenaphthene
Concen: 1169.412 ng
RT: 9.75 min Scan# 1303
Delta R.T. 0.02 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06

Tgt Ion:154 Resp: 1309259
Ion Ratio Lower Upper
154 100
153 112.4 89.1 133.7
152 54.9 43.8 65.6


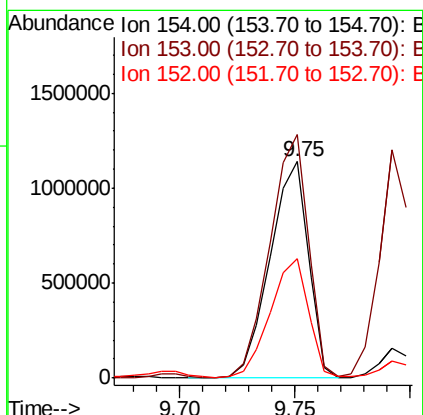






#53
3-Nitroaniline
Concen: 3.885 ng
RT: 9.75 min Scan# 1303
Delta R.T. 0.11 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06




Instrument :
BNA_F
ClientSampleId :
MW-1ADL


Tot Ion:138 Resp: 1599
Ion Ratio Lower Upper
138 100
108 315.8 7.9 11.9#
92 726.8 85.0 127.6#

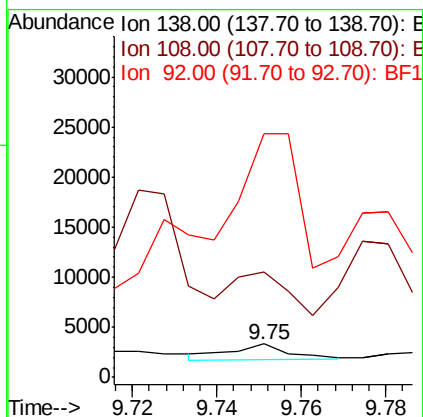

#54
2,4-Dinitrophenol
Concen: 421.373 ng
RT: 9.87 min Scan# 1323
Delta R.T. 0.12 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06

Tgt Ion:184 Resp: 71490
Ion Ratio Lower Upper
184 100
63 237.2 47.4 71.0#
154 15.1 48.6 73.0#



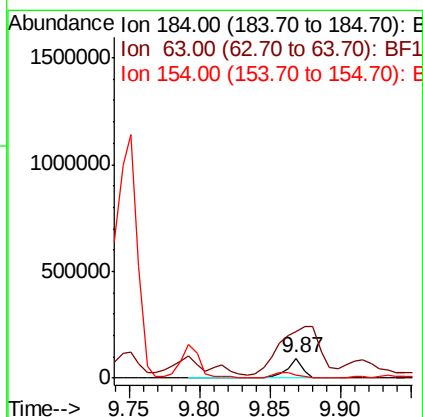



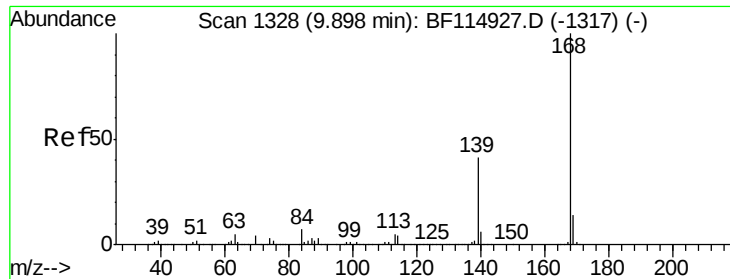

#55
Dibenzofuran
Concen: 936.384 ng
RT: 9.92 min Scan# 1331
Delta R.T. 0.02 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06




Instrument :
BNA_F
ClientSampleId :
MW-1ADL


Tot Ion:168 Resp: 1496526
Ion Ratio Lower Upper
168 100
139 39.9 33.0 49.4
169 14.7 11.6 17.4

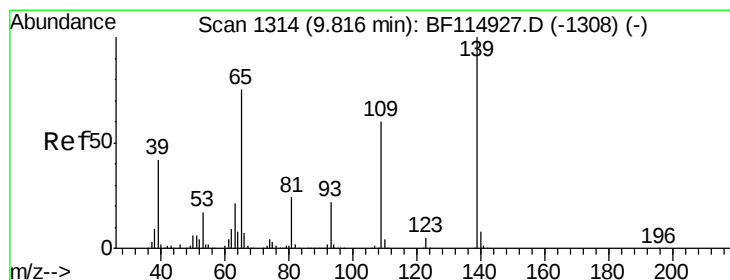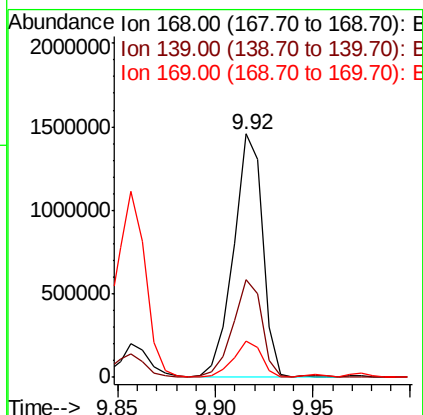

#56
4-Nitrophenol
Concen: 2025.488 ng
RT: 9.92 min Scan# 1331
Delta R.T. 0.10 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06

Tgt Ion:139 Resp: 594210
Ion Ratio Lower Upper
139 100
109 1.9 40.0 80.0#
65 5.2 55.0 95.0#



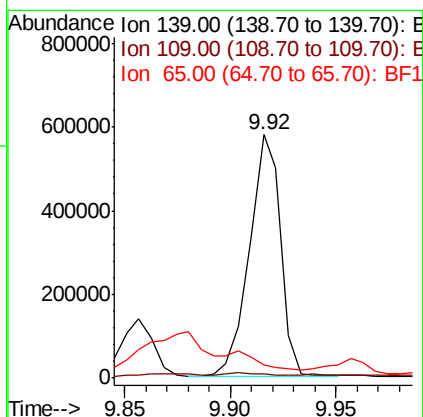



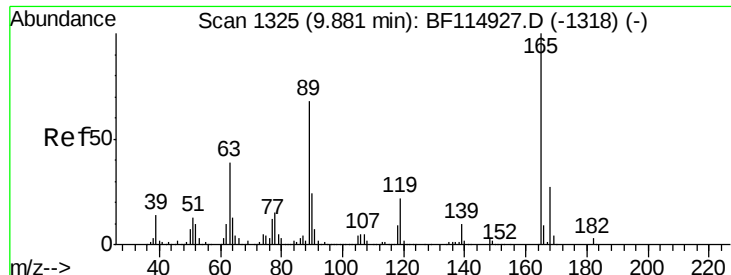

#57
 2,4-Dinitrotoluene
 Concen: 71.303 ng
 RT: 9.87 min Scan# 1323
 Delta R.T. -0.01 min
 Lab File: BF114965.D
 Acq: 12 Jun 2019 1:06




Instrument :
 BNA_F
 ClientSampleId :
 MW-1ADL


Tot Ion	Ratio	Lower	Upper
165	100		
63	580.7	31.8	47.6#
89	657.7	54.2	81.2#
182	9.1	2.1	3.1#

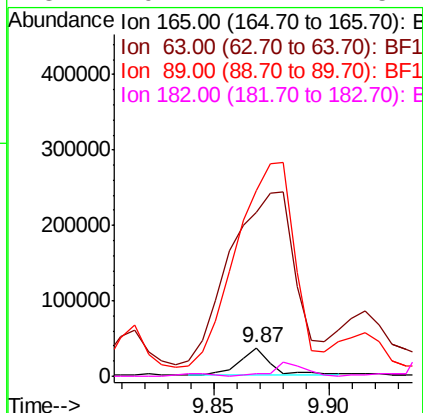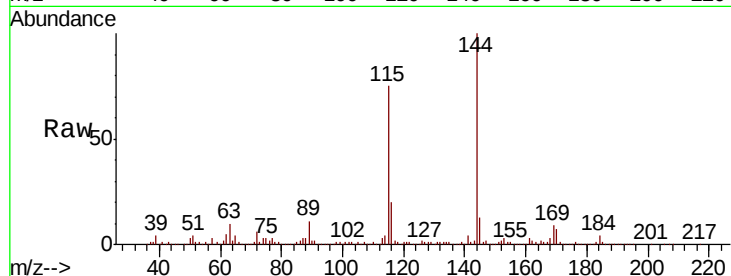

#58
 Fluorene
 Concen: 585.714 ng
 RT: 10.25 min Scan# 1388
 Delta R.T. 0.01 min
 Lab File: BF114965.D
 Acq: 12 Jun 2019 1:06

Tgt Ion	Ratio	Lower	Upper
166	100		
165	99.8	79.2	118.8
167	14.9	11.0	16.6


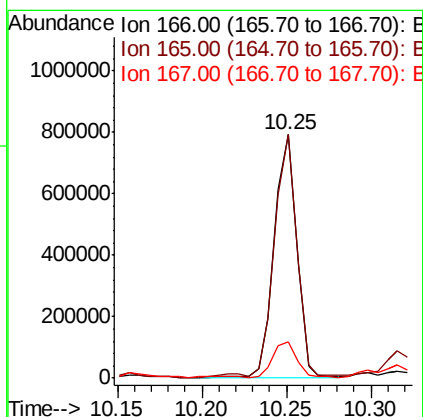

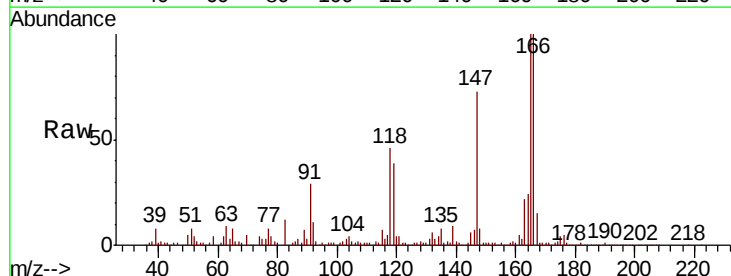


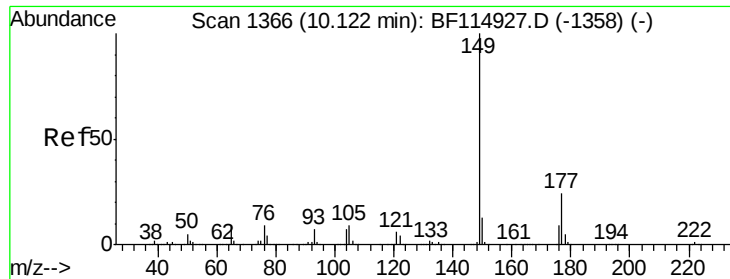

#60
Diethylphthalate
Concen: 28.495 ng
RT: 10.17 min Scan# 1374
Delta R.T. 0.05 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06




Instrument :
BNA_F
ClientSampled :
MW-1ADL


Tot Ion:149 Resp: 41333
Ion Ratio Lower Upper
149 100
177 42.9 19.1 28.7#
150 17.5 10.6 16.0#

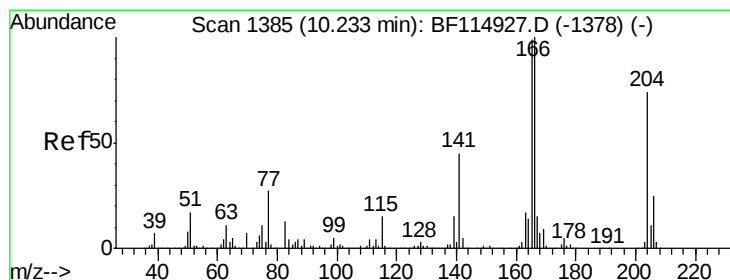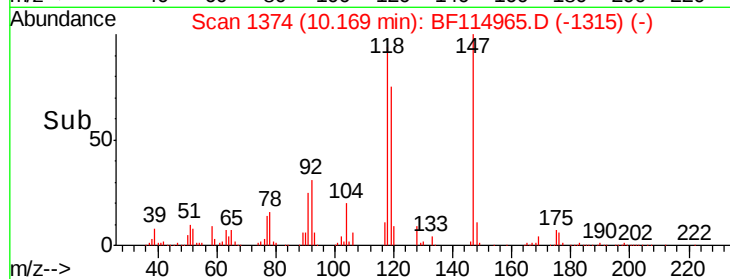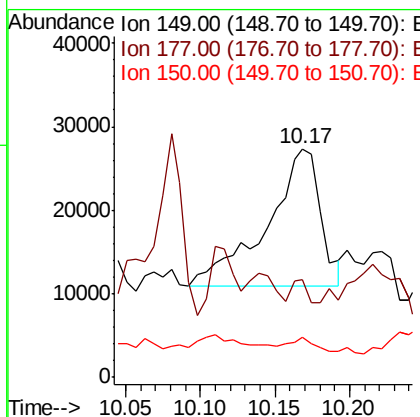

#61
4-Chlorophenyl-phenylether
Concen: 2.615 ng
RT: 10.30 min Scan# 1396
Delta R.T. 0.06 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06

Tgt Ion:204 Resp: 1613
Ion Ratio Lower Upper
204 100
206 49.6 26.8 40.2#
141 307.5 48.5 72.7#


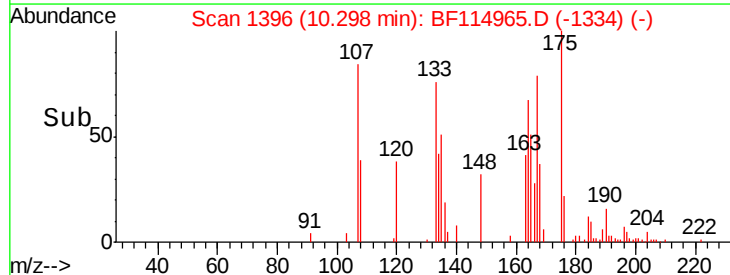
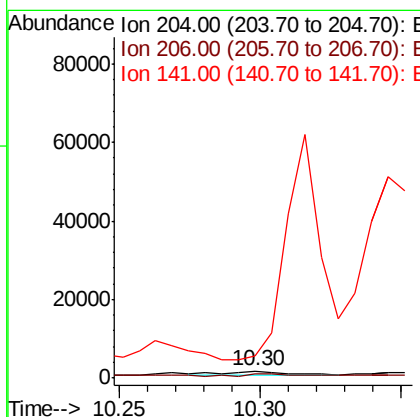



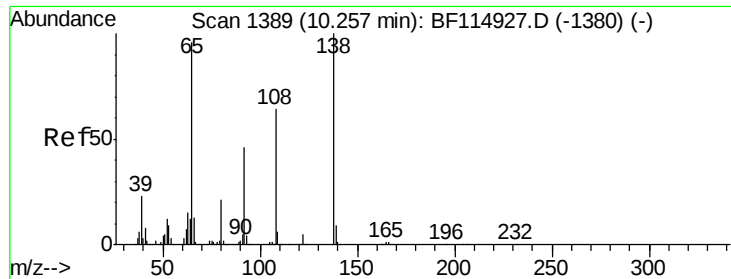

#62
4-Nitroaniline
Concen: 10.421 ng
RT: 10.53 min Scan# 1436
Delta R.T. 0.28 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06




Instrument :
BNA_F
ClientSampleId :
MW-1ADL


Tot Ion:138 Resp: 4396
Ion Ratio Lower Upper
138 100
92 63.8 26.0 66.0
108 58.6 44.0 84.0

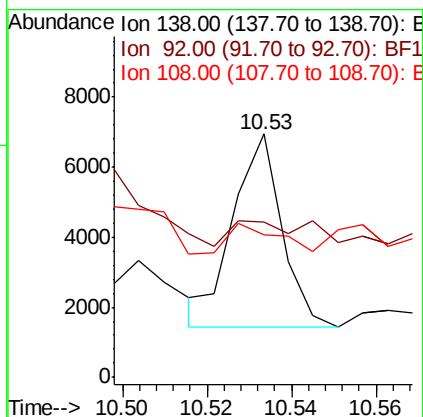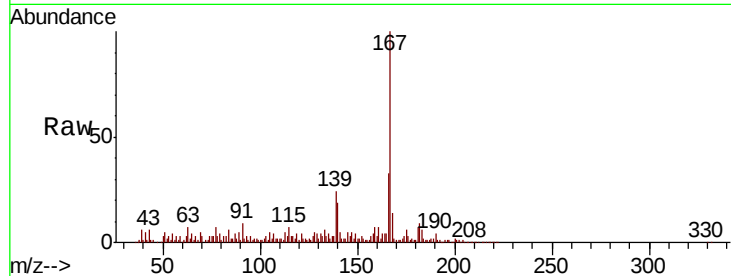

#63
Azobenzene
Concen: 150.787 ng
RT: 10.47 min Scan# 1426
Delta R.T. 0.08 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06

Tgt Ion: 77 Resp: 190372
Ion Ratio Lower Upper
77 100
182 22.5 10.8 50.8
105 24.3 5.3 45.3
51 69.4 6.8 46.8#

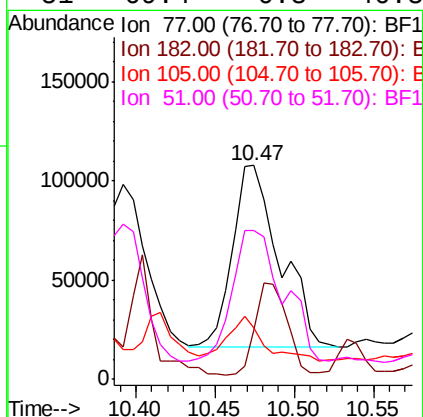


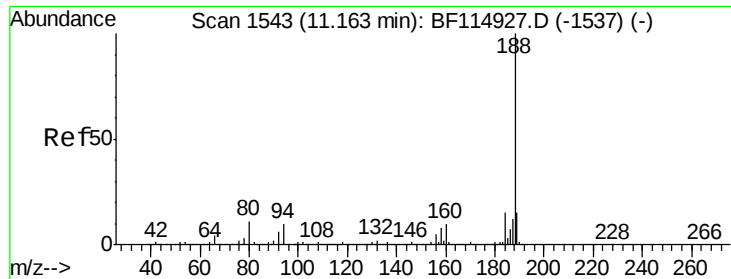




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.17 min Scan# 1545
Delta R.T. 0.01 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06

Instrument :
BNA_F
ClientSampleId :
MW-1ADL

Tot Ion	Ratio	Lower	Upper
188	100		
94	9.2	8.1	12.1
80	10.3	8.6	12.8

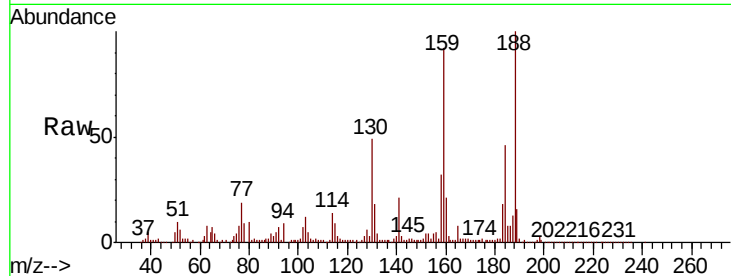


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1


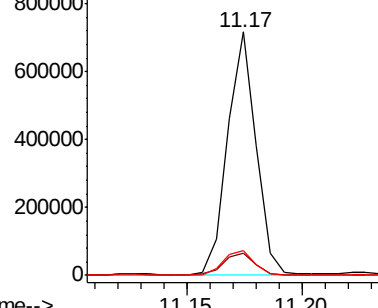



#65
4,6-Dinitro-2-methylphenol
Concen: 7.492 ng
RT: 10.32 min Scan# 1400
Delta R.T. 0.03 min
Lab File: BF114965.D
Acq: 12 Jun 2019 1:06

Tgt Ion	Ratio	Lower	Upper
198	100		
51	70.1	16.8	56.8#
105	48.2	23.5	63.5



Abundance Ion 198.00 (197.70 to 198.70): E
Ion 51.00 (50.70 to 51.70): BF1
Ion 105.00 (104.70 to 105.70): E




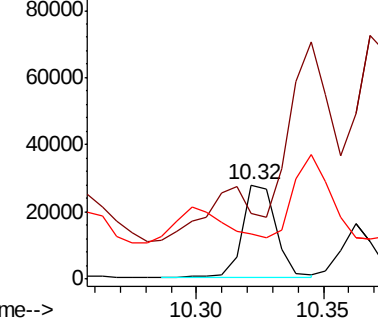




#66
 n-Nitrosodiphenylamine
 Concen: 3.147 ng
 RT: 10.12 min Scan# 1365
 Delta R.T. -0.24 min
 Lab File: BF114965.D
 Acq: 12 Jun 2019 1:06




Instrument :
 BNA_F
 ClientSampleId :
 MW-1ADL


Tot Ion	Ratio	Lower	Upper
169	100		
168	78.7	54.2	81.2
167	34.1	29.4	44.2

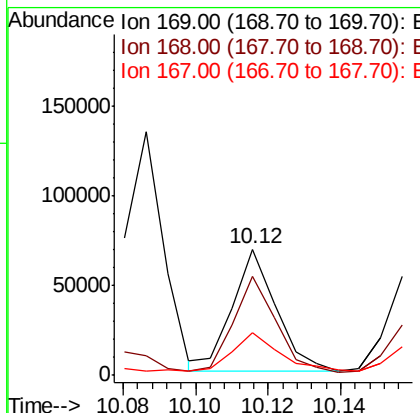

#67
 4-Bromophenyl-phenylether
 Concen: 2.328 ng
 RT: 10.49 min Scan# 1429
 Delta R.T. -0.22 min
 Lab File: BF114965.D
 Acq: 12 Jun 2019 1:06

Tgt Ion	Ratio	Lower	Upper
248	100		
250	204.3	77.4	116.0#
141	689.5	61.8	92.6#

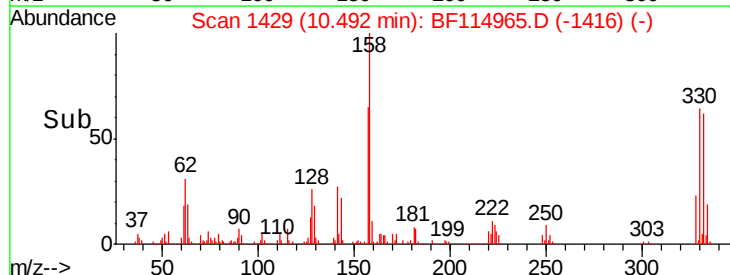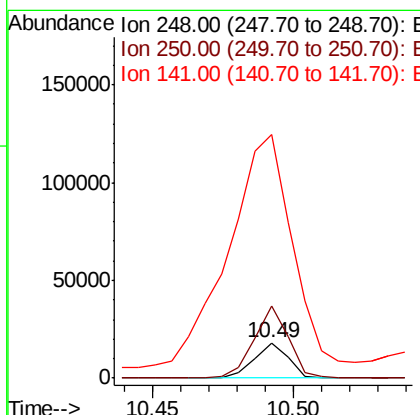

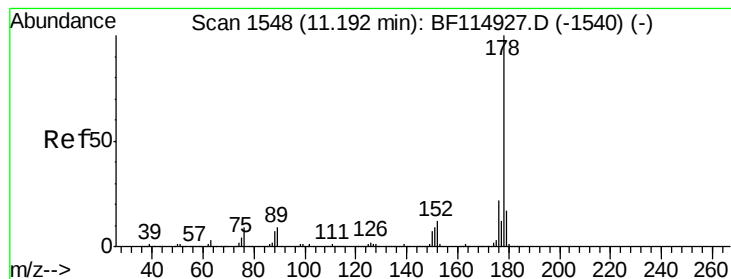

#71

Phenanthrene

Concen: 17.458 ng

RT: 11.20 min Scan# 1549

Delta R.T. 0.01 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06

Instrument :

BNA_F

ClientSampleId :

MW-1ADL


Tot Ion:178 Resp: 518936

Ion Ratio Lower Upper

178 100

176 20.6 17.4 26.2




179 15.7 13.6 20.4



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

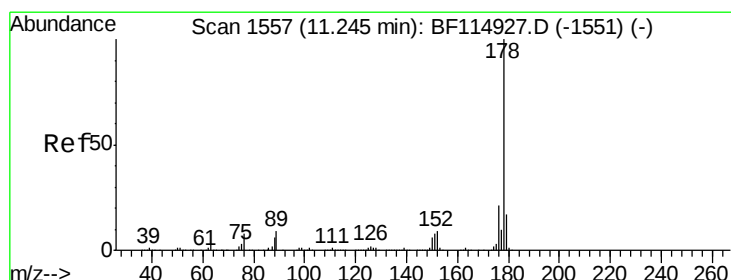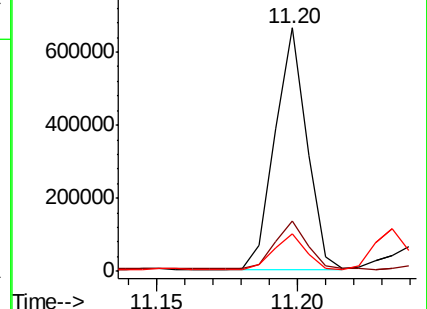

#72

Anthracene

Concen: 17.201 ng

RT: 11.20 min Scan# 1549

Delta R.T. -0.05 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06


Tgt Ion:178 Resp: 518936

Ion Ratio Lower Upper

178 100

176 20.6 16.6 25.0



179 15.7 13.4 20.2




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

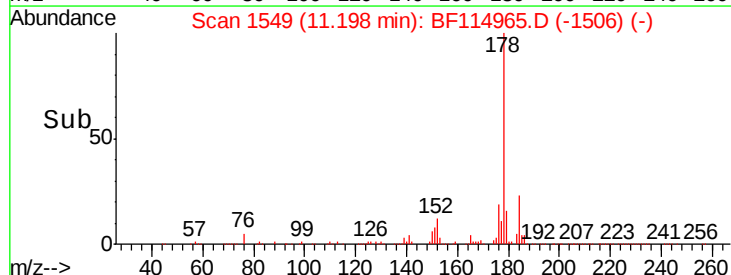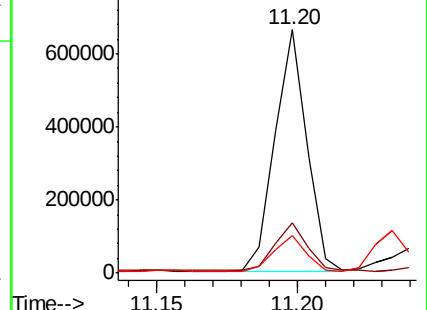



#73

Carbazole

Concen: 16.872 ng

RT: 11.42 min Scan# 1586

Delta R.T. 0.02 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06

Instrument :

BNA_F

ClientSampleId :

MW-1ADL


Tot Ion:167 Resp: 463433

Ion Ratio Lower Upper

167 100

166 21.2 18.8 28.2




139 14.2 11.6 17.4



Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

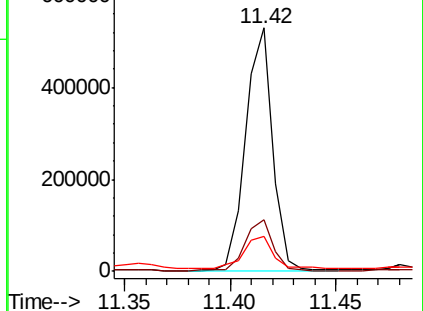

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.79 min Scan# 1990

Delta R.T. -0.00 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06


Tgt Ion:240 Resp: 531394

Ion Ratio Lower Upper

240 100

120 13.5 9.2 13.8



236 28.2 21.7 32.5




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

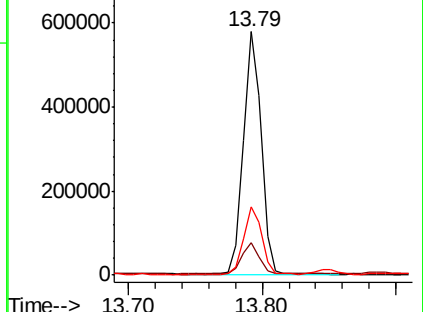



#79

Terphenyl-d14

Concen: 44.385 ng

RT: 12.75 min Scan# 1813

Delta R.T. 0.01 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06

Instrument :


BNA_F

ClientSampleId :

MW-1ADL

Tot Ion:244 Resp: 1185997




Ion	Ratio	Lower	Upper
244	100		
212	6.7	6.2	9.2
122	11.4	10.2	15.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

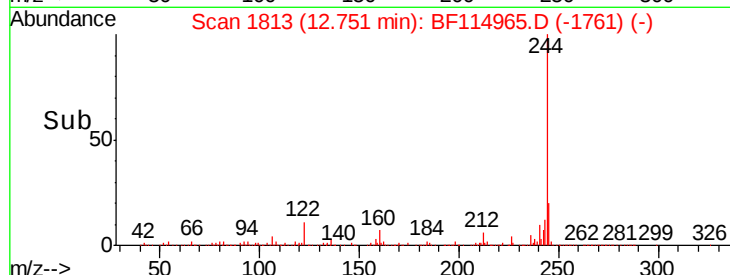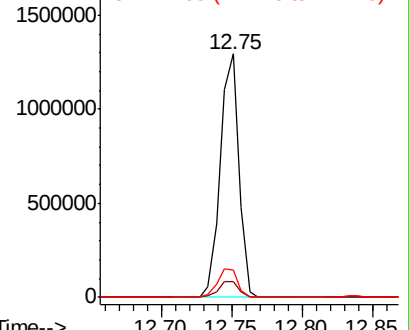

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.17 min Scan# 2225


Delta R.T. 0.01 min

Lab File: BF114965.D

Acq: 12 Jun 2019 1:06

Tgt Ion:264 Resp: 423786

Ion	Ratio	Lower	Upper
264	100		
260	24.7	19.7	29.5
265	22.7	17.5	26.3



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

