


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061119\
 Data File : BF114948.D
 Acq On : 11 Jun 2019 17:31
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 10 16:44:00 2019

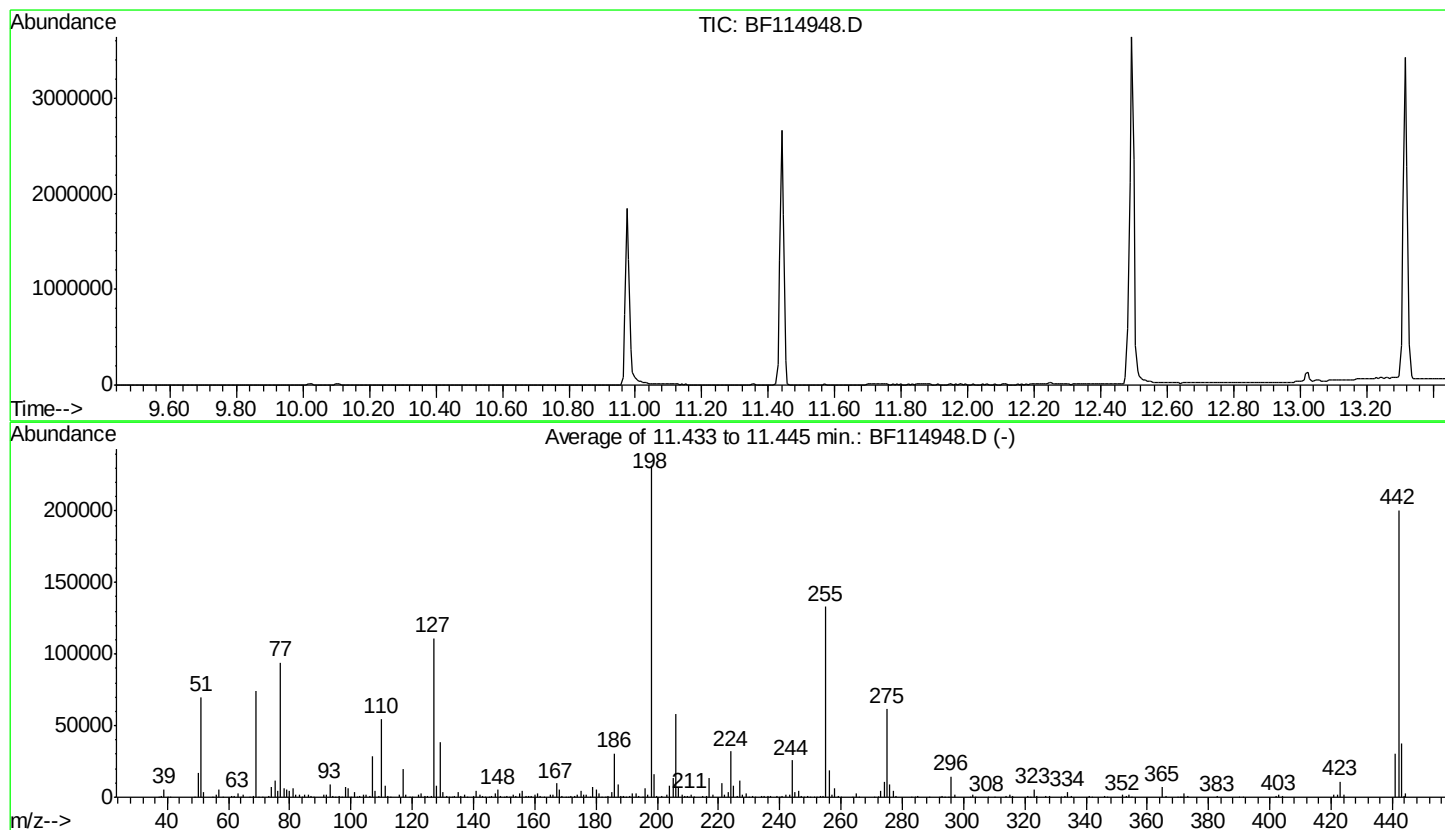

AutoFind: Scans 1589, 1590, 1591; Background Corrected with Scan 1584

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.3	70165	PASS
68	69	0.00	2	1.8	1353	PASS
69	198	0.00	100	32.2	74597	PASS
70	69	0.00	2	0.6	438	PASS
127	198	10	80	47.9	111005	PASS
197	198	0.00	2	0.6	1436	PASS
198	198	100	100	100.0	231594	PASS
199	198	5	9	6.9	15940	PASS
275	198	10	60	26.7	61760	PASS
365	198	1	100	3.1	7227	PASS
441	198	0.01	100	13.0	30185	PASS
442	198	50	100	86.5	200352	PASS
443	442	15	24	18.8	37604	PASS