
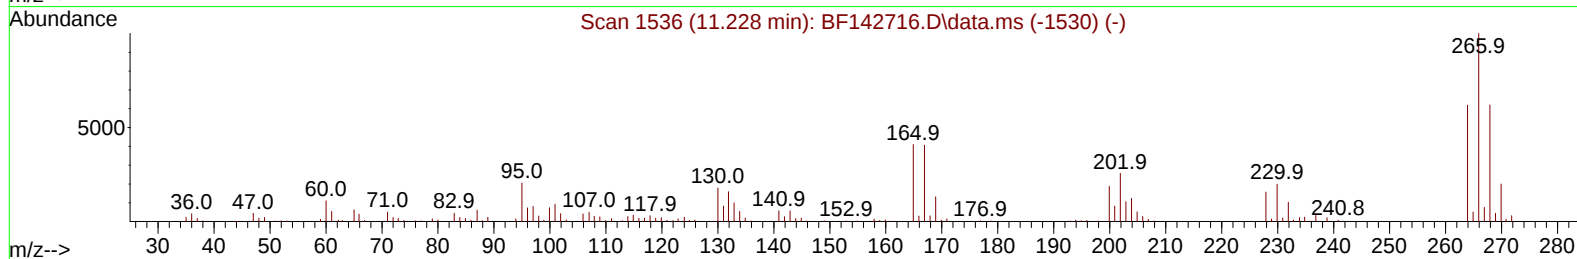
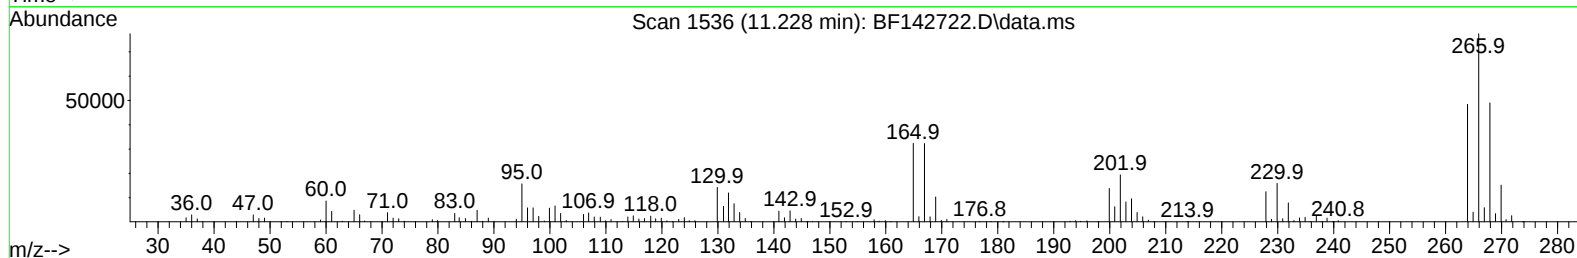


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061125\
Data File : BF142722.D
Acq On : 11 Jun 2025 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 11:00:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 11 05:56:09 2025
Response via : Initial Calibration

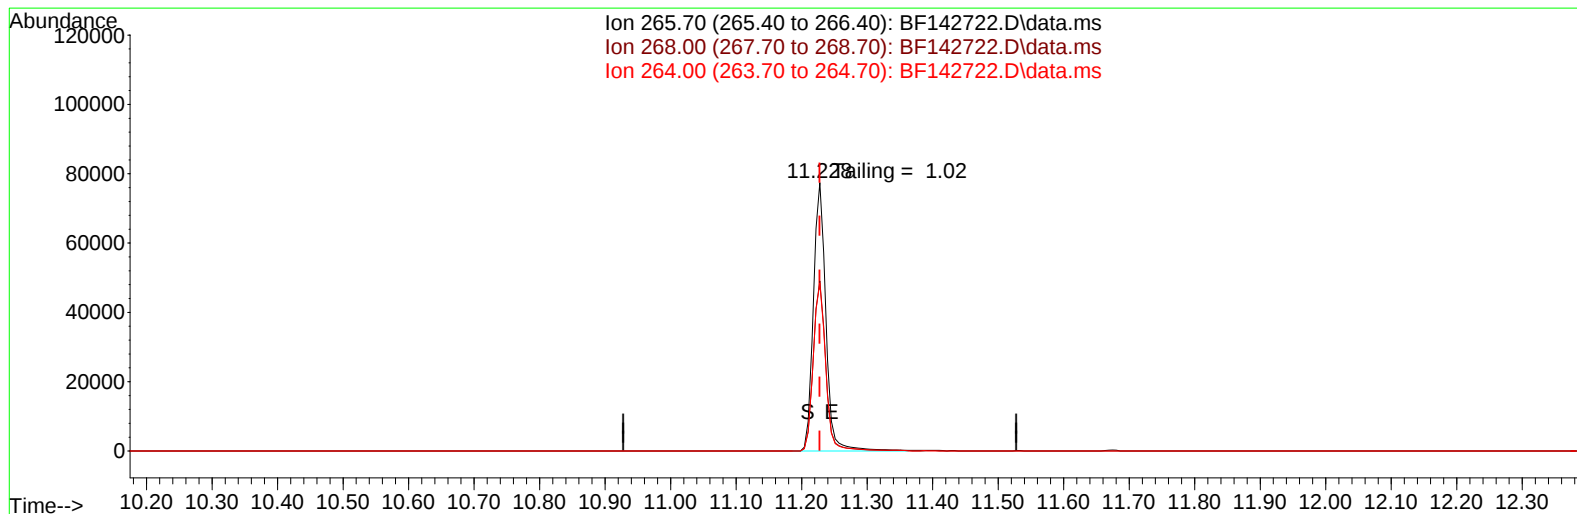

TIC: BF142722.D\data.ms

(70) Pentachlorophenol (C)




11.228min (+ 0.000) 36233.28 ng

response 103277

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.00	63.33
264.00	61.90	62.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061125\
Data File : BF142722.D
Acq On : 11 Jun 2025 08:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 11 11:00:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 11 05:56:09 2025
Response via : Initial Calibration

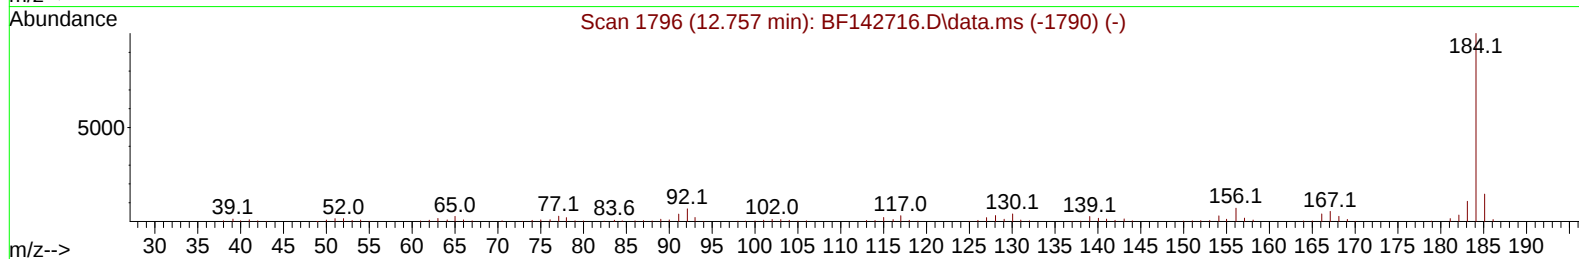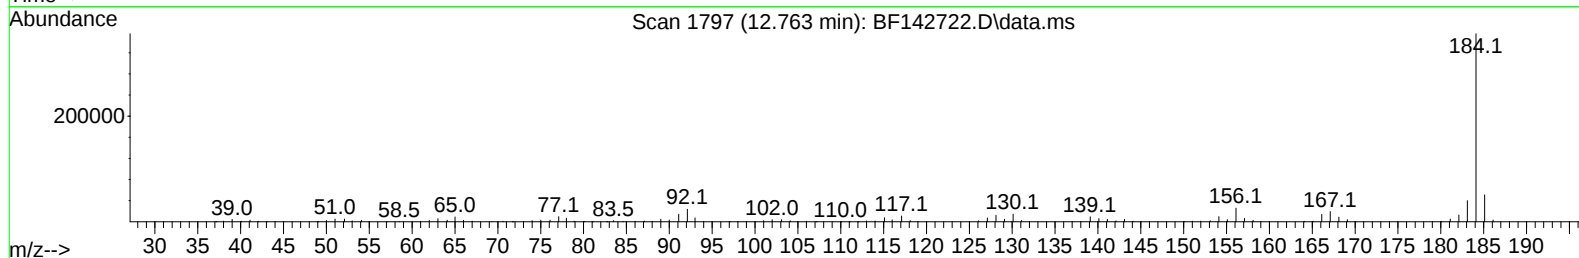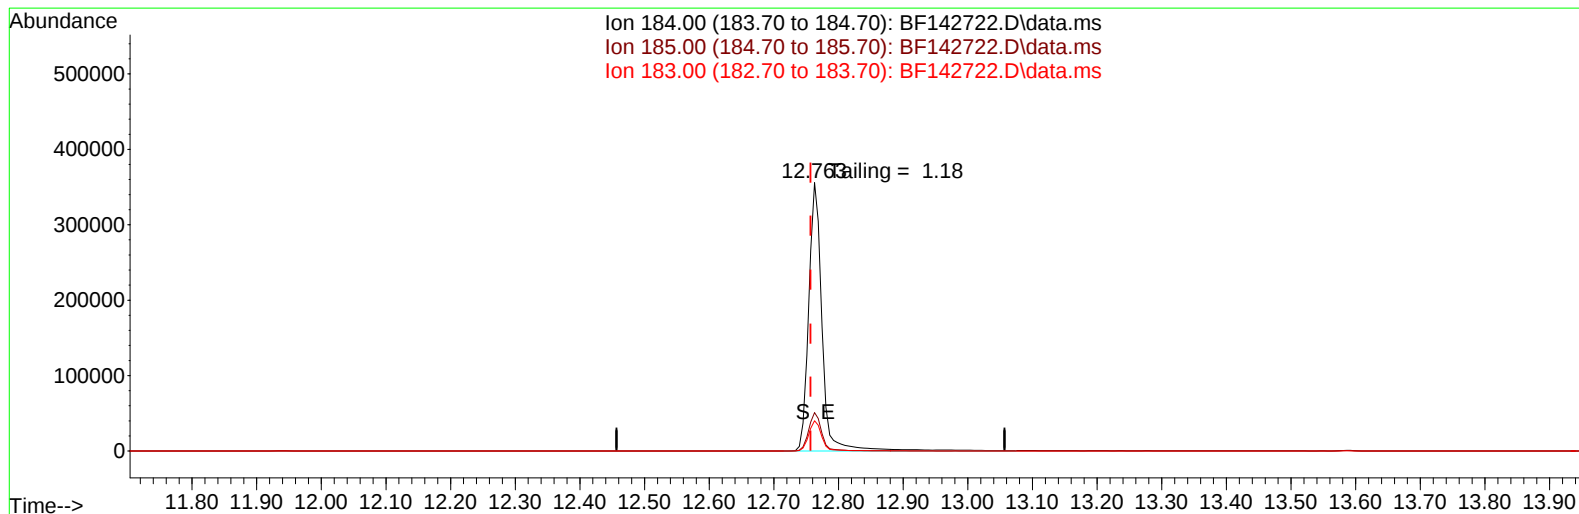

TIC: BF142722.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 11814.89 ng

response 510816

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.33
183.00	10.70	11.31
0.00	0.00	0.00