

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061125\
 Data File : BF142731.D
 Acq On : 11 Jun 2025 13:18
 Operator : RC/JU
 Sample : PB168378BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB168378BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF142731.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.516	559	565	570	rBV	992054	1291132	49.22%	9.852%
2	6.516	728	735	740	rBV	905676	1243134	47.39%	9.486%
3	6.887	793	798	804	rBV	336062	420526	16.03%	3.209%
4	7.451	887	894	899	rBV	890975	1255658	47.87%	9.581%
5	8.175	1010	1017	1038	rBV	416347	553404	21.10%	4.223%
6	9.251	1193	1200	1205	rBV	1986922	2622937	100.00%	20.014%
7	9.934	1310	1316	1333	rBV	504800	651913	24.85%	4.974%
8	10.722	1445	1450	1477	rBV	816130	1062499	40.51%	8.107%
9	11.422	1564	1569	1576	rBV	547940	689450	26.29%	5.261%
10	13.010	1833	1839	1844	rBV	1924631	2531429	96.51%	19.316%
11	14.063	2013	2018	2032	rBV	316296	430671	16.42%	3.286%
12	15.563	2266	2273	2289	rBV	211338	352855	13.45%	2.692%




Sum of corrected areas: 13105608

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061125\
Data File : BF142731.D
Acq On : 11 Jun 2025 13:18
Operator : RC/JU
Sample : PB168378BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168378BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

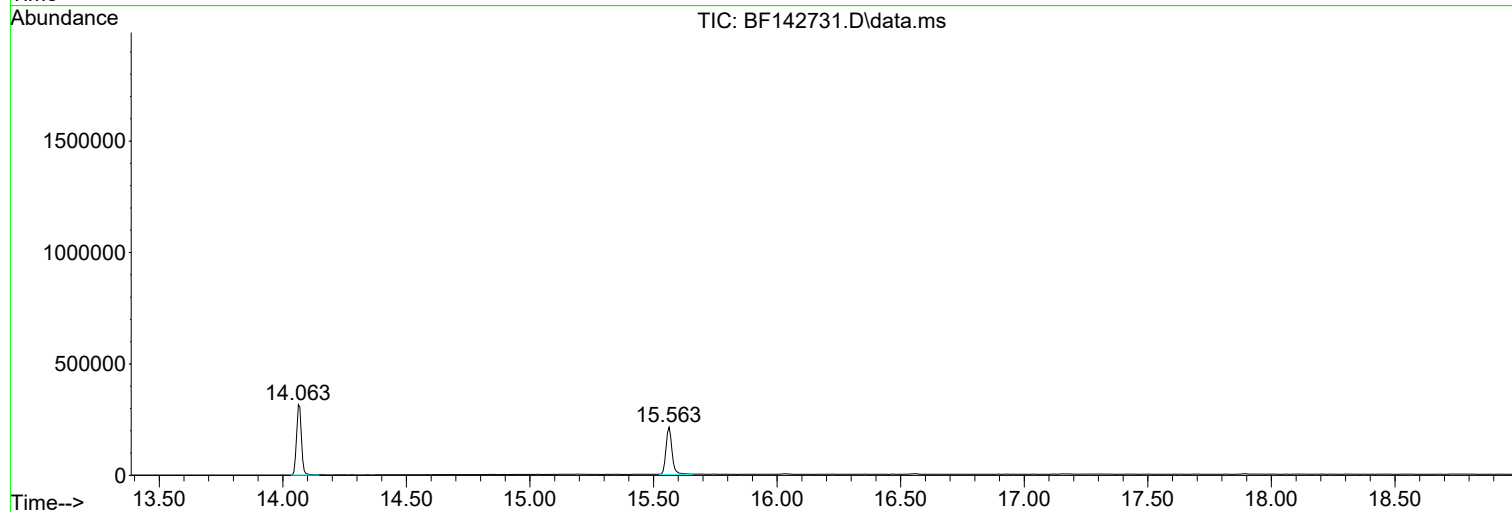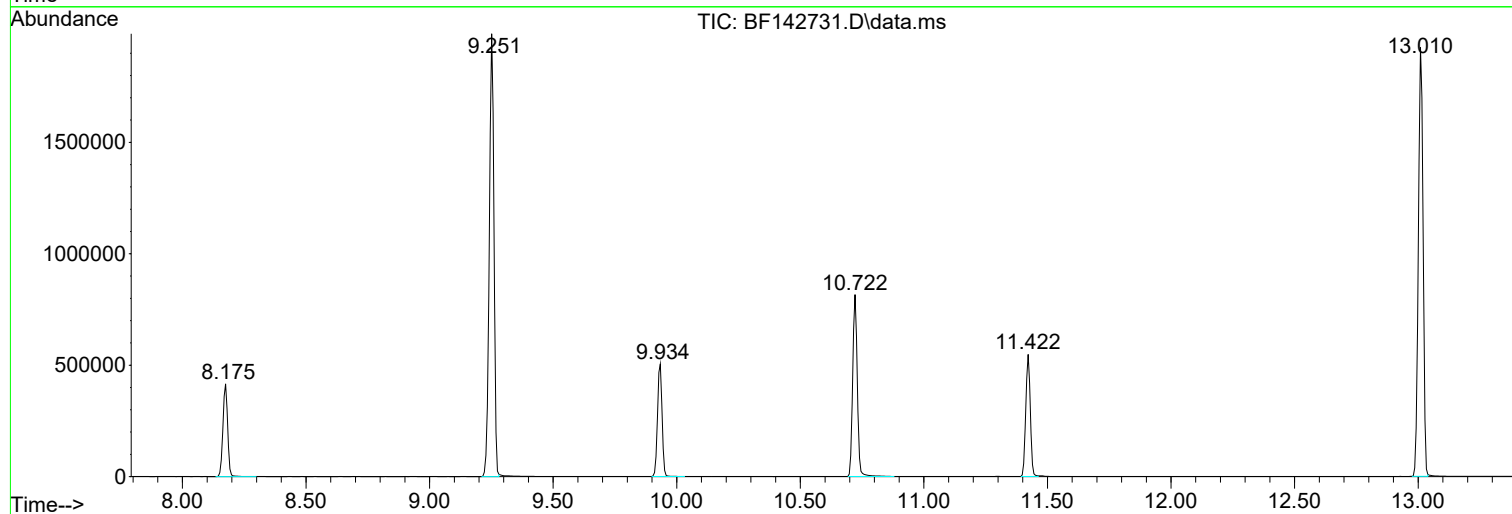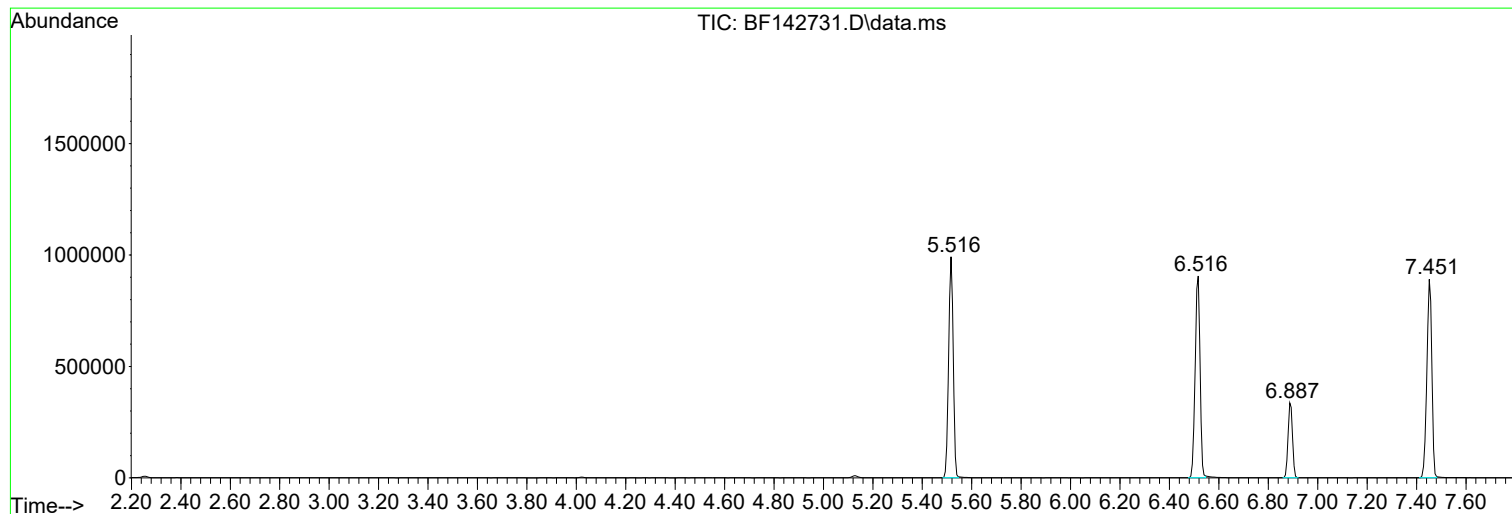

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061125\
Data File : BF142731.D
Acq On : 11 Jun 2025 13:18
Operator : RC/JU
Sample : PB168378BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168378BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061125\
Data File : BF142731.D
Acq On : 11 Jun 2025 13:18
Operator : RC/JU
Sample : PB168378BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168378BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------