

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061218\
 Data File : BF106338.D
 Acq On : 12 Jun 2018 12:28
 Operator : JU/SJ
 Sample : J3214-03RX
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MS-CON-2RX

Quant Time: Jun 13 01:27:39 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 11 15:00:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	172551	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	659275	20.00	ng	0.00
38) Acenaphthene-d10	10.01	164	328616	20.00	ng	0.00
63) Phenanthrene-d10	11.50	188	638726	20.00	ng	0.00
75) Chrysene-d12	14.15	240	496966	20.00	ng	0.00
86) Perylene-d12	15.71	264	517148	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	578133	56.71	ng	0.00
7) Phenol-d6	6.59	99	787671	61.15	ng	0.00
23) Nitrobenzene-d5	7.53	82	532465	47.51	ng	0.00
41) 2,4,6-Tribromophenol	10.80	330	197821	62.56	ng	0.00
44) 2-Fluorobiphenyl	9.32	172	989950	44.80	ng	0.00
78) Terphenyl-d14	13.09	244	1174342	58.69	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.72	163	85551	3.644	ng	Qvalue # 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061218\
Data File : BF106338.D
Acq On : 12 Jun 2018 12:28
Operator : JU/SJ
Sample : J3214-03RX
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MS-CON-2RX

Quant Time: Jun 13 01:27:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 11 15:00:22 2018
Response via : Initial Calibration

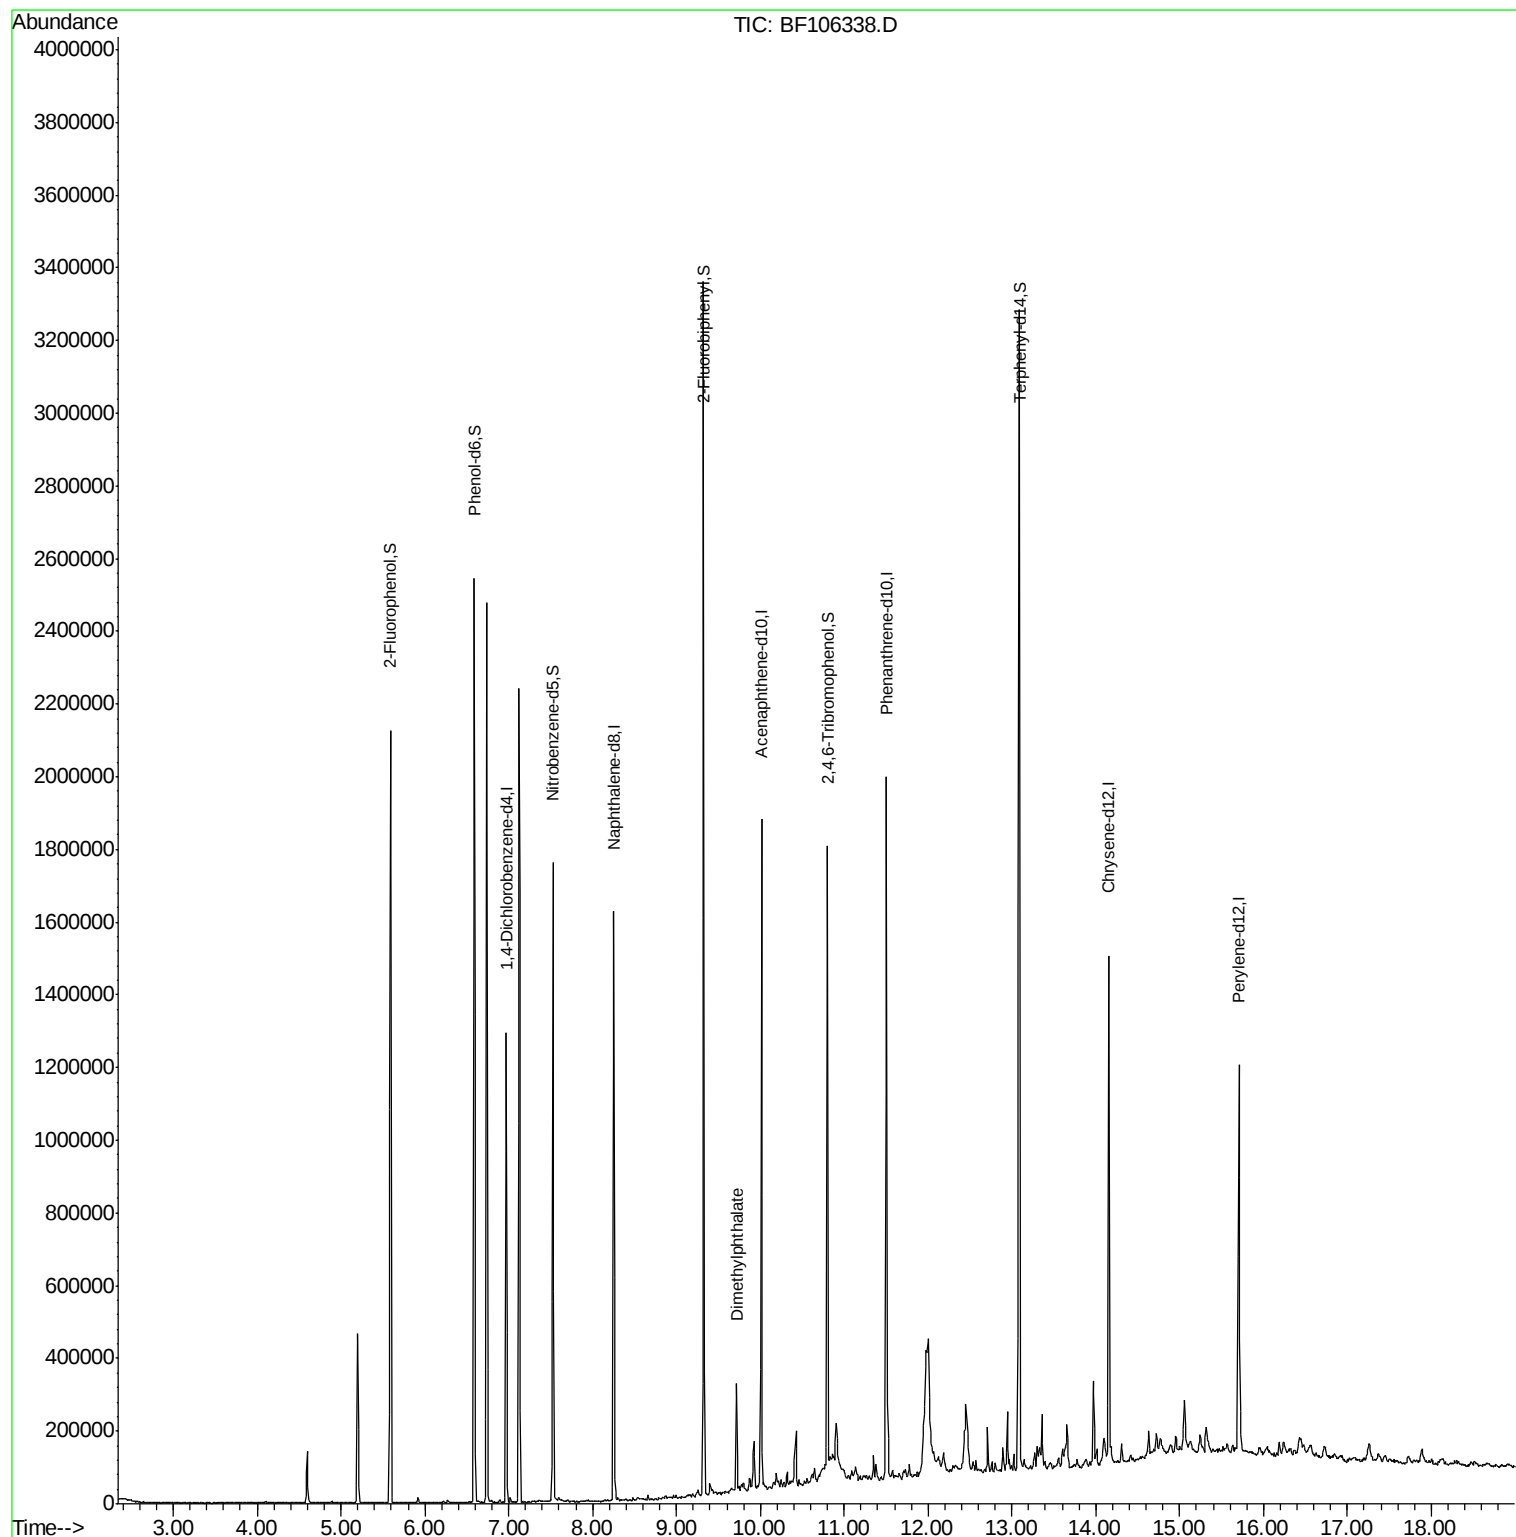




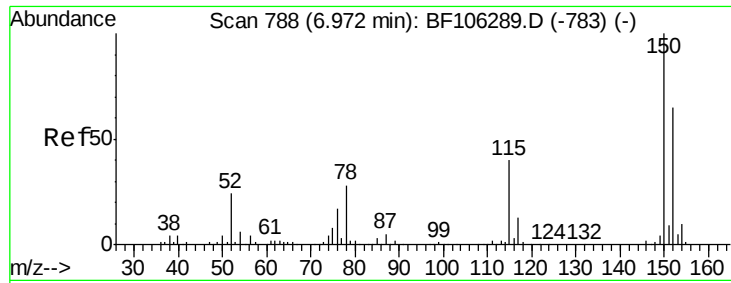


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 788
Delta R.T. 0.00 min
Lab File: BF106338.D
Acq: 12 Jun 2018 12:28

Instrument :
BNA_F
ClientSampleId :
MS-CON-2RX




Tot Ion:152 Resp: 172551
Ion Ratio Lower Upper
152 100
150 157.8 124.6 186.8
115 61.6 50.1 75.1

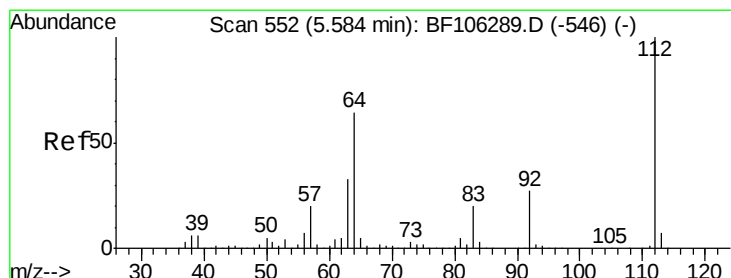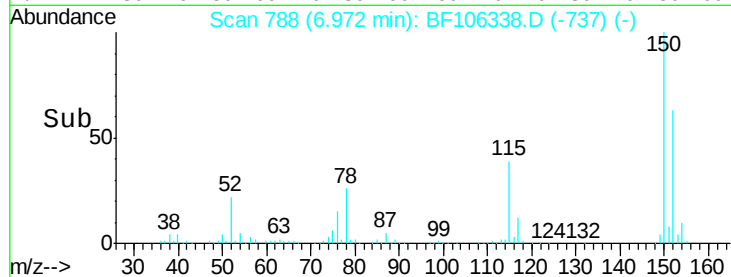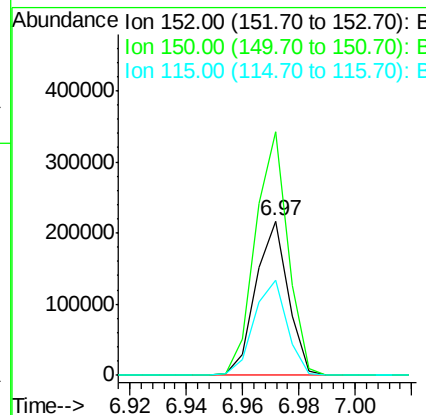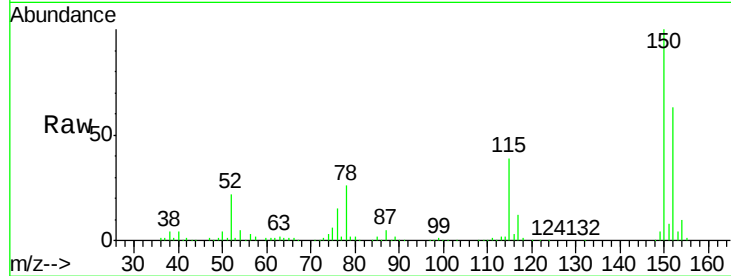

#5

2-Fluorophenol
Concen: 56.707 ng
RT: 5.59 min Scan# 553
Delta R.T. 0.01 min
Lab File: BF106338.D
Acq: 12 Jun 2018 12:28

Tgt Ion:112 Resp: 578133
Ion Ratio Lower Upper
112 100
64 64.2 47.9 71.9
63 32.0 23.7 35.5

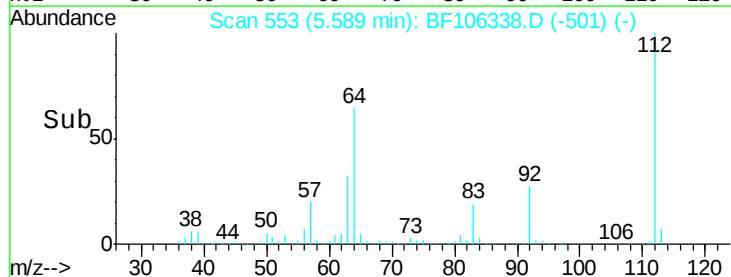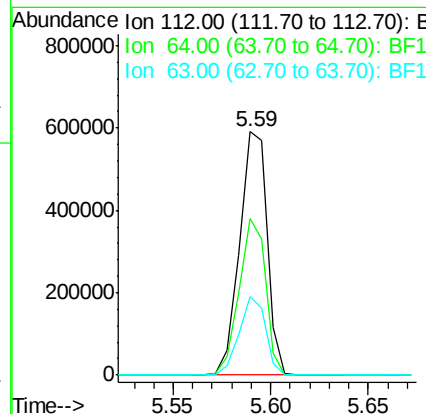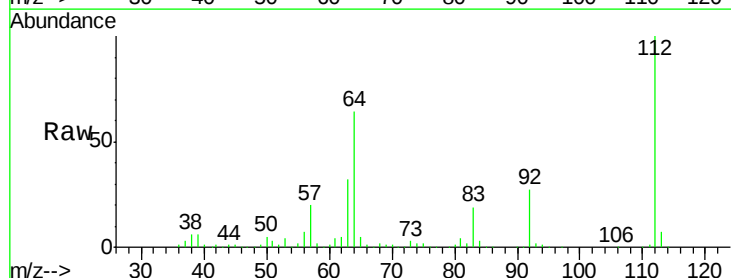



#7

Phenol-d6

Concen: 61.152 ng

RT: 6.59 min Scan# 723

Delta R.T. 0.00 min

Lab File: BF106338.D

Acq: 12 Jun 2018 12:28

Instrument :

BNA_F

ClientSampleId :

MS-CON-2RX


Tot Ion: 99 Resp: 787671

Ion Ratio Lower Upper




99 100

42 18.3 14.5 21.7

71 34.3 25.4 38.0

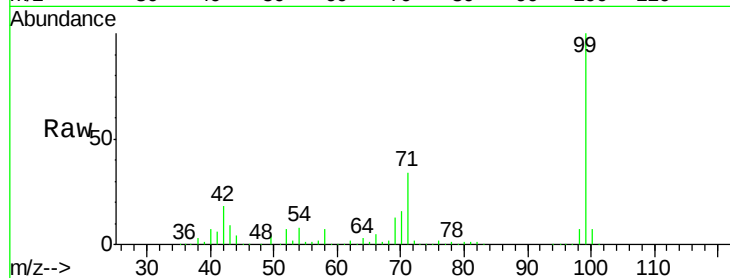

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

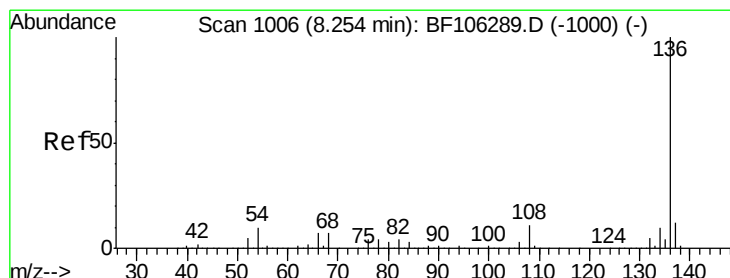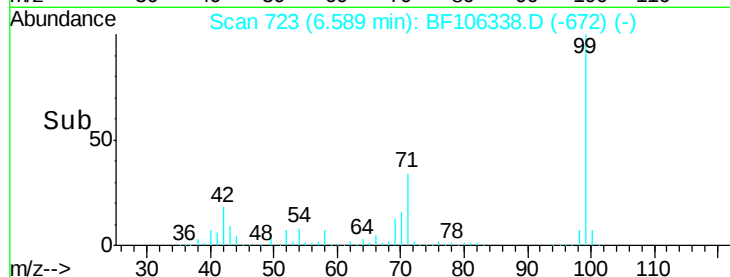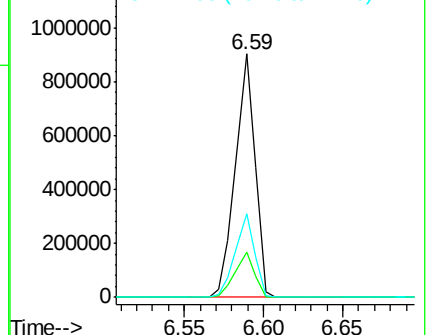

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.25 min Scan# 1006

Delta R.T. 0.00 min

Lab File: BF106338.D

Acq: 12 Jun 2018 12:28

Tgt Ion: 136 Resp: 659275


Ion Ratio Lower Upper

136 100



137 11.3 8.9 13.3


54 8.5 6.6 9.8

68 6.8 5.0 7.4

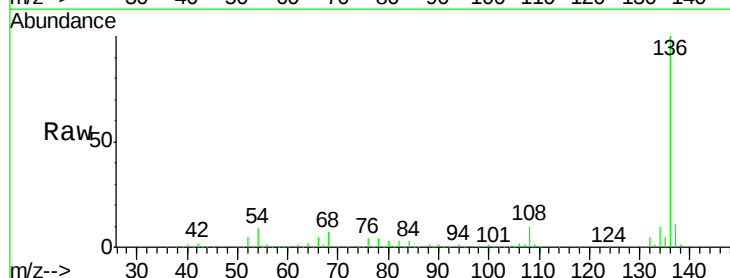

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

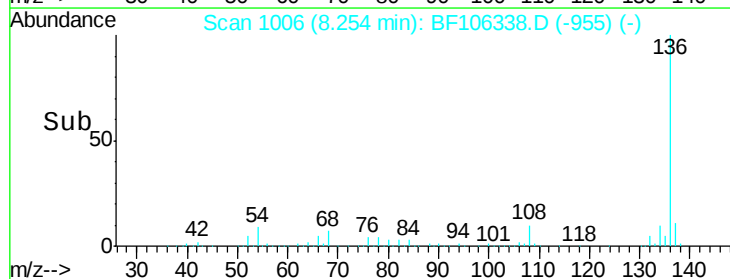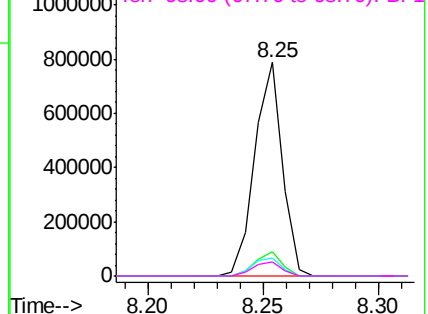


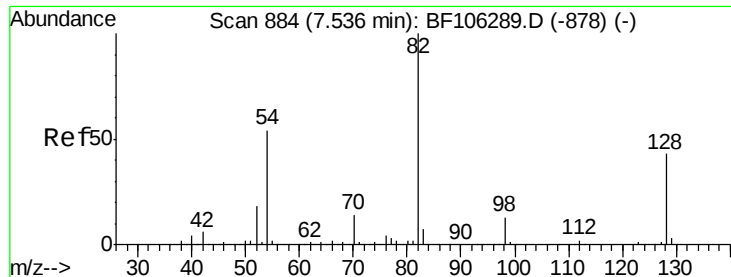




#23
Nitrobenzene-d5
Concen: 47.513 ng
RT: 7.53 min Scan# 883
Delta R.T. -0.01 min
Lab File: BF106338.D
Acq: 12 Jun 2018 12:28

Instrument :
BNA_F
ClientSampleId :
MS-CON-2RX

Tot Ion: 82 Resp: 532465
Ion Ratio Lower Upper
82 100
128 43.0 36.1 54.1
54 51.3 41.4 62.2

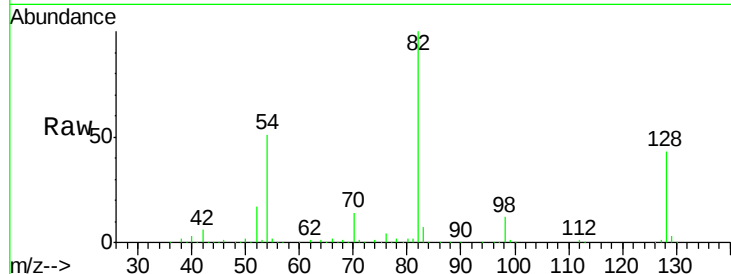


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

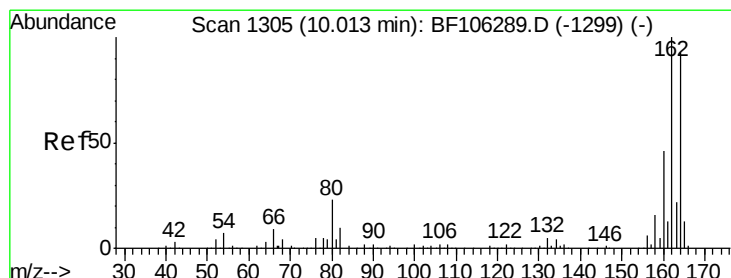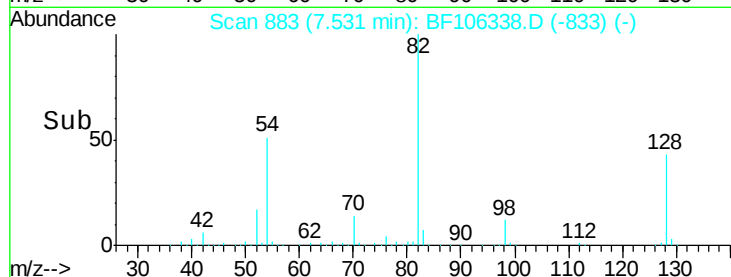
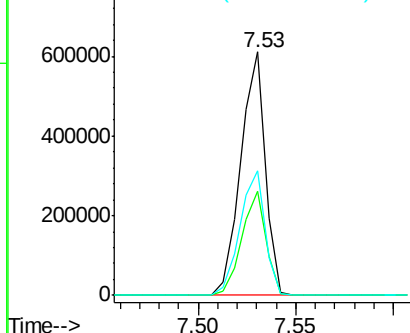



#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.01 min Scan# 1305
Delta R.T. 0.00 min
Lab File: BF106338.D
Acq: 12 Jun 2018 12:28

Tgt Ion:164 Resp: 328616
Ion Ratio Lower Upper
164 100
162 103.3 86.1 129.1
160 47.2 38.3 57.5

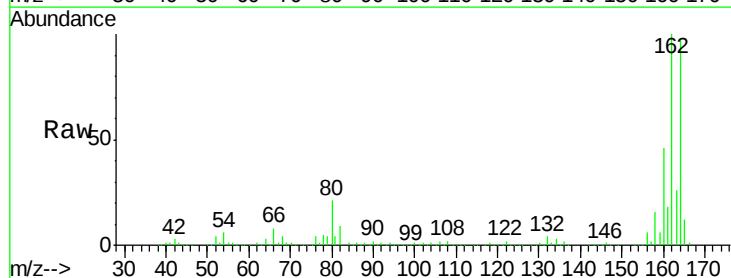

Abundance Ion 164.00 (163.70 to 164.70): BF1
Ion 162.00 (161.70 to 162.70): BF1
Ion 160.00 (159.70 to 160.70): BF1

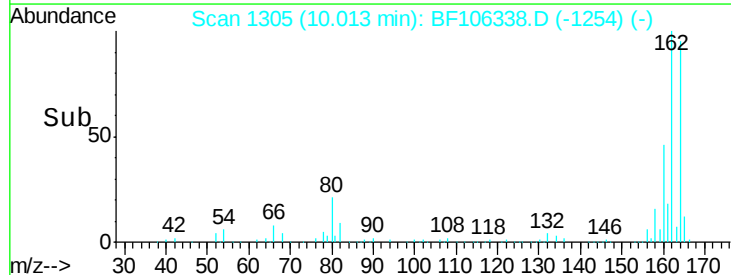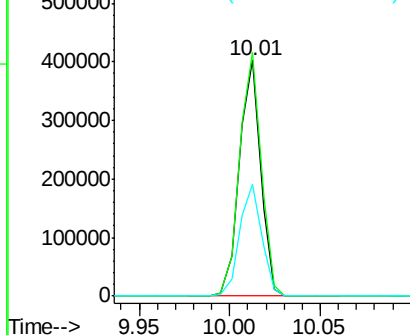


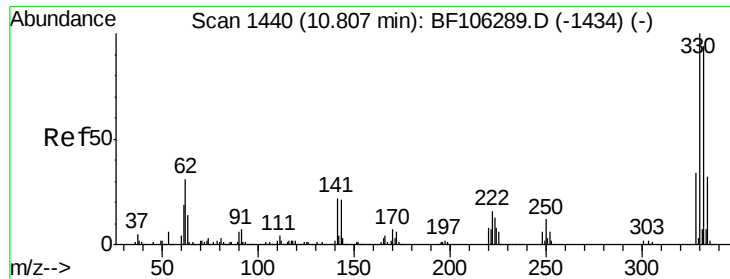




#41
 2,4,6-Tribromophenol
 Concen: 62.565 ng
 RT: 10.80 min Scan# 1439
 Delta R.T. -0.01 min
 Lab File: BF106338.D
 Acq: 12 Jun 2018 12:28

Instrument :
 BNA_F
 ClientSampleId :
 MS-CON-2RX

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.2	77.0	115.6
141	32.2	29.9	44.9

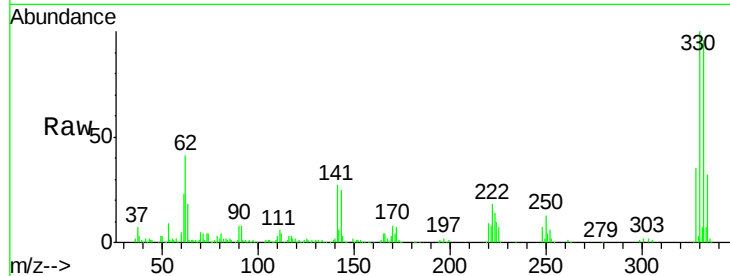


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

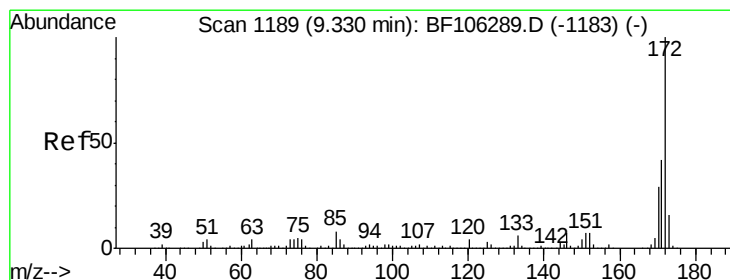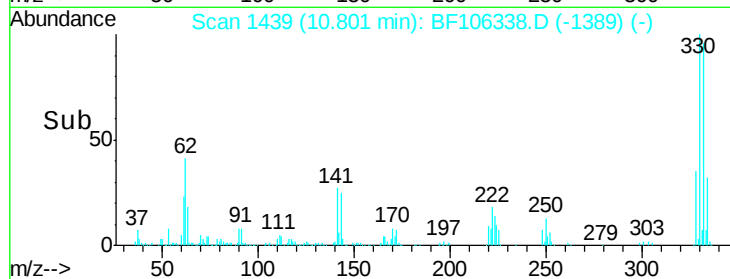
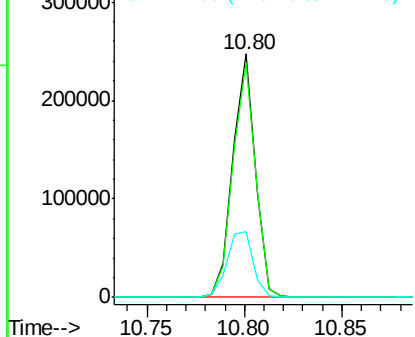



#44
 2-Fluorobiphenyl
 Concen: 44.796 ng
 RT: 9.32 min Scan# 1188
 Delta R.T. -0.01 min
 Lab File: BF106338.D
 Acq: 12 Jun 2018 12:28

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.7	29.7	44.5
170	25.7	19.6	29.4

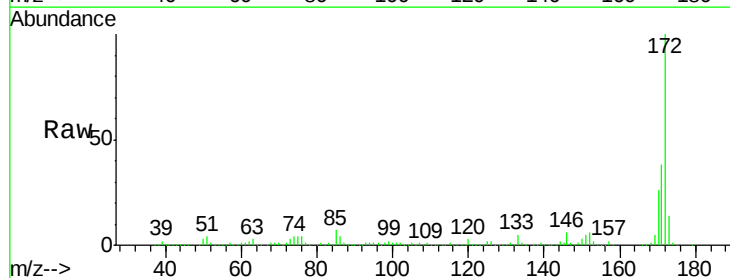

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

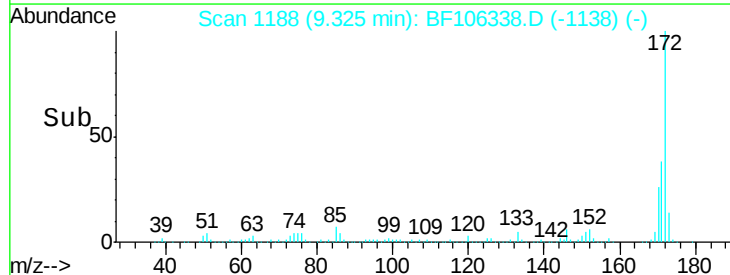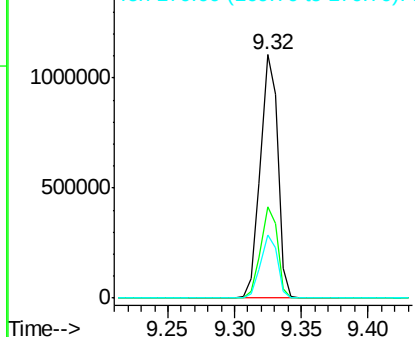

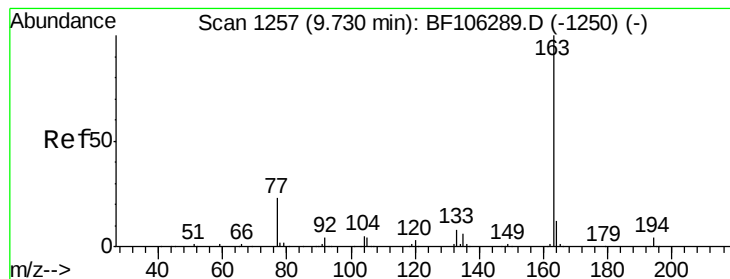

#49

Dimethylphthalate

Concen: 3.644 ng

RT: 9.72 min Scan# 1255

Delta R.T. -0.01 min

Lab File: BF106338.D

Acq: 12 Jun 2018 12:28

Instrument :

BNA_F

ClientSampleId :

MS-CON-2RX


Tot Ion:163 Resp: 85551

Ion Ratio Lower Upper

163 100

194 4.6 2.7 4.1#




164 9.5 8.2 12.2

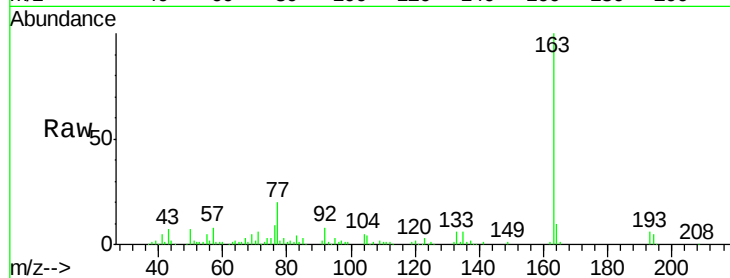

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

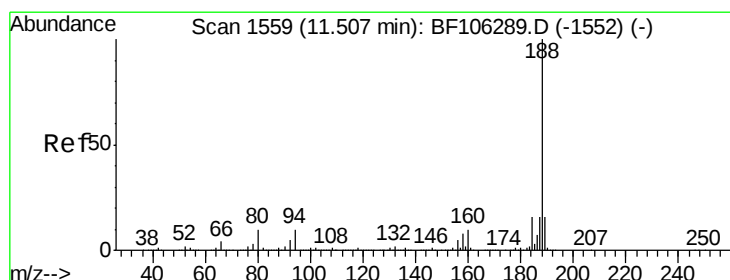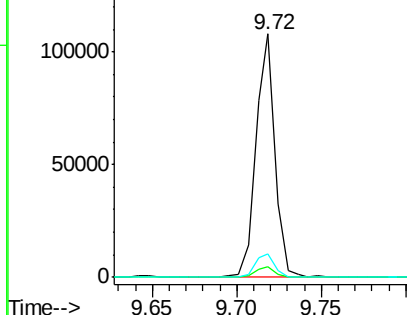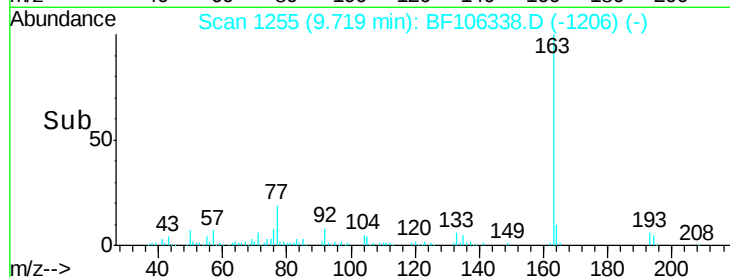

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.50 min Scan# 1558

Delta R.T. -0.01 min

Lab File: BF106338.D

Acq: 12 Jun 2018 12:28


Tgt Ion:188 Resp: 638726

Ion Ratio Lower Upper

188 100

94 10.9 8.5 12.7



80 11.6 9.2 13.8

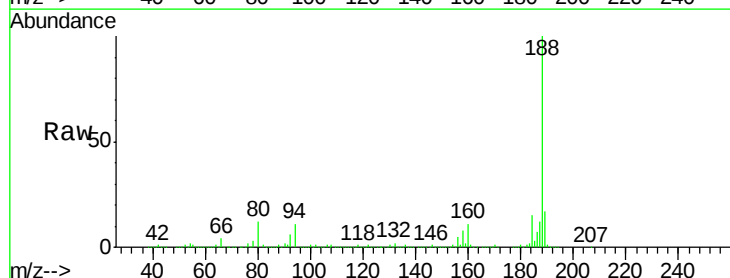


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

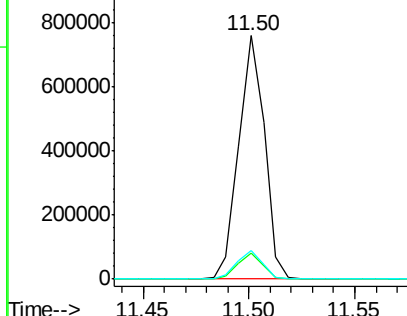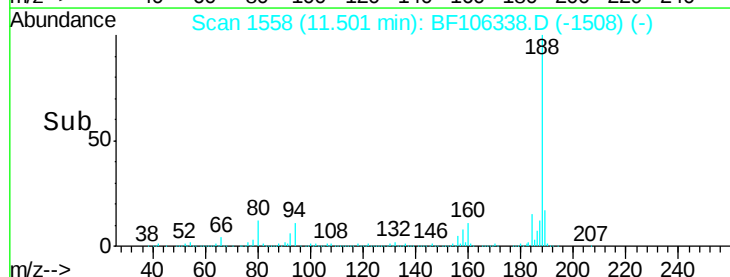

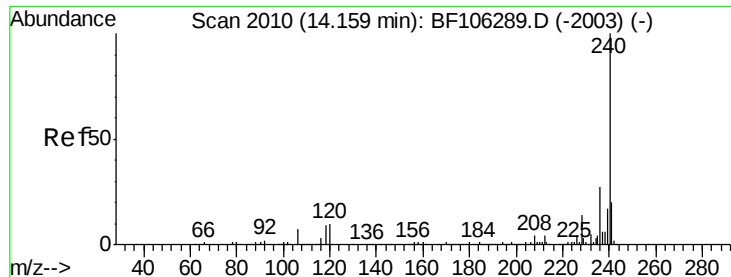

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.15 min Scan# 2009

Delta R.T. -0.01 min

Lab File: BF106338.D

Acq: 12 Jun 2018 12:28

Instrument :

BNA_F

ClientSampleId :

MS-CON-2RX


Tot Ion:240 Resp: 496966

Ion Ratio Lower Upper

240 100

120 12.4 9.5 14.3




236 27.2 20.7 31.1

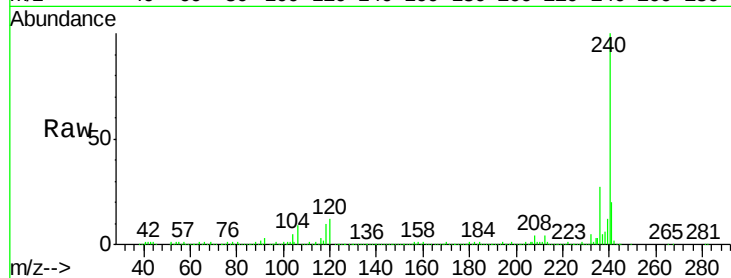

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

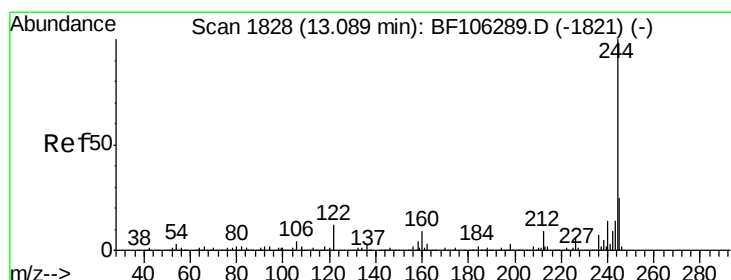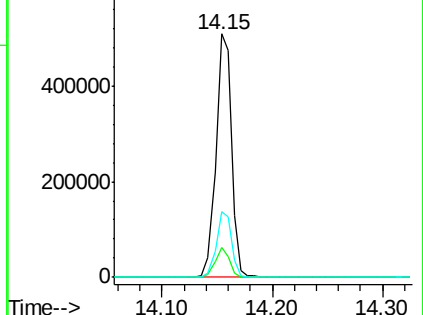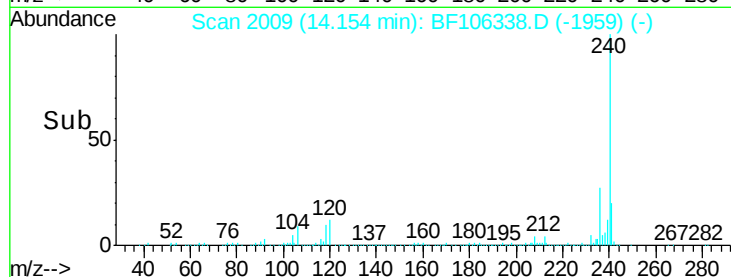

#78

Terphenyl-d14

Concen: 58.692 ng

RT: 13.09 min Scan# 1828

Delta R.T. 0.00 min

Lab File: BF106338.D

Acq: 12 Jun 2018 12:28


Tgt Ion:244 Resp: 1174342

Ion Ratio Lower Upper

244 100

212 7.1 5.4 8.0



122 9.5 11.0 16.4#

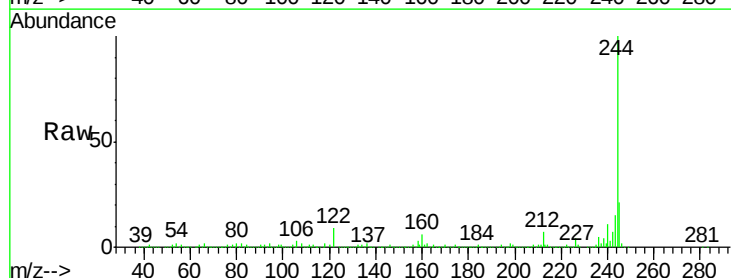


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

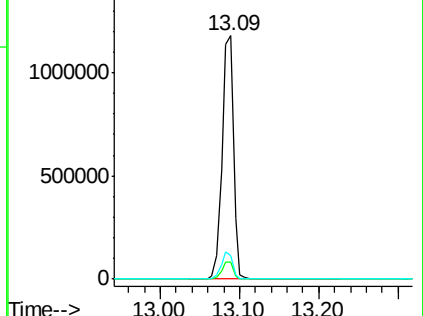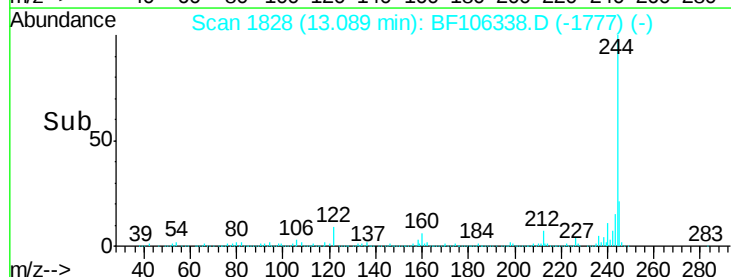

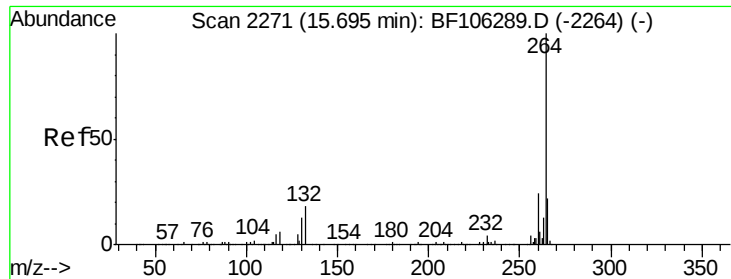

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.71 min Scan# 2273
Delta R.T. 0.01 min
Lab File: BF106338.D
Acq: 12 Jun 2018 12:28

Instrument :
BNA_F
ClientSampleId :
MS-CON-2RX

Tot Ion:264 Resp: 517148
Ion Ratio Lower Upper
264 100
260 23.7 19.2 28.8
265 21.5 17.5 26.3

