

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061218\
 Data File : BF106350.D
 Acq On : 12 Jun 2018 17:47
 Operator : JU/SJ
 Sample : J3415-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-33COMP

Quant Time: Jun 13 02:25:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 11 15:00:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	147799	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	491478	20.00	ng	0.00
38) Acenaphthene-d10	10.01	164	195983	20.00	ng	0.00
63) Phenanthrene-d10	11.51	188	394592	20.00	ng	0.00
75) Chrysene-d12	14.16	240	452425	20.00	ng	0.00
86) Perylene-d12	15.71	264	346119	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	785220	89.92	ng	0.01
7) Phenol-d6	6.60	99	935156	84.76	ng	0.00
23) Nitrobenzene-d5	7.53	82	587054	70.27	ng	0.00
41) 2,4,6-Tribromophenol	10.80	330	210887	111.84	ng	0.00
44) 2-Fluorobiphenyl	9.33	172	880838	77.62	ng	0.00
78) Terphenyl-d14	13.09	244	1080982	59.35	ng	0.00
Target Compounds						
10) Phenol	6.61	94	25746	2.138	ng	94
49) Dimethylphthalate	9.72	163	163956	11.710	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061218\
Data File : BF106350.D
Acq On : 12 Jun 2018 17:47
Operator : JU/SJ
Sample : J3415-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-33COMP

Quant Time: Jun 13 02:25:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 11 15:00:22 2018
Response via : Initial Calibration

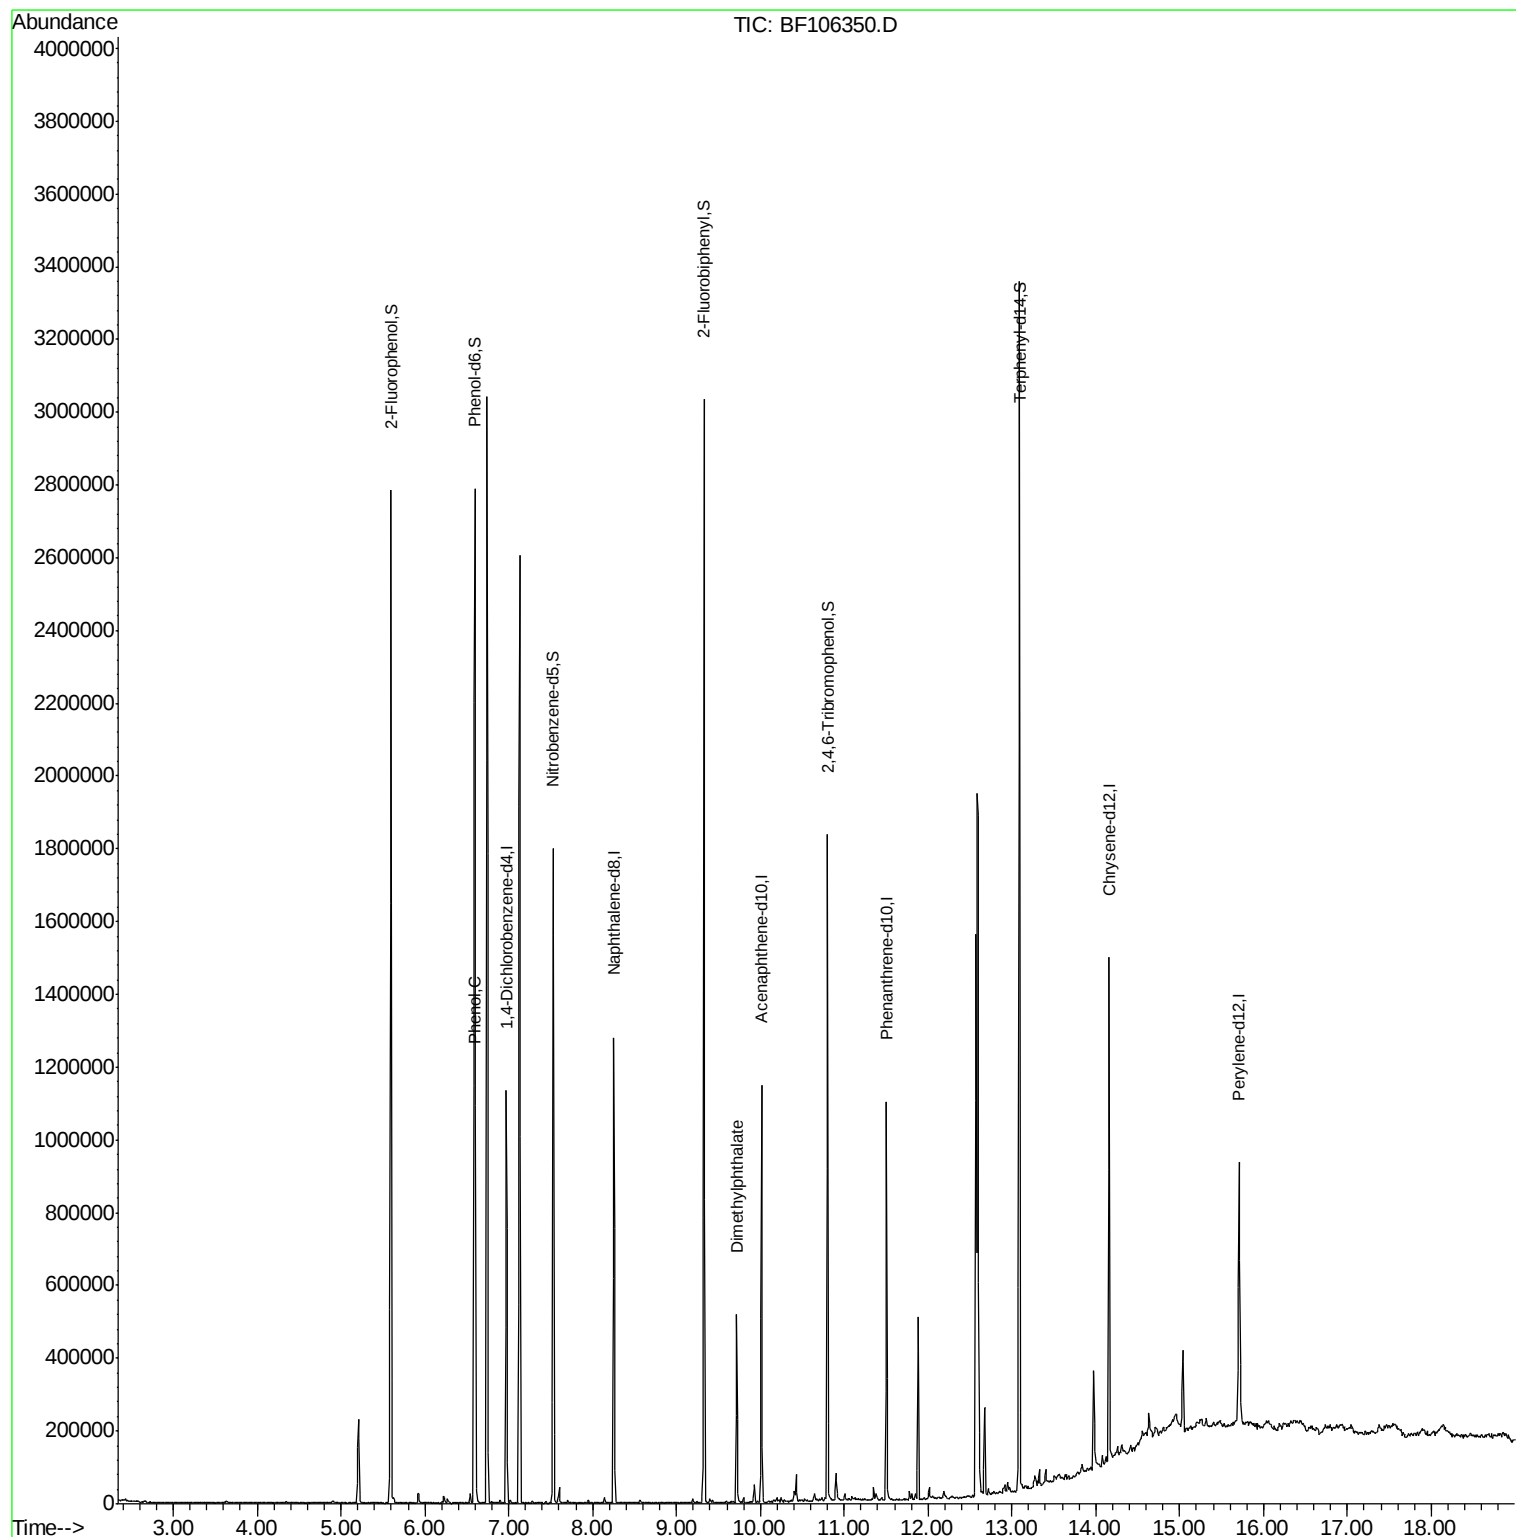




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 788
Delta R.T. 0.00 min
Lab File: BF106350.D
Acq: 12 Jun 2018 17:47

Instrument :
BNA_F
ClientSampleId :
SB-33COMP

Tot Ion:152 Resp: 147799
Ion Ratio Lower Upper
152 100
150 155.9 124.6 186.8
115 63.3 50.1 75.1

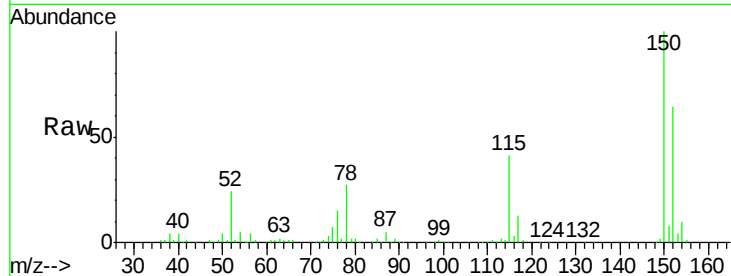


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

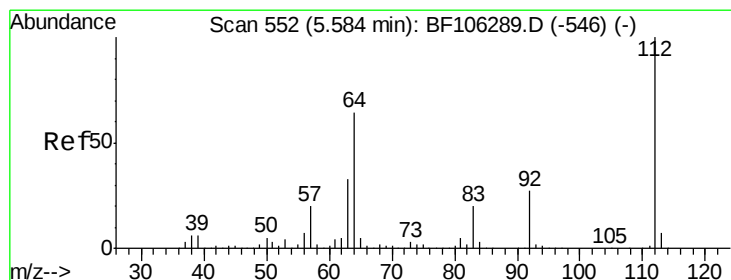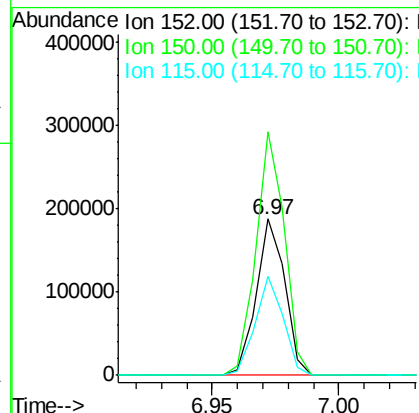



#5

2-Fluorophenol
Concen: 89.918 ng
RT: 5.60 min Scan# 554
Delta R.T. 0.01 min
Lab File: BF106350.D
Acq: 12 Jun 2018 17:47

Tgt Ion:112 Resp: 785220
Ion Ratio Lower Upper
112 100
64 64.2 47.9 71.9
63 32.1 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

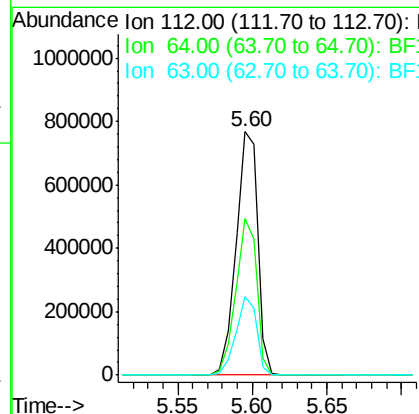



#7

Phenol-d6

Concen: 84.761 ng

RT: 6.60 min Scan# 724

Delta R.T. 0.01 min

Lab File: BF106350.D

Acq: 12 Jun 2018 17:47

Instrument :

BNA_F

ClientSampleId :

SB-33COMP


Tot Ion: 99 Resp: 935156

Ion Ratio Lower Upper




99 100

42 18.2 14.5 21.7

71 35.2 25.4 38.0

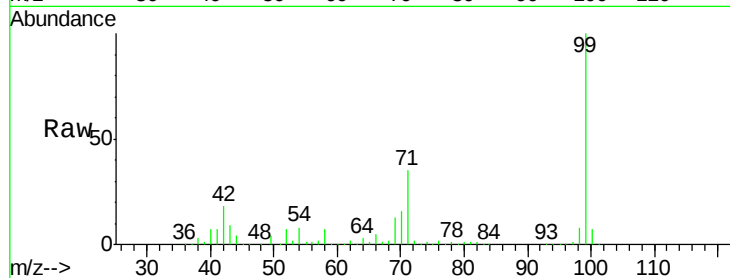

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

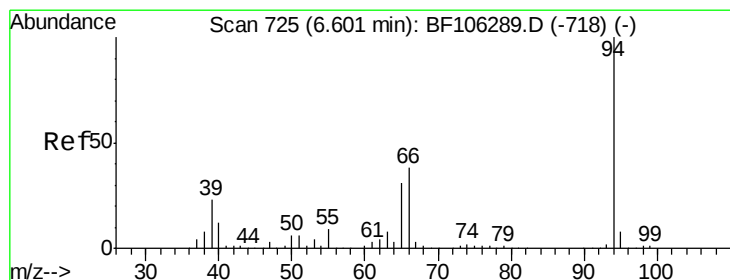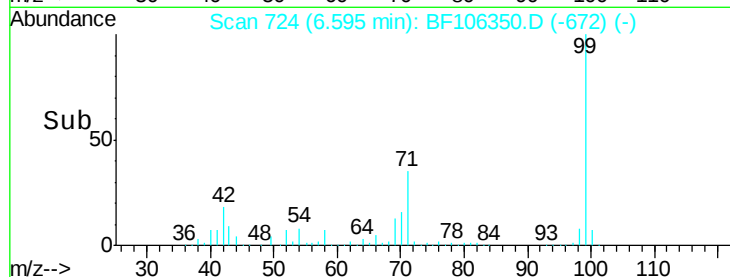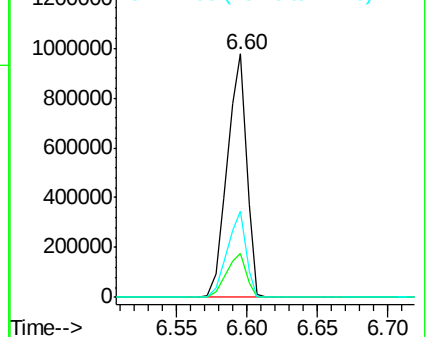

#10

Phenol

Concen: 2.138 ng

RT: 6.61 min Scan# 726

Delta R.T. 0.01 min

Lab File: BF106350.D

Acq: 12 Jun 2018 17:47


Tgt Ion: 94 Resp: 25746

Ion Ratio Lower Upper



94 100


65 25.6 7.9 47.9

66 32.1 16.2 56.2

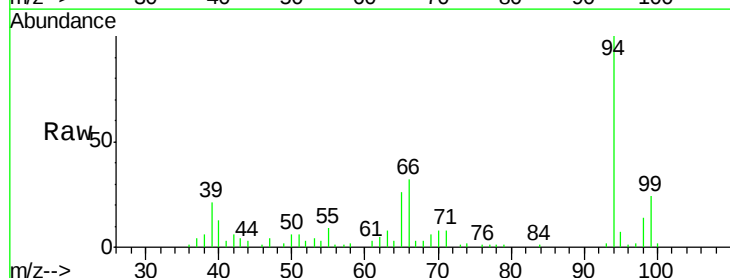

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

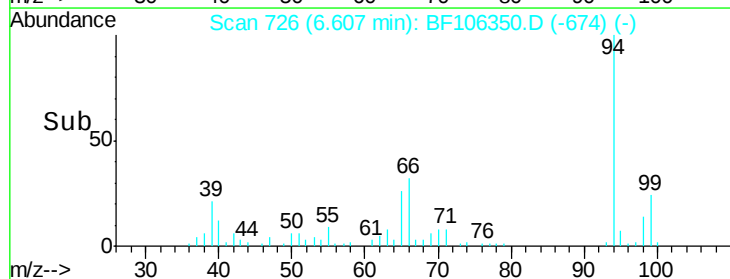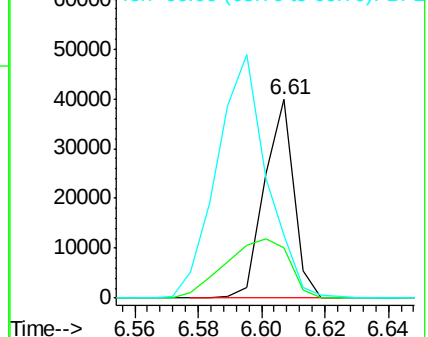


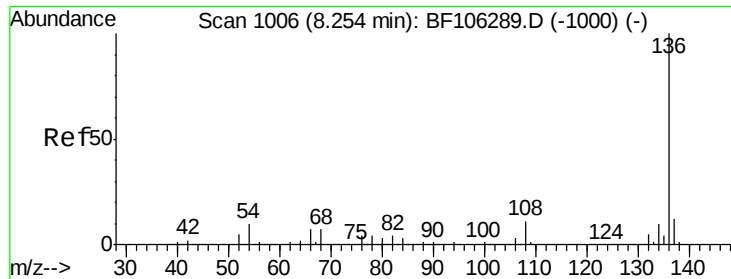




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.25 min Scan# 1006
Delta R.T. 0.00 min
Lab File: BF106350.D
Acq: 12 Jun 2018 17:47

Instrument :
BNA_F
ClientSampleId :
SB-33COMP

Tot Ion:136	Resp:	491478
Ion Ratio	Lower	Upper
136	100	
137	11.1	8.9 13.3
54	8.9	6.6 9.8
68	7.0	5.0 7.4




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

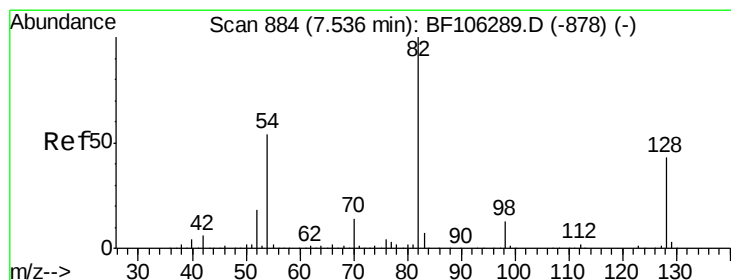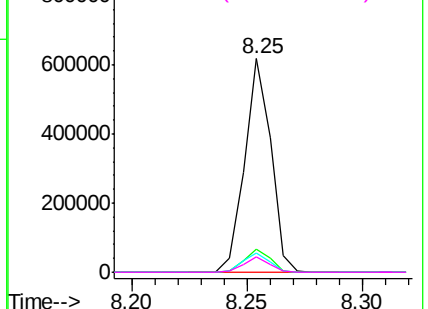




#23
Nitrobenzene-d5
Concen: 70.269 ng
RT: 7.53 min Scan# 883
Delta R.T. -0.01 min
Lab File: BF106350.D
Acq: 12 Jun 2018 17:47

Tgt Ion: 82	Resp:	587054
Ion Ratio	Lower	Upper
82	100	
128	41.0	36.1 54.1
54	51.7	41.4 62.2



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

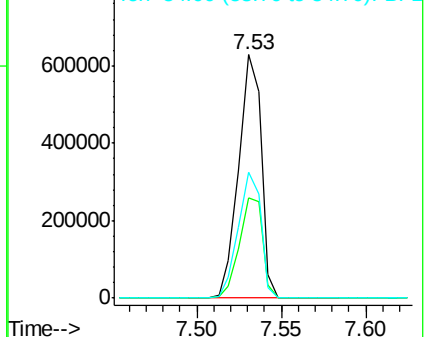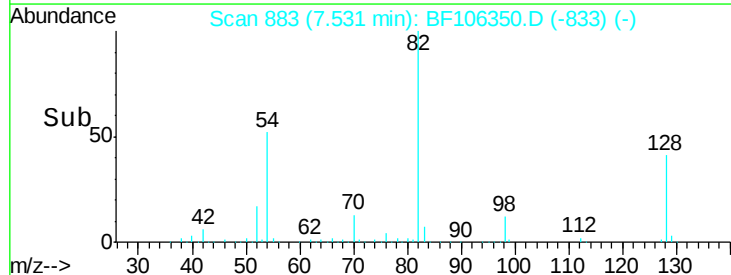



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.01 min Scan# 1305

Delta R.T. 0.00 min

Lab File: BF106350.D

Acq: 12 Jun 2018 17:47

Instrument :

BNA_F

ClientSampleId :

SB-33COMP


Tot Ion:164 Resp: 195983

Ion Ratio Lower Upper

164 100

162 106.7 86.1 129.1




160 47.2 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

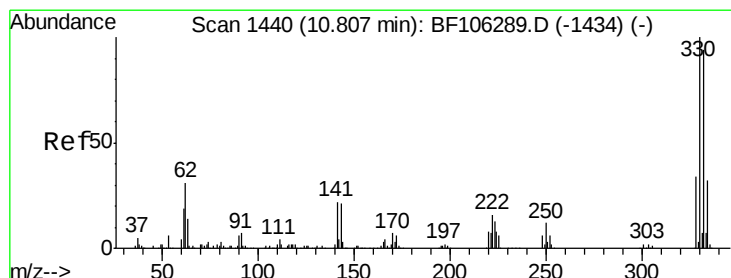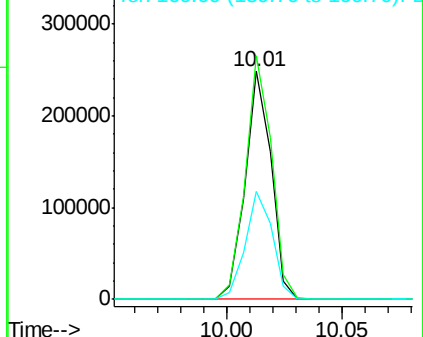

#41

2,4,6-Tribromophenol

Concen: 111.835 ng

RT: 10.80 min Scan# 1439

Delta R.T. -0.01 min

Lab File: BF106350.D

Acq: 12 Jun 2018 17:47


Tgt Ion:330 Resp: 210887

Ion Ratio Lower Upper

330 100

332 96.4 77.0 115.6



141 29.9 29.9 44.9#




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

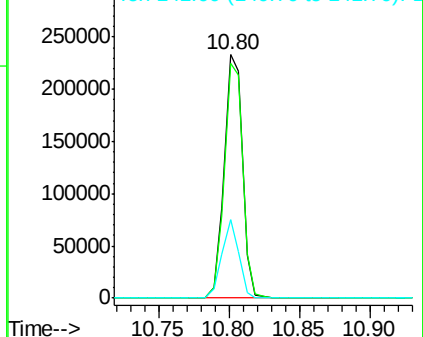

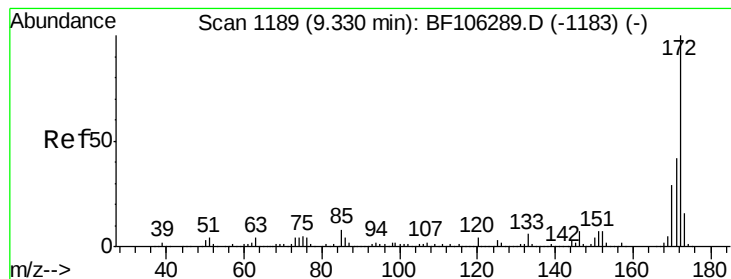

#44

2-Fluorobiphenyl

Concen: 77.618 ng

RT: 9.33 min Scan# 1189

Delta R.T. 0.00 min

Lab File: BF106350.D

Acq: 12 Jun 2018 17:47

Instrument :

BNA_F

ClientSampleId :

SB-33COMP


Tot Ion:172 Resp: 880838

Ion Ratio Lower Upper

172 100

171 37.5 29.7 44.5




170 25.4 19.6 29.4



Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

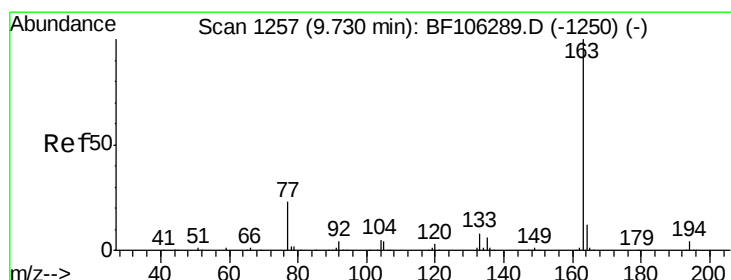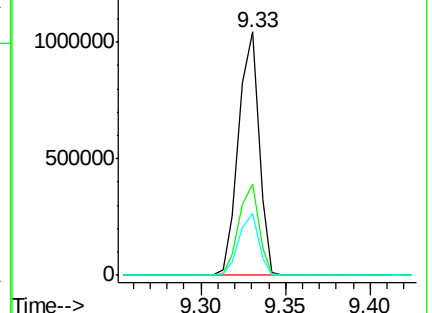

#49

Dimethylphthalate

Concen: 11.710 ng

RT: 9.72 min Scan# 1255

Delta R.T. -0.01 min

Lab File: BF106350.D

Acq: 12 Jun 2018 17:47


Tgt Ion:163 Resp: 163956

Ion Ratio Lower Upper

163 100

194 3.7 2.7 4.1



164 9.7 8.2 12.2




Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E



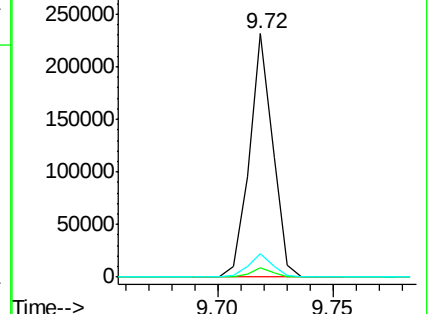



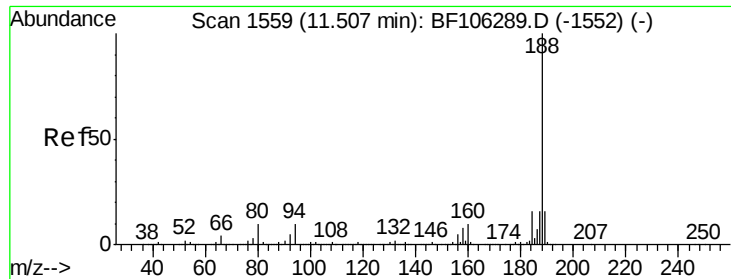

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.51 min Scan# 1559
Delta R.T. 0.00 min
Lab File: BF106350.D
Acq: 12 Jun 2018 17:47




Instrument :
BNA_F
ClientSampleId :
SB-33COMP


Tot Ion:188 Resp: 394592
Ion Ratio Lower Upper
188 100
94 9.0 8.5 12.7
80 9.3 9.2 13.8

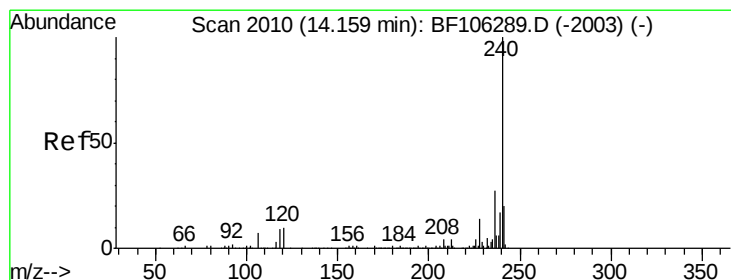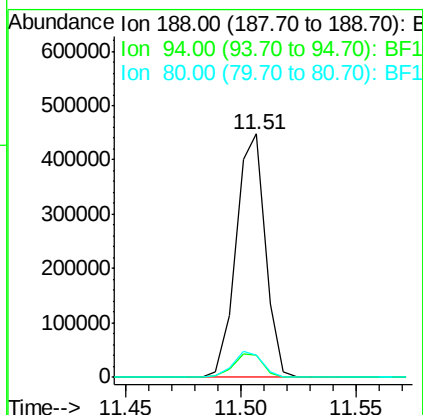

#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.16 min Scan# 2010
Delta R.T. 0.00 min
Lab File: BF106350.D
Acq: 12 Jun 2018 17:47

Tgt Ion:240 Resp: 452425
Ion Ratio Lower Upper
240 100
120 11.1 9.5 14.3
236 25.7 20.7 31.1

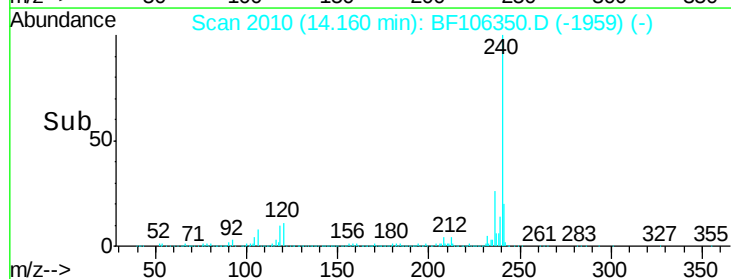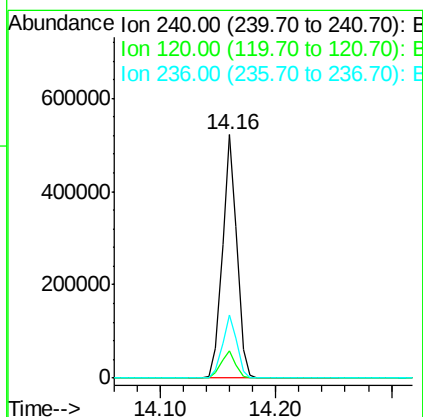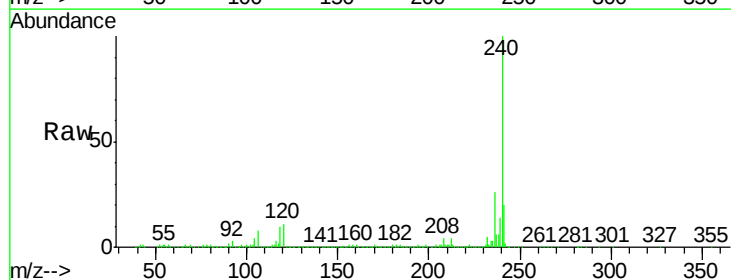



#78

Terphenyl-d14

Concen: 59.345 ng

RT: 13.09 min Scan# 1828

Delta R.T. 0.00 min

Lab File: BF106350.D

Acq: 12 Jun 2018 17:47

Instrument :

BNA_F

ClientSampleId :

SB-33COMP


Tot Ion:244 Resp: 1080982

Ion Ratio Lower Upper

244 100

212 7.2 5.4 8.0




122 11.0 11.0 16.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

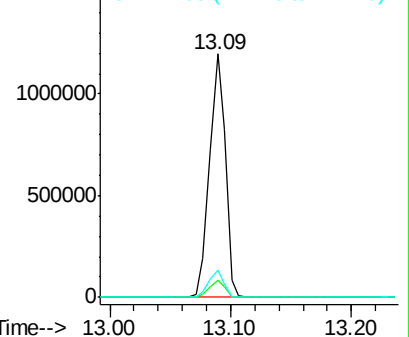

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.71 min Scan# 2274

Delta R.T. 0.02 min

Lab File: BF106350.D

Acq: 12 Jun 2018 17:47


Tgt Ion:264 Resp: 346119

Ion Ratio Lower Upper

264 100

260 23.8 19.2 28.8

265 21.8 17.5 26.3



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

