

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061218\
 Data File : BF106353.D
 Acq On : 12 Jun 2018 19:09
 Operator : JU/SJ
 Sample : J3415-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-36COMP

Quant Time: Jun 13 03:08:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 11 15:00:22 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	136688	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	459519	20.00	ng	0.00
38) Acenaphthene-d10	10.01	164	188673	20.00	ng	0.00
63) Phenanthrene-d10	11.51	188	378259	20.00	ng	0.00
75) Chrysene-d12	14.15	240	427607	20.00	ng	0.00
86) Perylene-d12	15.69	264	322525	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	732744	90.73	ng	0.01
7) Phenol-d6	6.60	99	863163	84.60	ng	0.00
23) Nitrobenzene-d5	7.53	82	528684	67.68	ng	0.00
41) 2,4,6-Tribromophenol	10.80	330	193321	106.49	ng	0.00
44) 2-Fluorobiphenyl	9.33	172	795556	70.92	ng	0.00
78) Terphenyl-d14	13.09	244	984812	57.20	ng	0.00
Target Compounds						
10) Phenol	6.61	94	24354	2.186	ng	99
49) Dimethylphthalate	9.72	163	140333	10.411	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061218\
Data File : BF106353.D
Acq On : 12 Jun 2018 19:09
Operator : JU/SJ
Sample : J3415-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-36COMP

Quant Time: Jun 13 03:08:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 11 15:00:22 2018
Response via : Initial Calibration

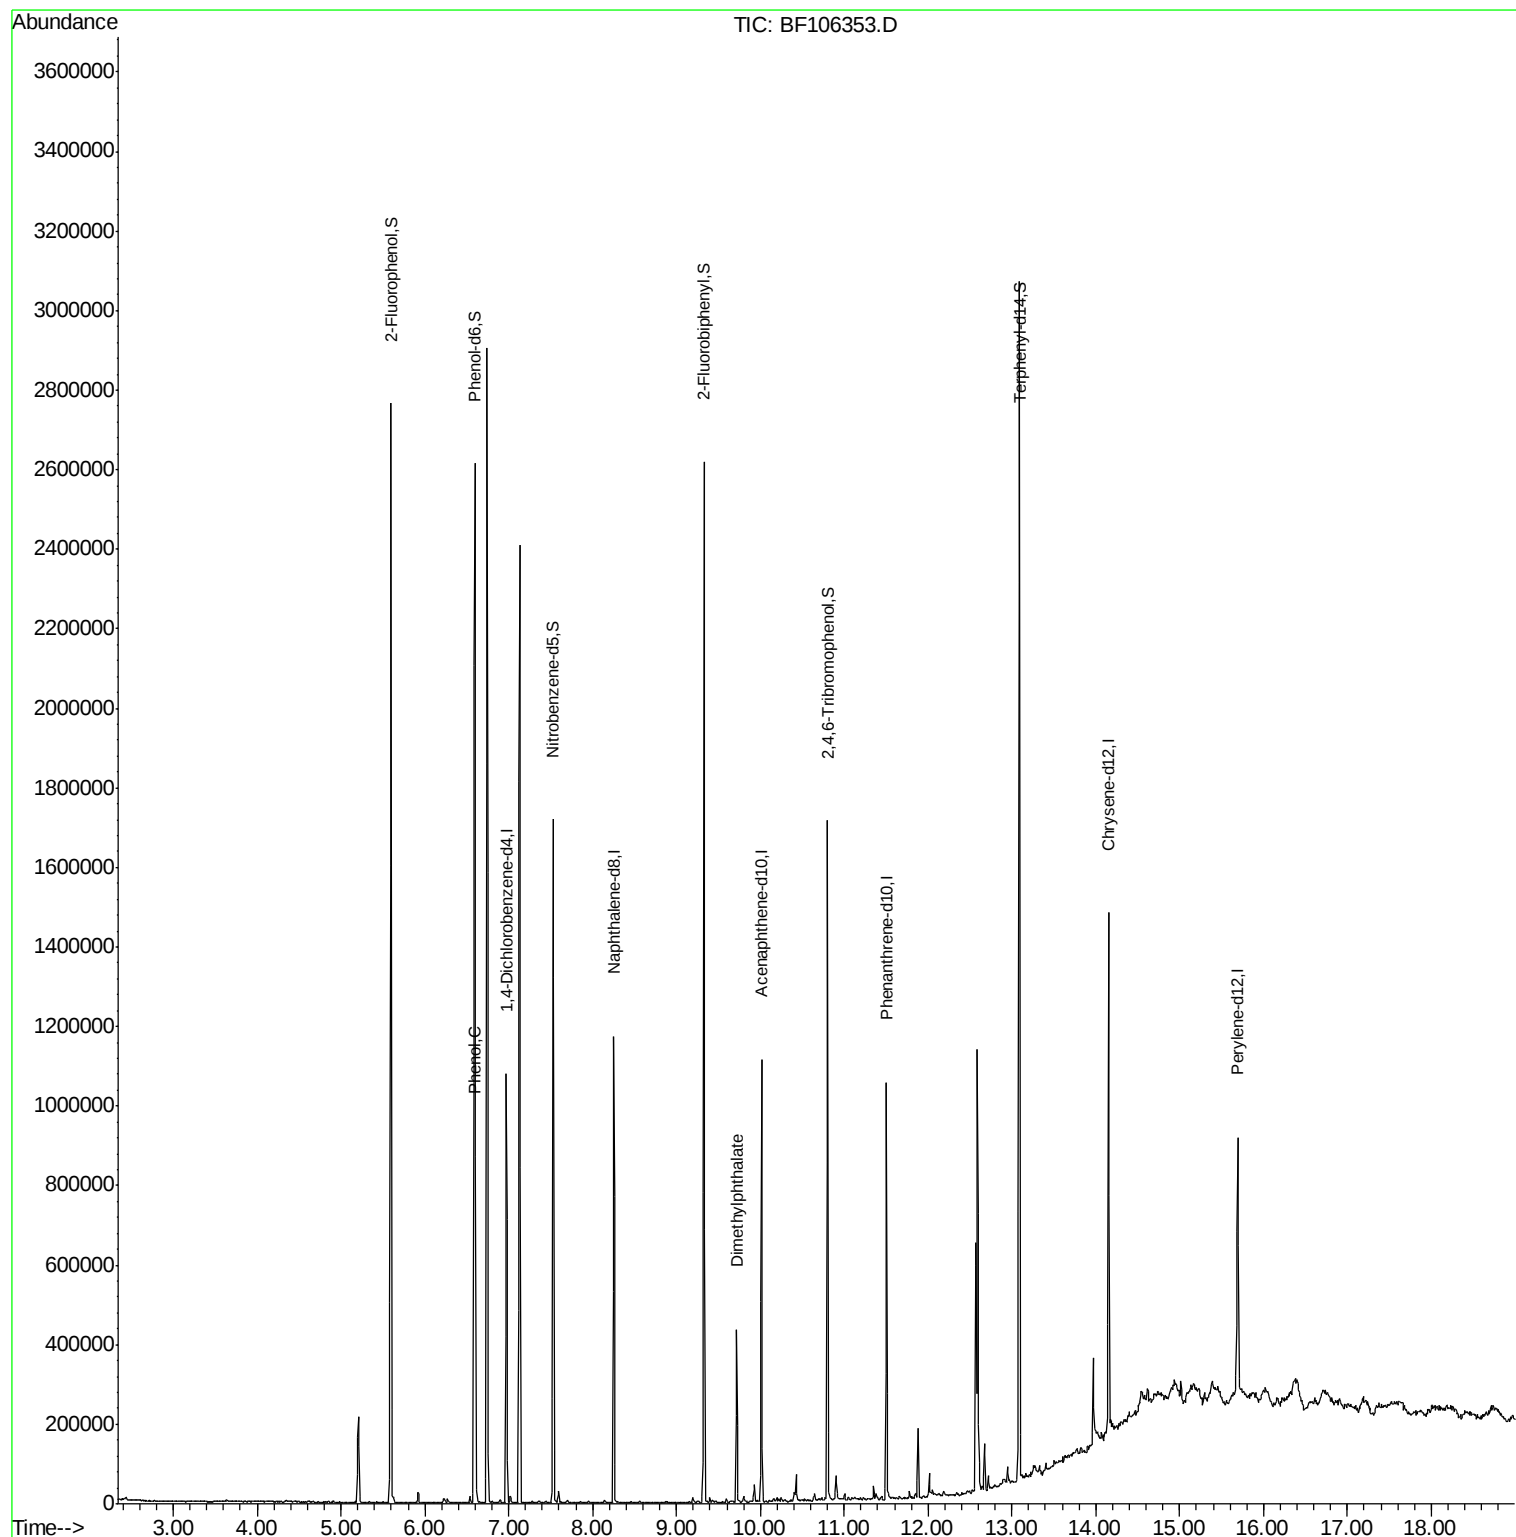

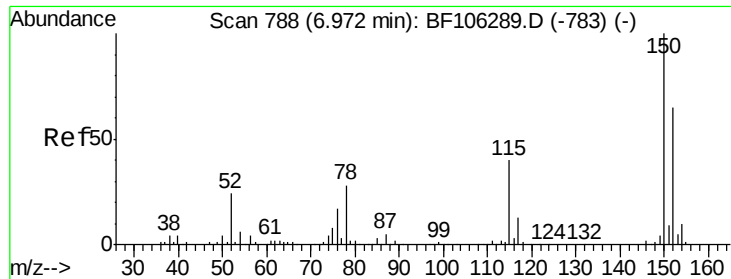


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 788
Delta R.T. 0.00 min
Lab File: BF106353.D
Acq: 12 Jun 2018 19:09

Instrument :
BNA_F
ClientSampleId :
SB-36COMP

Tot Ion:152 Resp: 136688
Ion Ratio Lower Upper
152 100
150 161.1 124.6 186.8
115 64.6 50.1 75.1

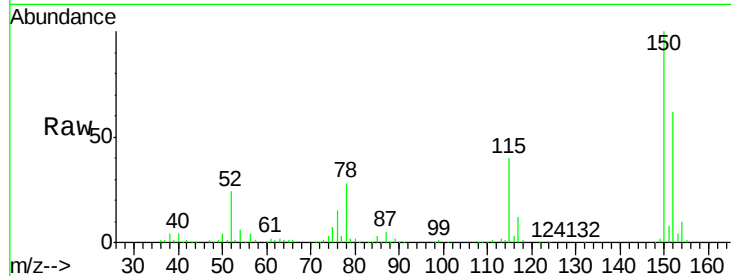


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

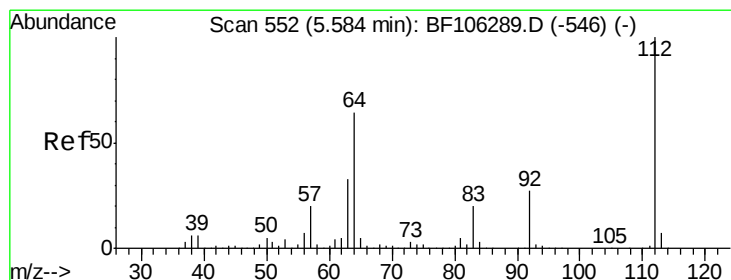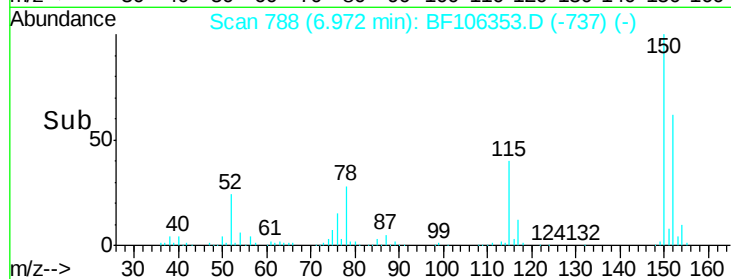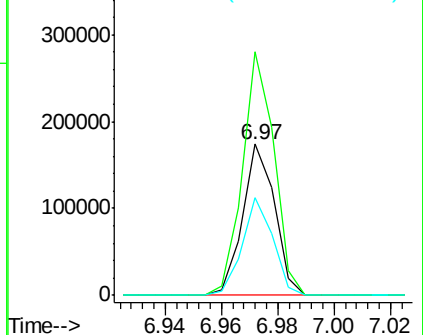



#5


2-Fluorophenol
Concen: 90.730 ng
RT: 5.60 min Scan# 554
Delta R.T. 0.01 min
Lab File: BF106353.D
Acq: 12 Jun 2018 19:09

Tgt Ion:112 Resp: 732744
Ion Ratio Lower Upper
112 100
64 61.3 47.9 71.9
63 31.3 23.7 35.5

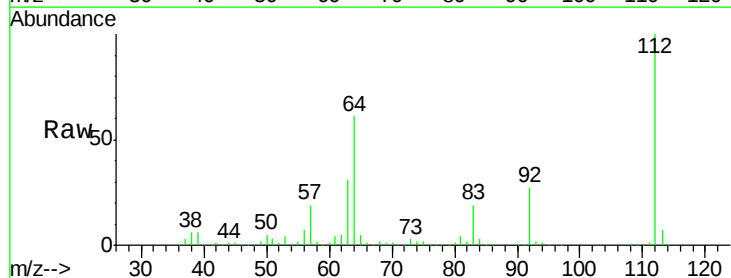

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

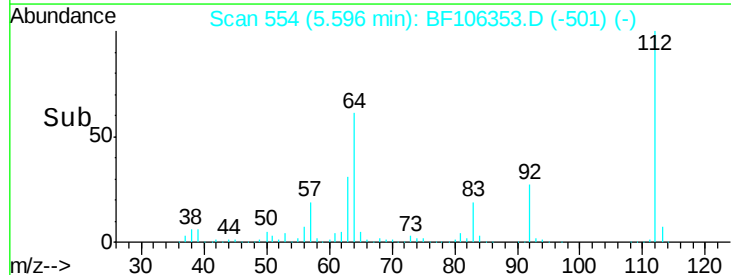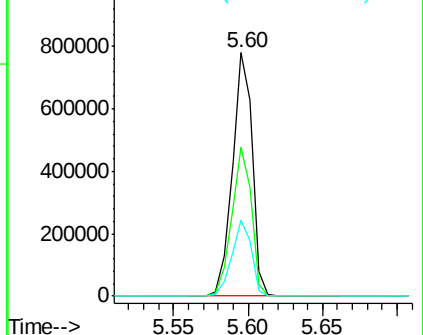

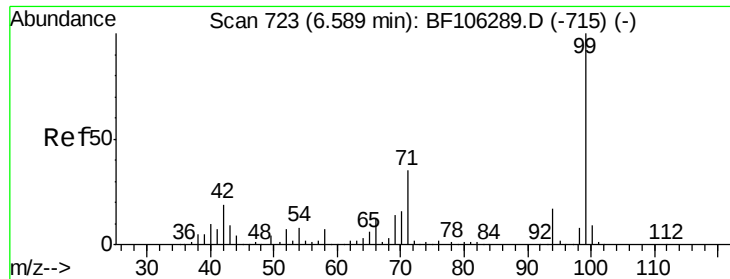

#7

Phenol-d6

Concen: 84.596 ng

RT: 6.60 min Scan# 724

Delta R.T. 0.01 min

Lab File: BF106353.D

Acq: 12 Jun 2018 19:09

Instrument :

BNA_F

ClientSampleId :

SB-36COMP


Tot Ion: 99 Resp: 863163

Ion Ratio Lower Upper




99 100

42 18.0 14.5 21.7

71 34.0 25.4 38.0

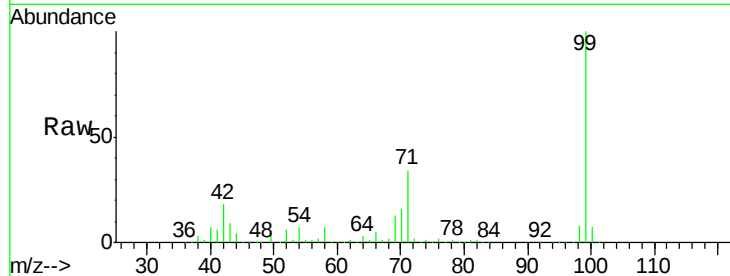

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

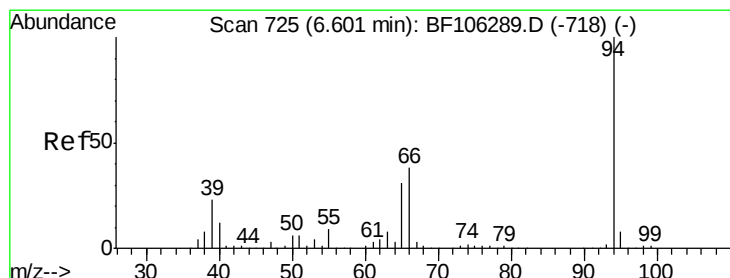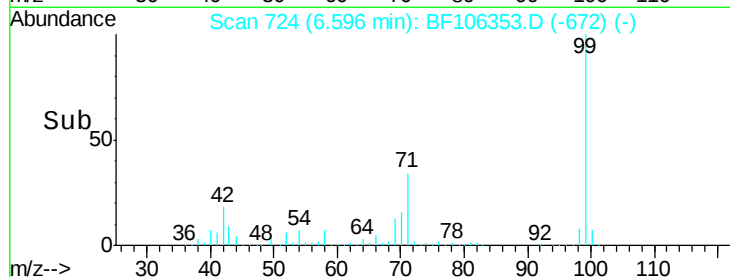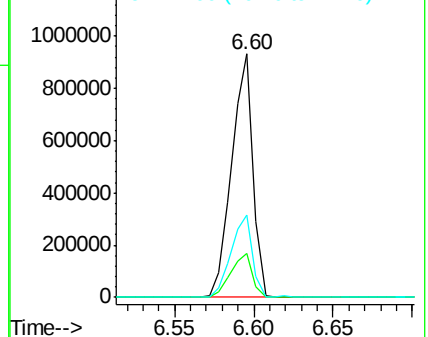

#10

Phenol

Concen: 2.186 ng

RT: 6.61 min Scan# 726

Delta R.T. 0.01 min

Lab File: BF106353.D

Acq: 12 Jun 2018 19:09


Tgt Ion: 94 Resp: 24354

Ion Ratio Lower Upper



94 100


65 27.7 7.9 47.9

66 35.2 16.2 56.2

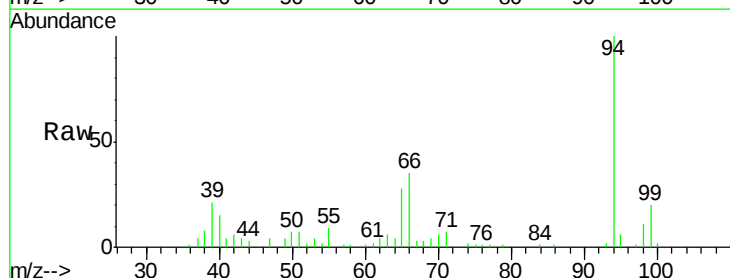

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

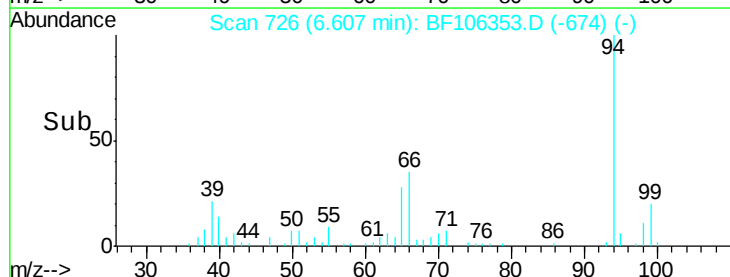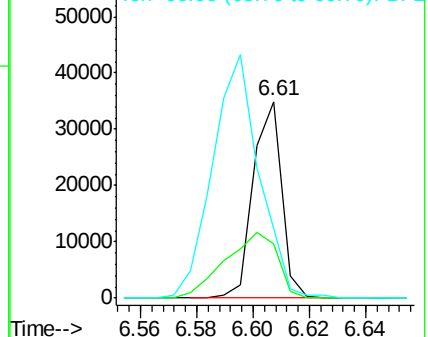


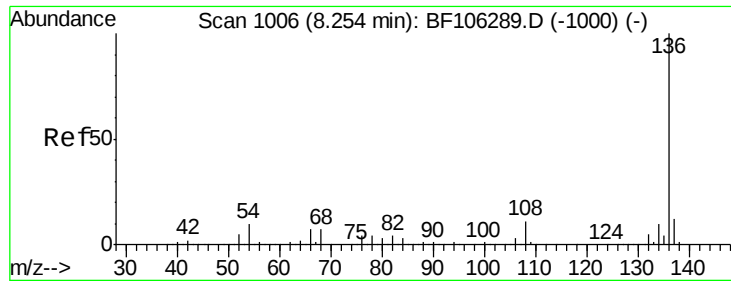




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.25 min Scan# 1006
Delta R.T. 0.00 min
Lab File: BF106353.D
Acq: 12 Jun 2018 19:09

Instrument :
BNA_F
ClientSampleId :
SB-36COMP

Tot Ion:136 Resp: 459519
Ion Ratio Lower Upper
136 100
137 11.2 8.9 13.3
54 9.0 6.6 9.8
68 6.6 5.0 7.4

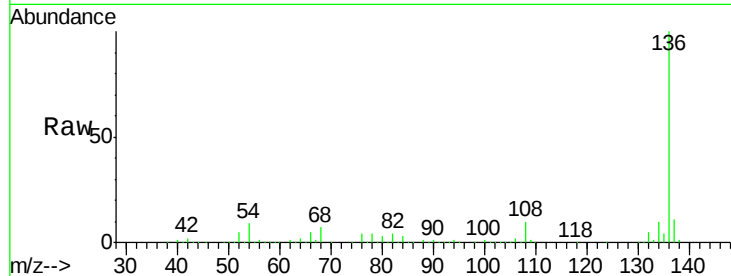


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

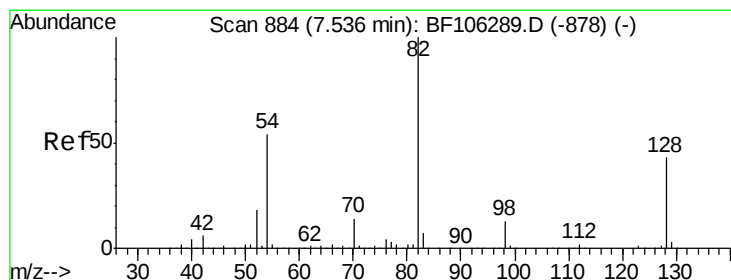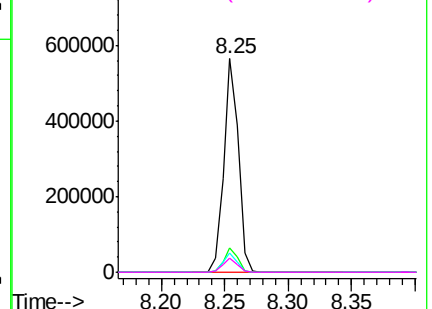
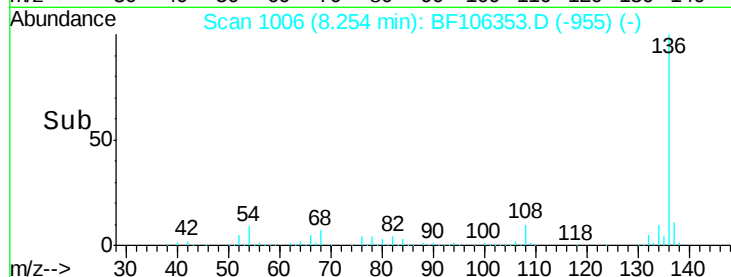



#23
Nitrobenzene-d5
Concen: 67.683 ng
RT: 7.53 min Scan# 883
Delta R.T. -0.01 min
Lab File: BF106353.D
Acq: 12 Jun 2018 19:09

Tgt Ion: 82 Resp: 528684
Ion Ratio Lower Upper
82 100
128 42.4 36.1 54.1
54 53.7 41.4 62.2

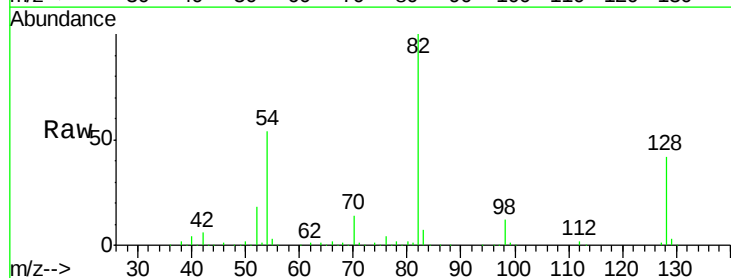

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

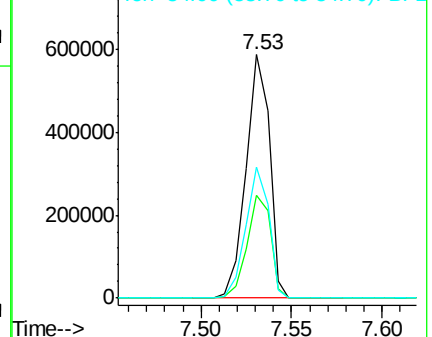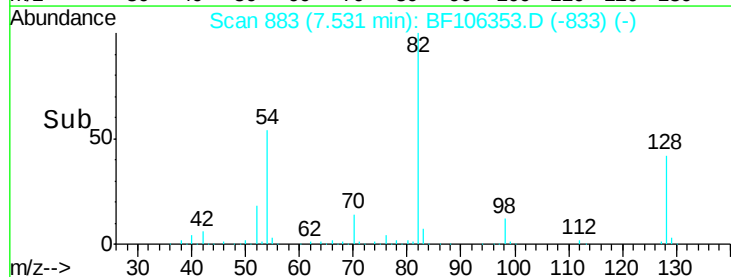

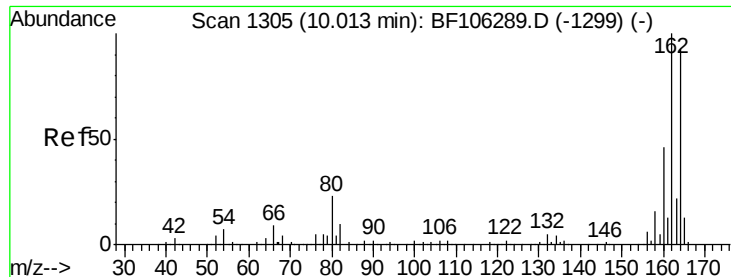

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.01 min Scan# 1305

Delta R.T. 0.00 min

Lab File: BF106353.D

Acq: 12 Jun 2018 19:09

Instrument :

BNA_F

ClientSampleId :

SB-36COMP


Tot Ion:164 Resp: 188673

Ion Ratio Lower Upper

164 100

162 101.6 86.1 129.1




160 47.4 38.3 57.5

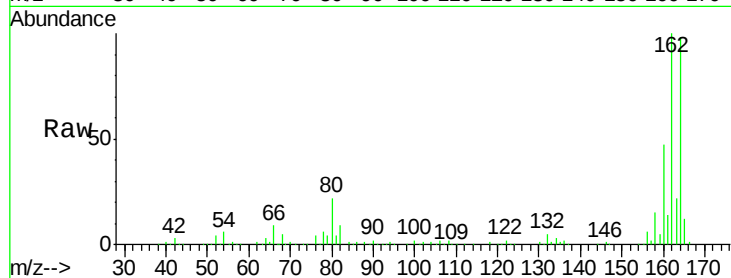

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

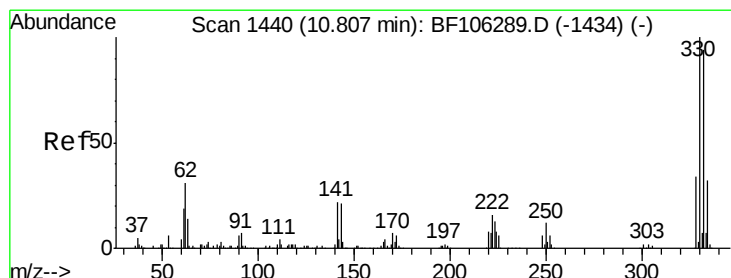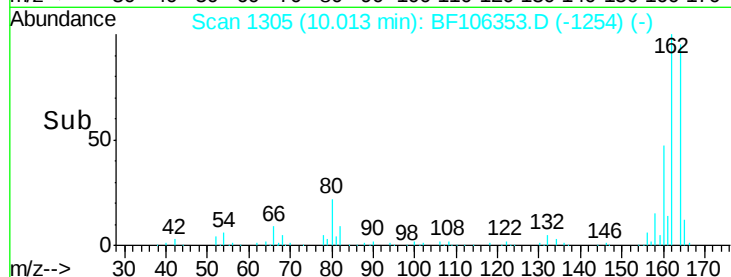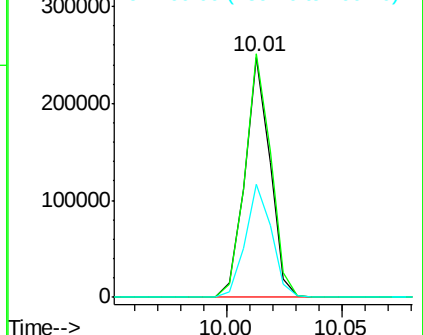

#41

2,4,6-Tribromophenol

Concen: 106.492 ng

RT: 10.80 min Scan# 1439

Delta R.T. -0.01 min

Lab File: BF106353.D

Acq: 12 Jun 2018 19:09


Tgt Ion:330 Resp: 193321

Ion Ratio Lower Upper

330 100

332 94.9 77.0 115.6



141 30.5 29.9 44.9

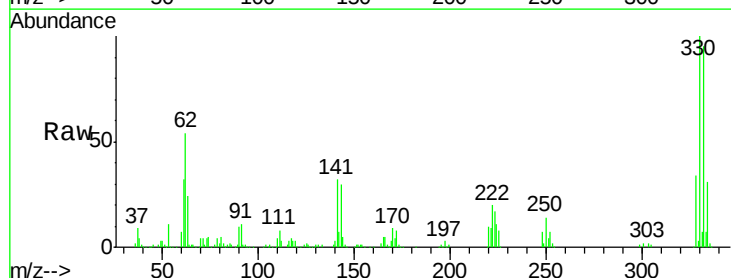


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

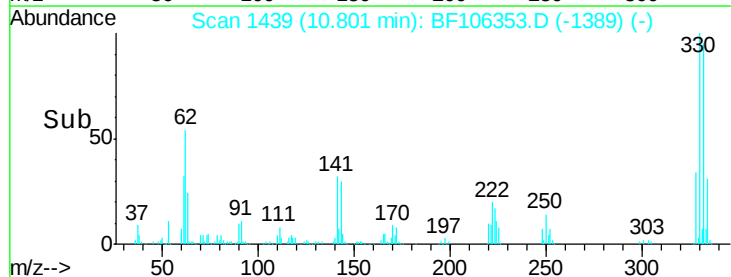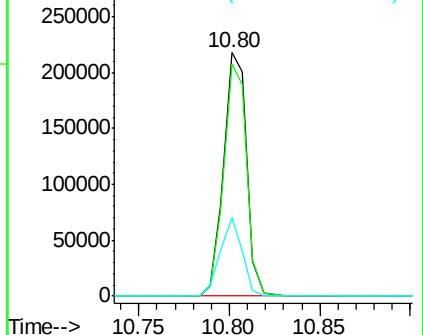


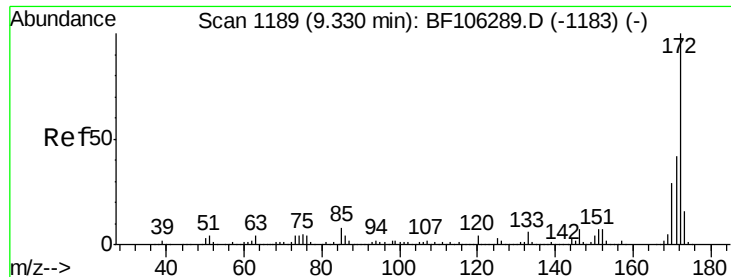




#44
2-Fluorobiphenyl
Concen: 70.923 ng
RT: 9.33 min Scan# 1189
Delta R.T. 0.00 min
Lab File: BF106353.D
Acq: 12 Jun 2018 19:09

Instrument :
BNA_F
ClientSampleId :
SB-36COMP

Tot Ion:172 Resp: 795556
Ion Ratio Lower Upper
172 100
171 36.4 29.7 44.5
170 25.1 19.6 29.4

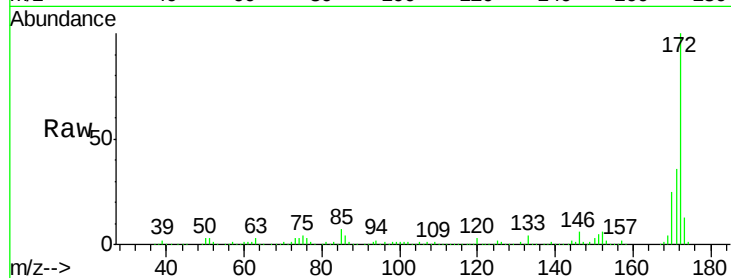


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

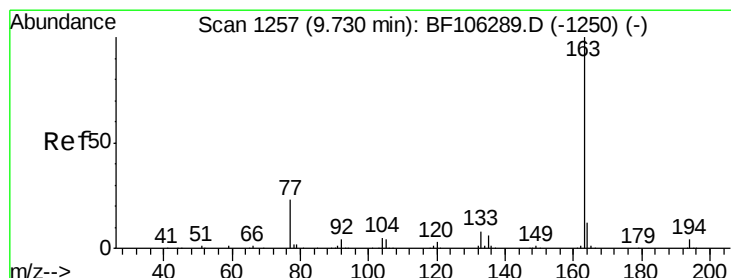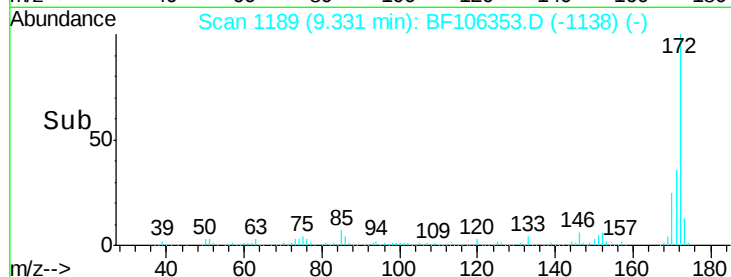
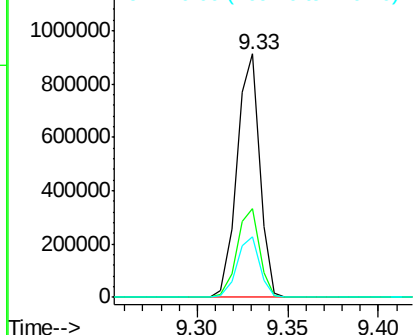



#49
Dimethylphthalate
Concen: 10.411 ng
RT: 9.72 min Scan# 1255
Delta R.T. -0.01 min
Lab File: BF106353.D
Acq: 12 Jun 2018 19:09

Tgt Ion:163 Resp: 140333
Ion Ratio Lower Upper
163 100
194 3.7 2.7 4.1
164 10.4 8.2 12.2

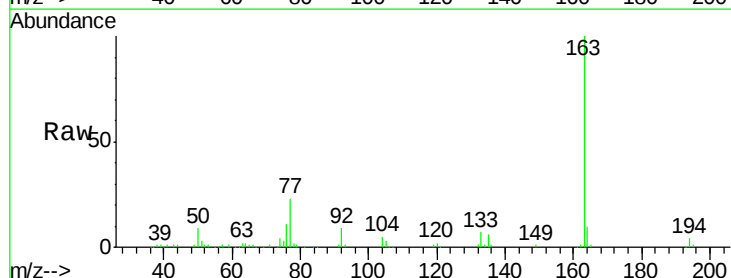

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

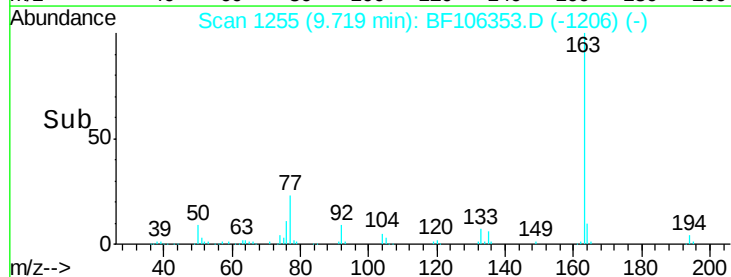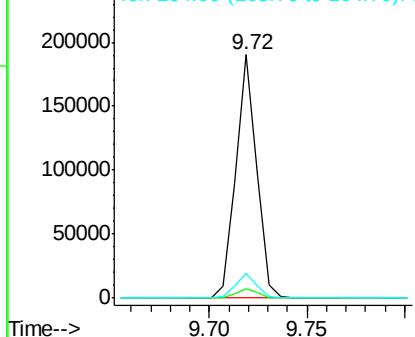


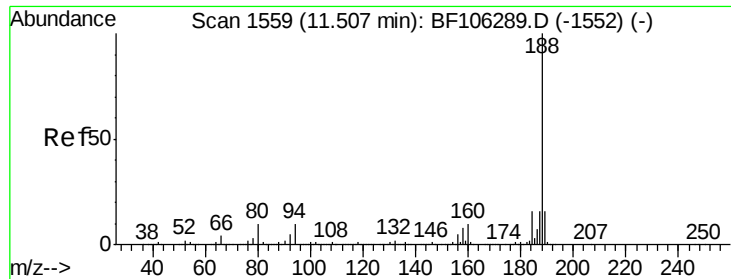




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.51 min Scan# 1559
Delta R.T. 0.00 min
Lab File: BF106353.D
Acq: 12 Jun 2018 19:09

Instrument :
BNA_F
ClientSampleId :
SB-36COMP

Tot Ion:188 Resp: 378259
Ion Ratio Lower Upper
188 100
94 8.9 8.5 12.7
80 9.8 9.2 13.8

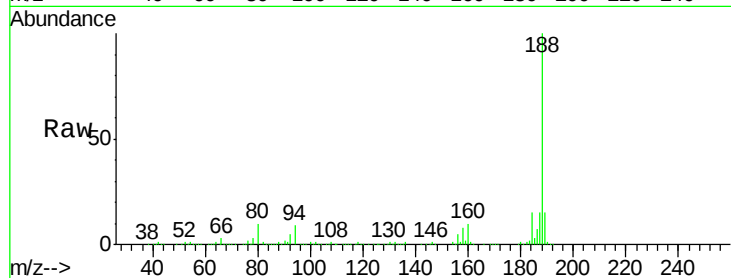


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

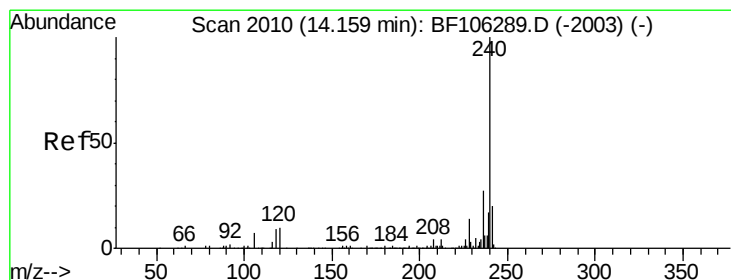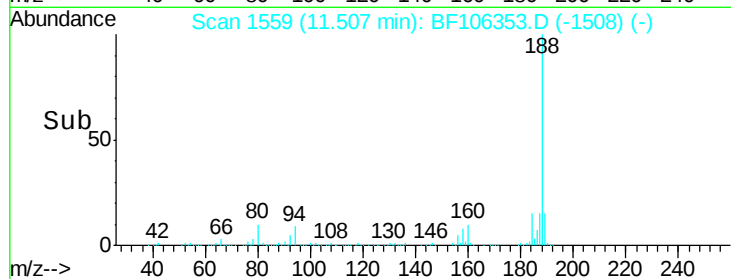
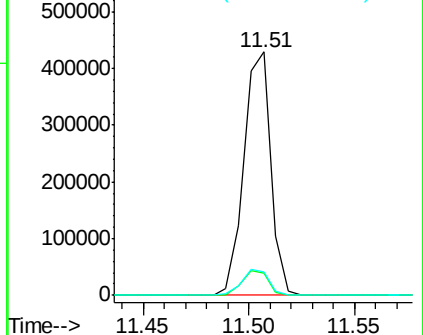



#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.15 min Scan# 2009
Delta R.T. -0.01 min
Lab File: BF106353.D
Acq: 12 Jun 2018 19:09

Tgt Ion:240 Resp: 427607
Ion Ratio Lower Upper
240 100
120 10.4 9.5 14.3
236 26.0 20.7 31.1

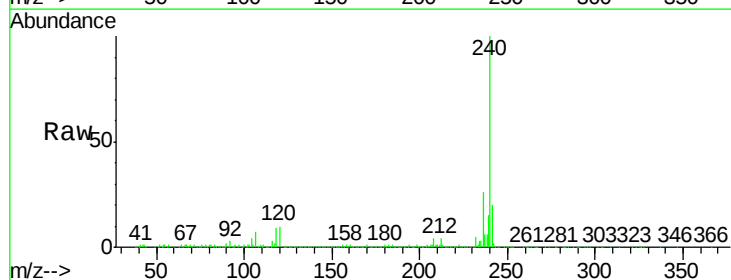

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

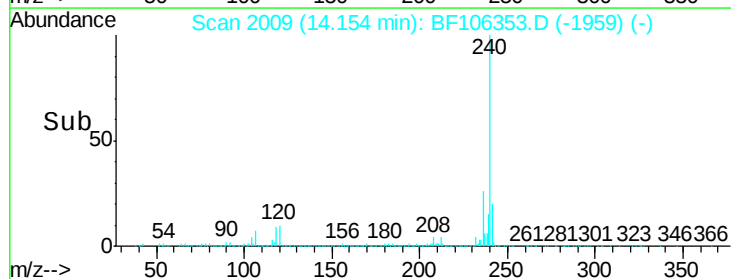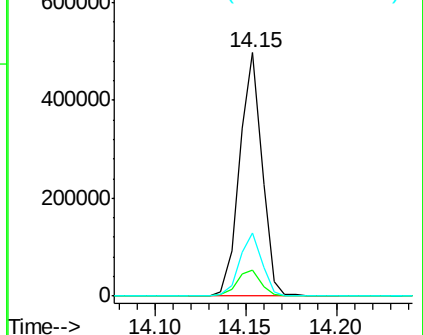

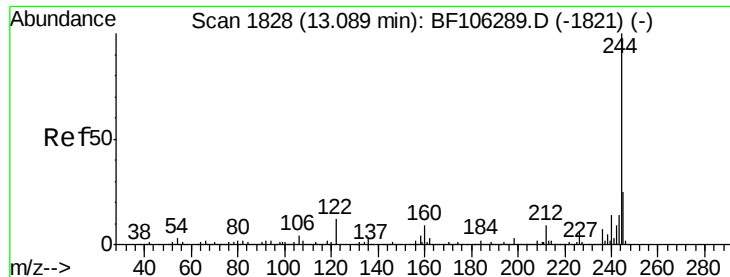

#78

Terphenyl-d14

Concen: 57.203 ng

RT: 13.09 min Scan# 1828

Delta R.T. 0.00 min

Lab File: BF106353.D

Acq: 12 Jun 2018 19:09

Instrument :

BNA_F

ClientSampled :

SB-36COMP


Tot Ion:244 Resp: 984812

Ion Ratio Lower Upper

244 100

212 7.2 5.4 8.0




122 10.7 11.0 16.4#

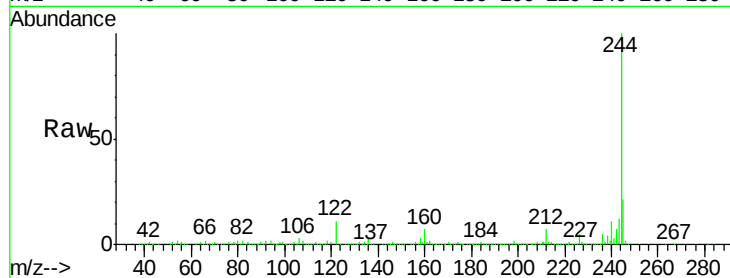

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

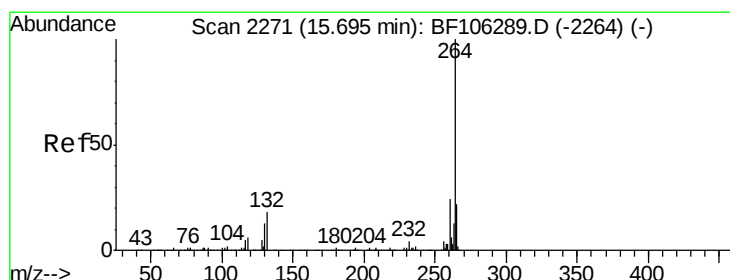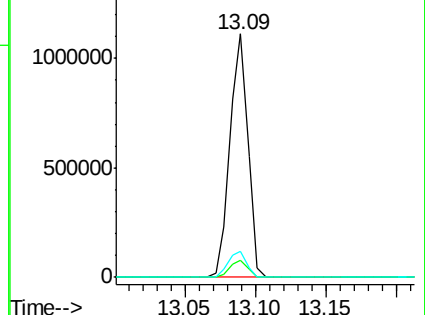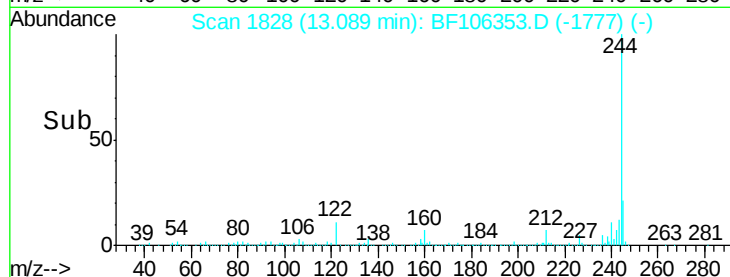

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.69 min Scan# 2271

Delta R.T. 0.00 min

Lab File: BF106353.D

Acq: 12 Jun 2018 19:09


Tgt Ion:264 Resp: 322525

Ion Ratio Lower Upper

264 100

260 23.4 19.2 28.8

265 22.0 17.5 26.3

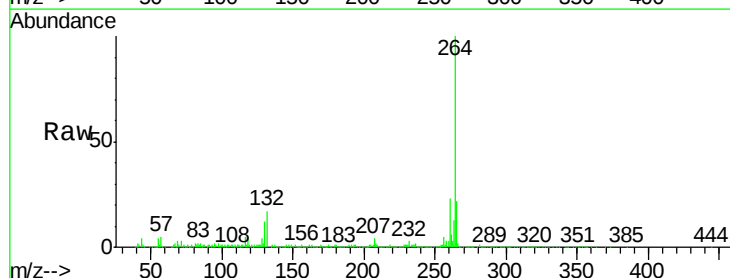

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

