


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061218\
Data File : BF106336.D
Acq On : 12 Jun 2018 11:26
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 13 10:51:26 2018

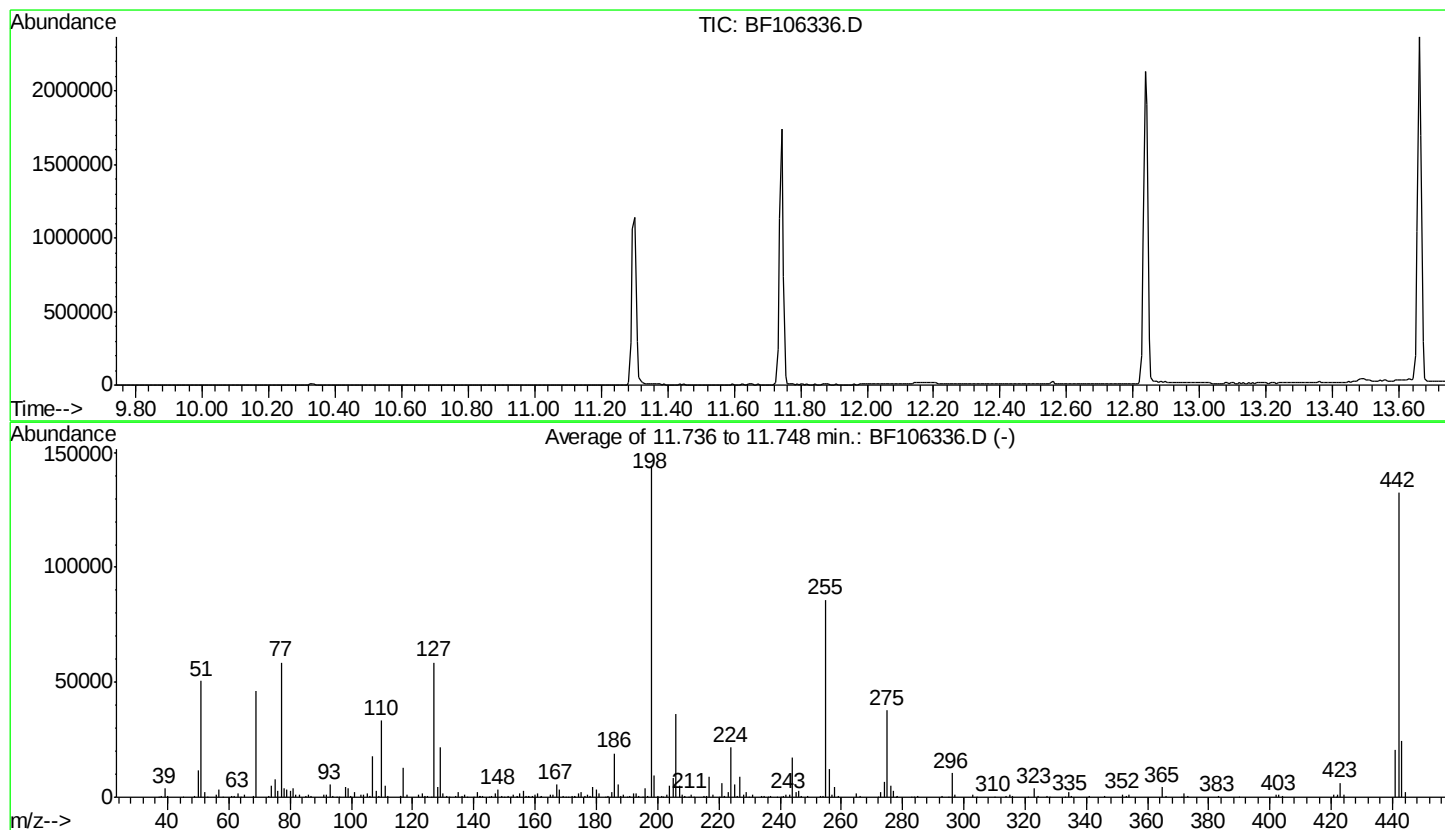

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	50424	PASS
68	69	0.00	2	1.7	760	PASS
69	198	0.00	100	31.9	46008	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.6	58584	PASS
197	198	0.00	2	0.6	854	PASS
198	198	100	100	100.0	144280	PASS
199	198	5	9	6.5	9435	PASS
275	198	10	60	26.1	37642	PASS
365	198	1	100	2.9	4242	PASS
441	443	0.01	100	82.5	20415	PASS
442	198	50	100	91.8	132426	PASS
443	442	15	24	18.7	24749	PASS