


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061218\
 Data File : BF106363.D
 Acq On : 13 Jun 2018 00:04
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 13 10:51:26 2018

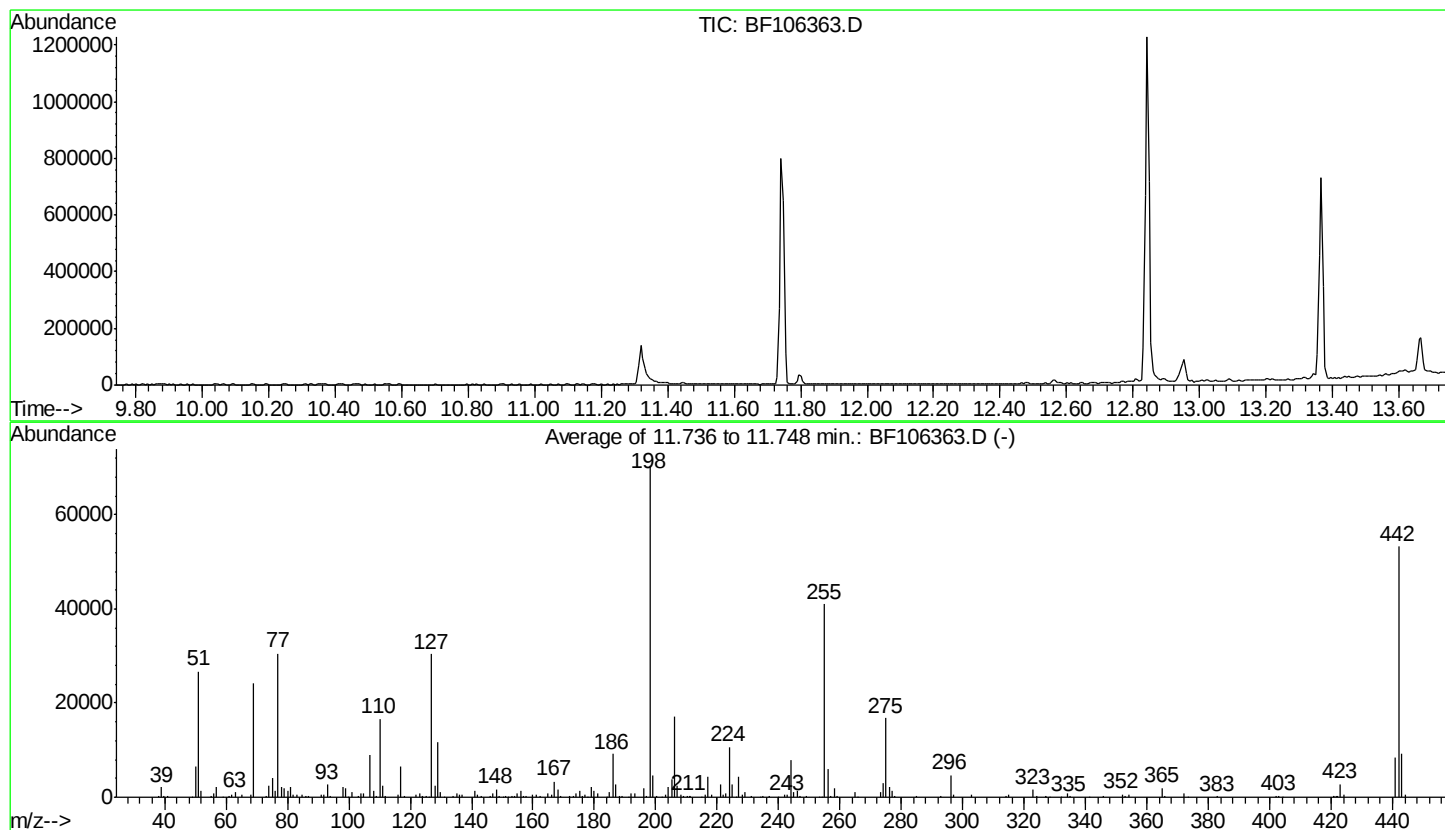

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	26722	PASS
68	69	0.00	2	1.8	428	PASS
69	198	0.00	100	34.6	24349	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.1	30376	PASS
197	198	0.00	2	0.3	207	PASS
198	198	100	100	100.0	70453	PASS
199	198	5	9	6.5	4604	PASS
275	198	10	60	23.9	16818	PASS
365	198	1	100	2.7	1934	PASS
441	443	0.01	100	91.4	8500	PASS
442	198	50	100	75.5	53205	PASS
443	442	15	24	17.5	9295	PASS