
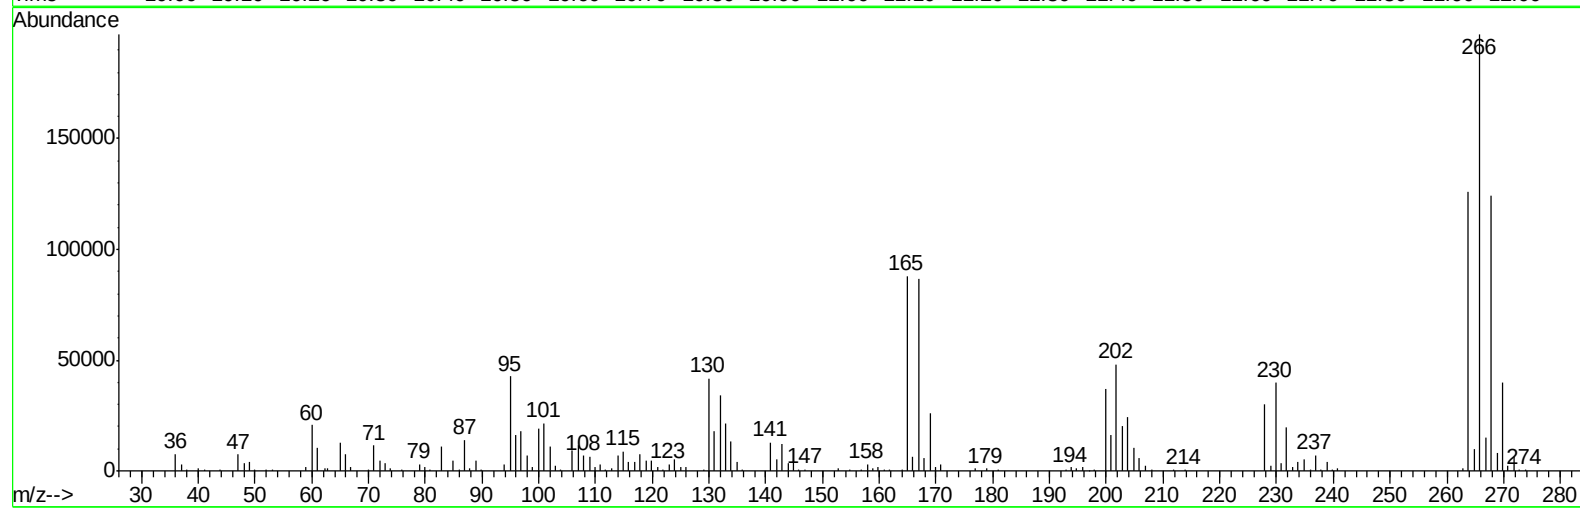


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF061219\
Data File : BF114966.D
Acq On : 12 Jun 2019 9:56
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 03:16:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 12 15:42:37 2019
Response via : Initial Calibration

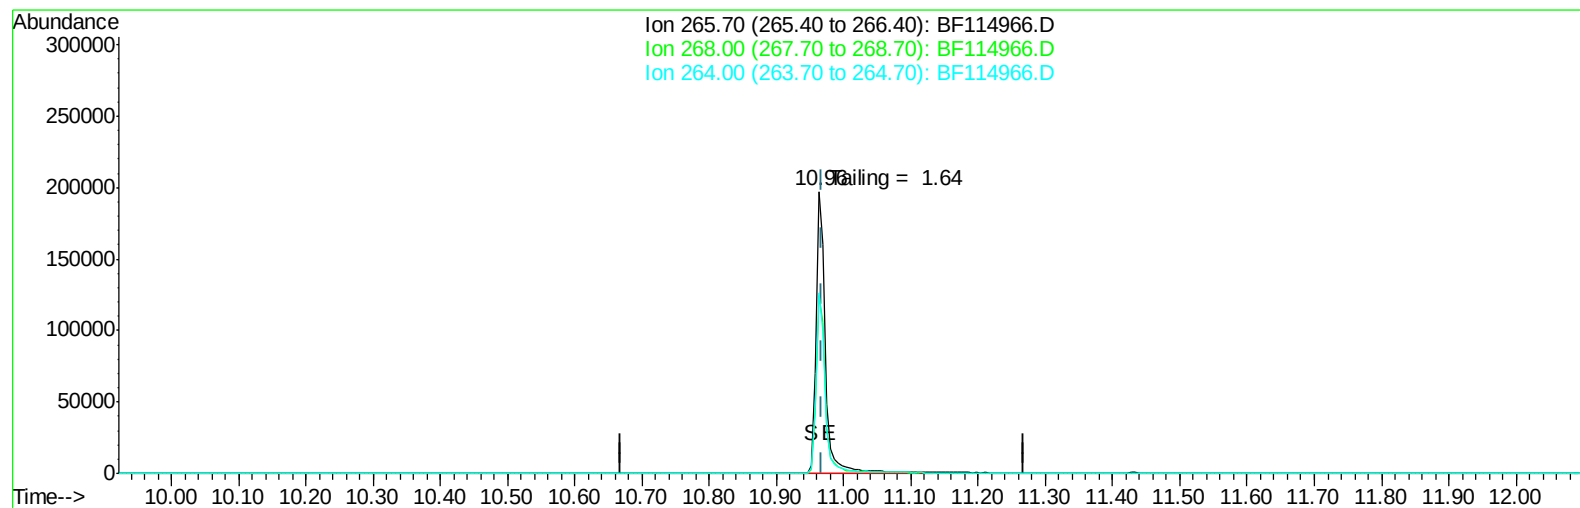

TIC: BF114966.D

(70) Pentachlorophenol (C)



10.963min (-0.006) 0.00ng

response 194082

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	63.13
264.00	62.90	63.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF061219\
Data File : BF114966.D
Acq On : 12 Jun 2019 9:56
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 03:16:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 12 15:42:37 2019
Response via : Initial Calibration

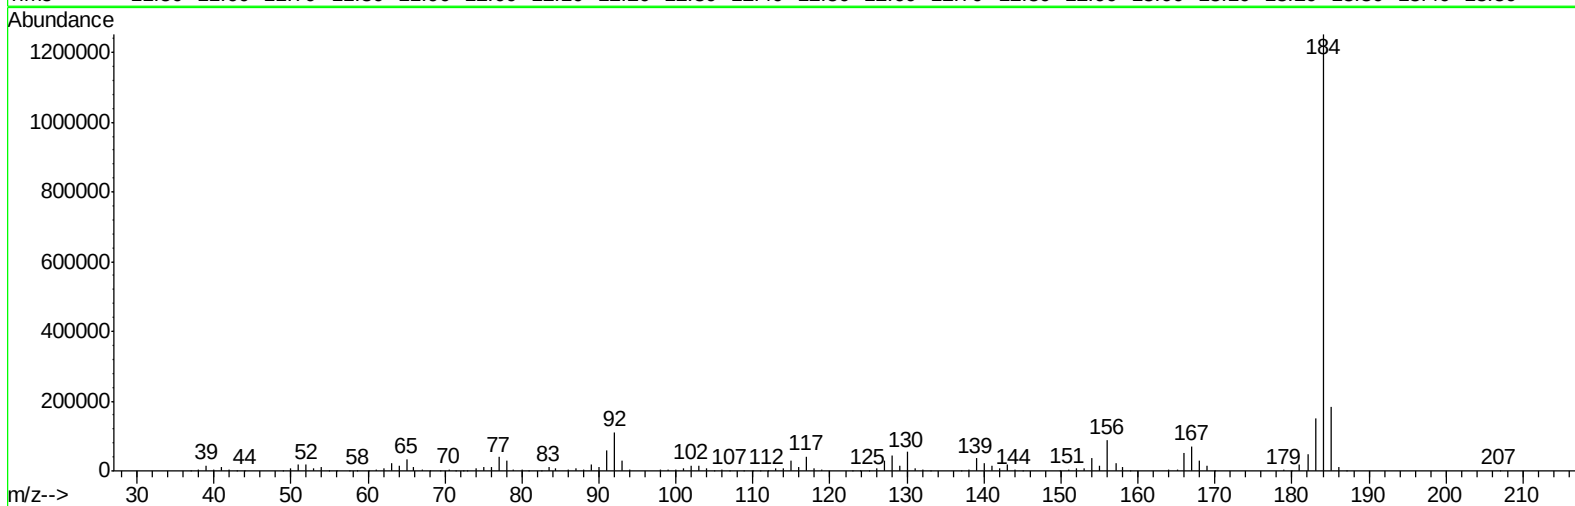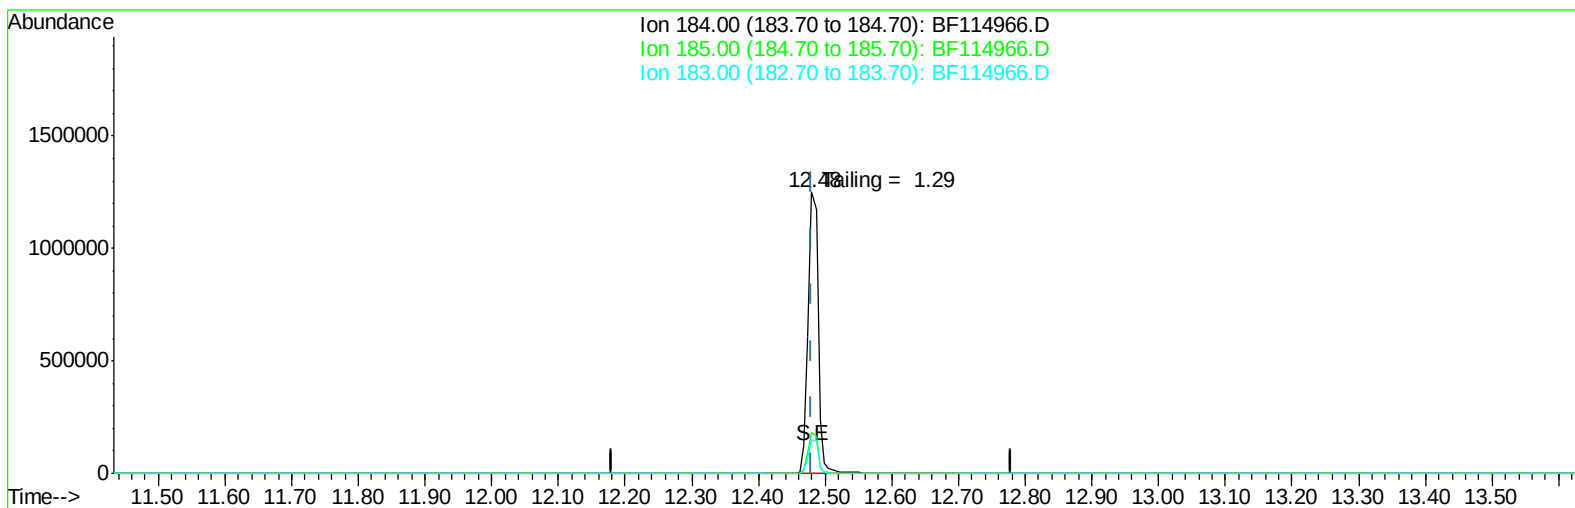

TIC: BF114966.D

(77) Benzidine

12.480min (-0.000) 31879.27ng

response 1253337

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.78
183.00	12.20	12.01
0.00	0.00	0.00