

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061219\
 Data File : BF114981.D
 Acq On : 12 Jun 2019 18:10
 Operator : HP/JU
 Sample : PB120290BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120290BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.263	535	540	543	rBV	5188199	5873086	72.53%	9.699%
2	6.292	709	715	718	rBV	4874964	6039003	74.58%	9.973%
3	6.422	731	737	740	rBV	5574026	6279813	77.55%	10.371%
4	6.645	771	775	779	rBV	1857863	1484967	18.34%	2.452%
5	6.804	797	802	805	rBV	5431472	5111791	63.13%	8.442%
6	7.210	865	871	874	rBV	3718842	3998706	49.38%	6.603%
7	7.928	988	993	996	rBV	1977829	1942657	23.99%	3.208%
8	9.004	1170	1176	1179	rBV	6851539	7726260	95.41%	12.759%
9	9.675	1284	1290	1294	rBV	2422960	2277621	28.13%	3.761%
10	10.463	1417	1424	1427	rBV	4295220	4809826	59.40%	7.943%
11	11.145	1536	1540	1544	rBV	2670189	2491138	30.76%	4.114%
12	12.733	1805	1810	1813	rBV	7219609	8097674	100.00%	13.373%
13	13.768	1982	1986	1996	rBV	2600436	2320825	28.66%	3.833%
14	15.145	2215	2220	2227	rBV	1745595	2101154	25.95%	3.470%


Sum of corrected areas: 60554521

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061219\
Data File : BF114981.D
Acq On : 12 Jun 2019 18:10
Operator : HP/JU
Sample : PB120290BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120290BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

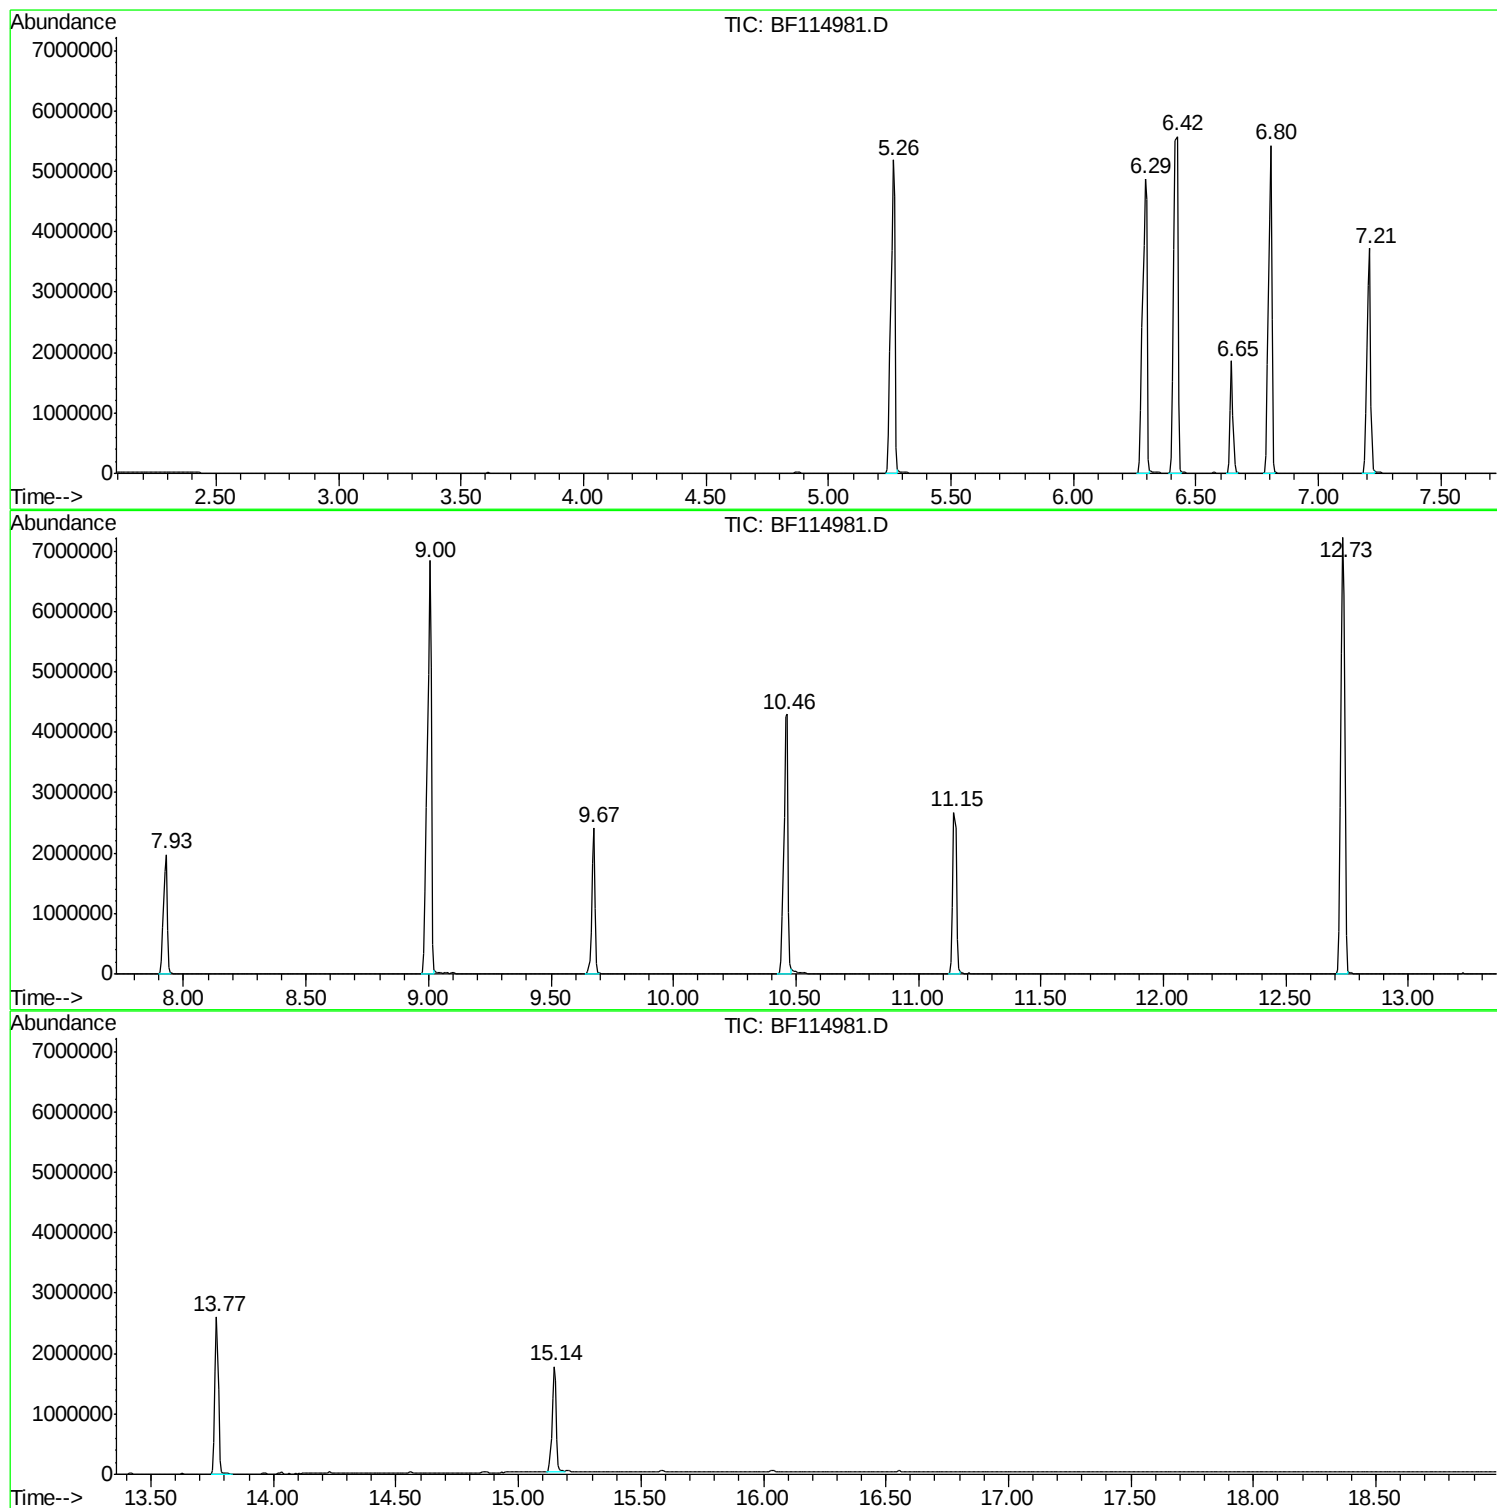

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061219\
Data File : BF114981.D
Acq On : 12 Jun 2019 18:10
Operator : HP/JU
Sample : PB120290BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120290BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.42 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.42	84.58 ng	6279810	1,4-Dichlorobenzene-d4	6.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	16
3		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

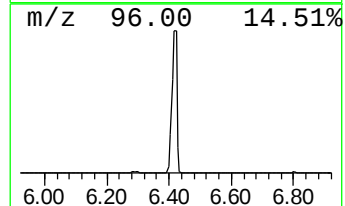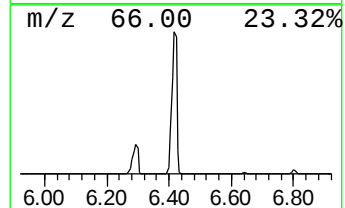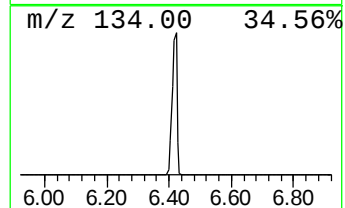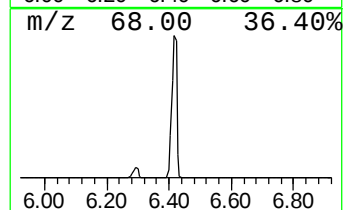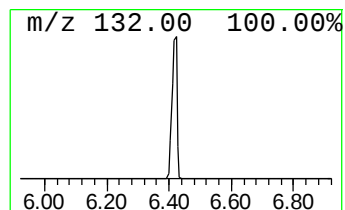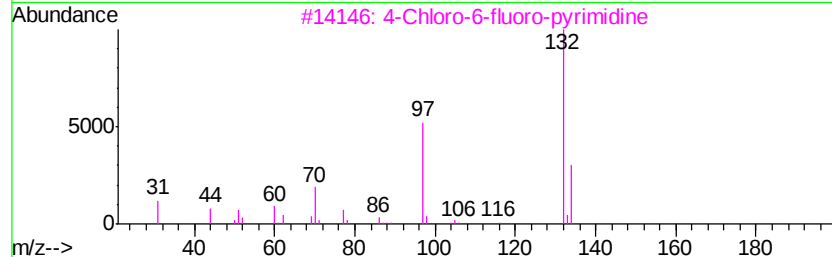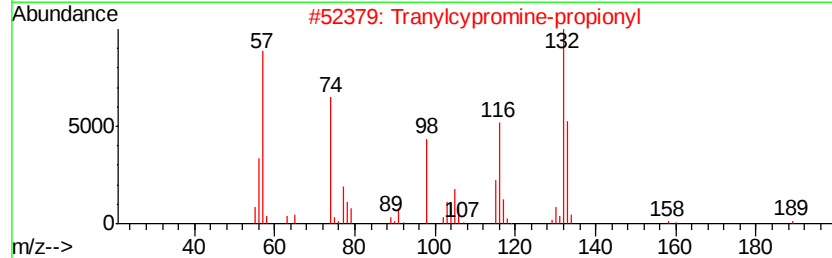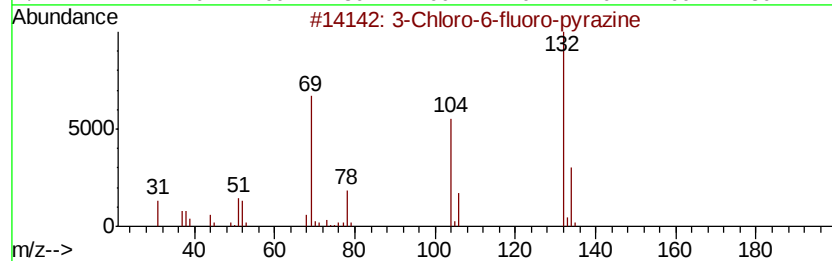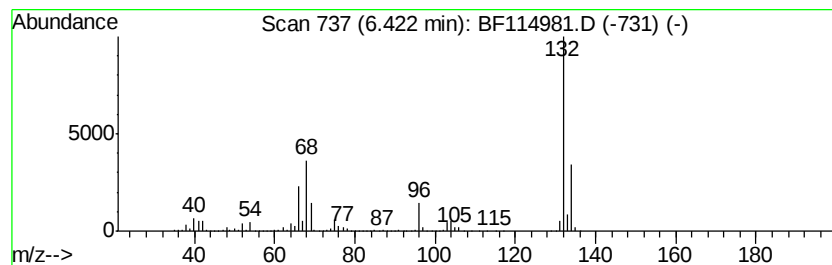

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061219\
Data File : BF114981.D
Acq On : 12 Jun 2019 18:10
Operator : HP/JU
Sample : PB120290BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120290BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.42	6.42	84.6	ng	6279810	1	6.65	1484970	20.0