


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061219\
 Data File : BF114966.D
 Acq On : 12 Jun 2019 9:56
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 12 15:42:37 2019

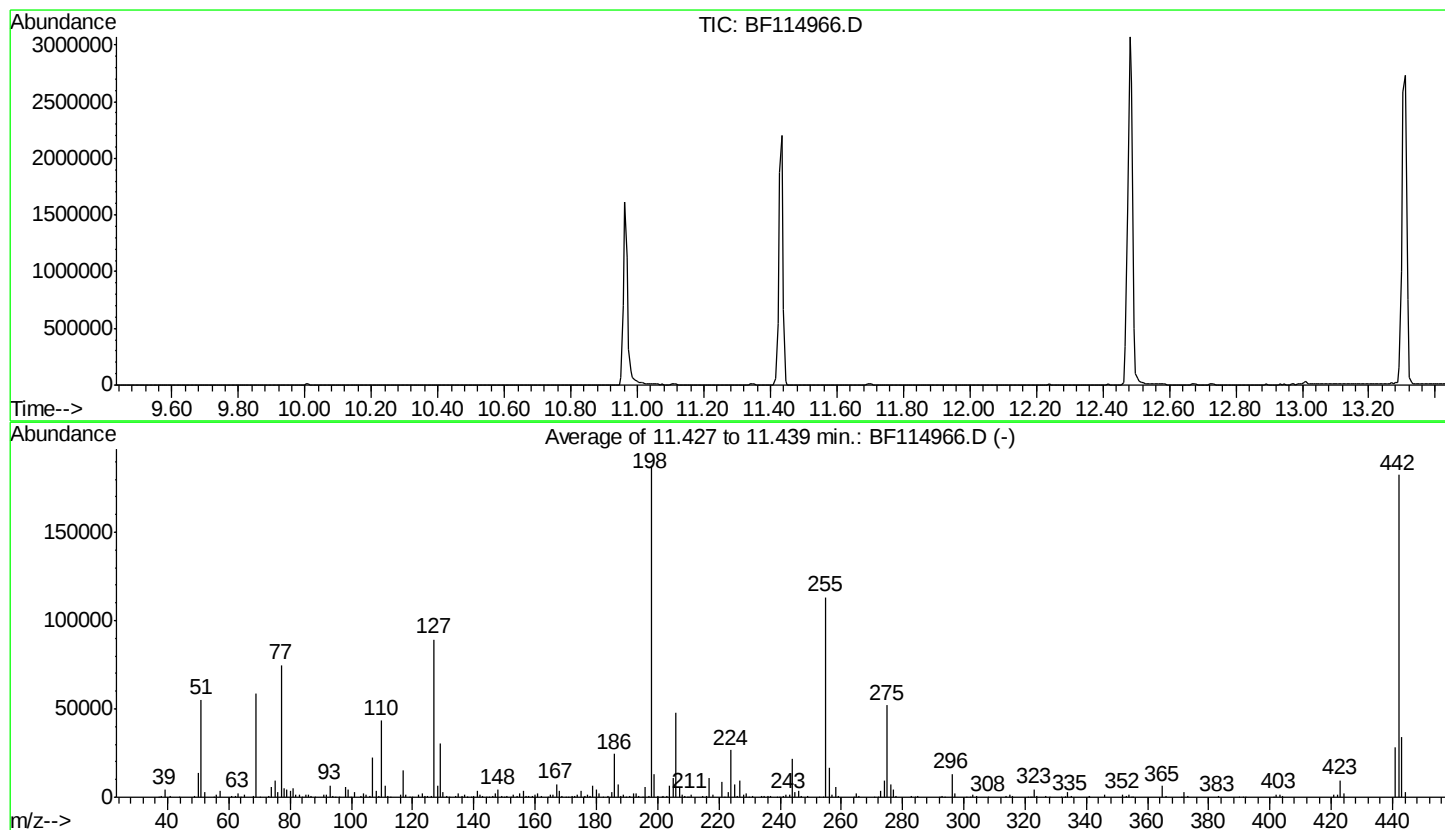

AutoFind: Scans 1588, 1589, 1590; Background Corrected with Scan 1582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	55144	PASS
68	69	0.00	2	1.5	894	PASS
69	198	0.00	100	31.3	58772	PASS
70	69	0.00	2	0.5	274	PASS
127	198	10	80	47.5	89184	PASS
197	198	0.00	2	0.6	1054	PASS
198	198	100	100	100.0	187685	PASS
199	198	5	9	6.8	12812	PASS
275	198	10	60	27.6	51885	PASS
365	198	1	100	3.3	6234	PASS
441	198	0.01	100	15.1	28330	PASS
442	198	50	100	97.1	182293	PASS
443	442	15	24	18.8	34336	PASS