


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061221\
 Data File : BF124277.D
 Acq On : 12 Jun 2021 10:03
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 10 01:53:56 2021

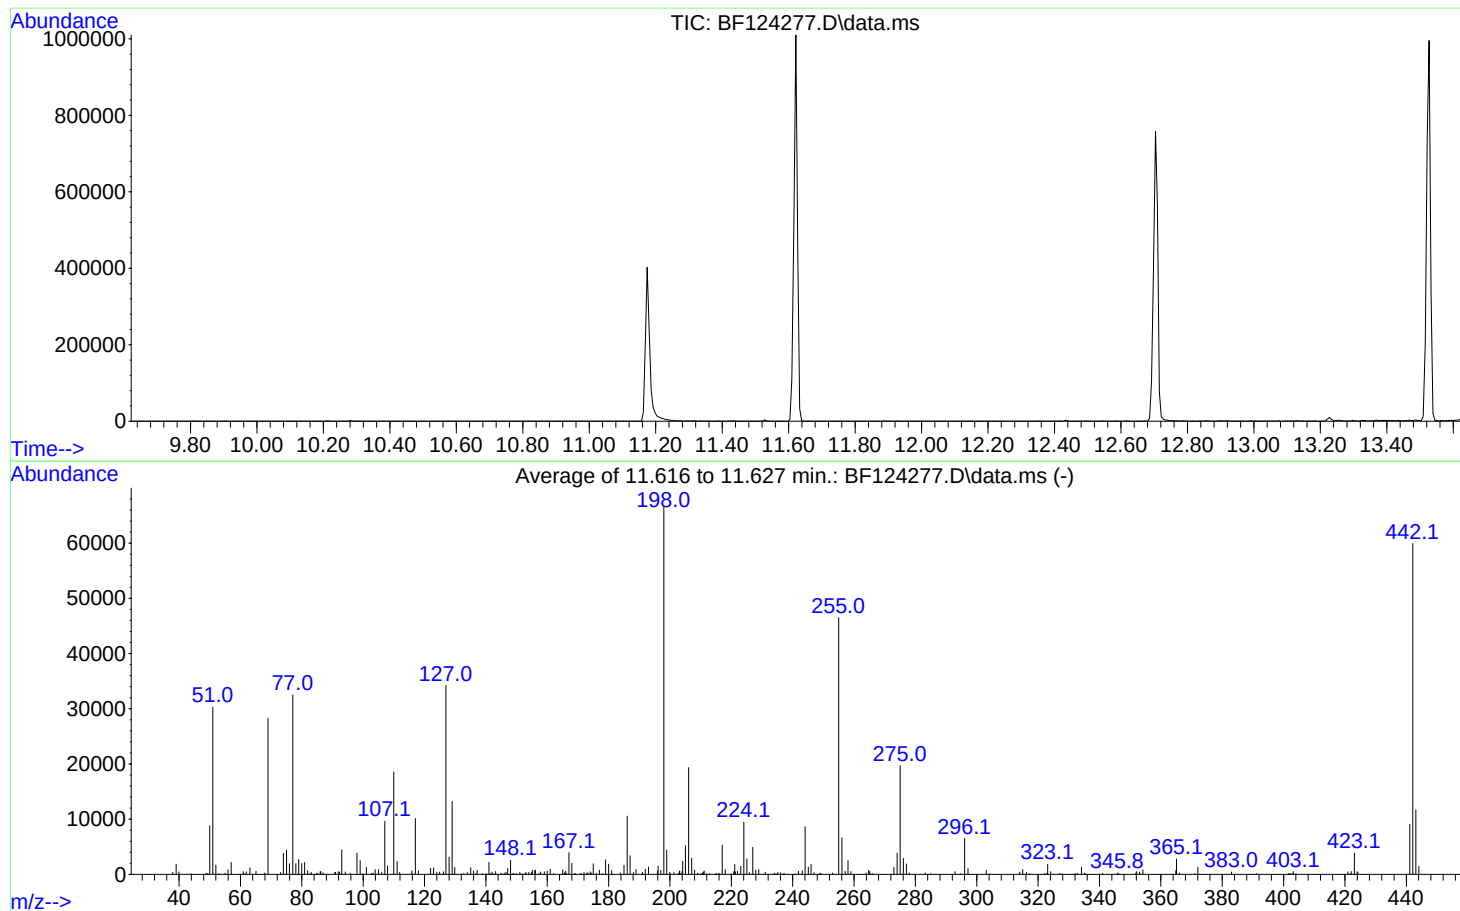




AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	30298	PASS
68	69	0.00	2	0.8	232	PASS
69	198	0.00	100	42.4	28266	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.4	34216	PASS
197	198	0.00	2	1.1	742	PASS
198	198	100	100	100.0	66629	PASS
199	198	5	9	6.6	4410	PASS
275	198	10	60	29.5	19672	PASS
365	198	1	100	4.2	2781	PASS
441	198	0.01	100	13.6	9033	PASS
442	442	50	100	100.0	59893	PASS
443	442	15	24	19.5	11680	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061221\
Data File : BF124277.D
Acq On : 12 Jun 2021 10:03
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 14 06:28:31 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 10 01:53:56 2021
Response via : Initial Calibration

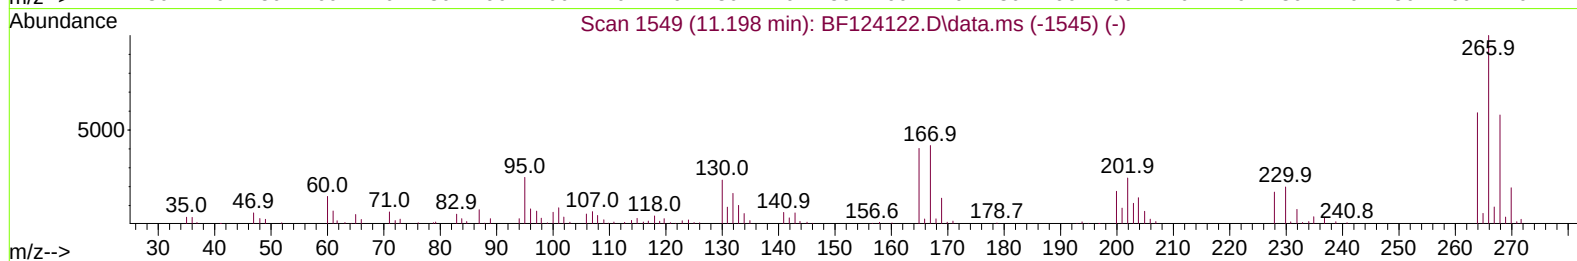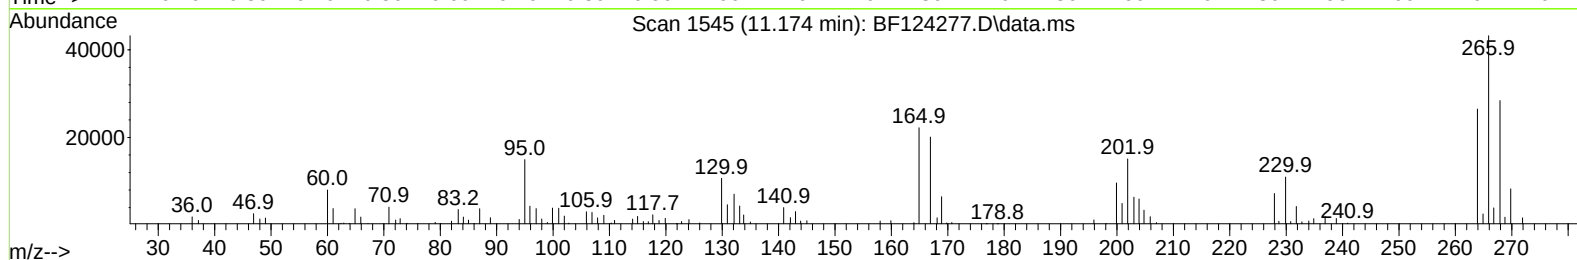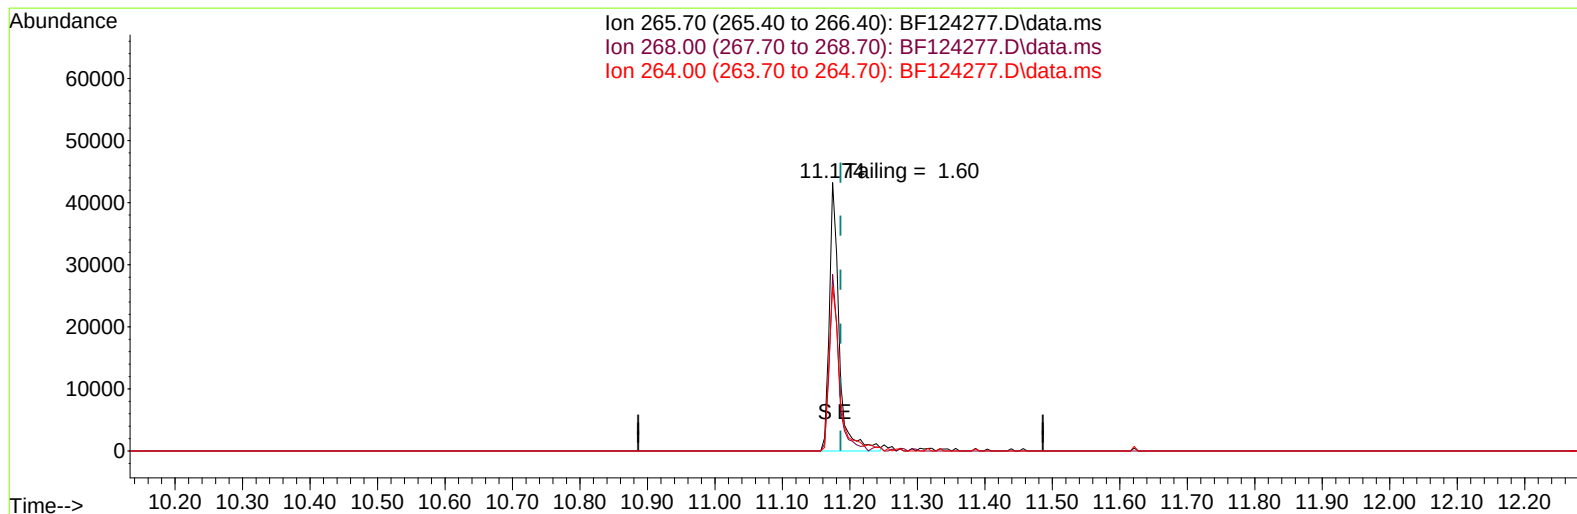

TIC: BF124277.D\data.ms

(70) Pentachlorophenol (C)

11.174min (-0.012) 14187.08 ng




response 44294

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	65.80
264.00	65.70	61.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061221\
 Data File : BF124277.D
 Acq On : 12 Jun 2021 10:03
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 14 06:28:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 10 01:53:56 2021
 Response via : Initial Calibration

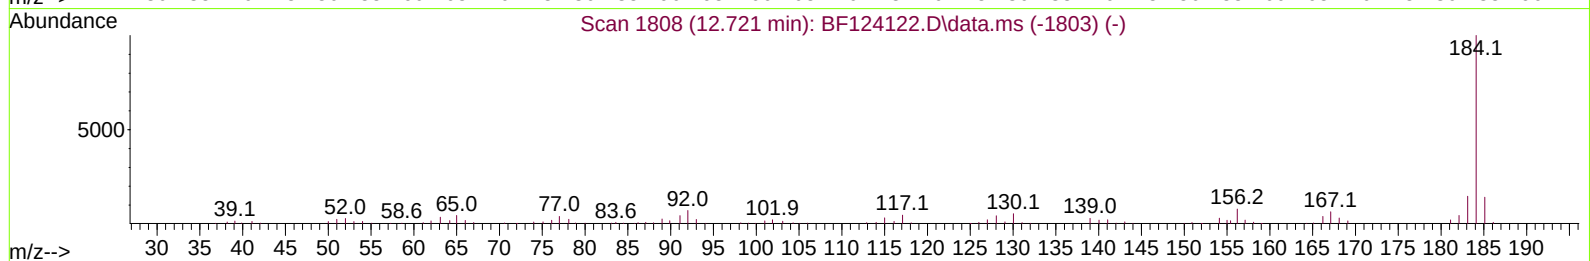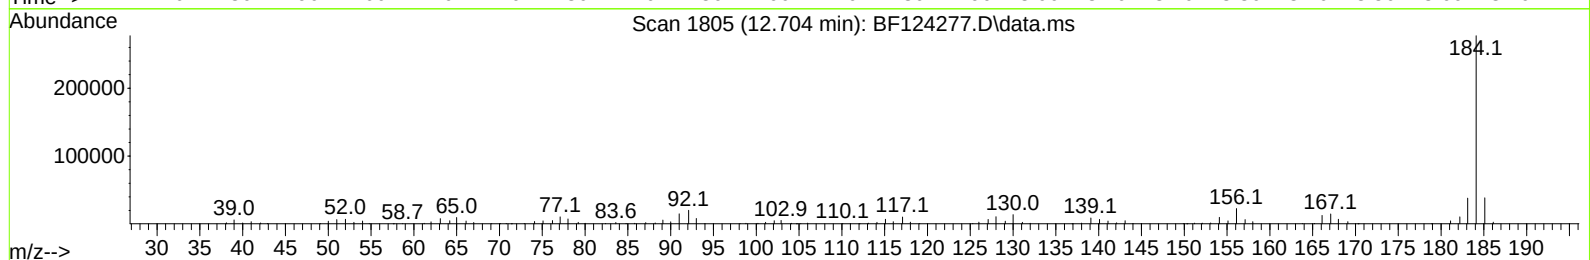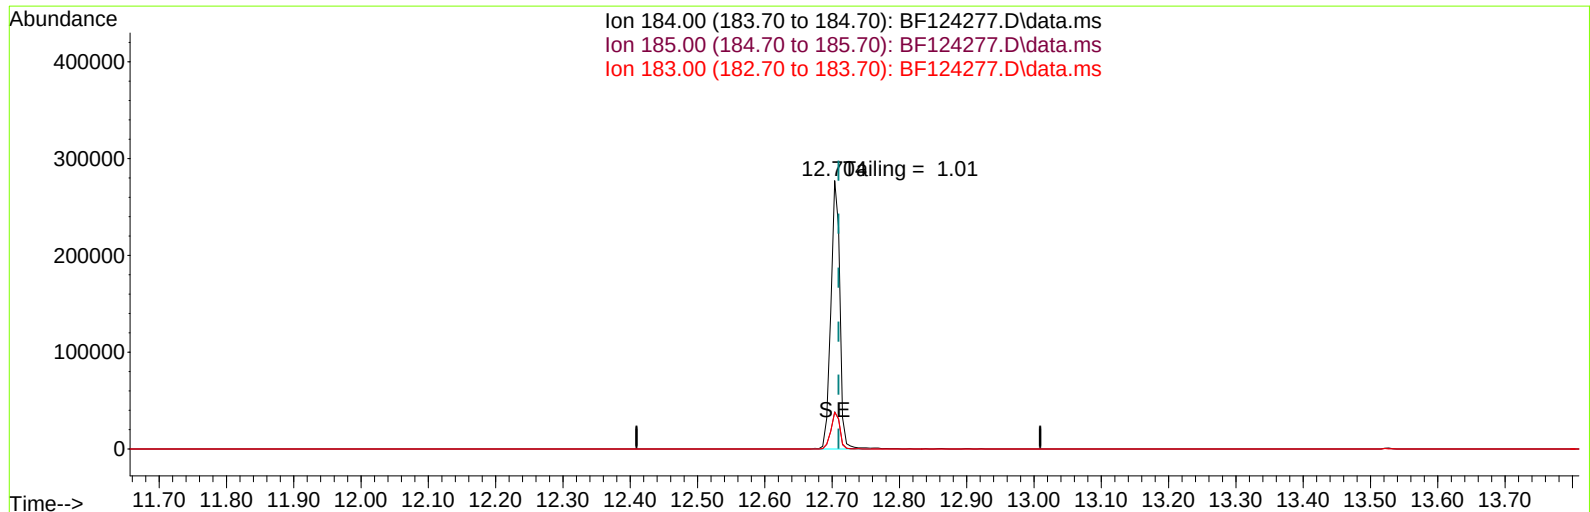

TIC: BF124277.D\data.ms

(77) Benzidine

12.704min (-0.006) 0.00 ng

response 259130

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.93
183.00	9.80	13.69#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/12/2021	BNA_F	<u>BF124277.D</u>
Compound Name	Response	Retention Time
DDT	147832	13.527
DDD	2799	13.227
DDE	389	12.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3188	151020	2.11

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP