


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061223\
Data File : BF133700.D
Acq On : 12 Jun 2023 12:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 12 16:32:43 2023

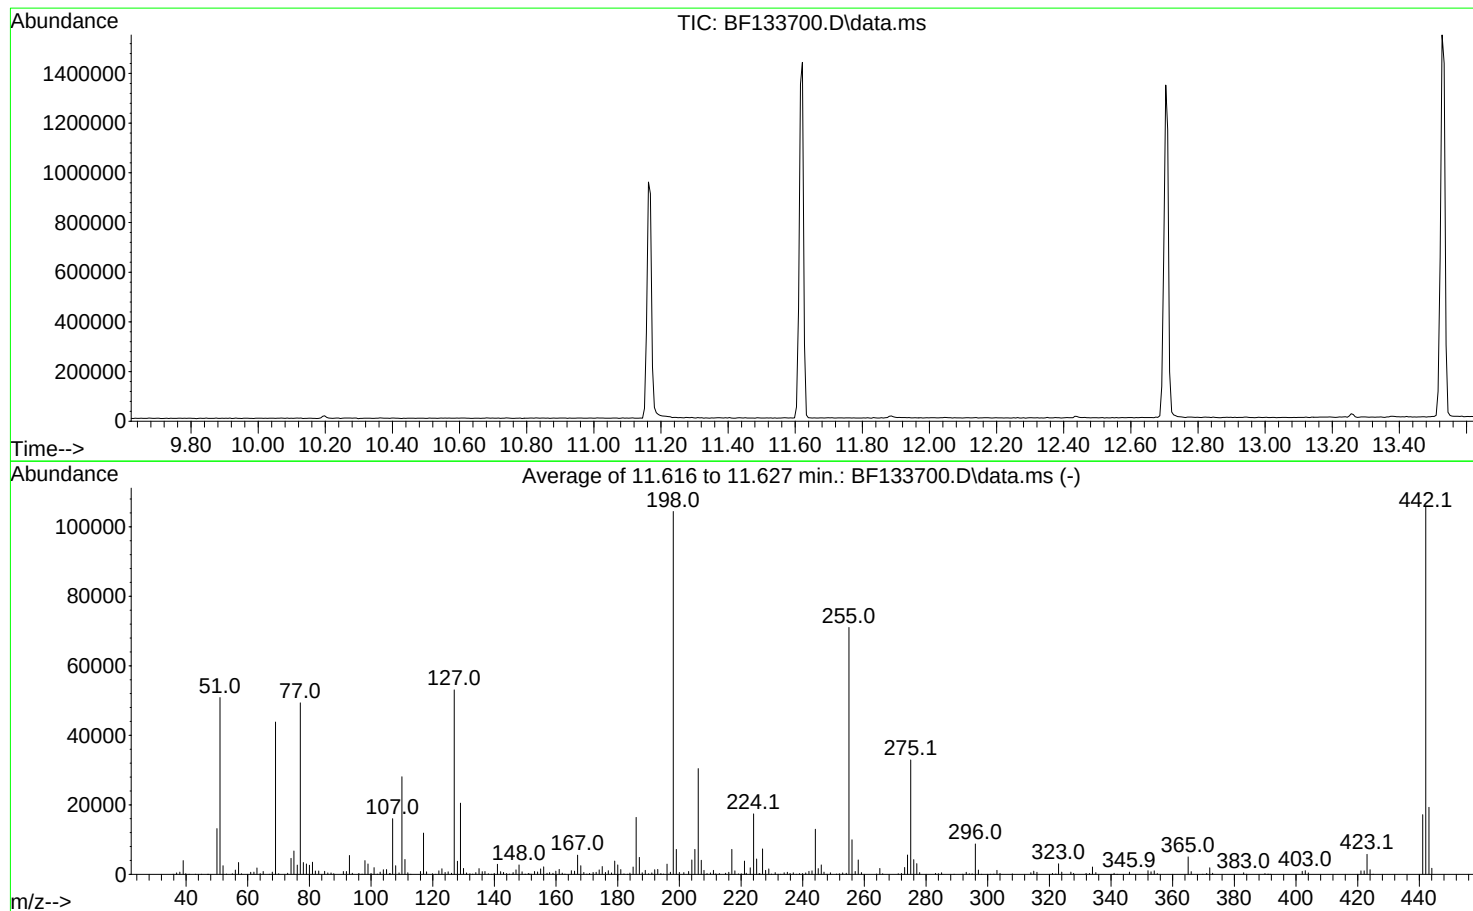

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.7	50858	PASS
68	69	0.00	2	1.5	638	PASS
69	198	0.00	100	42.0	43848	PASS
70	69	0.00	2	0.5	199	PASS
127	198	10	80	50.8	53062	PASS
197	198	0.00	2	0.6	607	PASS
198	198	100	100	100.0	104397	PASS
199	198	5	9	6.9	7191	PASS
275	198	10	60	31.5	32928	PASS
365	198	1	100	4.8	5001	PASS
441	198	0.01	100	16.5	17184	PASS
442	442	50	100	100.0	105840	PASS
443	442	15	24	18.2	19270	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/12/2023	BNA_F	<u>BF133700.D</u>
Compound Name	Response	Retention Time
DDT	256075	13.533
DDD	2617	13.257
DDE	62	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2679	258754	1.04

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061223\
Data File : BF133700.D
Acq On : 12 Jun 2023 12:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 12 14:14:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 09 15:37:41 2023
Response via : Initial Calibration

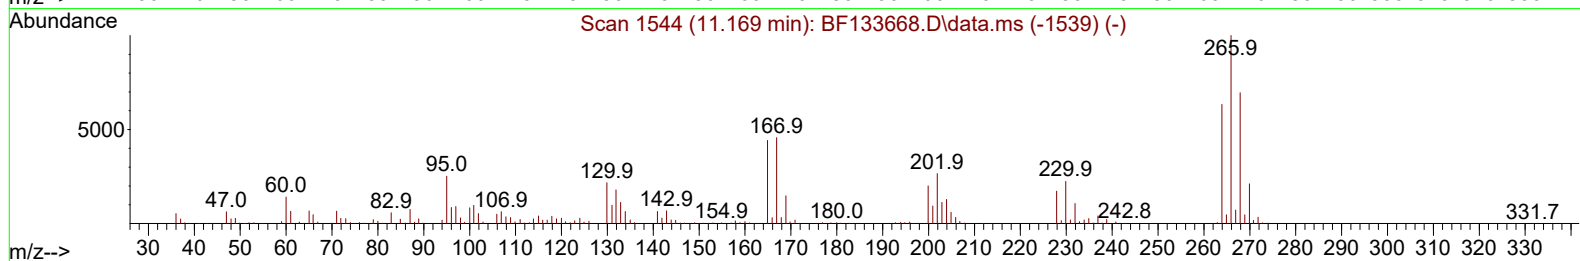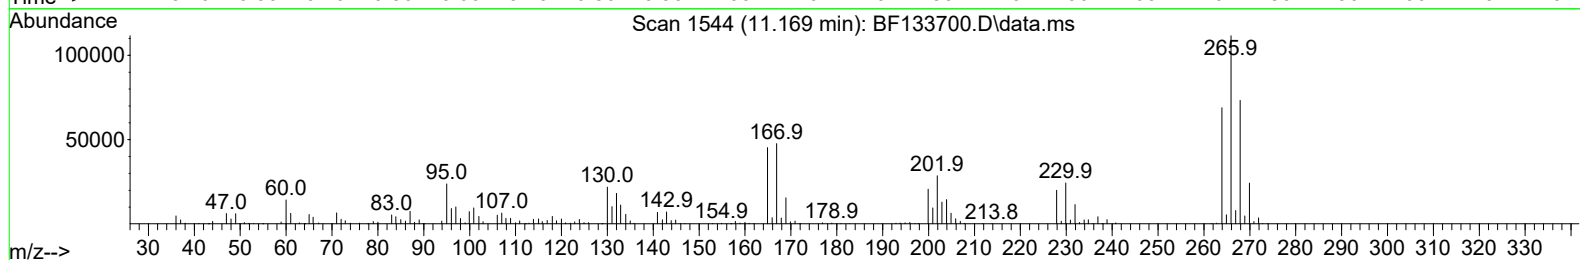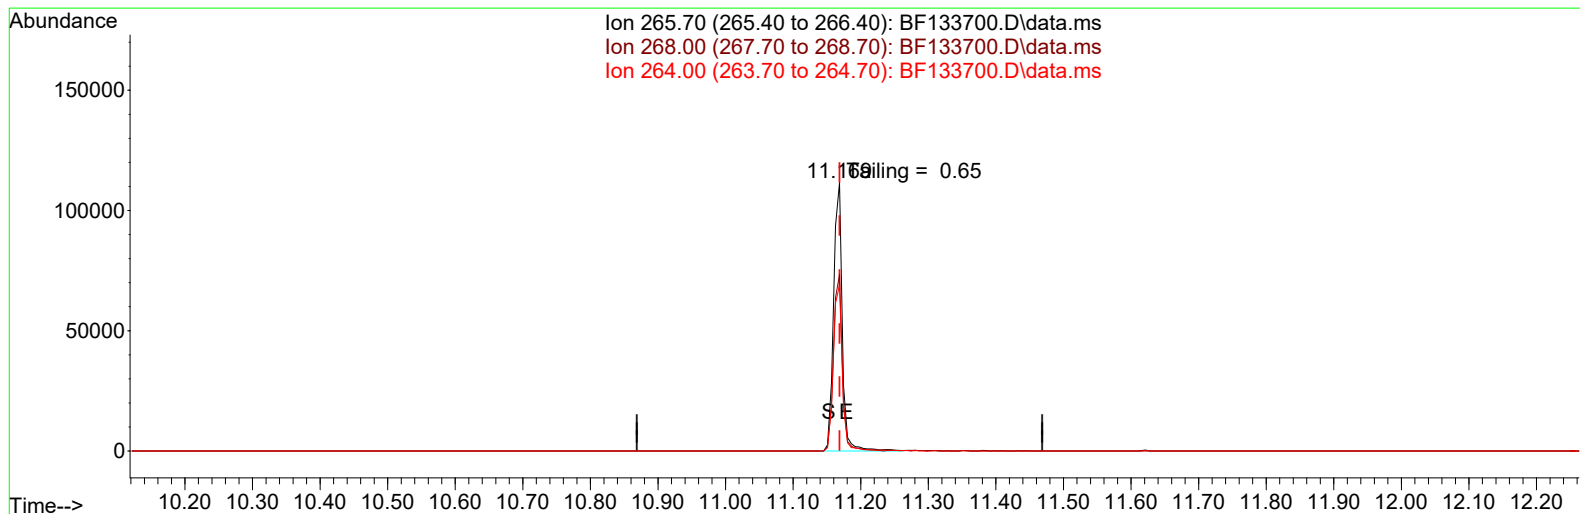

TIC: BF133700.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.000) 24169.87 ng




response 99714

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.60	65.69
264.00	63.40	61.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061223\
Data File : BF133700.D
Acq On : 12 Jun 2023 12:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 12 14:14:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 09 15:37:41 2023
Response via : Initial Calibration

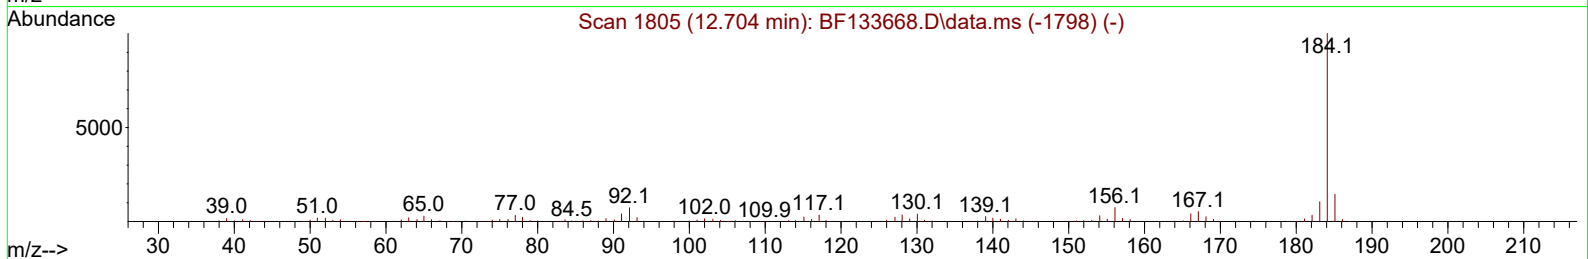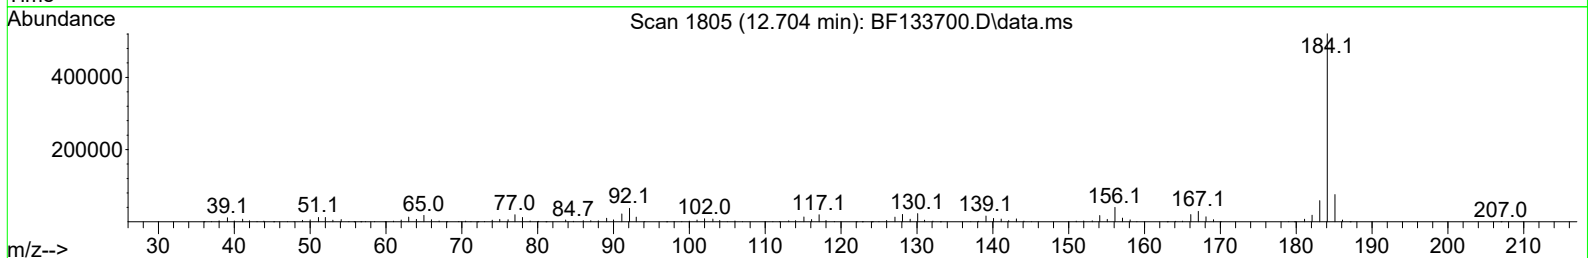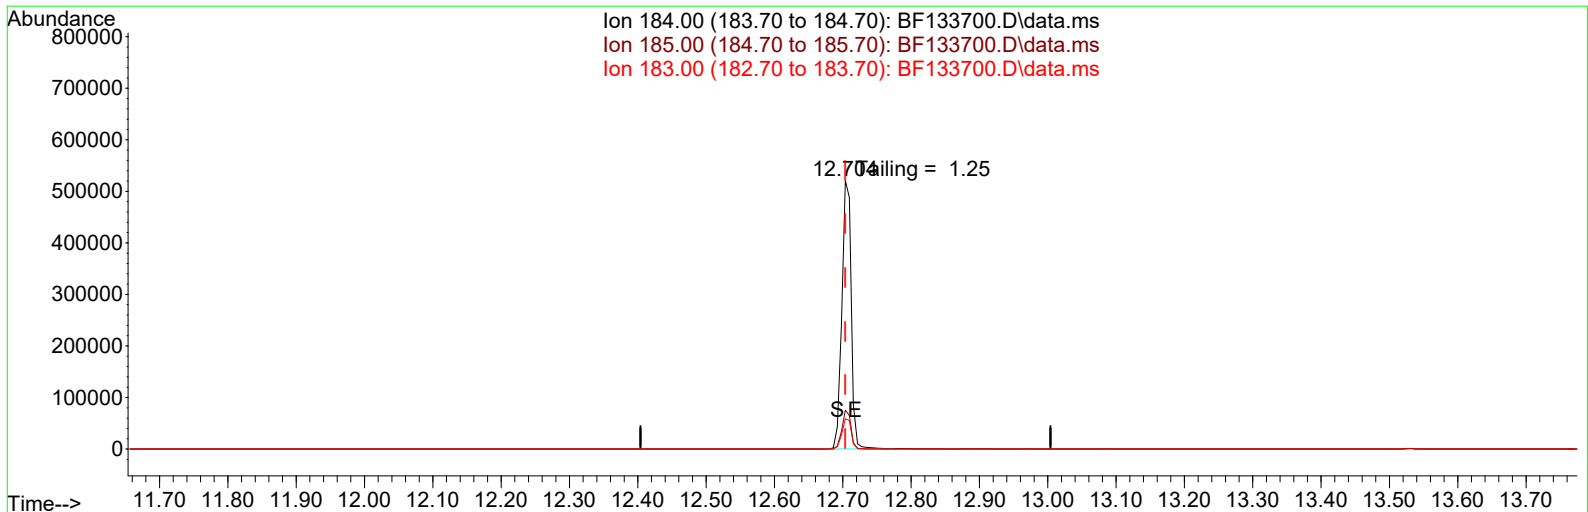

TIC: BF133700.D\data.ms

(77) Benzidine

12.704min (-0.000) 0.00 ng

response 496796

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.48
183.00	10.50	11.26
0.00	0.00	0.00