
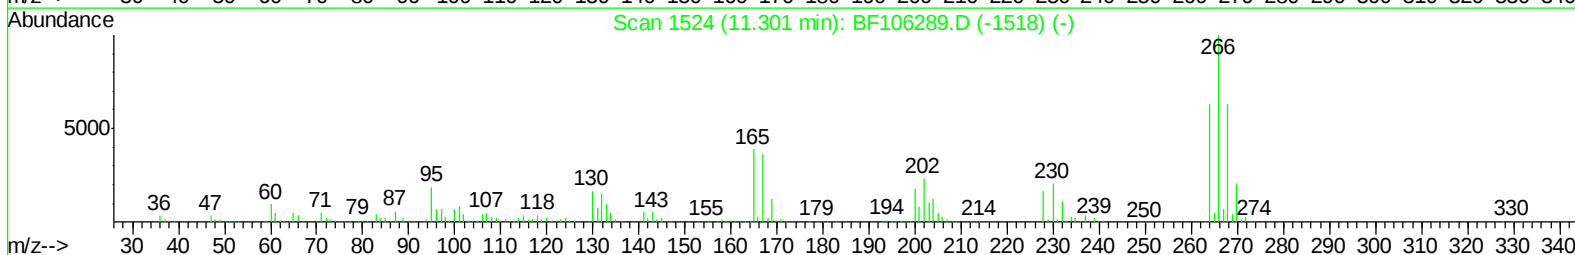
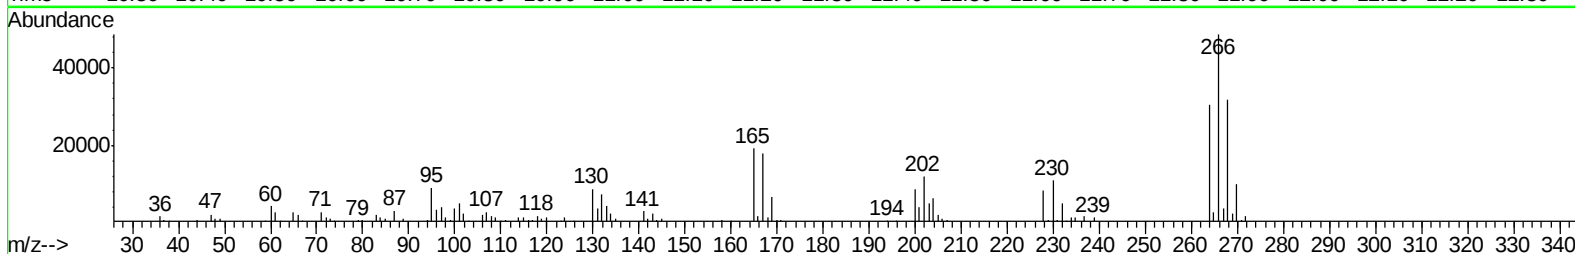


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061318\
Data File : BF106413.D
Acq On : 14 Jun 2018 1:41
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 04:08:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 13 10:51:26 2018
Response via : Initial Calibration

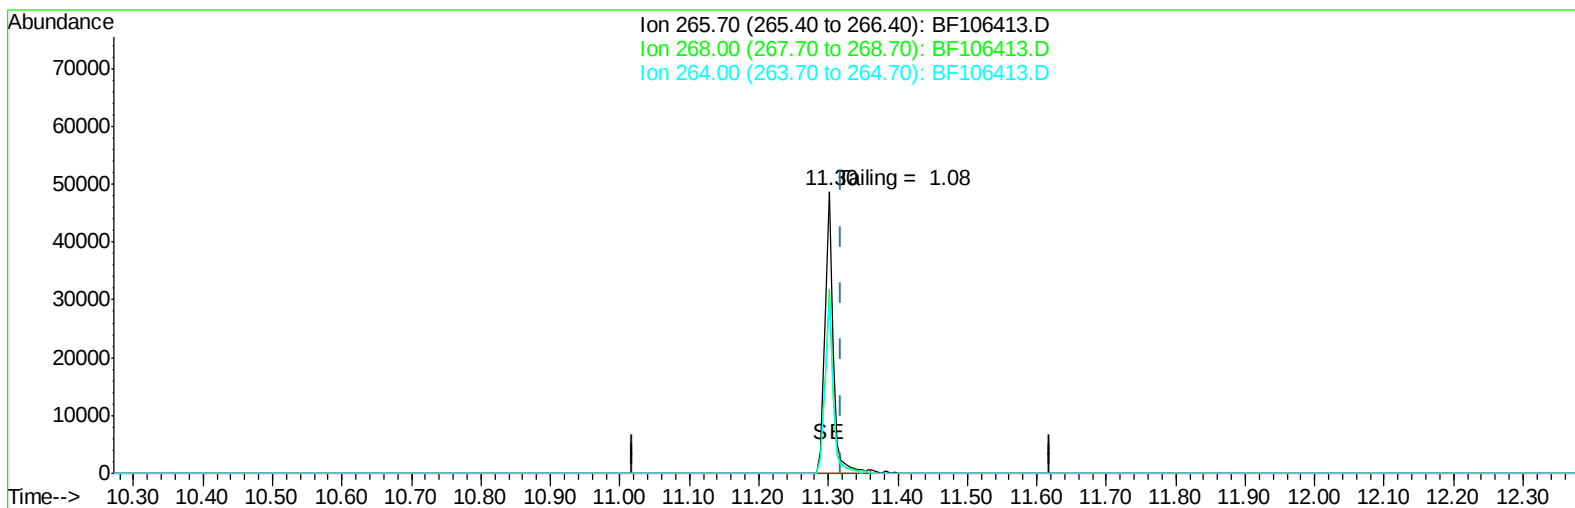

TIC: BF106413.D

(69) Pentachlorophenol (C)




11.301min (-0.018) 16905.08ng

response 41006

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.29
264.00	61.90	62.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061318\
Data File : BF106413.D
Acq On : 14 Jun 2018 1:41
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 04:08:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 13 10:51:26 2018
Response via : Initial Calibration

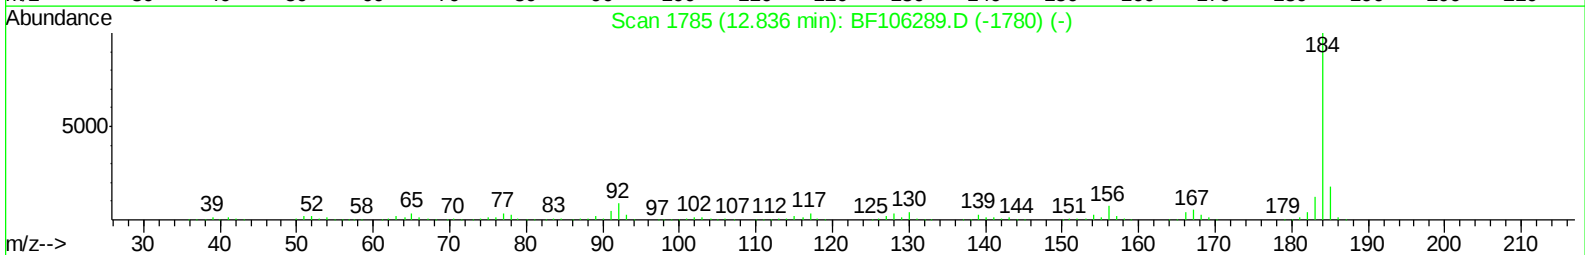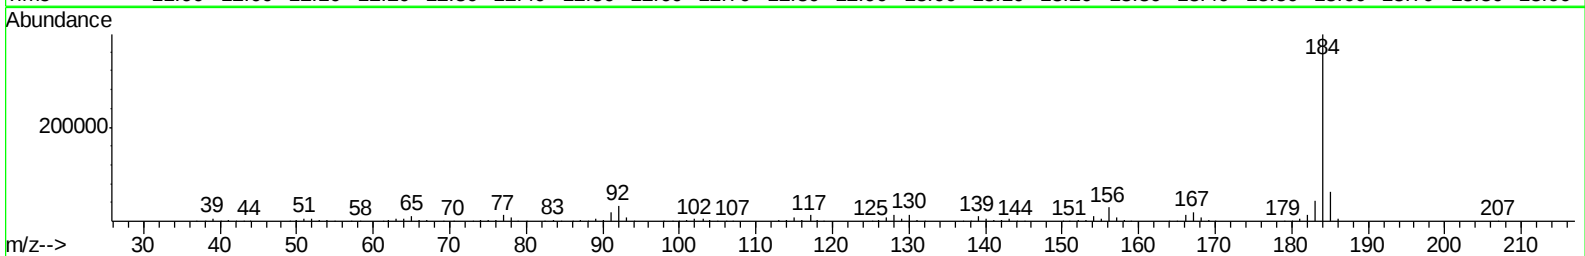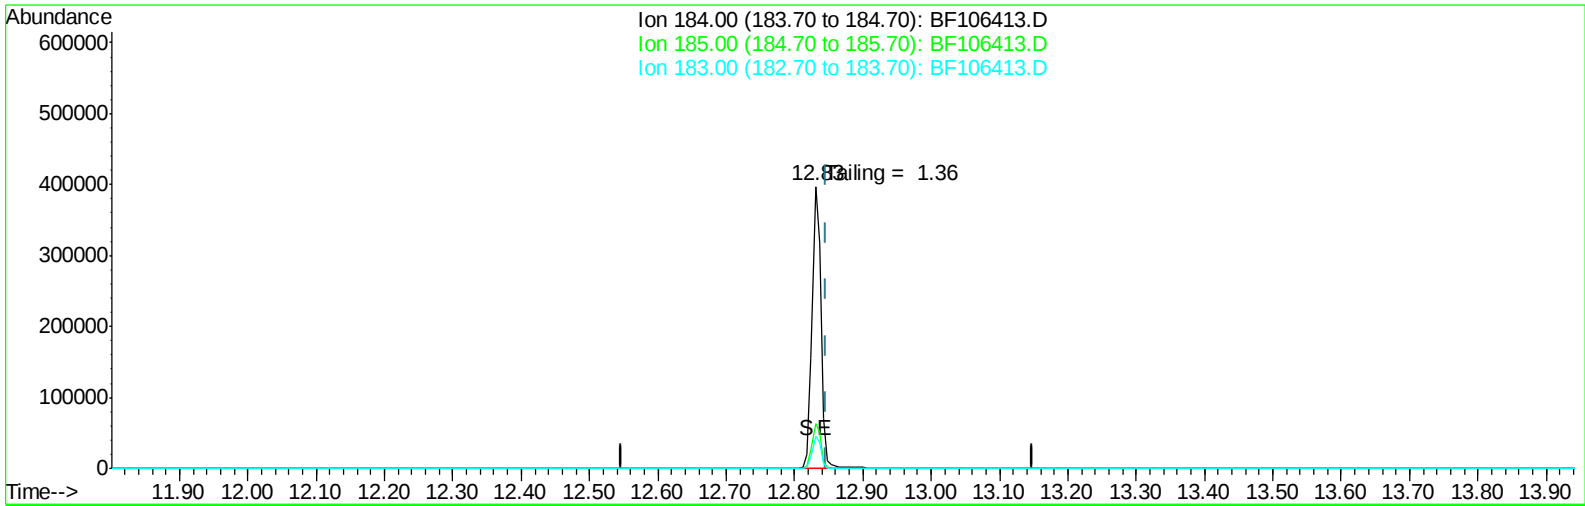

TIC: BF106413.D

(76) Benzidine

12.830min (-0.018) 0.00ng

response 351396

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.15
183.00	11.60	11.37
0.00	0.00	0.00