


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061318\
 Data File : BF106386.D
 Acq On : 13 Jun 2018 12:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 14 11:27:54 2018

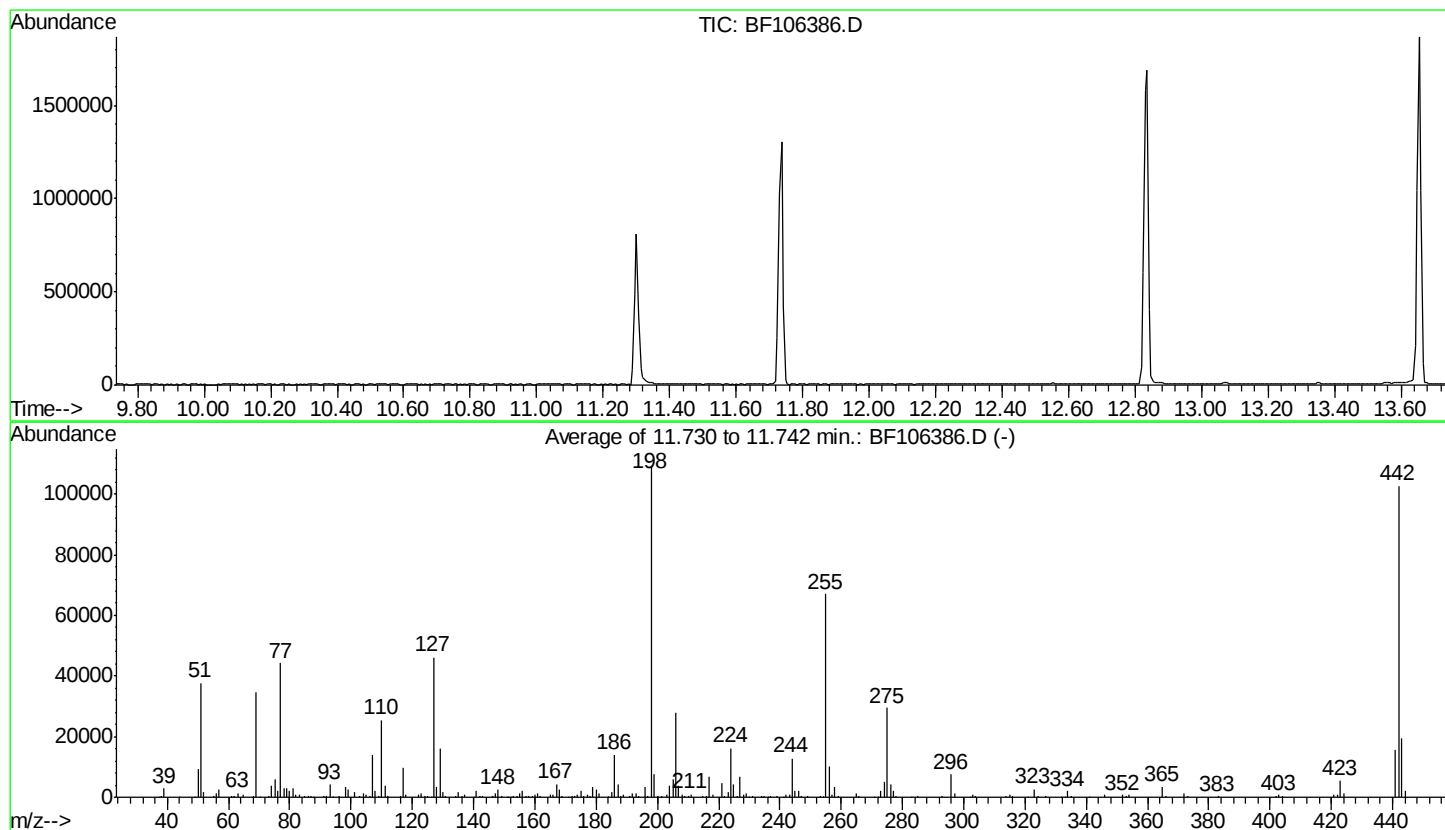

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	37687	PASS
68	69	0.00	2	1.6	540	PASS
69	198	0.00	100	31.5	34489	PASS
70	69	0.00	2	0.4	124	PASS
127	198	10	80	42.3	46252	PASS
197	198	0.00	2	0.5	509	PASS
198	198	100	100	100.0	109392	PASS
199	198	5	9	7.0	7613	PASS
275	198	10	60	27.0	29524	PASS
365	198	1	100	3.2	3534	PASS
441	443	0.01	100	79.4	15570	PASS
442	198	50	100	93.9	102696	PASS
443	442	15	24	19.1	19609	PASS