

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061319\
 Data File : BF114992.D
 Acq On : 13 Jun 2019 9:59
 Operator : HP/JU
 Sample : K3159-01 2X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-03-061119-A

Quant Time: Jun 13 17:31:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 15:42:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.65	152	302416	20.00	ng	0.00
21) Naphthalene-d8	7.93	136	1180389	20.00	ng	0.00
39) Acenaphthene-d10	9.67	164	538783	20.00	ng	0.00
64) Phenanthrene-d10	11.15	188	873495	20.00	ng	0.00
76) Chrysene-d12	13.77	240	571267	20.00	ng	-0.01
87) Perylene-d12	15.15	264	609448	20.00	ng	0.00

System Monitoring Compounds						
5) 2-Fluorophenol	5.25	112	859820	47.47	ng	0.00
7) Phenol-d6	6.29	99	1055536	48.31	ng	-0.01
23) Nitrobenzene-d5	7.20	82	621654	31.70	ng	-0.01
42) 2,4,6-Tribromophenol	10.46	330	240875	41.75	ng	-0.01
45) 2-Fluorobiphenyl	9.00	172	1125567	35.41	ng	0.00
79) Terphenyl-d14	12.73	244	806869	26.57	ng	-0.01


Target Compounds				Qvalue		
9) Benzaldehyde	6.42	77	18304	Below Cal		87
19) n-Nitroso-di-n-propylamine	7.20	70	80959	6.099 ng	#	77
25) Isophorone	7.20	82	610864	16.632 ng	#	62
31) Naphthalene	7.95	128	116859	2.092 ng		95
50) Dimethylphthalate	9.40	163	164276	4.054 ng		98
51) 2,6-Dinitrotoluene	9.67	165	71369	7.765 ng	#	37
52) Acenaphthene	9.70	154	81925	2.668 ng		97
56) 4-Nitrophenol	9.87	139	30581	3.938 ng	#	16
57) 2,4-Dinitrotoluene	9.67	165	71369	6.101 ng	#	30
58) Fluorene	10.22	166	111659	Below Cal		99
61) 4-Chlorophenyl-phenylether	10.05	204	127	Below Cal	#	27
71) Phenanthrene	11.17	178	628564	13.937 ng		97
72) Anthracene	11.22	178	175675	3.861 ng		97
75) Fluoranthene	12.35	202	634923	13.768 ng		99
78) Pyrene	12.57	202	568771	10.929 ng		98
81) Benzo(a)anthracene	13.76	228	290917	6.805 ng		98
83) Chrysene	13.79	228	259041	6.094 ng		95
86) Indeno(1,2,3-cd)pyrene	16.44	276	111188	2.978 ng		95
88) Benzo(b)fluoranthene	14.77	252	429490	10.601 ng		98
89) Benzo(k)fluoranthene	14.77	252	429490	12.078 ng	#	96
90) Benzo(a)pyrene	15.09	252	232779	6.659 ng		97
92) Benzo(g,h,i)perylene	16.83	276	98023	3.193 ng		99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061319\
Data File : BF114992.D
Acq On : 13 Jun 2019 9:59
Operator : HP/JU
Sample : K3159-01 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-03-061119-A

Quant Time: Jun 13 17:31:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 12 15:42:37 2019
Response via : Initial Calibration

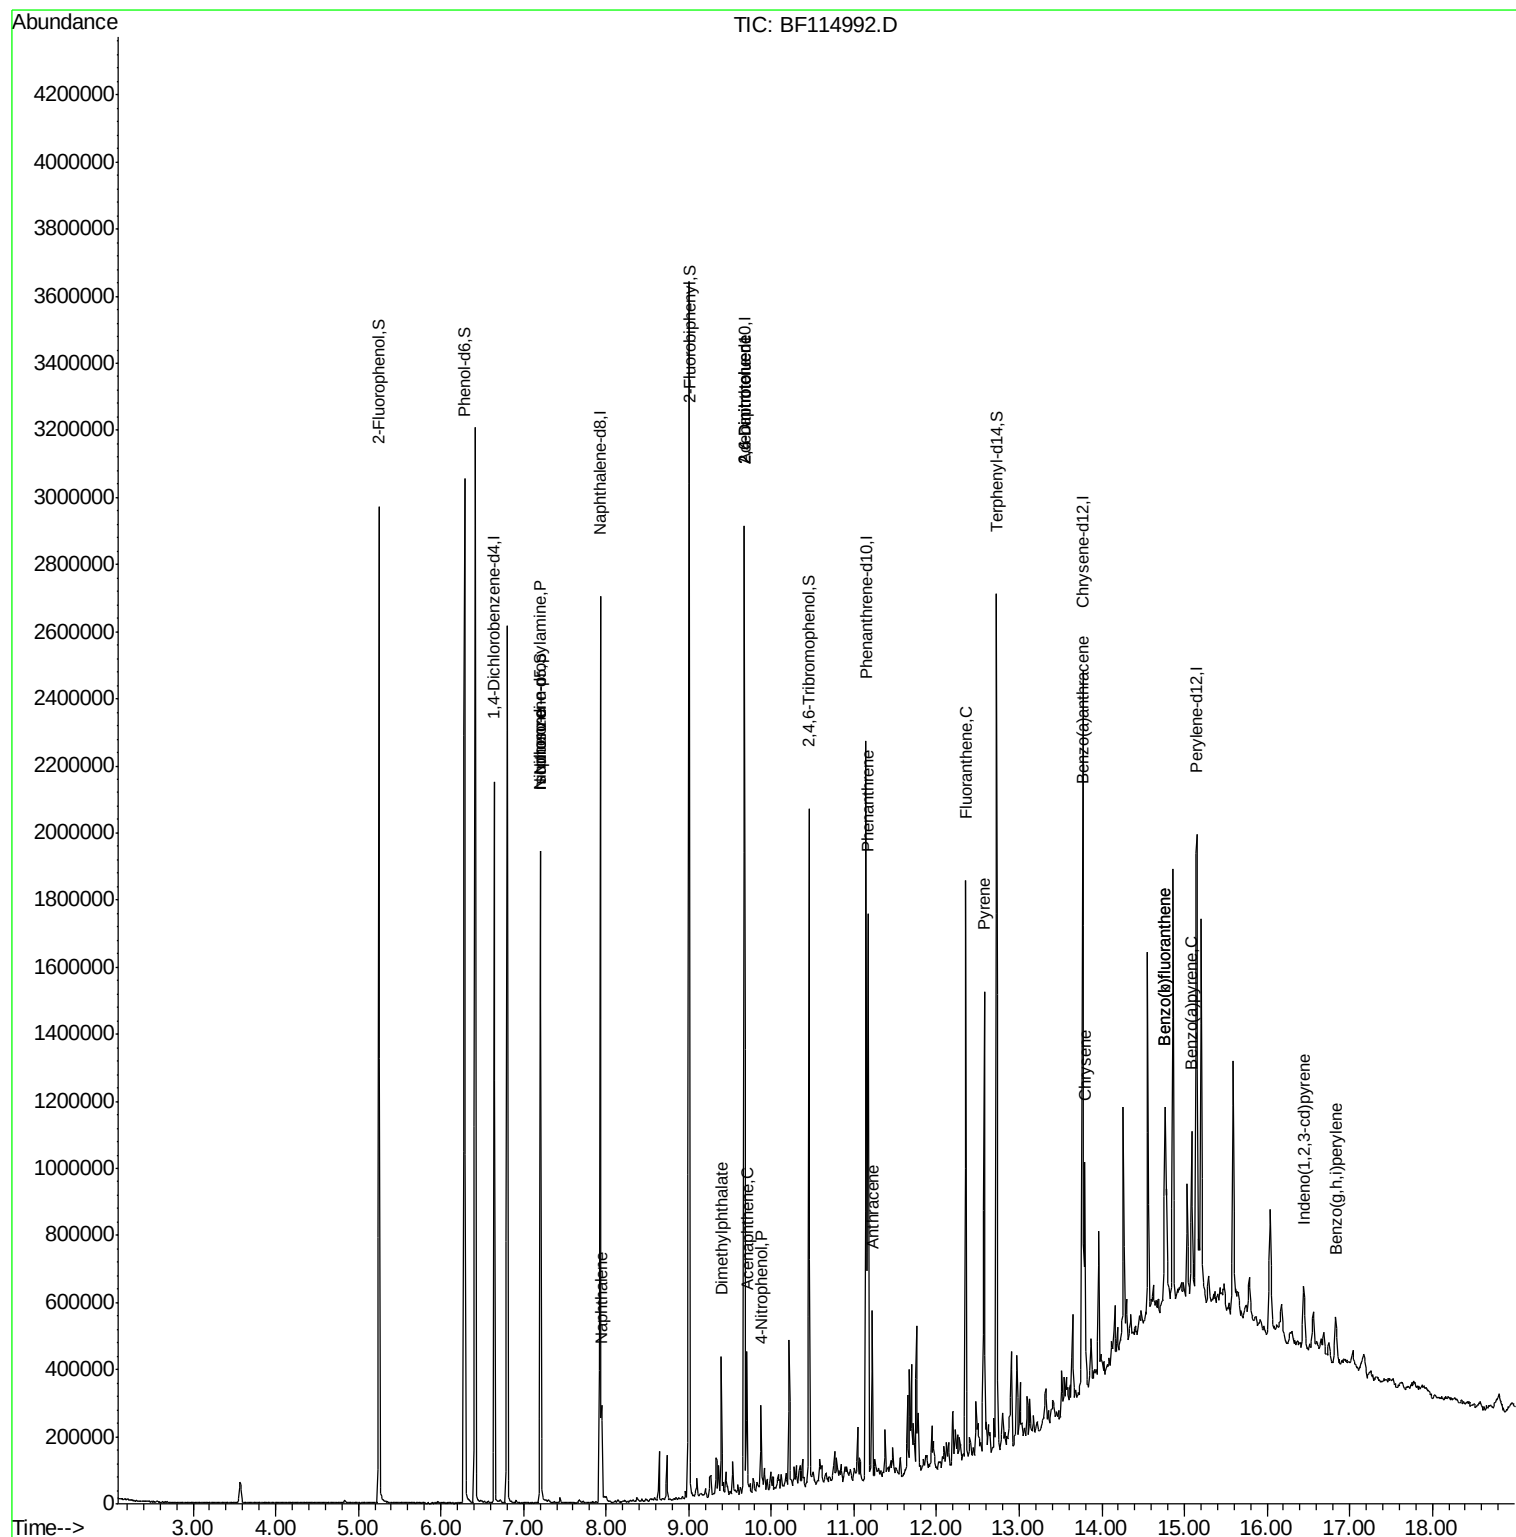




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.65 min Scan# 775
Delta R.T. -0.01 min
Lab File: BF114992.D
Acq: 13 Jun 2019 9:59

Instrument :
BNA_F
ClientSampleId :
OR-03-061119-A

Tot Ion:152 Resp: 302416
Ion Ratio Lower Upper
152 100
150 156.1 127.4 191.0
115 60.2 46.0 69.0

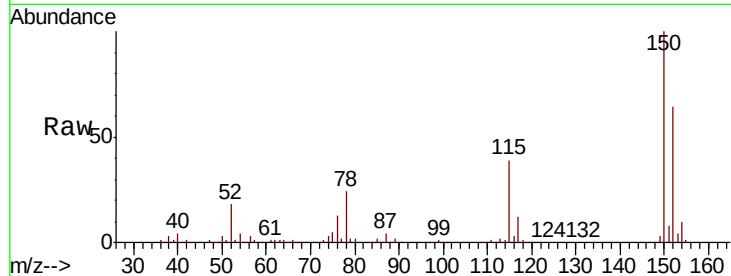


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

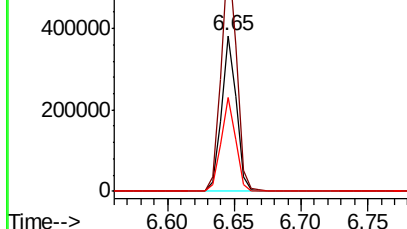



#5


2-Fluorophenol
Concen: 47.475 ng
RT: 5.25 min Scan# 538
Delta R.T. -0.01 min
Lab File: BF114992.D
Acq: 13 Jun 2019 9:59

Tgt Ion:112 Resp: 859820
Ion Ratio Lower Upper
112 100
64 52.7 41.6 62.4
63 26.5 20.9 31.3



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

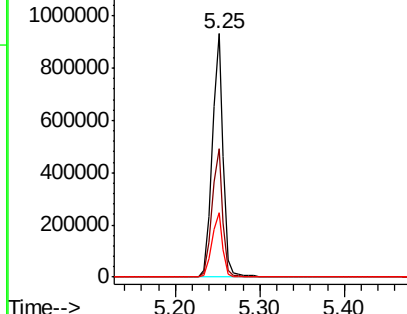



#7

Phenol-d6

Concen: 48.315 ng

RT: 6.29 min Scan# 714

Delta R.T. -0.01 min

Lab File: BF114992.D

Acq: 13 Jun 2019 9:59

Instrument :

BNA_F

ClientSampleId :

OR-03-061119-A


Tot Ion: 99 Resp: 1055536

Ion Ratio Lower Upper

99 100

42 15.8 13.4 20.2

71 32.1 26.4 39.6



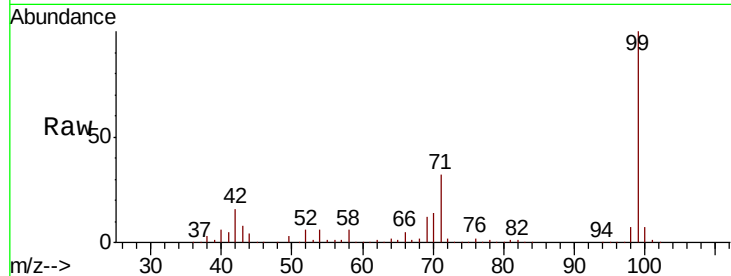


Abundance

Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

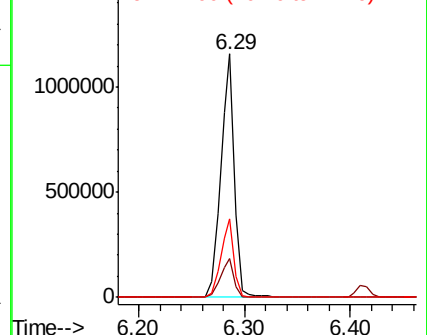

#19

n-Nitroso-di-n-propylamine

Concen: 6.099 ng

RT: 7.20 min Scan# 870

Delta R.T. 0.12 min

Lab File: BF114992.D

Acq: 13 Jun 2019 9:59

Tgt Ion: 70 Resp: 80959


Ion Ratio Lower Upper

70 100

42 42.7 40.3 60.5

101 0.0 8.2 12.4#

130 2.7 20.3 30.5#





Abundance


Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

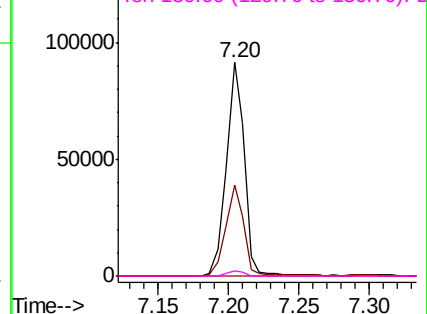




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.93 min Scan# 993
Delta R.T. -0.01 min
Lab File: BF114992.D
Acq: 13 Jun 2019 9:59




Instrument :
BNA_F
ClientSampleId :
OR-03-061119-A

Tot Ion:136 Resp: 1180389

Ion	Ratio	Lower	Upper
136	100		
137	11.3	9.0	13.4
54	6.8	5.4	8.0
68	5.8	4.6	7.0

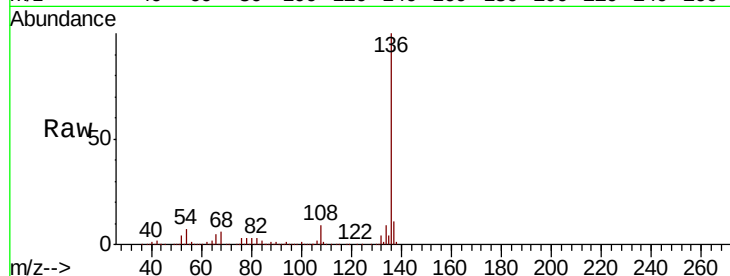


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

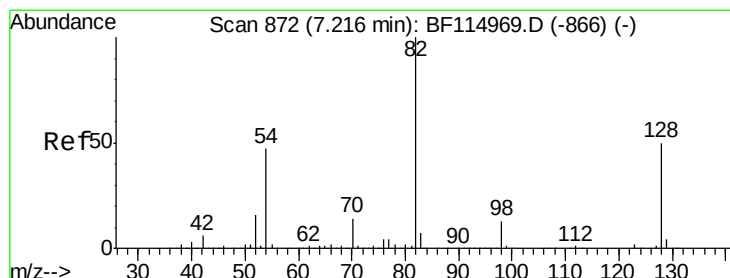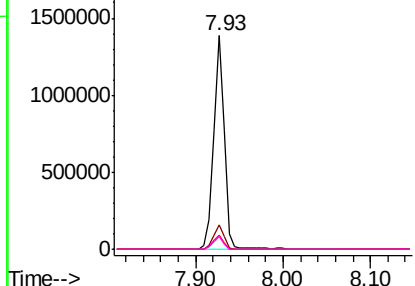



#23
Nitrobenzene-d5
Concen: 31.700 ng
RT: 7.20 min Scan# 870
Delta R.T. -0.01 min
Lab File: BF114992.D
Acq: 13 Jun 2019 9:59


Tgt Ion: 82 Resp: 621654

Ion	Ratio	Lower	Upper
82	100		
128	48.4	39.9	59.9
54	46.2	37.3	55.9

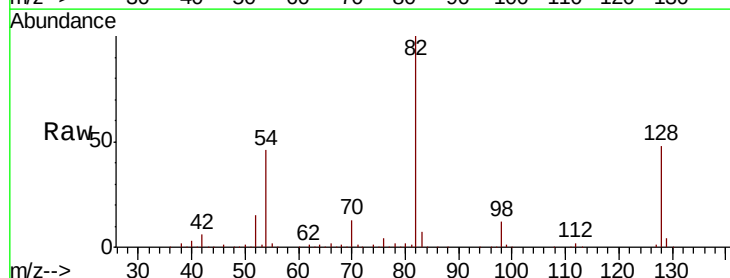

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

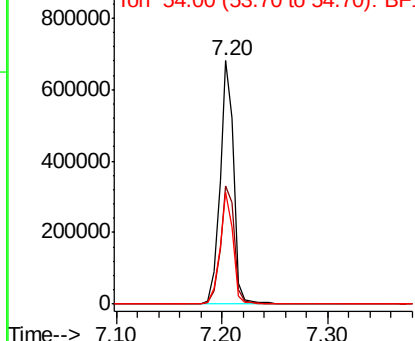



#25

Isophorone

Concen: 16.632 ng

RT: 7.20 min Scan# 870

Delta R.T. -0.28 min

Lab File: BF114992.D

Acq: 13 Jun 2019 9:59

Instrument :

BNA_F

ClientSampleId :

OR-03-061119-A


Tot Ion: 82 Resp: 610864

Ion Ratio Lower Upper

82 100

95 0.0 5.6 8.4#




138 0.0 16.1 24.1#

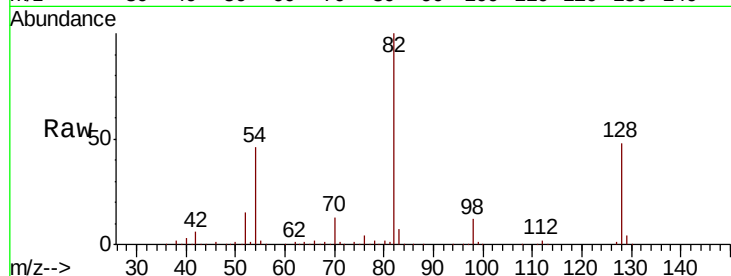

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

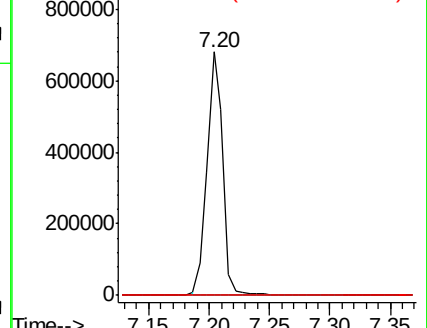

#31

Naphthalene

Concen: 2.092 ng

RT: 7.95 min Scan# 996

Delta R.T. -0.01 min

Lab File: BF114992.D

Acq: 13 Jun 2019 9:59


Tgt Ion: 128 Resp: 116859

Ion Ratio Lower Upper

128 100

129 10.4 9.5 14.3



127 12.2 11.5 17.3




Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E




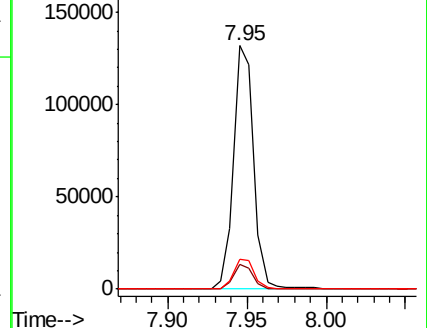




#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.67 min Scan# 1290
 Delta R.T. -0.01 min
 Lab File: BF114992.D
 Acq: 13 Jun 2019 9:59




Instrument :
 BNA_F
 ClientSampleId :
 OR-03-061119-A


Tot Ion:164 Resp: 538783
 Ion Ratio Lower Upper
 164 100
 162 103.7 82.6 124.0
 160 46.4 36.9 55.3

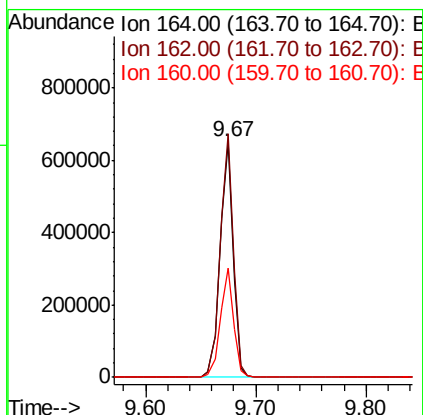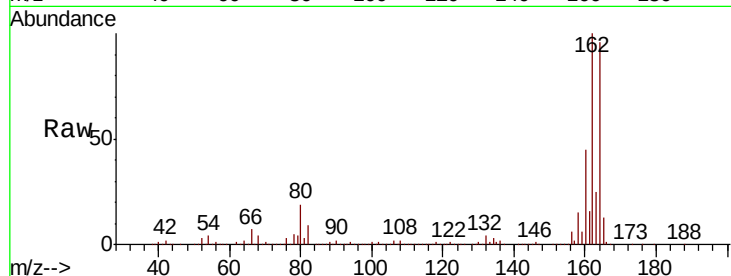

#42
 2,4,6-Tribromophenol
 Concen: 41.749 ng
 RT: 10.46 min Scan# 1423
 Delta R.T. -0.01 min
 Lab File: BF114992.D
 Acq: 13 Jun 2019 9:59

Tgt Ion:330 Resp: 240875
 Ion Ratio Lower Upper
 330 100
 332 95.7 77.6 116.4
 141 34.2 27.2 40.8



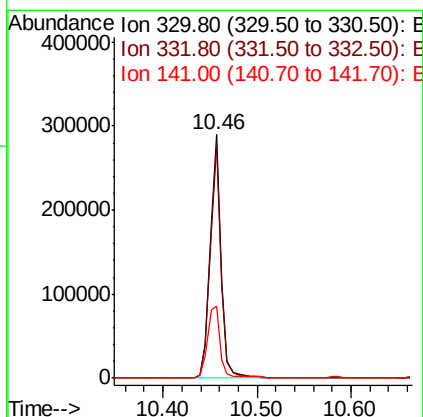





#45
2-Fluorobiphenyl
Concen: 35.407 ng
RT: 9.00 min Scan# 1176
Delta R.T. -0.01 min
Lab File: BF114992.D
Acq: 13 Jun 2019 9:59




Instrument :
BNA_F
ClientSampleId :
OR-03-061119-A


Tot Ion:172 Resp: 1125567
Ion Ratio Lower Upper
172 100
171 36.1 29.8 44.6
170 24.0 20.6 31.0

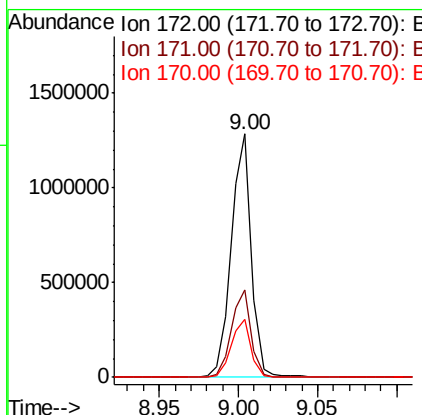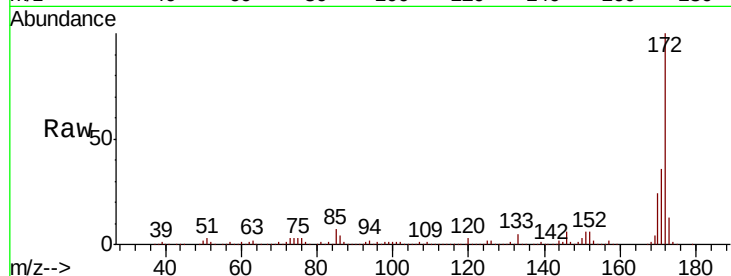

#50
Dimethylphthalate
Concen: 4.054 ng
RT: 9.40 min Scan# 1243
Delta R.T. -0.02 min
Lab File: BF114992.D
Acq: 13 Jun 2019 9:59

Tgt Ion:163 Resp: 164276
Ion Ratio Lower Upper
163 100
194 4.1 3.3 4.9
164 9.6 8.6 12.8

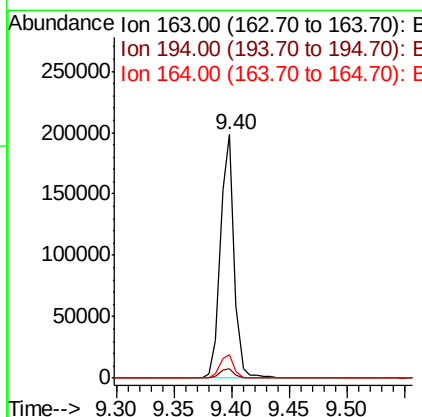



#51

2,6-Dinitrotoluene

Concen: 7.765 ng

RT: 9.67 min Scan# 1290

Delta R.T. 0.20 min

Lab File: BF114992.D

Acq: 13 Jun 2019 9:59

Instrument :

BNA_F

ClientSampleId :

OR-03-061119-A


Tot Ion:165 Resp: 71369

Ion Ratio Lower Upper

165 100

63 1.2 30.6 46.0#




89 1.6 34.4 51.6#

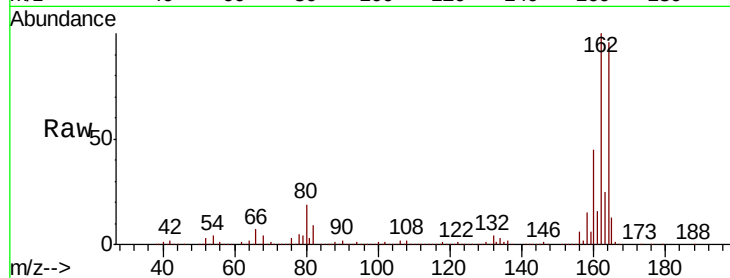

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

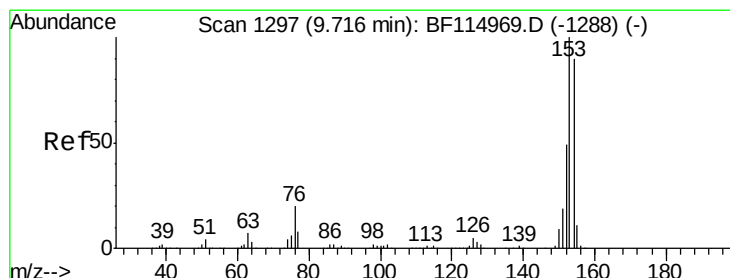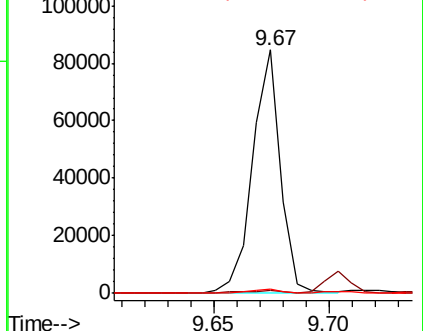

#52

Acenaphthene

Concen: 2.668 ng

RT: 9.70 min Scan# 1295

Delta R.T. -0.01 min

Lab File: BF114992.D

Acq: 13 Jun 2019 9:59


Tgt Ion:154 Resp: 81925

Ion Ratio Lower Upper

154 100

153 113.7 88.5 132.7



152 52.9 43.6 65.4

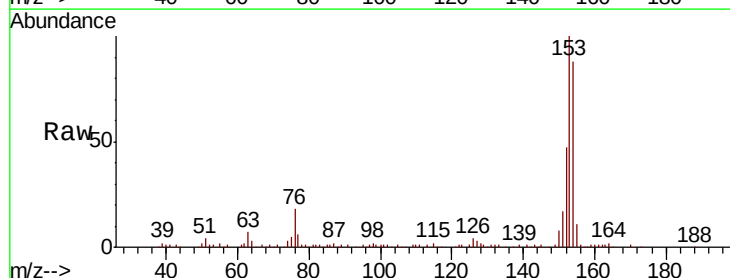


Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E




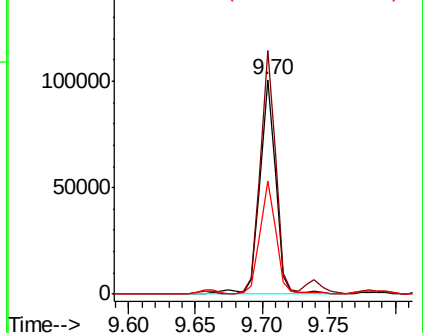




#56
4-Nitrophenol
Concen: 3.938 ng
RT: 9.87 min Scan# 1324
Delta R.T. 0.07 min
Lab File: BF114992.D
Acq: 13 Jun 2019 9:59




Instrument :
BNA_F
ClientSampleId :
OR-03-061119-A


Tot Ion	Ratio	Lower	Upper
139	100		
109	3.0	41.4	81.4#
65	2.1	62.7	102.7#

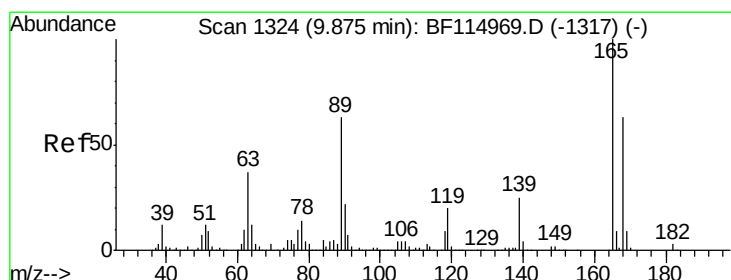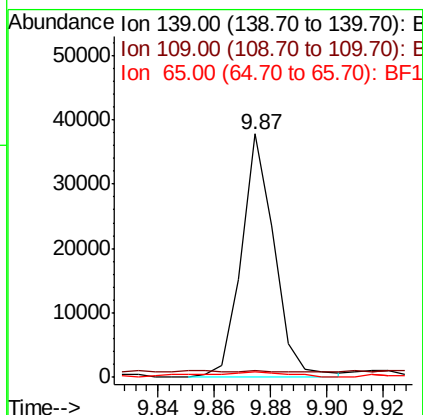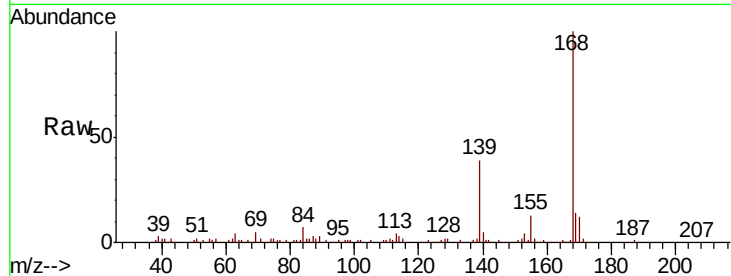

#57
2,4-Dinitrotoluene
Concen: 6.101 ng
RT: 9.67 min Scan# 1290
Delta R.T. -0.20 min
Lab File: BF114992.D
Acq: 13 Jun 2019 9:59

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.2	29.4	44.2#
89	1.6	50.6	75.8#
182	0.0	2.2	3.2#

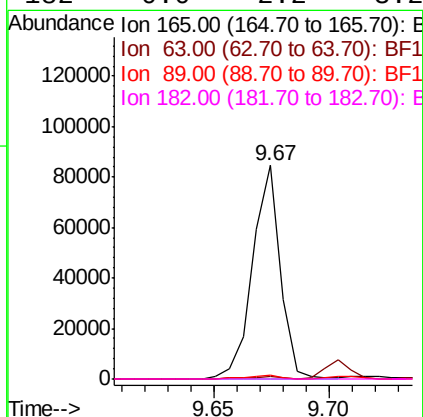

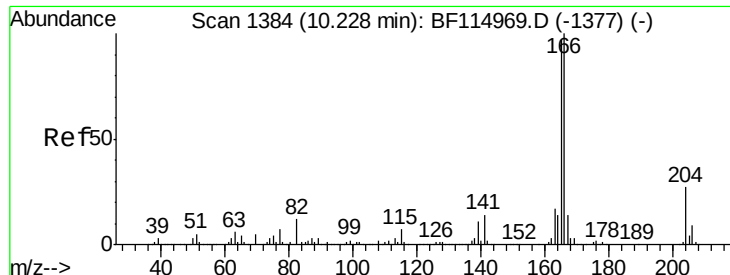

#58

Fluorene

Concen: Below Cal

RT: 10.22 min Scan# 1382

Delta R.T. -0.01 min

Lab File: BF114992.D

Acq: 13 Jun 2019 9:59

Instrument :

BNA_F

ClientSampleId :

OR-03-061119-A


Tot Ion:166 Resp: 111659

Ion Ratio Lower Upper

166 100

165 97.9 77.6 116.4



167 14.0 11.0 16.4

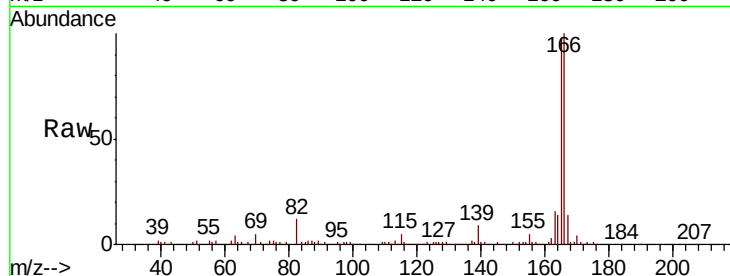

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

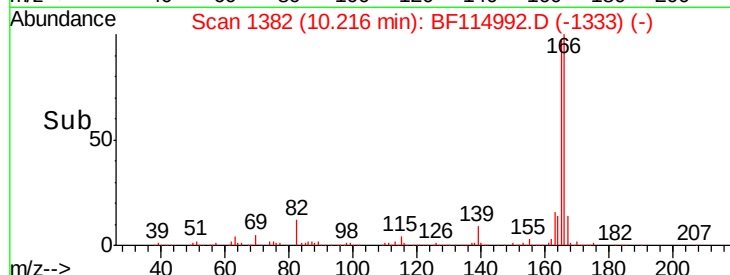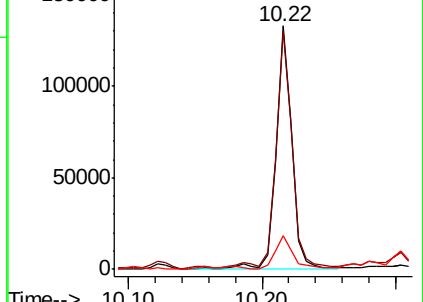

#61

4-Chlorophenyl-phenylether

Concen: Below Cal

RT: 10.05 min Scan# 1354

Delta R.T. -0.17 min

Lab File: BF114992.D

Acq: 13 Jun 2019 9:59


Tgt Ion:204 Resp: 127

Ion Ratio Lower Upper

204 100

206 0.0 26.5 39.7#



141 128.5 51.8 77.8#

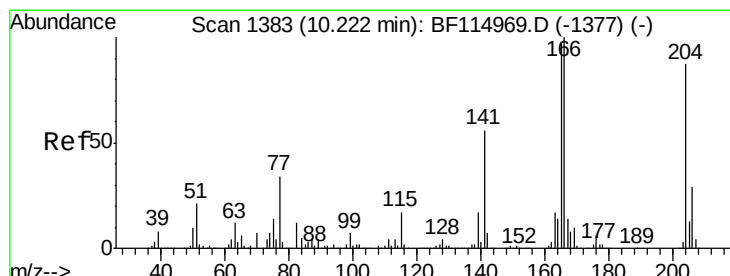


Abundance Ion 204.00 (203.70 to 204.70): E

Ion 206.00 (205.70 to 206.70): E

Ion 141.00 (140.70 to 141.70): E

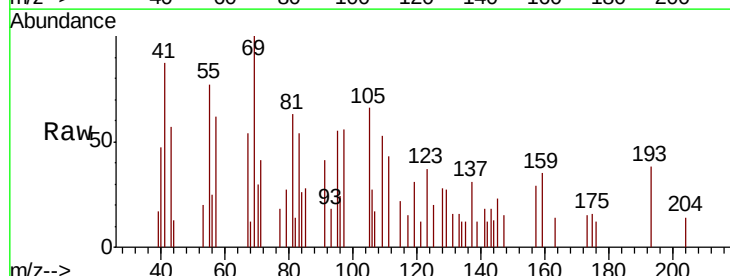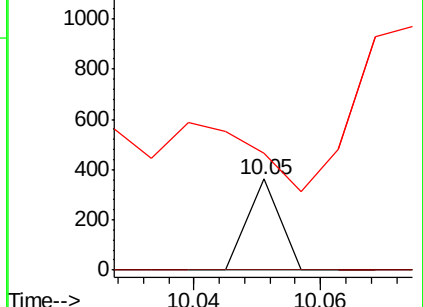







#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.15 min Scan# 1541
Delta R.T. -0.01 min
Lab File: BF114992.D
Acq: 13 Jun 2019 9:59

Instrument :
BNA_F
ClientSampleId :
OR-03-061119-A

Tot Ion:188 Resp: 873495
Ion Ratio Lower Upper
188 100
94 8.6 7.2 10.8
80 8.9 7.4 11.2




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1


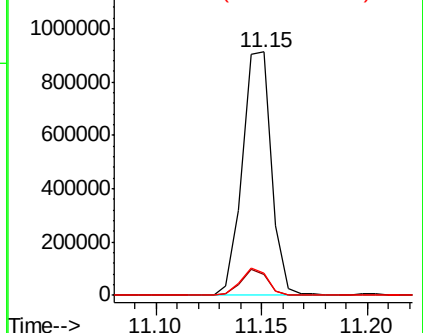



#71
Phenanthrene
Concen: 13.937 ng
RT: 11.17 min Scan# 1544
Delta R.T. -0.01 min
Lab File: BF114992.D
Acq: 13 Jun 2019 9:59

Tgt Ion:178 Resp: 628564
Ion Ratio Lower Upper
178 100
176 19.3 16.9 25.3
179 15.6 13.4 20.0



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

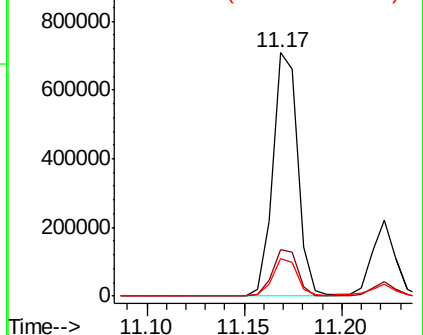

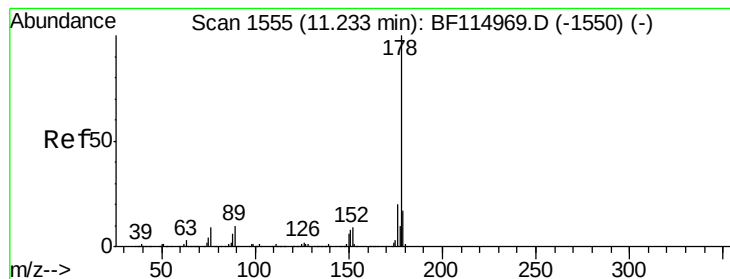

#72

Anthracene

Concen: 3.861 ng

RT: 11.22 min Scan# 1553

Delta R.T. -0.01 min

Lab File: BF114992.D

Acq: 13 Jun 2019 9:59

Instrument :

BNA_F

ClientSampleId :

OR-03-061119-A


Tot Ion:178 Resp: 175675

Ion Ratio Lower Upper

178 100

176 18.6 16.2 24.4




179 15.7 13.2 19.8

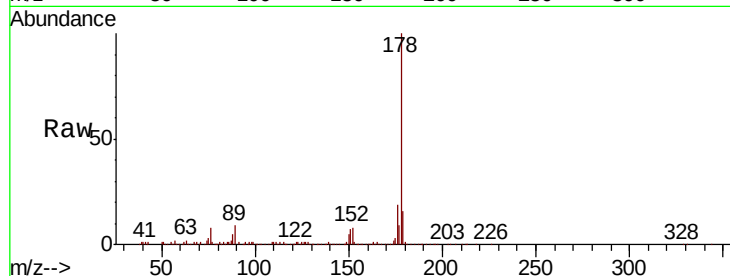

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

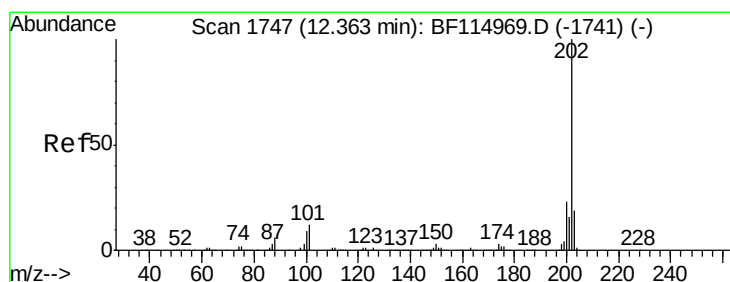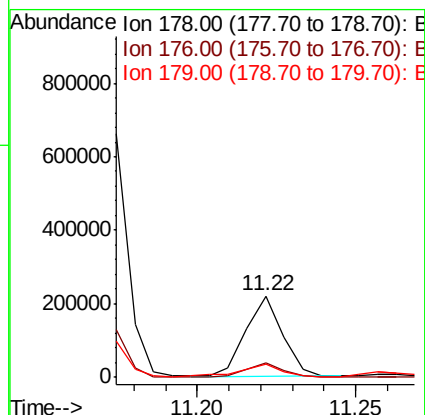

#75

Fluoranthene

Concen: 13.768 ng

RT: 12.35 min Scan# 1745

Delta R.T. -0.01 min

Lab File: BF114992.D

Acq: 13 Jun 2019 9:59


Tgt Ion:202 Resp: 634923

Ion Ratio Lower Upper

202 100

101 12.7 0.0 32.4



203 18.1 0.0 38.6

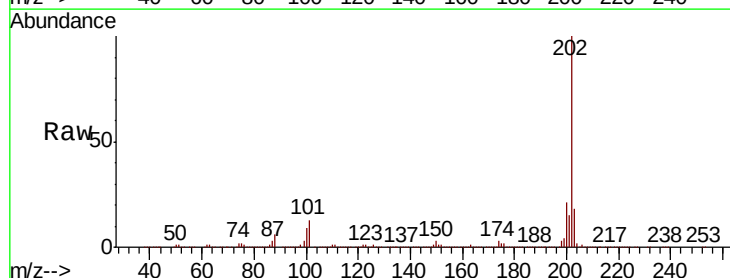


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E



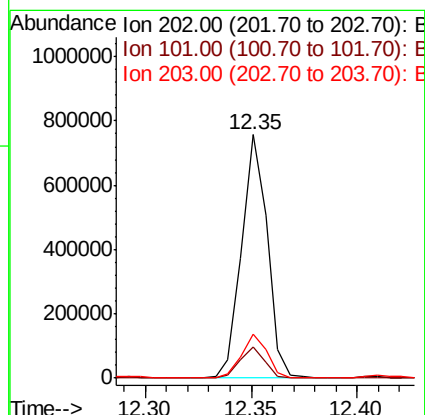





#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.77 min Scan# 1986
Delta R.T. -0.01 min
Lab File: BF114992.D
Acq: 13 Jun 2019 9:59




Instrument :
BNA_F
ClientSampleId :
OR-03-061119-A


Tot Ion:240 Resp: 571267
Ion Ratio Lower Upper
240 100
120 12.9 10.0 15.0
236 26.5 21.6 32.4

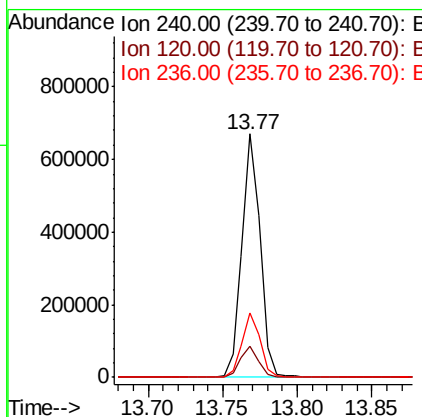

#78
Pyrene
Concen: 10.929 ng
RT: 12.57 min Scan# 1783
Delta R.T. -0.01 min
Lab File: BF114992.D
Acq: 13 Jun 2019 9:59

Tgt Ion:202 Resp: 568771
Ion Ratio Lower Upper
202 100
200 21.3 18.4 27.6
203 19.1 14.9 22.3

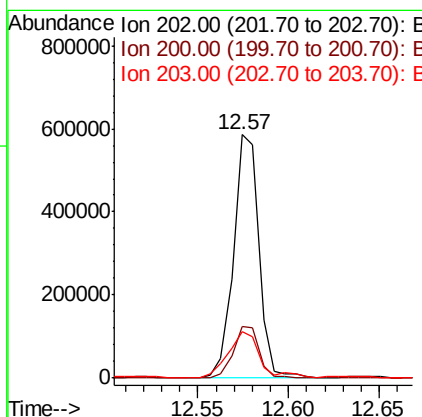



#79

Terphenyl-d14

Concen: 26.566 ng

RT: 12.73 min Scan# 1809

Delta R.T. -0.01 min

Lab File: BF114992.D

Acq: 13 Jun 2019 9:59

Instrument :

BNA_F

ClientSampleId :

OR-03-061119-A


Tot Ion:244 Resp: 806869

Ion Ratio Lower Upper

244 100

212 6.3 5.8 8.8




122 11.7 9.4 14.0

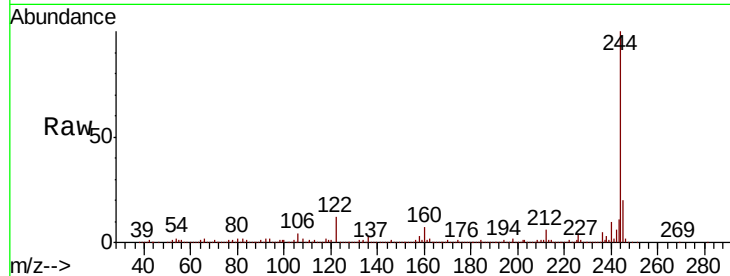

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

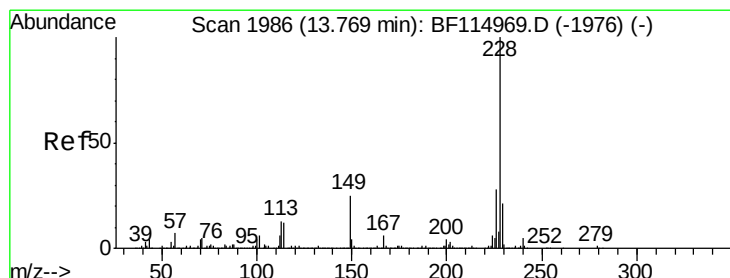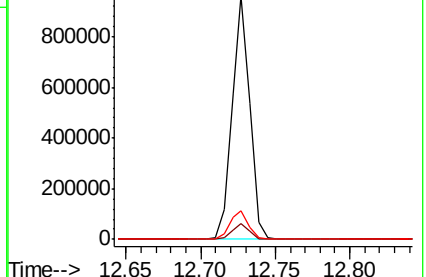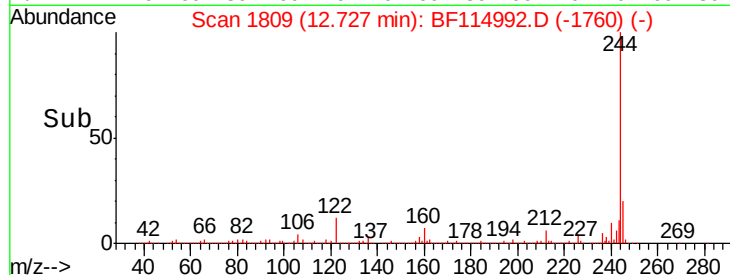

#81

Benzo(a)anthracene

Concen: 6.805 ng

RT: 13.76 min Scan# 1984

Delta R.T. -0.01 min

Lab File: BF114992.D

Acq: 13 Jun 2019 9:59


Tgt Ion:228 Resp: 290917

Ion Ratio Lower Upper

228 100

226 29.5 22.0 33.0



229 20.9 16.6 25.0

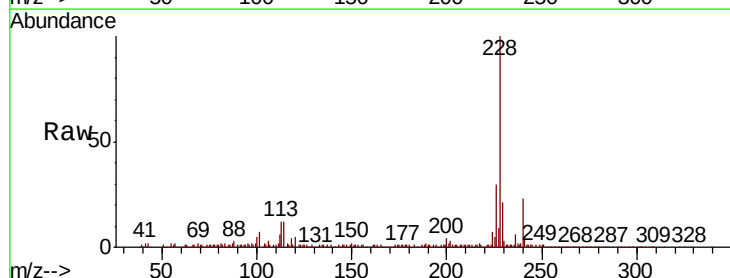


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

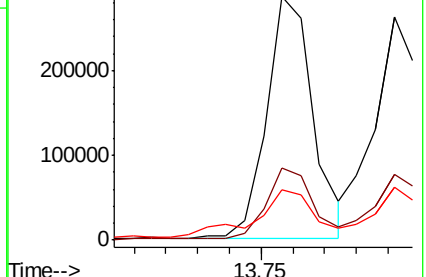



#83

Chrysene

Concen: 6.094 ng

RT: 13.79 min Scan# 1990

Delta R.T. -0.02 min

Lab File: BF114992.D

Acq: 13 Jun 2019 9:59

Instrument :

BNA_F

ClientSampleId :

OR-03-061119-A


Tot Ion:228 Resp: 259041

Ion Ratio Lower Upper

228 100

226 29.7 25.4 38.0




229 23.6 16.4 24.6

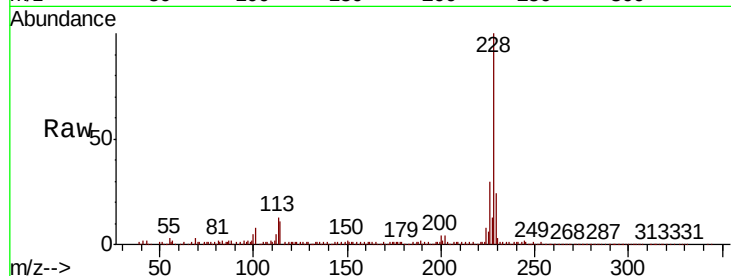

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

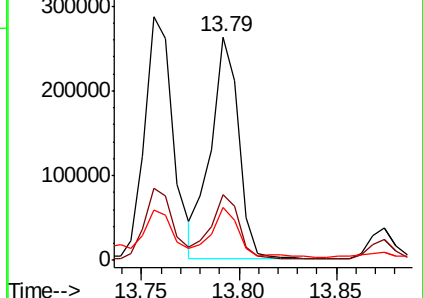

#86

Indeno(1,2,3-cd)pyrene

Concen: 2.978 ng

RT: 16.44 min Scan# 2441

Delta R.T. -0.02 min

Lab File: BF114992.D

Acq: 13 Jun 2019 9:59


Tgt Ion:276 Resp: 111188

Ion Ratio Lower Upper

276 100

138 24.5 23.0 34.4



277 24.3 20.6 30.8




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

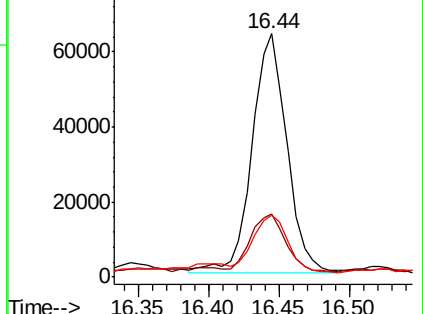



#87

Pervlene-d12

Concen: 20.000 ng

RT: 15.15 min Scan# 2221

Delta R.T. -0.00 min

Lab File: BF114992.D

Acq: 13 Jun 2019 9:59

Instrument :

BNA_F

ClientSampleId :

OR-03-061119-A


Tot Ion:264 Resp: 609448

Ion Ratio Lower Upper

264 100

260 24.4 19.9 29.9




265 22.3 17.6 26.4



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

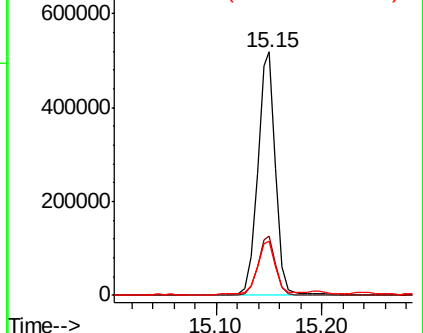

#88

Benzo(b)fluoranthene

Concen: 10.601 ng

RT: 14.77 min Scan# 2156

Delta R.T. -0.01 min

Lab File: BF114992.D

Acq: 13 Jun 2019 9:59


Tgt Ion:252 Resp: 429490

Ion Ratio Lower Upper

252 100

253 23.7 18.1 27.1



125 12.8 9.4 14.0




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E




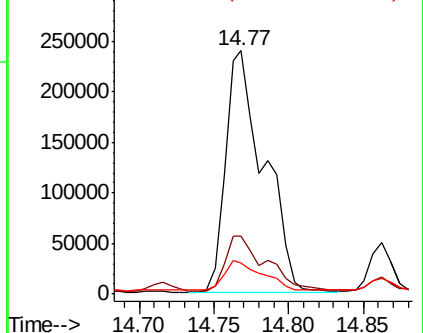




#89
Benzo(k)fluoranthene
Concen: 12.078 ng
RT: 14.77 min Scan# 2156
Delta R.T. -0.04 min
Lab File: BF114992.D
Acq: 13 Jun 2019 9:59




Instrument :
BNA_F
ClientSampleId :
OR-03-061119-A


Tot Ion	Ratio	Lower	Upper
252	100		
253	23.7	18.0	27.0
125	12.8	8.2	12.4

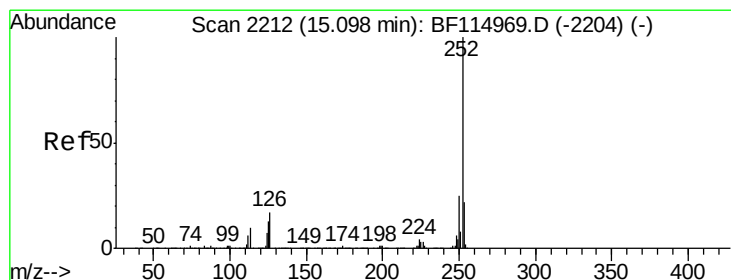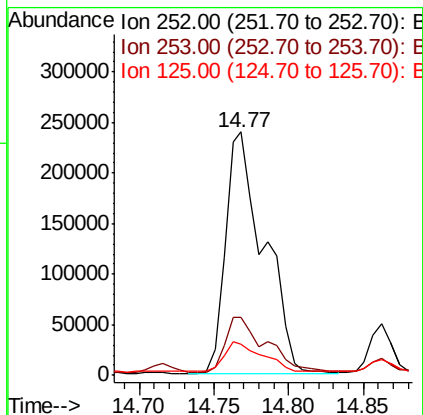

#90
Benzo(a)pyrene
Concen: 6.659 ng
RT: 15.09 min Scan# 2211
Delta R.T. -0.01 min
Lab File: BF114992.D
Acq: 13 Jun 2019 9:59

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.6	17.8	26.8
125	12.3	10.7	16.1

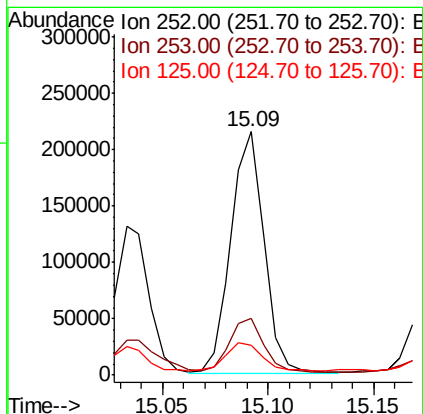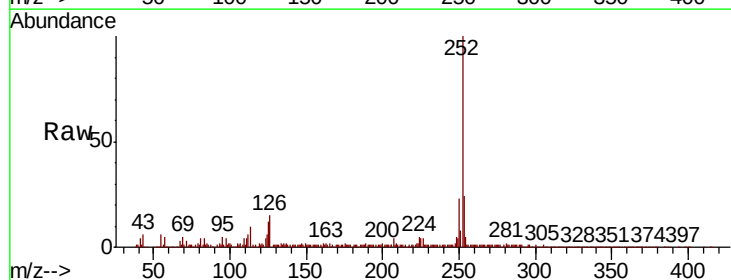

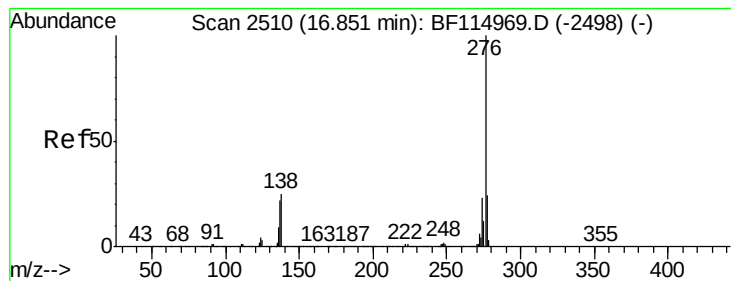

#92

Benzo(a,h,i)perylene

Concen: 3.193 ng

RT: 16.83 min Scan# 2507

Delta R.T. -0.02 min

Lab File: BF114992.D

Acq: 13 Jun 2019 9:59

Instrument :

BNA_F

ClientSampleId :

OR-03-061119-A


Tot Ion: 276 Resp: 98023

Ion Ratio Lower Upper

276 100

277 23.2 18.8 28.2

138 26.2 20.2 30.4

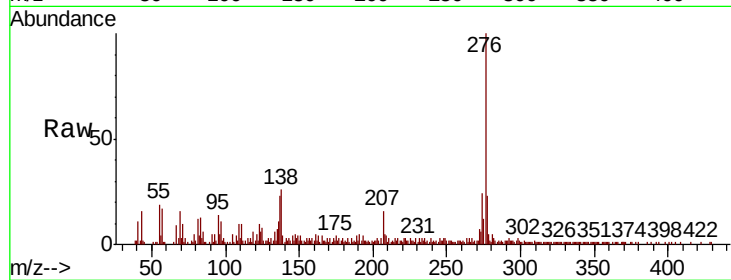

Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

