
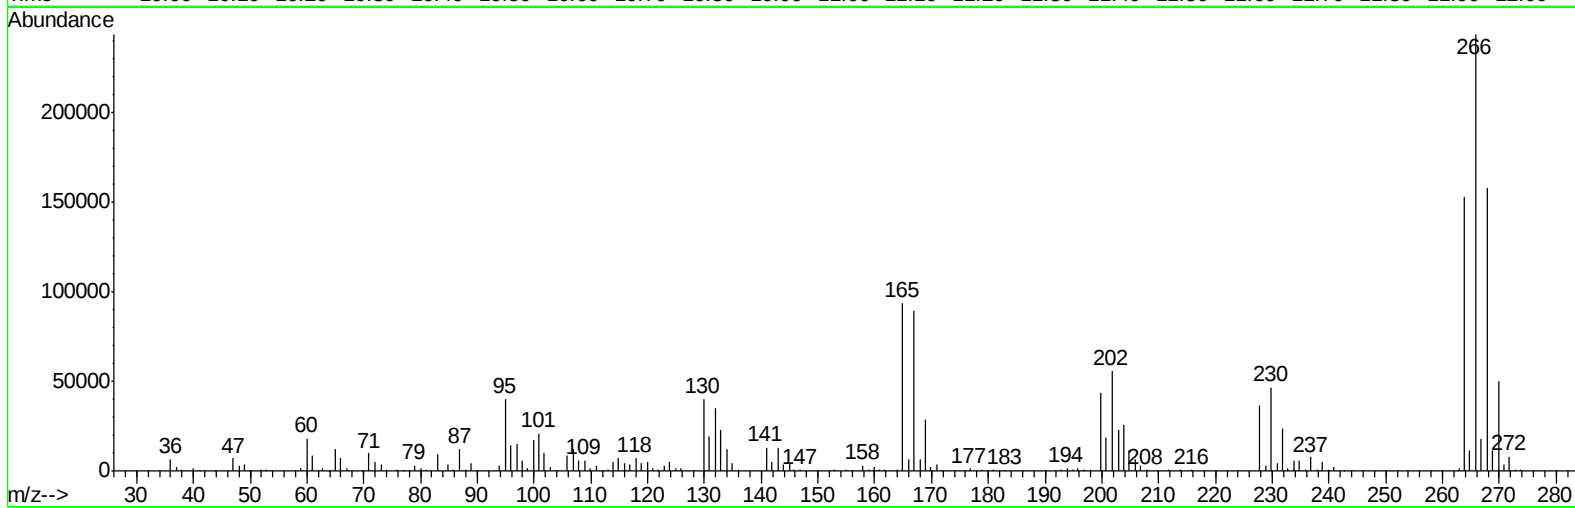


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF061319\
Data File : BF114987.D
Acq On : 13 Jun 2019 7:47
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 08:55:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 12 15:42:37 2019
Response via : Initial Calibration

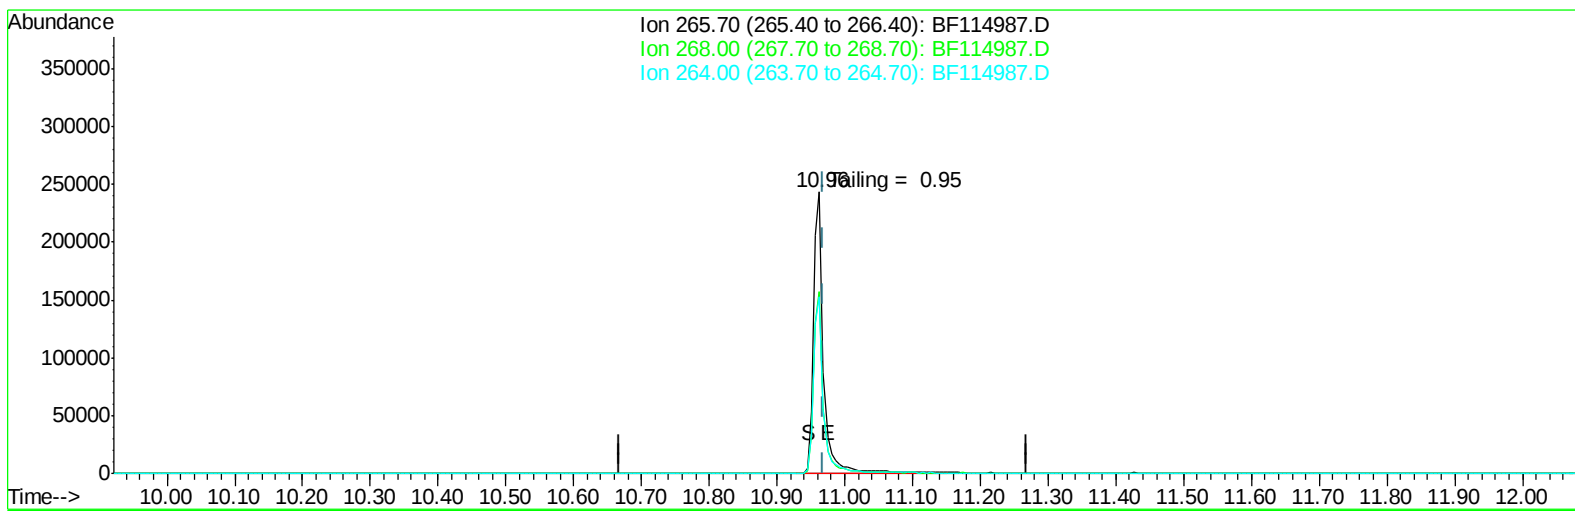

TIC: BF114987.D

(70) Pentachlorophenol (C)



10.963min (-0.006) 73823.73ng m

response 251651

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	64.78
264.00	62.90	62.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF061319\
Data File : BF114987.D
Acq On : 13 Jun 2019 7:47
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 08:55:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 12 15:42:37 2019
Response via : Initial Calibration

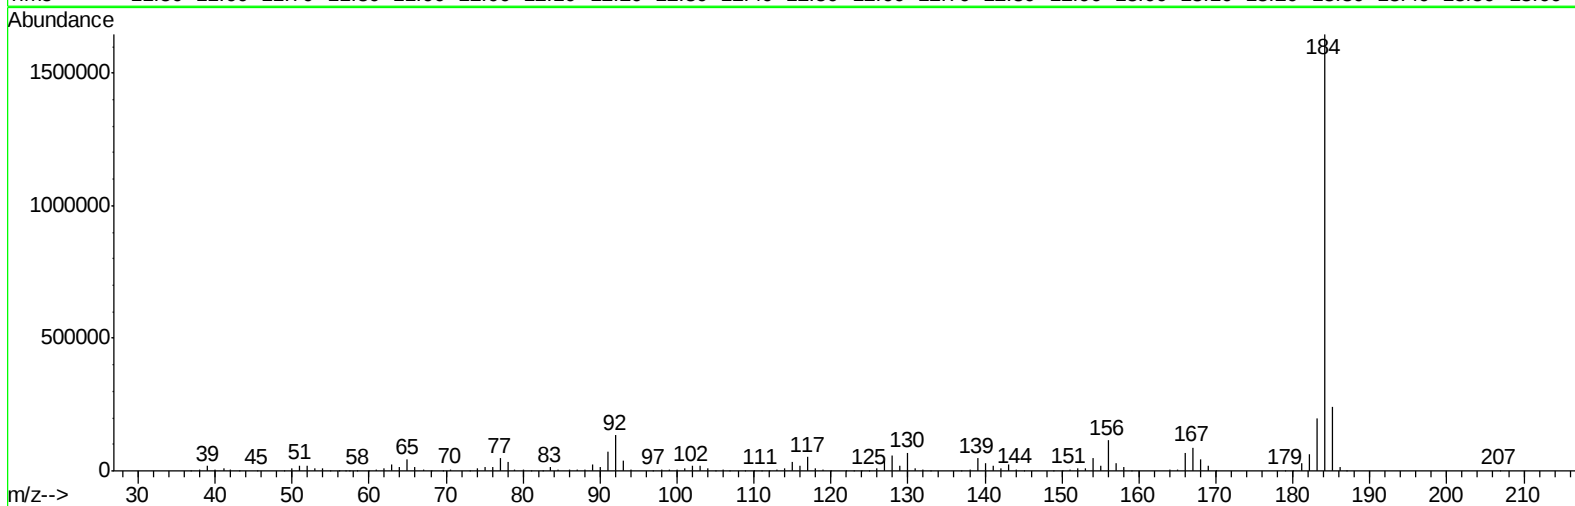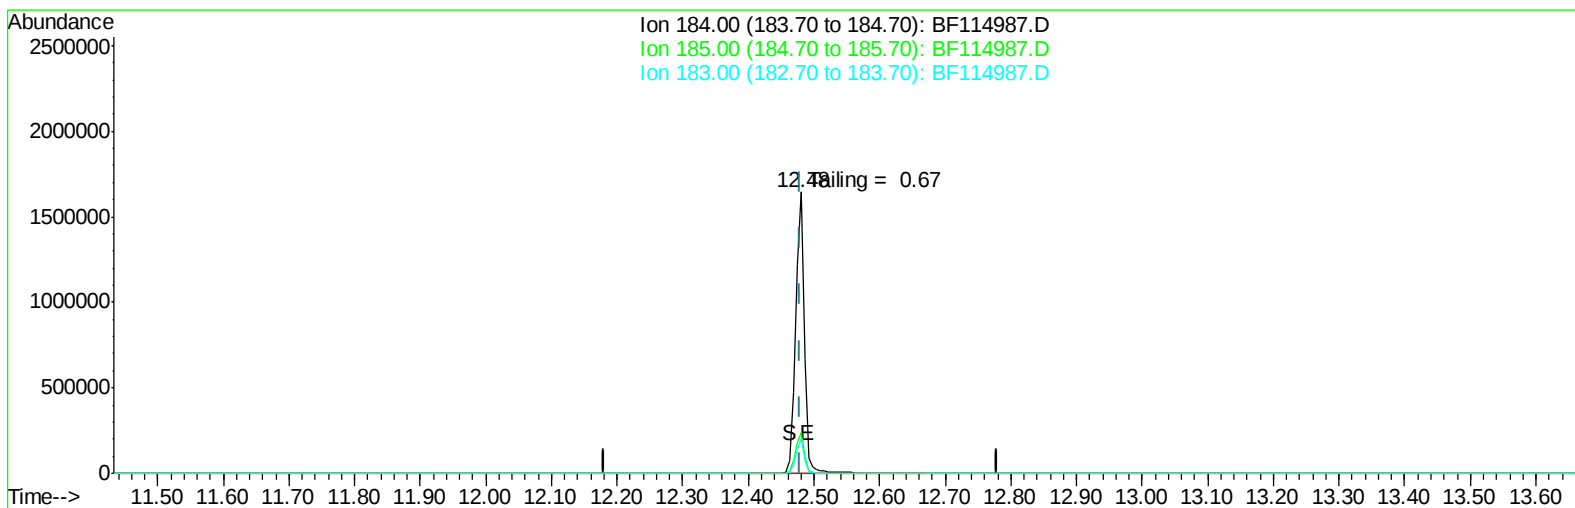

TIC: BF114987.D

(77) Benzidine

12.480min (-0.000) 4461.82ng m

response 1529666

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.65
183.00	12.20	12.08
0.00	0.00	0.00