
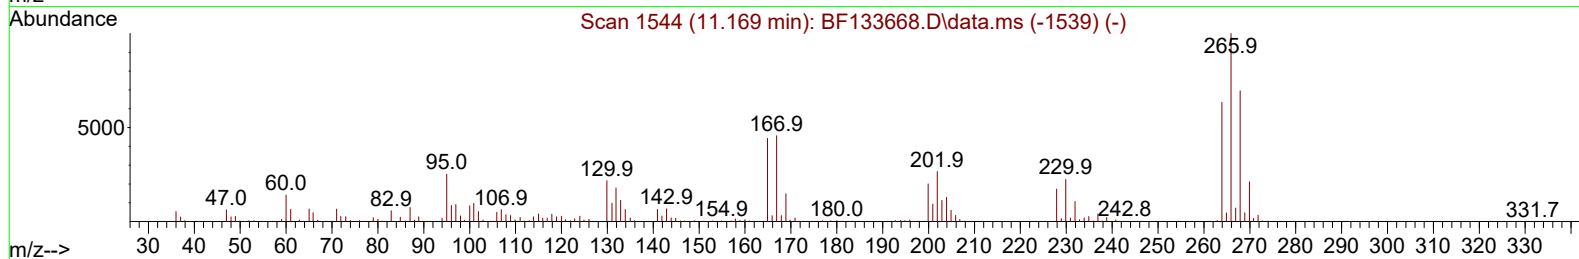
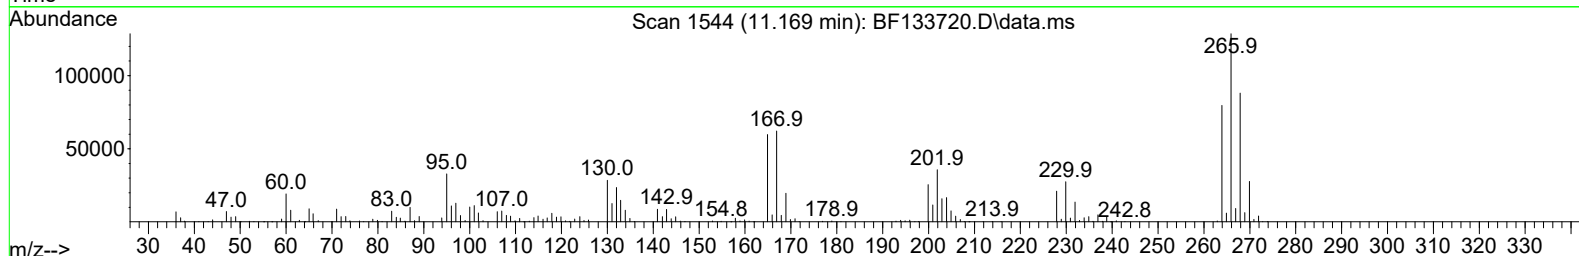


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061323\
 Data File : BF133720.D
 Acq On : 13 Jun 2023 09:16
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 11:30:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 13 11:26:55 2023
 Response via : Initial Calibration

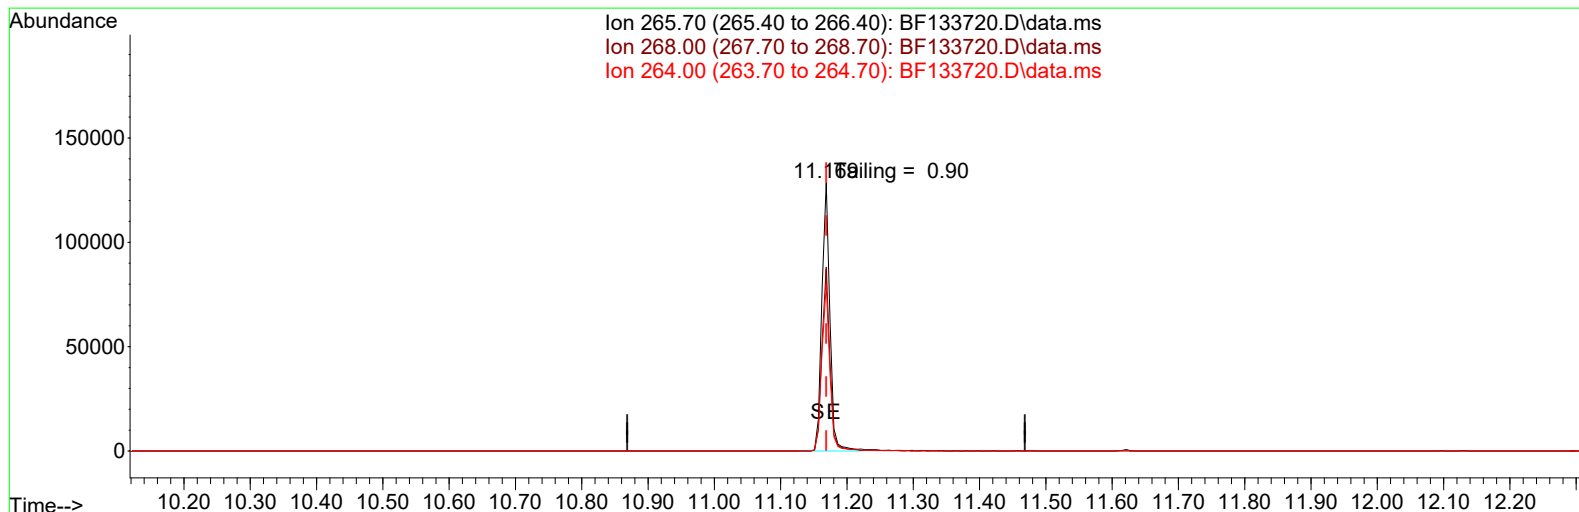

TIC: BF133720.D\data.ms

(70) Pentachlorophenol (C)




11.169min (+ 0.000) 26161.30 ng

response 110320

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.60	68.50
264.00	63.40	61.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061323\
Data File : BF133720.D
Acq On : 13 Jun 2023 09:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 11:30:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 13 11:26:55 2023
Response via : Initial Calibration

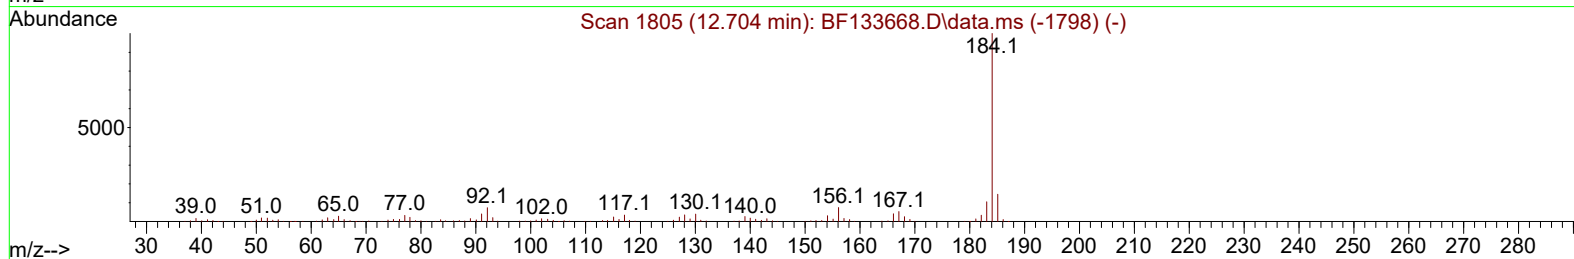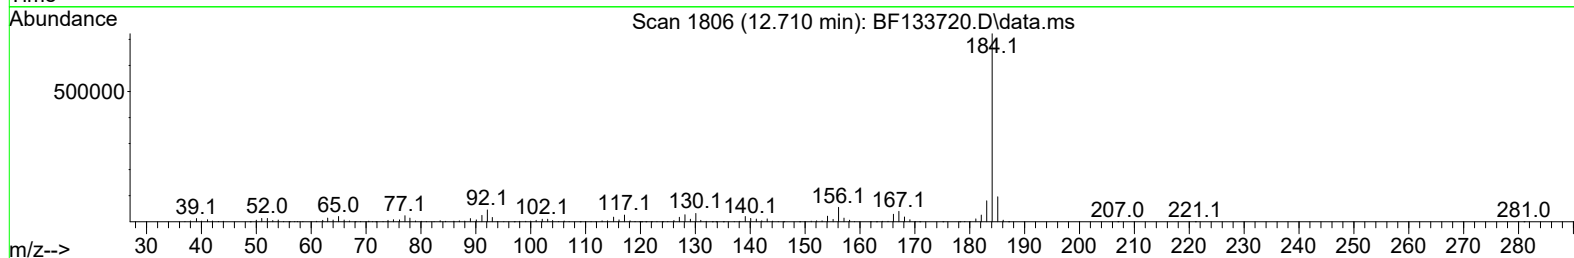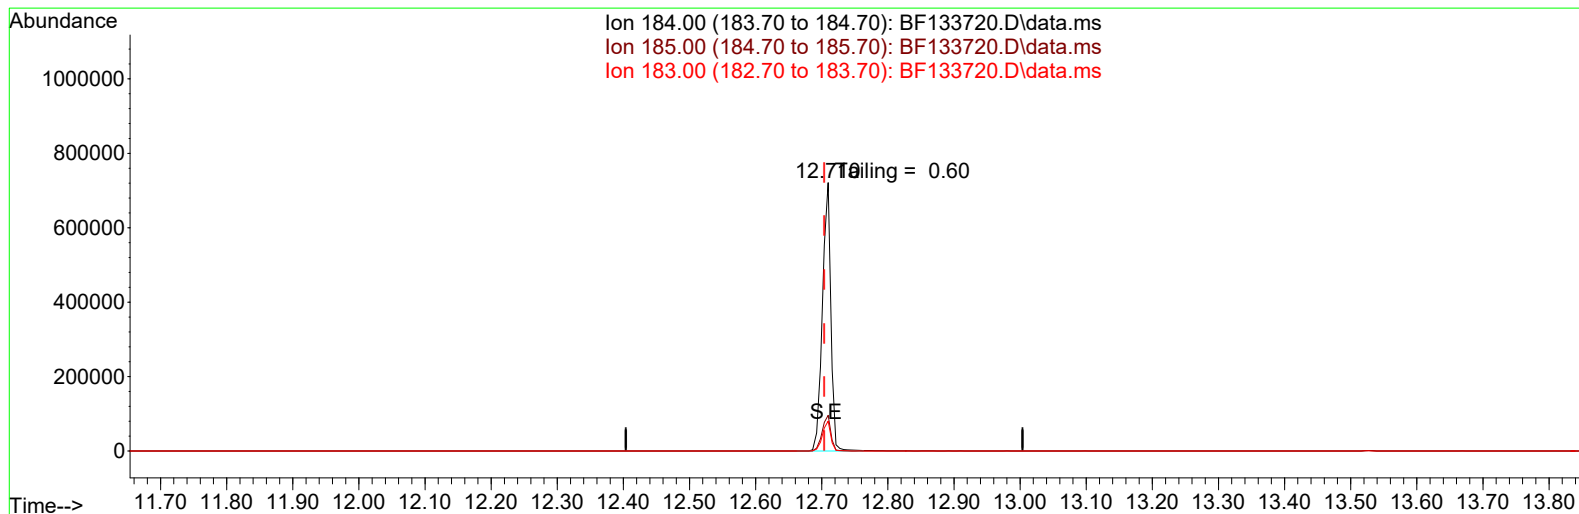

TIC: BF133720.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 91911.02 ng

response 641506

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.29
183.00	10.50	11.18
0.00	0.00	0.00