

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061323\
 Data File : BF133722.D
 Acq On : 13 Jun 2023 10:18
 Operator : CG\JU
 Sample : PB153230BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB153230BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133722.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.146	5	10	16	rVB	52953	73631	1.90%	0.343%
2	5.081	505	509	516	rVB	30689	44527	1.15%	0.207%
3	5.457	568	573	576	rBV	2549904	2817355	72.79%	13.119%
4	6.469	739	745	748	rBV	2564161	2842441	73.44%	13.236%
5	6.834	803	807	810	rBV	735864	542890	14.03%	2.528%
6	7.404	898	904	906	rBV	1921175	1898081	49.04%	8.838%
7	8.116	1021	1025	1029	rBV	870118	686688	17.74%	3.198%
8	9.198	1204	1209	1212	rBV	4119059	3416585	88.27%	15.909%
9	9.875	1320	1324	1327	rBV	983684	775955	20.05%	3.613%
10	10.669	1454	1459	1462	rBV	2688114	2368943	61.20%	11.031%
11	11.363	1573	1577	1581	rBV	1059422	857041	22.14%	3.991%
12	12.957	1843	1848	1851	rBV	3714129	3870514	100.00%	18.023%
13	14.010	2023	2027	2031	rBV	825464	719274	18.58%	3.349%
14	15.474	2272	2276	2284	rVB	455853	561803	14.51%	2.616%




Sum of corrected areas: 21475728

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061323\
Data File : BF133722.D
Acq On : 13 Jun 2023 10:18
Operator : CG\JU
Sample : PB153230BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153230BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

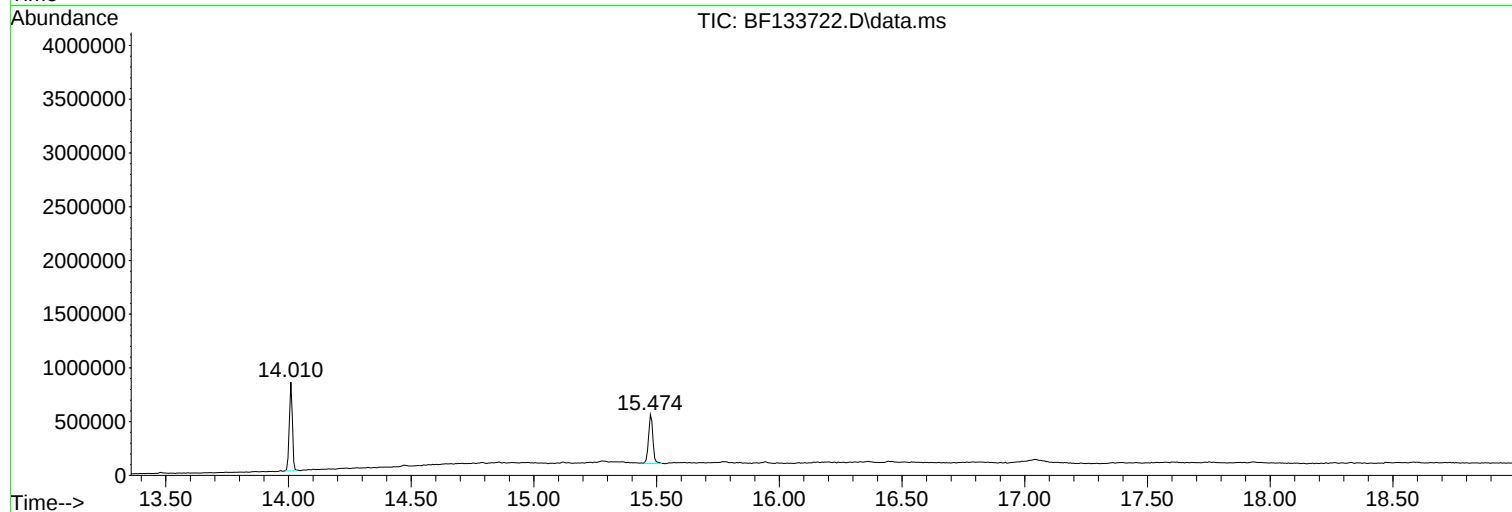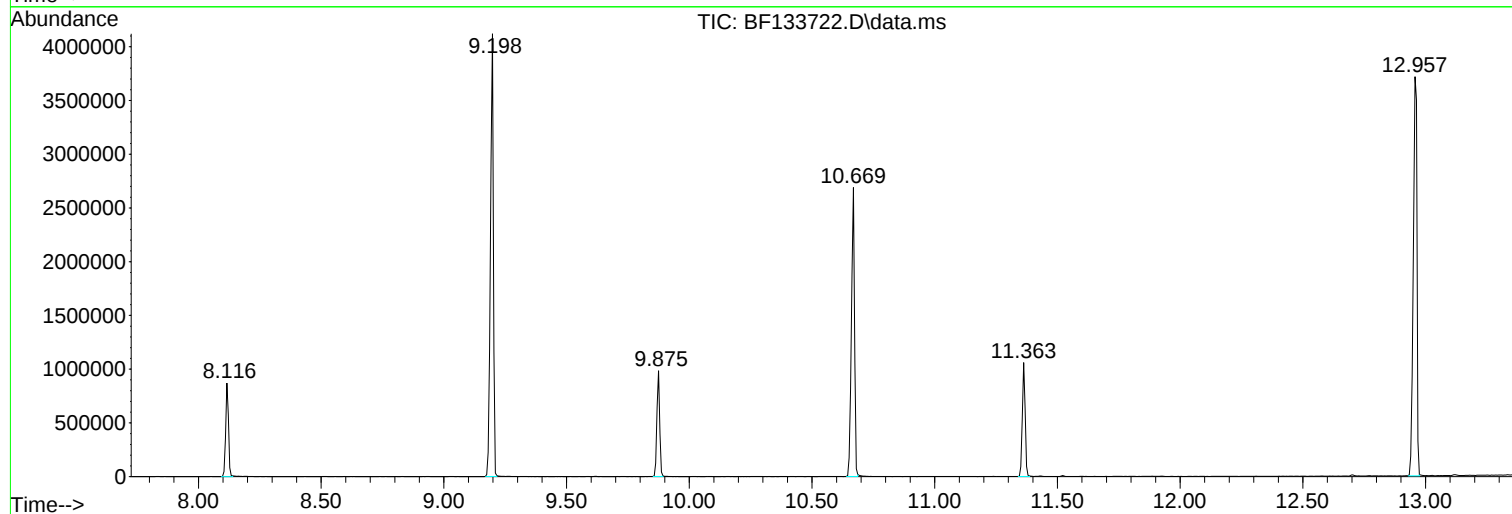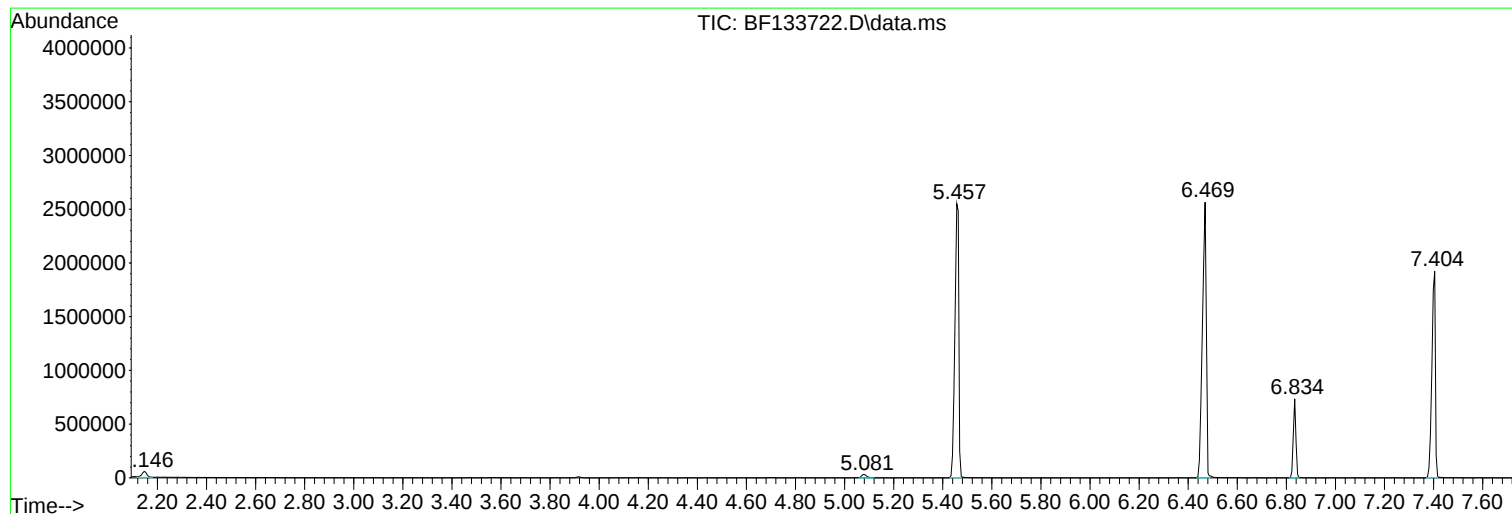

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061323\
Data File : BF133722.D
Acq On : 13 Jun 2023 10:18
Operator : CG\JU
Sample : PB153230BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153230BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.146	2.71 ng	73631	1,4-Dichlorobenzene-d4	6.834

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	45
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
4			Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	36
5			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	28

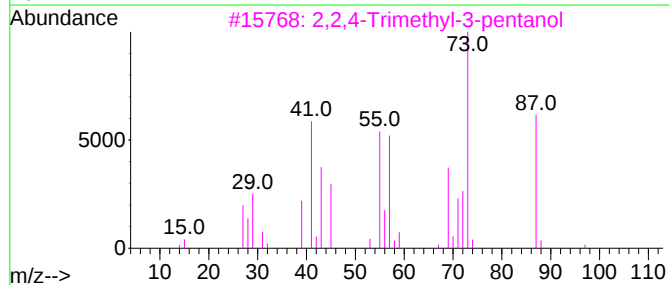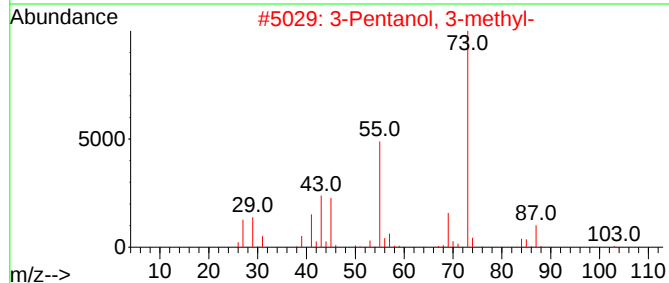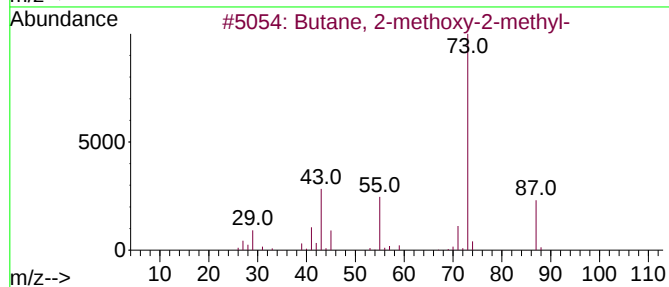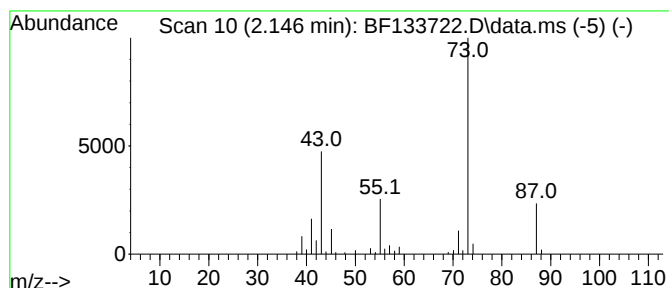

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061323\
Data File : BF133722.D
Acq On : 13 Jun 2023 10:18
Operator : CG\JU
Sample : PB153230BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153230BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.146	2.7	ng	73631	1	6.834	542890	20.0