
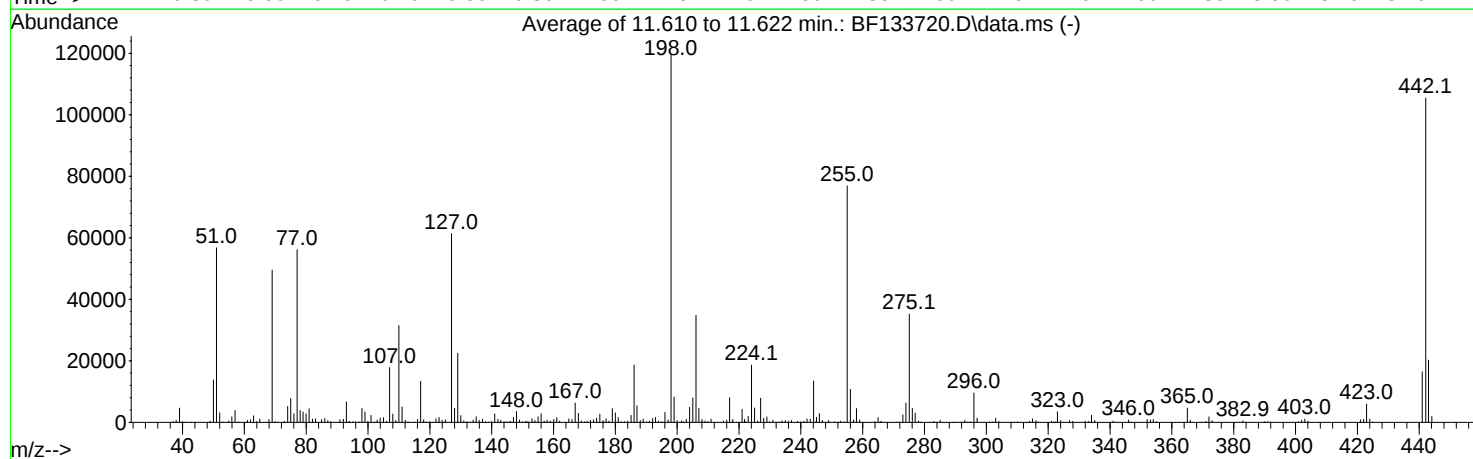


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061323\
 Data File : BF133720.D
 Acq On : 13 Jun 2023 09:16
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 13 11:26:55 2023

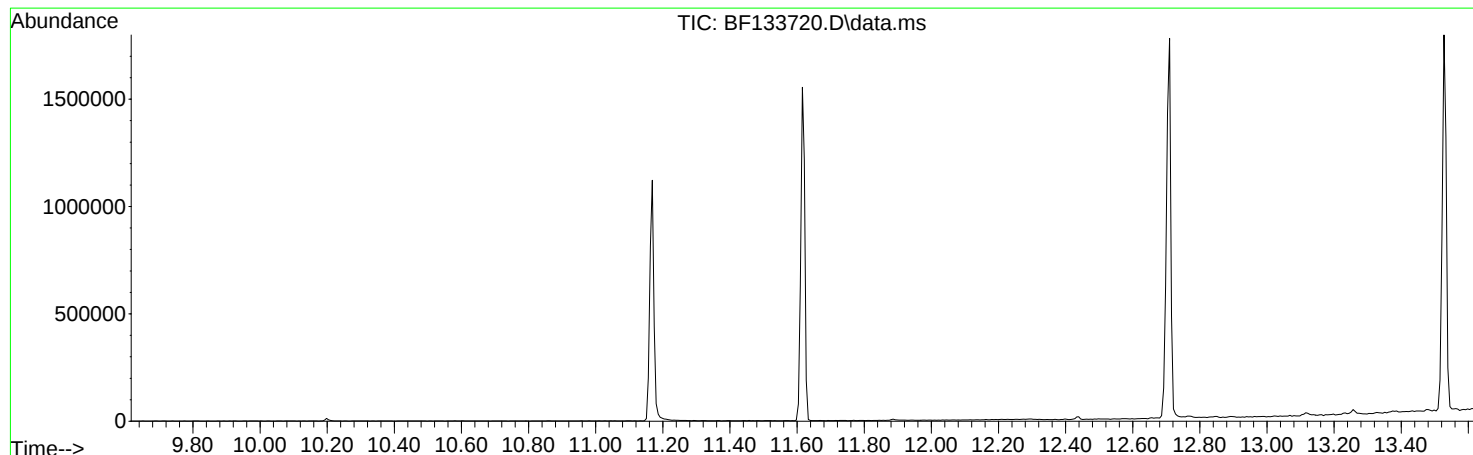

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.5	56773	PASS
68	69	0.00	2	1.7	866	PASS
69	198	0.00	100	41.4	49549	PASS
70	69	0.00	2	0.5	265	PASS
127	198	10	80	51.3	61349	PASS
197	198	0.00	2	0.7	817	PASS
198	198	100	100	100.0	119611	PASS
199	198	5	9	6.9	8296	PASS
275	198	10	60	29.4	35163	PASS
365	198	1	100	3.9	4616	PASS
441	198	0.01	100	13.8	16463	PASS
442	442	50	100	100.0	105440	PASS
443	442	15	24	19.2	20240	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
6/13/2023	BNA_F	<u>BF133720.D</u>
Compound Name	Response	Retention Time
DDT	274156	13.527
DDD	5147	13.257
DDE	231	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5378	279534	1.92

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061323\
Data File : BF133720.D
Acq On : 13 Jun 2023 09:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 13 11:30:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 13 11:26:55 2023
Response via : Initial Calibration

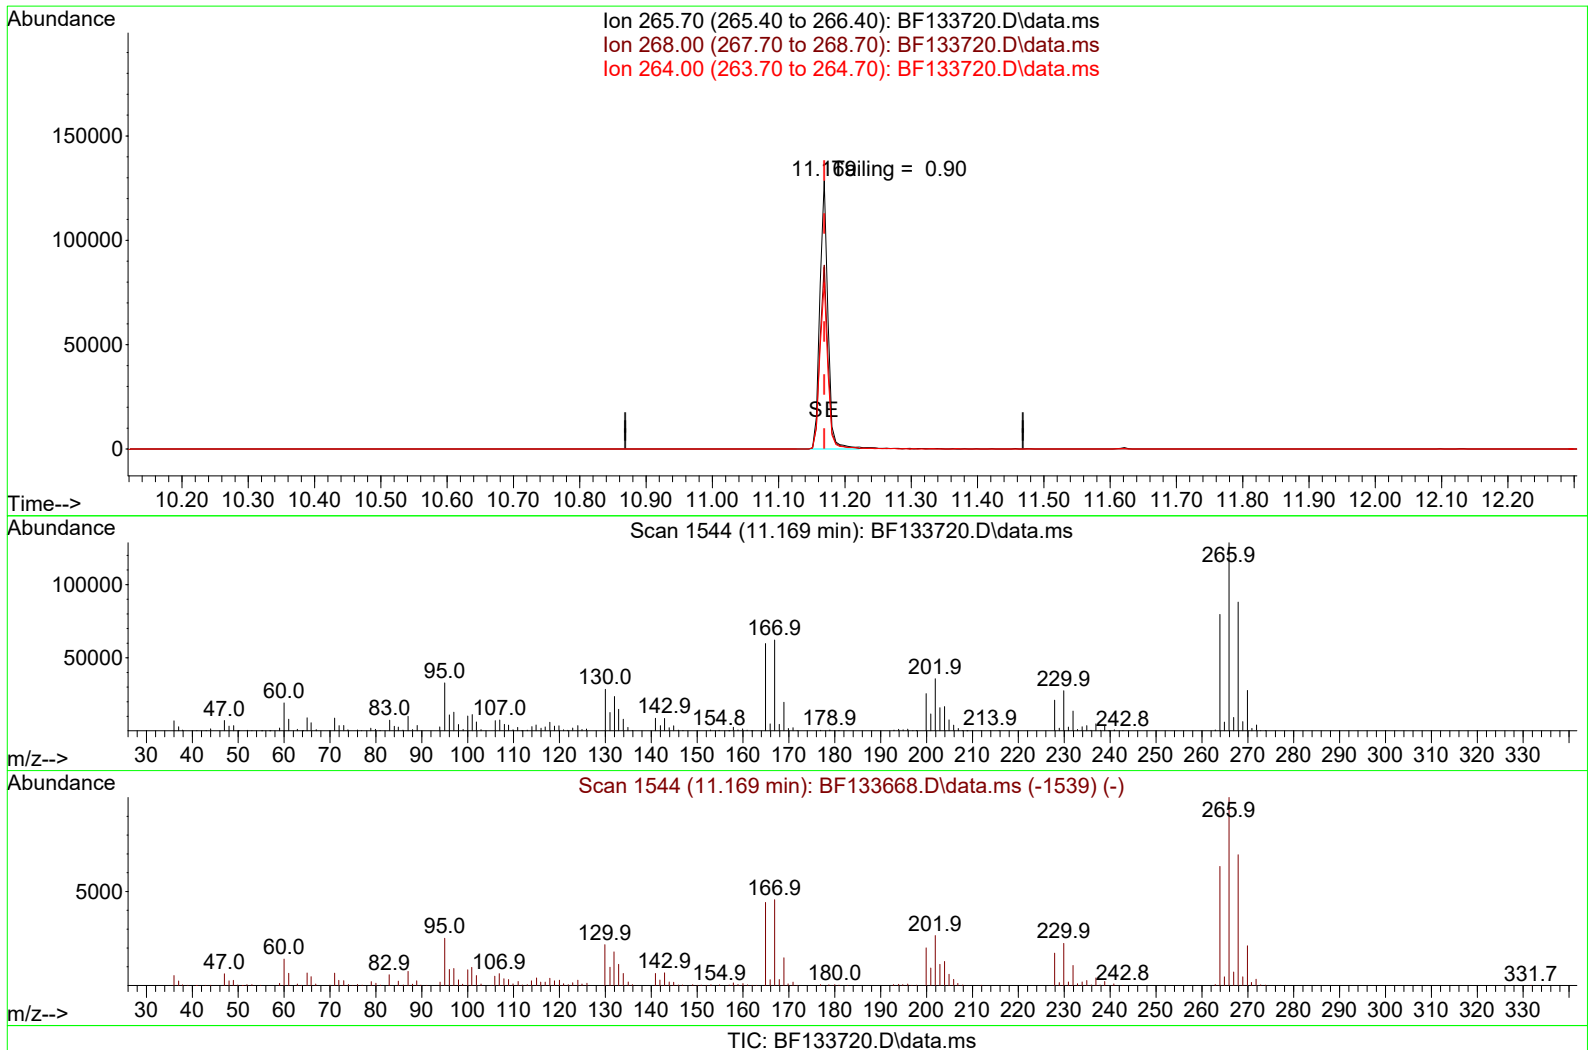

TIC: BF133720.D\data.ms

(70) Pentachlorophenol (C)

11.169min (+ 0.000) 26161.30 ng




response 110320

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.60	68.50
264.00	63.40	61.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061323\
Data File : BF133720.D
Acq On : 13 Jun 2023 09:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 13 11:30:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 13 11:26:55 2023
Response via : Initial Calibration

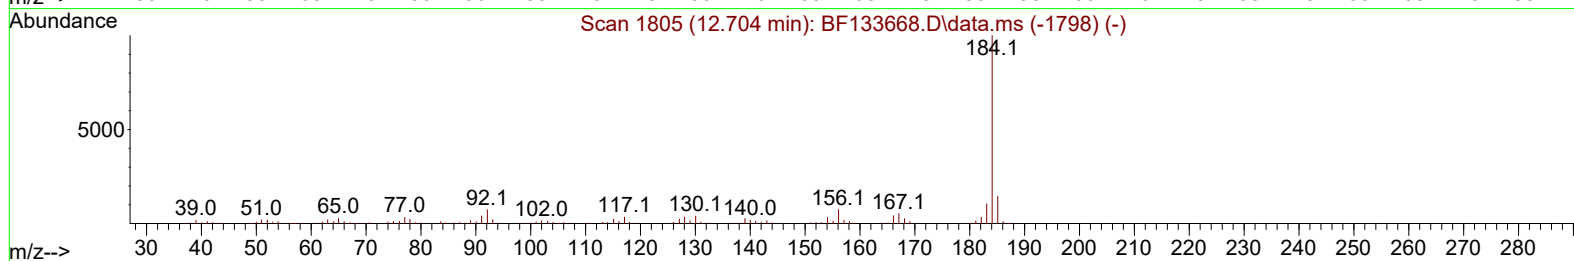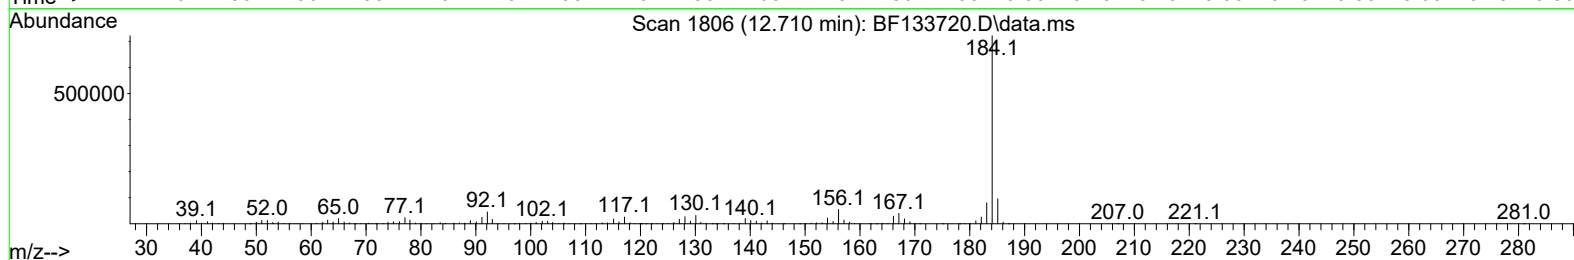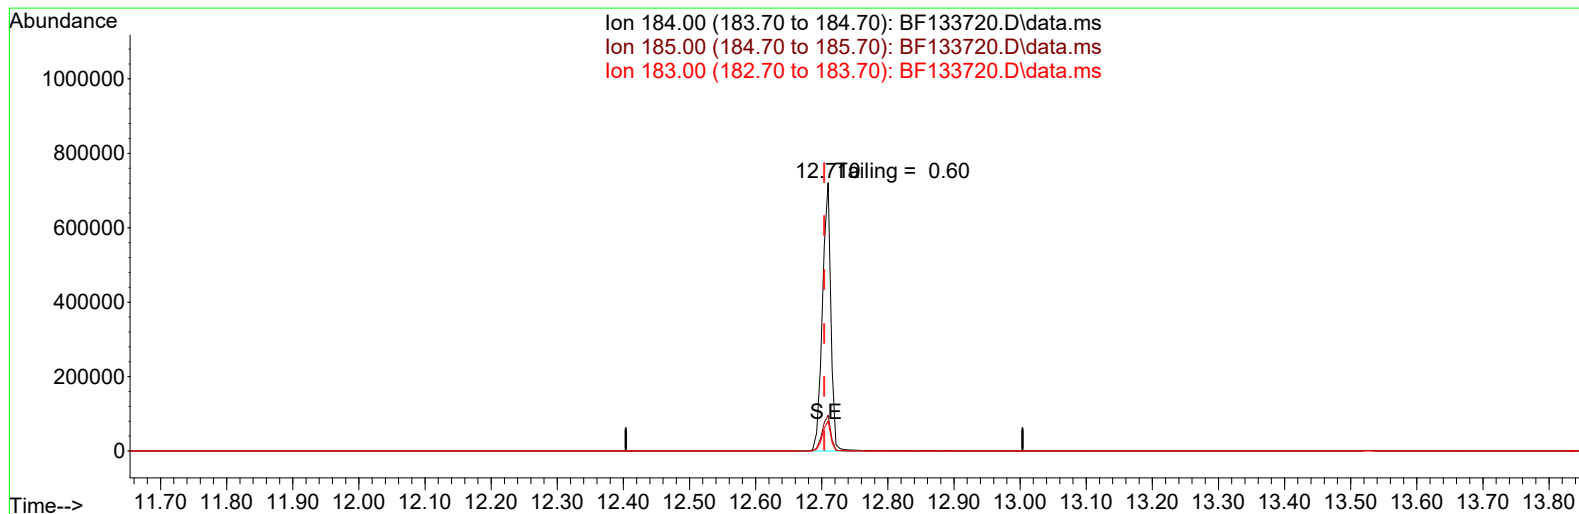

TIC: BF133720.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 91911.02 ng

response 641506

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.29
183.00	10.50	11.18
0.00	0.00	0.00