

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061418\
 Data File : BF106470.D
 Acq On : 15 Jun 2018 4:11
 Operator : JU/SJ
 Sample : J3474-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 061118-DBRI-E-D-S

Quant Time: Jun 15 08:26:58 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 14 18:39:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	106669	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	346779	20.00	ng	0.00
38) Acenaphthene-d10	10.01	164	134802	20.00	ng	0.00
63) Phenanthrene-d10	11.50	188	268977	20.00	ng	0.00
75) Chrysene-d12	14.15	240	284265	20.00	ng	-0.01
86) Perylene-d12	15.68	264	194890	20.00	ng	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.61	112	298701	47.39	ng	0.00
7) Phenol-d6	6.61	99	232371	29.18	ng	0.00
23) Nitrobenzene-d5	7.53	82	624910	106.01	ng	0.00
41) 2,4,6-Tribromophenol	10.80	330	144139	111.13	ng	0.00
44) 2-Fluorobiphenyl	9.32	172	952768	171.17	ng	0.00
78) Terphenyl-d14	13.08	244	1123006	98.12	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
19) n-Nitroso-di-n-propylamine	7.53	70	83837	14.034	ng	# 74
25) Isophorone	7.53	82	624904	54.274	ng	# 64
49) Dimethylphthalate	9.71	163	51670	5.365	ng	# 99
50) 2,6-Dinitrotoluene	10.01	165	16926	8.604	ng	# 24
56) 2,4-Dinitrotoluene	10.01	165	16926	6.851	ng	# 21
64) 4,6-Dinitro-2-methylphenol	10.80	198	294	6.471	ng	# 1
66) 4-Bromophenyl-phenylether	10.80	248	9598	3.137	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061418\
Data File : BF106470.D
Acq On : 15 Jun 2018 4:11
Operator : JU/SJ
Sample : J3474-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
061118-DBRI-E-D-S

Quant Time: Jun 15 08:26:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 14 18:39:24 2018
Response via : Initial Calibration

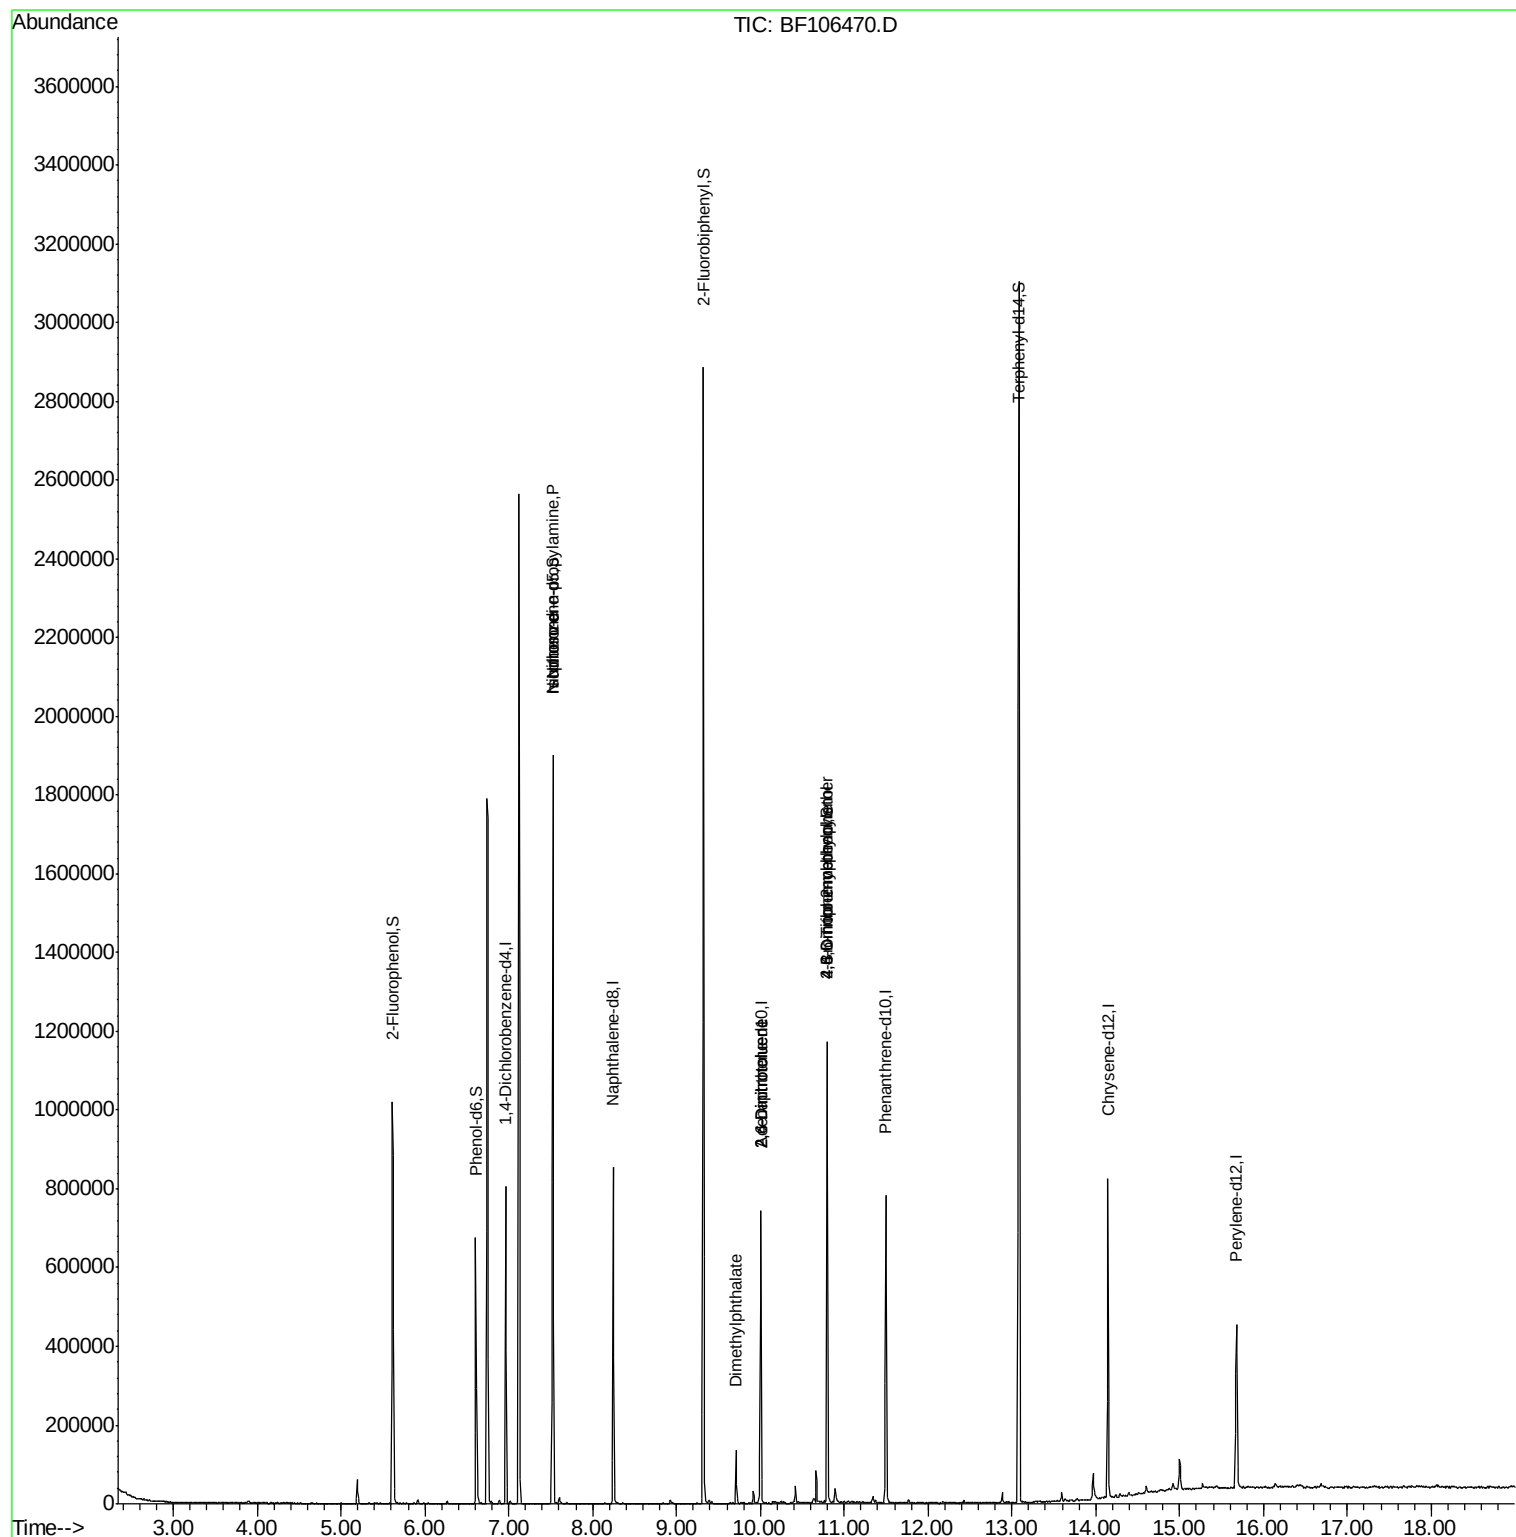

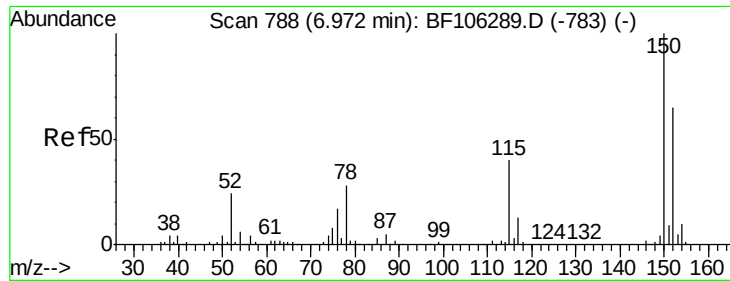


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 787
Delta R.T. -0.00 min
Lab File: BF106470.D
Acq: 15 Jun 2018 4:11

Instrument :
BNA_F
ClientSampleId :
061118-DBRI-E-D-S

Tgt Ion:152 Resp: 106669
Ion Ratio Lower Upper
152 100
150 159.5 124.6 186.8
115 60.3 50.1 75.1

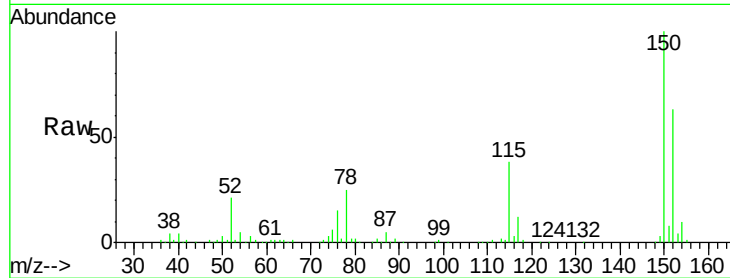


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

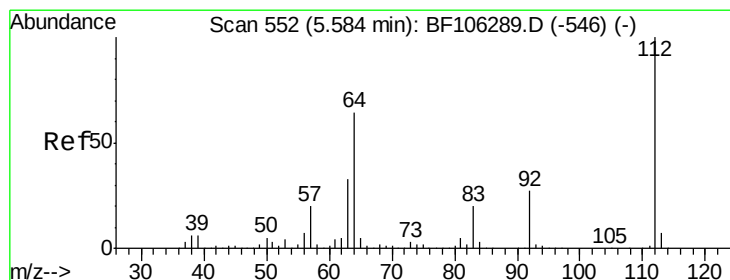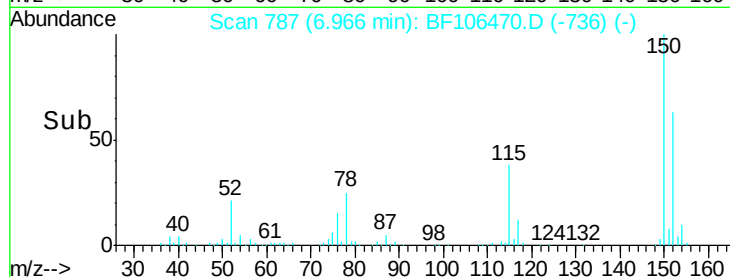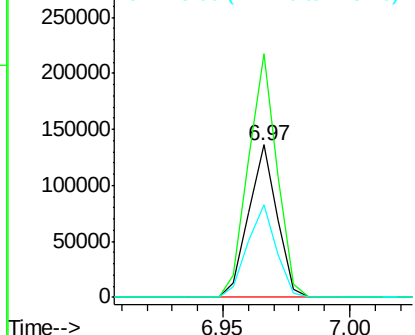



#5




2-Fluorophenol
Concen: 47.394 ng
RT: 5.61 min Scan# 557
Delta R.T. -0.00 min
Lab File: BF106470.D
Acq: 15 Jun 2018 4:11

Tgt Ion:112 Resp: 298701
Ion Ratio Lower Upper
112 100
64 64.0 47.9 71.9
63 31.4 23.7 35.5

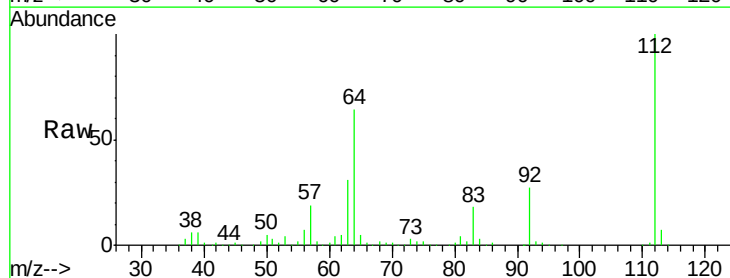

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

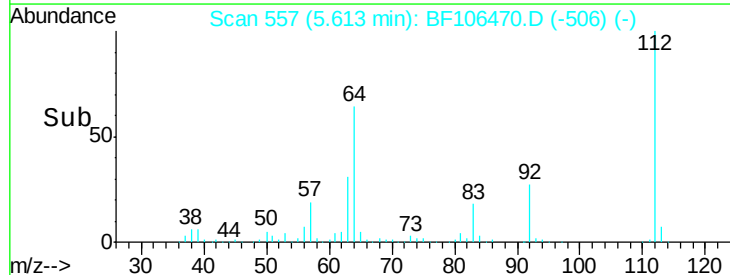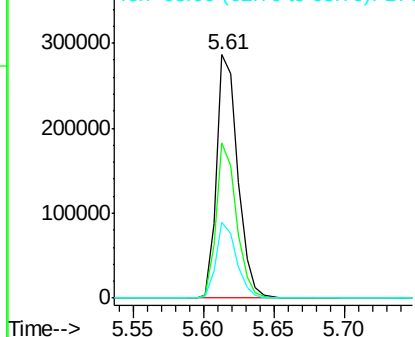

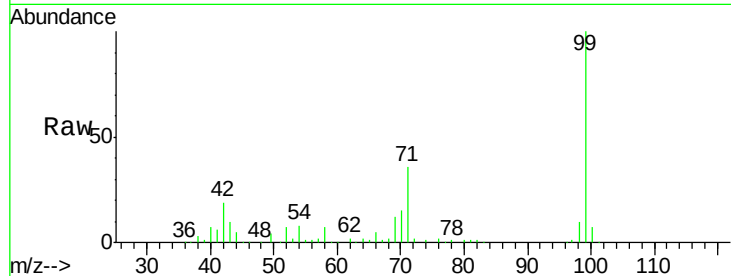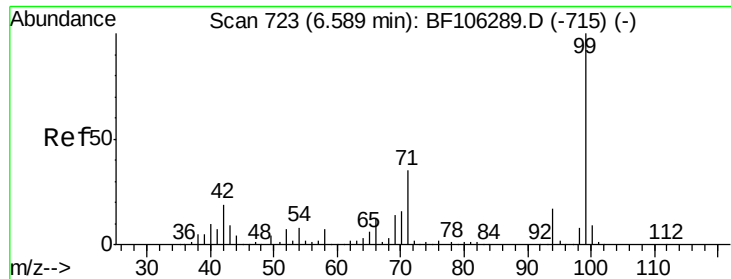

#7

Phenol-d6

Concen: 29.183 ng

RT: 6.61 min Scan# 726

Delta R.T. -0.01 min

Lab File: BF106470.D

Acq: 15 Jun 2018 4:11

Instrument :

BNA_F

ClientSampleId :

061118-DBRI-E-D-S





Tgt Ion: 99 Resp: 232371

Ion Ratio Lower Upper

99 100

42 19.0 14.5 21.7

71 35.6 25.4 38.0

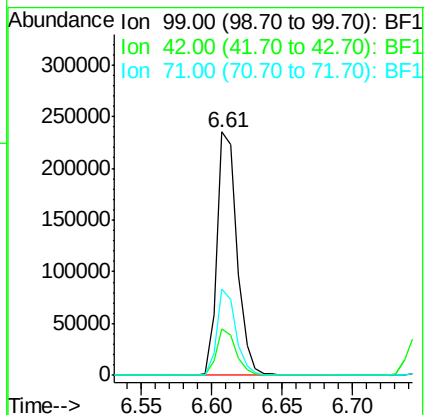

#19

n-Nitroso-di-n-propylamine

Concen: 14.034 ng

RT: 7.53 min Scan# 883

Delta R.T. 0.15 min

Lab File: BF106470.D

Acq: 15 Jun 2018 4:11

Tgt Ion: 70 Resp: 83837


Ion Ratio Lower Upper


70 100

42 44.0 47.5 71.3#

101 0.0 7.4 11.2#

130 2.1 16.6 25.0#

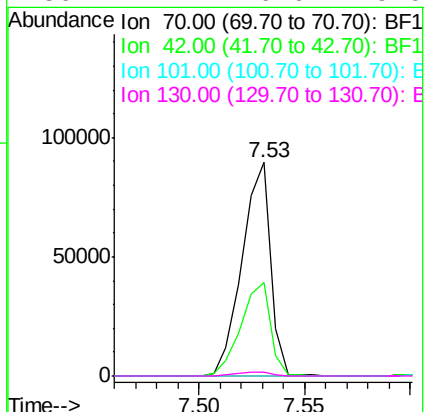


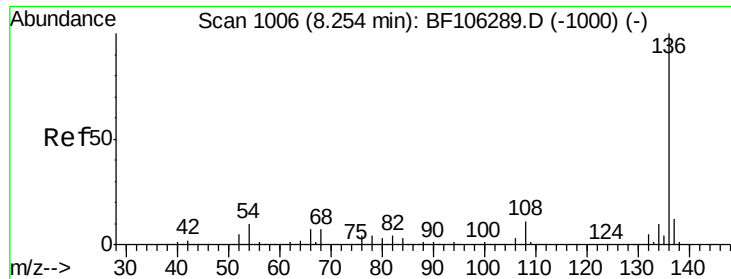




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.25 min Scan# 1005
Delta R.T. -0.01 min
Lab File: BF106470.D
Acq: 15 Jun 2018 4:11

Instrument :
BNA_F
ClientSampleId :
061118-DBRI-E-D-S

Tgt Ion: 136 Resp: 346779
Ion Ratio Lower Upper
136 100
137 10.8 8.9 13.3
54 8.4 6.6 9.8
68 6.5 5.0 7.4




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

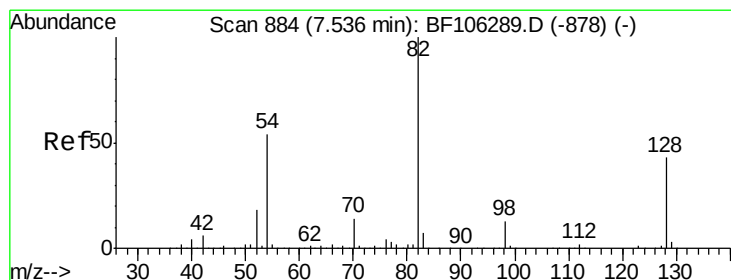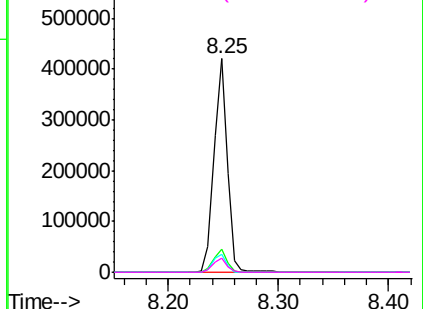




#23
Nitrobenzene-d5
Concen: 106.011 ng
RT: 7.53 min Scan# 883
Delta R.T. -0.01 min
Lab File: BF106470.D
Acq: 15 Jun 2018 4:11

Tgt Ion: 82 Resp: 624910
Ion Ratio Lower Upper
82 100
128 44.8 36.1 54.1
54 49.5 41.4 62.2



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

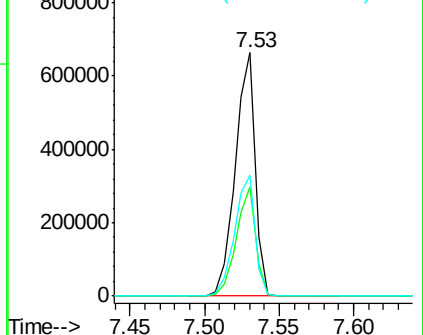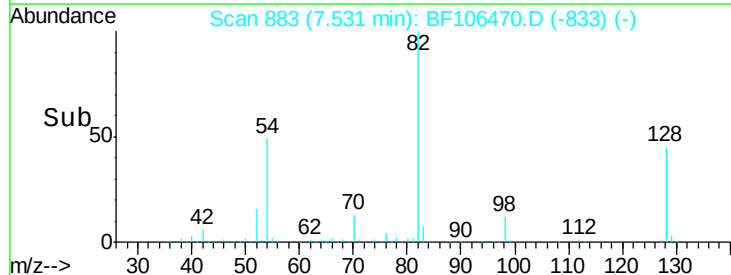

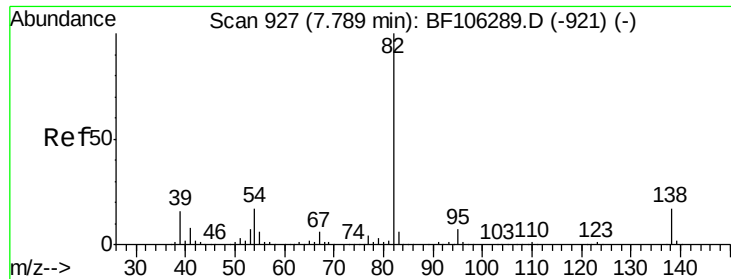

#25

Isophorone

Concen: 54.274 ng

RT: 7.53 min Scan# 883

Delta R.T. -0.26 min

Lab File: BF106470.D

Acq: 15 Jun 2018 4:11

Instrument :

BNA_F

ClientSampleId :

061118-DBRI-E-D-S


Tgt Ion: 82 Resp: 624904

Ion Ratio Lower Upper

82 100

95 0.0 5.2 7.8#




138 0.0 14.9 22.3#

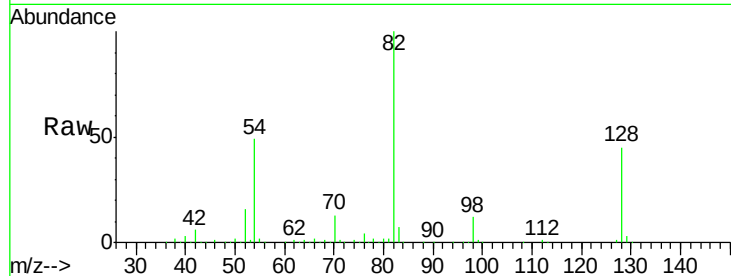

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

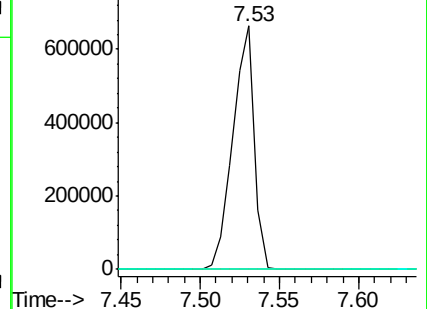

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.01 min Scan# 1304

Delta R.T. -0.01 min

Lab File: BF106470.D

Acq: 15 Jun 2018 4:11


Tgt Ion: 164 Resp: 134802

Ion Ratio Lower Upper

164 100

162 103.7 86.1 129.1



160 47.2 38.3 57.5




Abundance Ion 164.00 (163.70 to 164.70): BF1

Ion 162.00 (161.70 to 162.70): BF1

Ion 160.00 (159.70 to 160.70): BF1

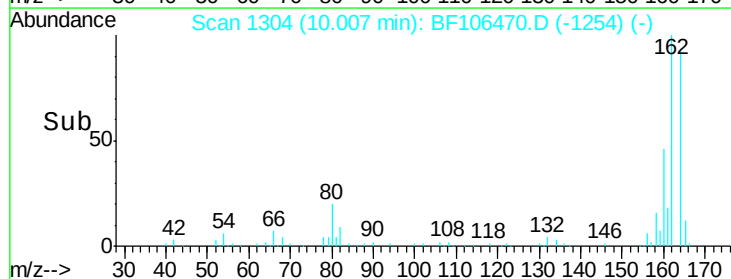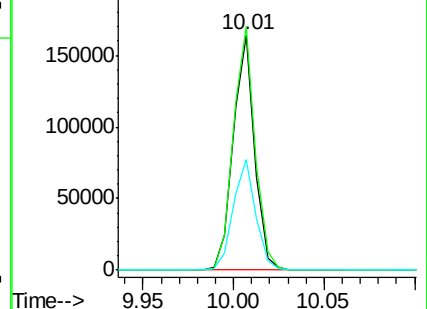







#41
 2,4,6-Tribromophenol
 Concen: 111.130 ng
 RT: 10.80 min Scan# 1439
 Delta R.T. -0.01 min
 Lab File: BF106470.D
 Acq: 15 Jun 2018 4:11

Instrument :
 BNA_F
 ClientSampleId :
 061118-DBRI-E-D-S

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.8	77.0	115.6
141	28.5	29.9	44.9#

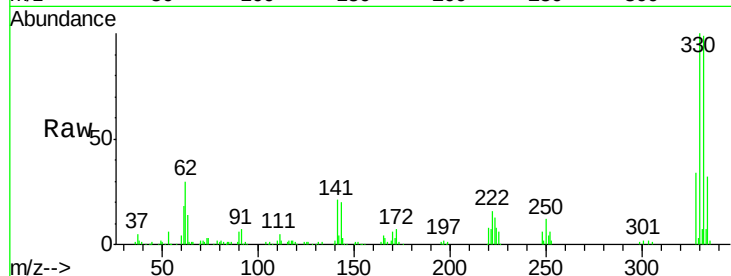


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


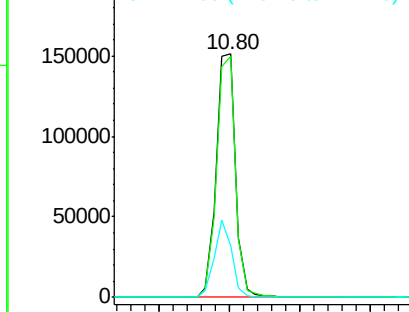



#44
 2-Fluorobiphenyl
 Concen: 171.166 ng
 RT: 9.32 min Scan# 1188
 Delta R.T. -0.00 min
 Lab File: BF106470.D
 Acq: 15 Jun 2018 4:11

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.0	29.7	44.5
170	25.3	19.6	29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

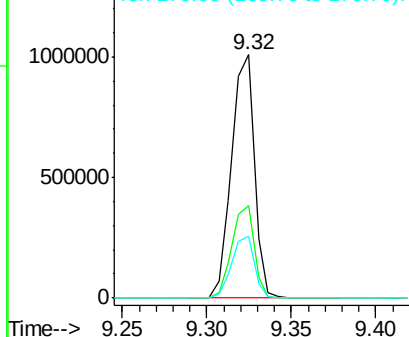

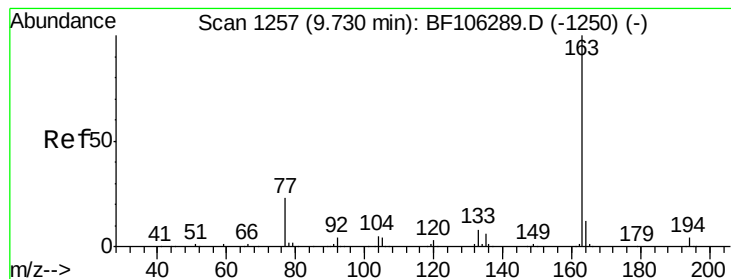

#49

Dimethylphthalate

Concen: 5.365 ng

RT: 9.71 min Scan# 1254

Delta R.T. -0.01 min

Lab File: BF106470.D

Acq: 15 Jun 2018 4:11

Instrument :

BNA_F

ClientSampleId :

061118-DBRI-E-D-S


Tgt Ion:163 Resp: 51670

Ion Ratio Lower Upper

163 100

194 4.2 2.7 4.1#




164 10.3 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

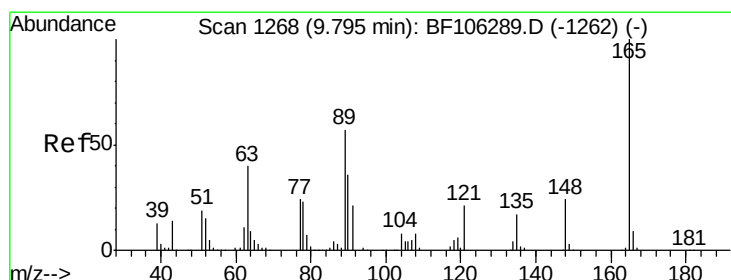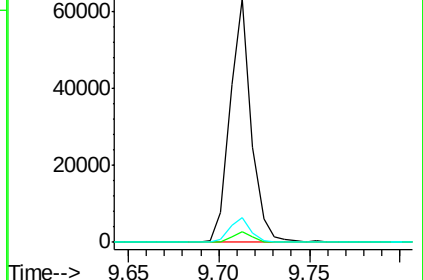

#50

2,6-Dinitrotoluene

Concen: 8.604 ng

RT: 10.01 min Scan# 1304

Delta R.T. 0.21 min

Lab File: BF106470.D

Acq: 15 Jun 2018 4:11


Tgt Ion:165 Resp: 16926

Ion Ratio Lower Upper

165 100

63 0.0 44.7 67.1#



89 0.0 44.0 66.0#




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

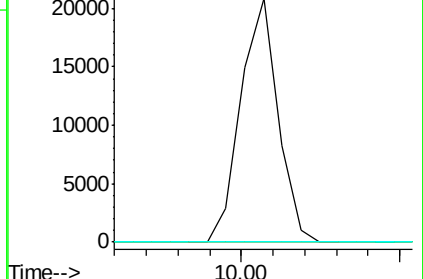




#56
 2,4-Dinitrotoluene
 Concen: 6.851 ng
 RT: 10.01 min Scan# 1304
 Delta R.T. -0.19 min
 Lab File: BF106470.D
 Acq: 15 Jun 2018 4:11

Instrument :
 BNA_F
 ClientSampleId :
 061118-DBRI-E-D-S

Tgt Ion:	165	Resp:	16926
Ion Ratio	Lower	Upper	
165	100		
63	0.0	36.4	54.6#
89	0.0	57.8	86.6#
182	0.0	1.6	2.4#



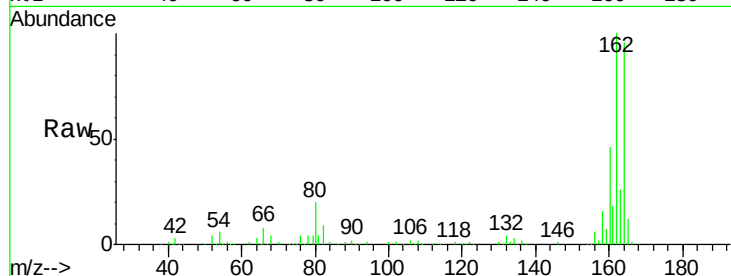


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1


Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

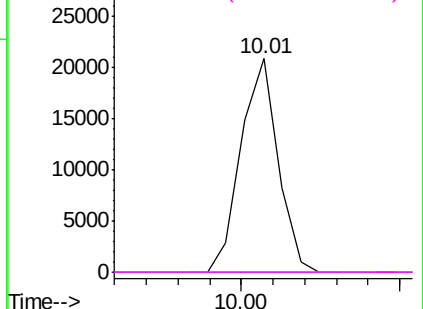

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.50 min Scan# 1557
 Delta R.T. -0.01 min
 Lab File: BF106470.D
 Acq: 15 Jun 2018 4:11



Tgt Ion:	188	Resp:	268977
Ion Ratio	Lower	Upper	
188	100		
94	10.3	8.5	12.7
80	12.0	9.2	13.8




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

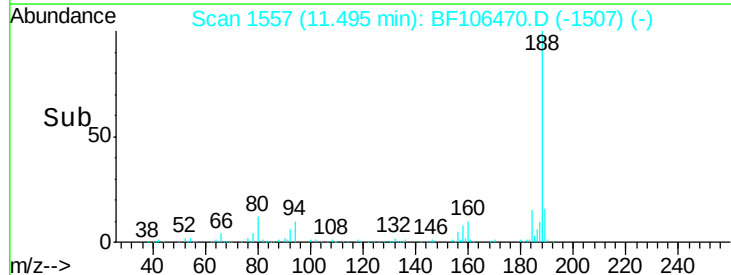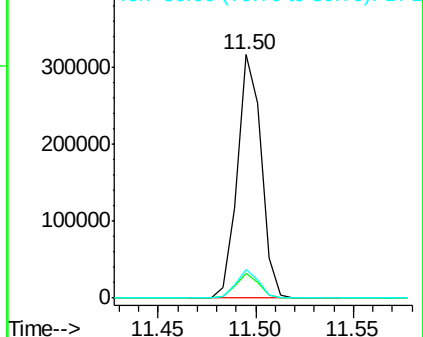


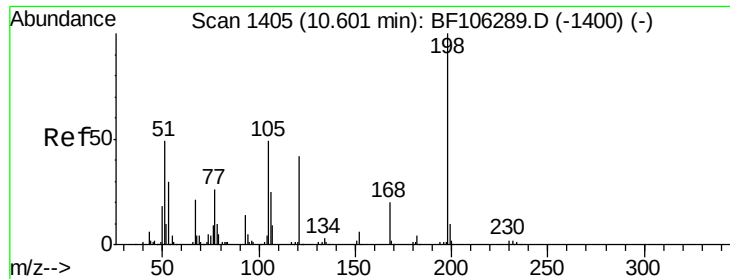




#64
 4,6-Dinitro-2-methylphenol
 Concen: 6.471 ng
 RT: 10.80 min Scan# 1438
 Delta R.T. 0.19 min
 Lab File: BF106470.D
 Acq: 15 Jun 2018 4:11

Instrument :
 BNA_F
 ClientSampleId :
 061118-DBRI-E-D-S

Tgt Ion:198 Resp: 294
 Ion Ratio Lower Upper
 198 100
 51 141.3 37.7 77.7#
 105 170.5 36.3 76.3#

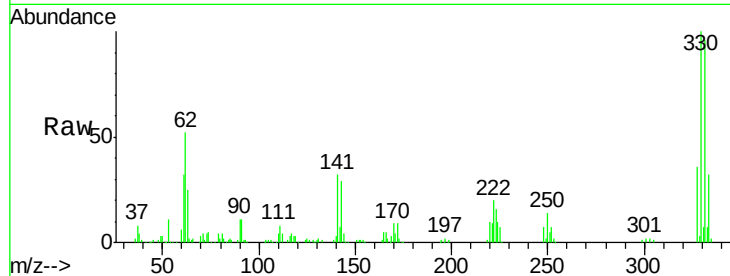


Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BF1
 Ion 105.00 (104.70 to 105.70): E

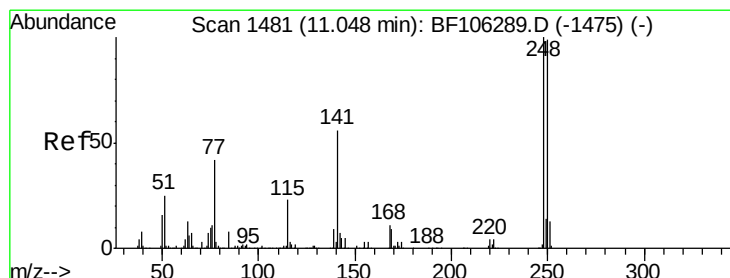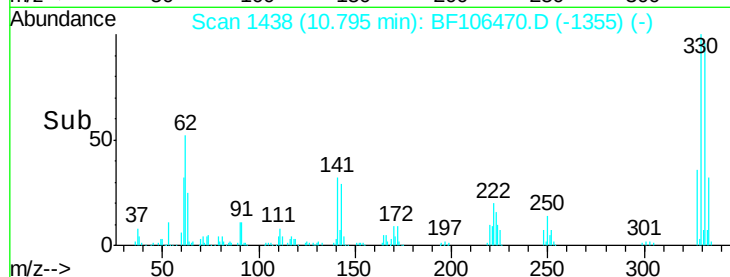
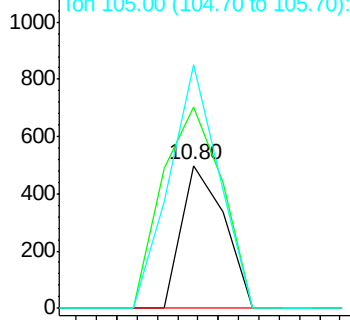



#66
 4-Bromophenyl-phenylether
 Concen: 3.137 ng
 RT: 10.80 min Scan# 1438
 Delta R.T. -0.25 min
 Lab File: BF106470.D
 Acq: 15 Jun 2018 4:11

Tgt Ion:248 Resp: 9598
 Ion Ratio Lower Upper
 248 100
 250 192.4 76.9 115.3#
 141 446.2 74.4 111.6#

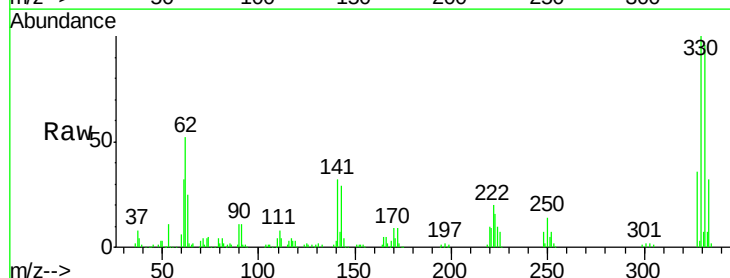

Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

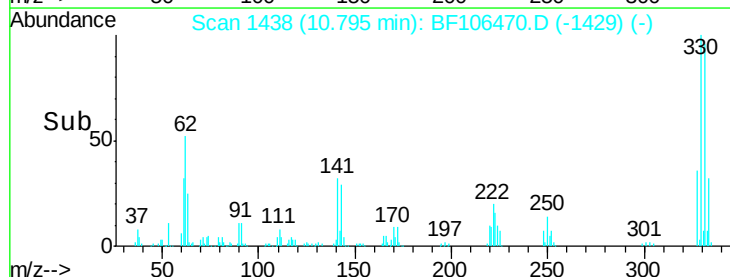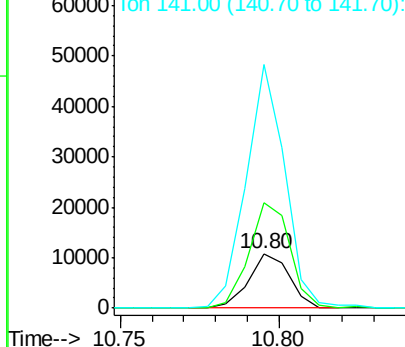



#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.15 min Scan# 2008

Delta R.T. -0.01 min

Lab File: BF106470.D

Acq: 15 Jun 2018 4:11

Instrument :

BNA_F

ClientSampleId :

061118-DBRI-E-D-S


Tgt Ion:240 Resp: 284265

Ion Ratio Lower Upper

240 100

120 9.5 9.5 14.3#




236 26.1 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

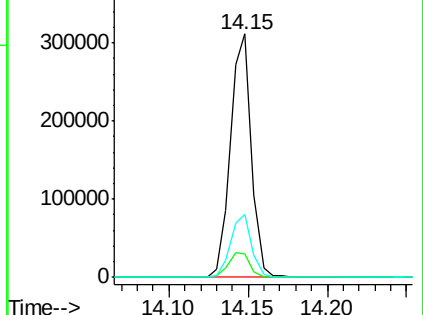

#78

Terphenyl-d14

Concen: 98.123 ng

RT: 13.08 min Scan# 1827

Delta R.T. -0.01 min

Lab File: BF106470.D

Acq: 15 Jun 2018 4:11


Tgt Ion:244 Resp: 1123006

Ion Ratio Lower Upper

244 100

212 7.2 5.4 8.0



122 10.3 11.0 16.4#






Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

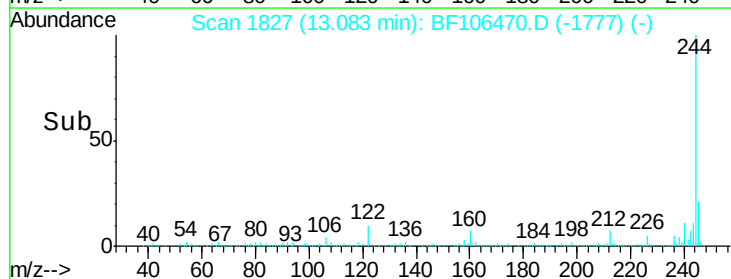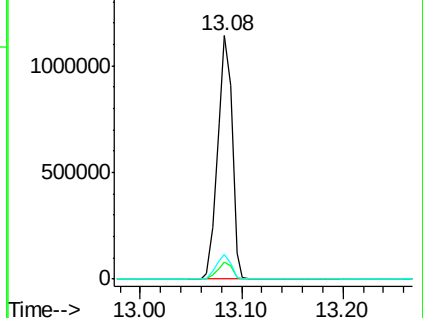

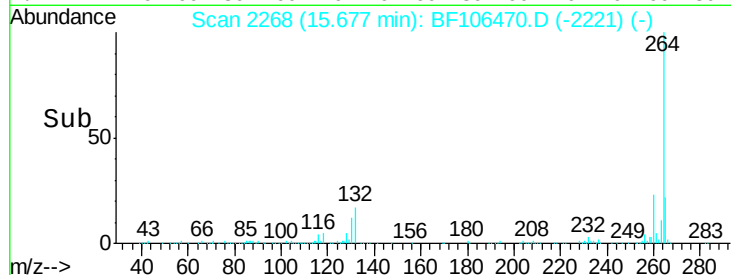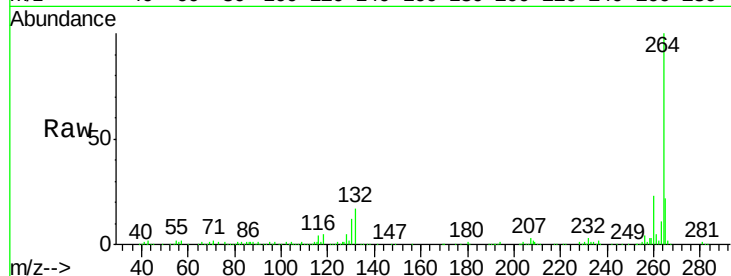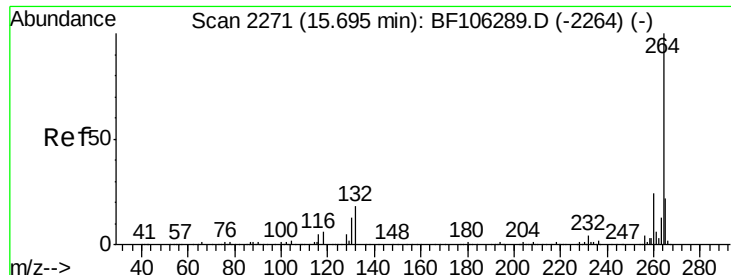

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.68 min Scan# 2268
Delta R.T. -0.02 min
Lab File: BF106470.D
Acq: 15 Jun 2018 4:11

Instrument :
BNA_F
ClientSampleId :
061118-DBRI-E-D-S

Tgt Ion:	264	Resp:	194890
Ion	Ratio	Lower	Upper
264	100		
260	23.1	19.2	28.8
265	21.8	17.5	26.3

