

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061418\
 Data File : BF106475.D
 Acq On : 15 Jun 2018 6:23
 Operator : JU/SJ
 Sample : J3475-02
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 061218-DBRI-F-D-M

Quant Time: Jun 15 08:27:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 14 18:39:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	111778	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	377286	20.00	ng	0.00
38) Acenaphthene-d10	10.01	164	148731	20.00	ng	0.00
63) Phenanthrene-d10	11.50	188	293679	20.00	ng	0.00
75) Chrysene-d12	14.15	240	309627	20.00	ng	-0.01
86) Perylene-d12	15.68	264	210884	20.00	ng	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.61	112	331173	50.14	ng	0.00
7) Phenol-d6	6.61	99	268472	32.18	ng	0.00
23) Nitrobenzene-d5	7.53	82	658553	102.69	ng	0.00
41) 2,4,6-Tribromophenol	10.80	330	157329	109.94	ng	0.00
44) 2-Fluorobiphenyl	9.32	172	1006301	153.34	ng	0.00
78) Terphenyl-d14	13.08	244	1167121	93.62	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
19) n-Nitroso-di-n-propylamine	7.53	70	88719	14.173	ng	# 74
25) Isophorone	7.53	82	658544	52.571	ng	# 64
49) Dimethylphthalate	9.71	163	107608	10.127	ng	100
56) 2,4-Dinitrotoluene	10.01	165	19384	7.112	ng	# 22
62) Azobenzene	10.72	77	52222	4.749	ng	# 1
64) 4,6-Dinitro-2-methylphenol	10.80	198	324	6.473	ng	# 1
66) 4-Bromophenyl-phenylether	10.80	248	10331	3.093	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061418\
Data File : BF106475.D
Acq On : 15 Jun 2018 6:23
Operator : JU/SJ
Sample : J3475-02
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
061218-DBRI-F-D-M

Quant Time: Jun 15 08:27:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 14 18:39:24 2018
Response via : Initial Calibration




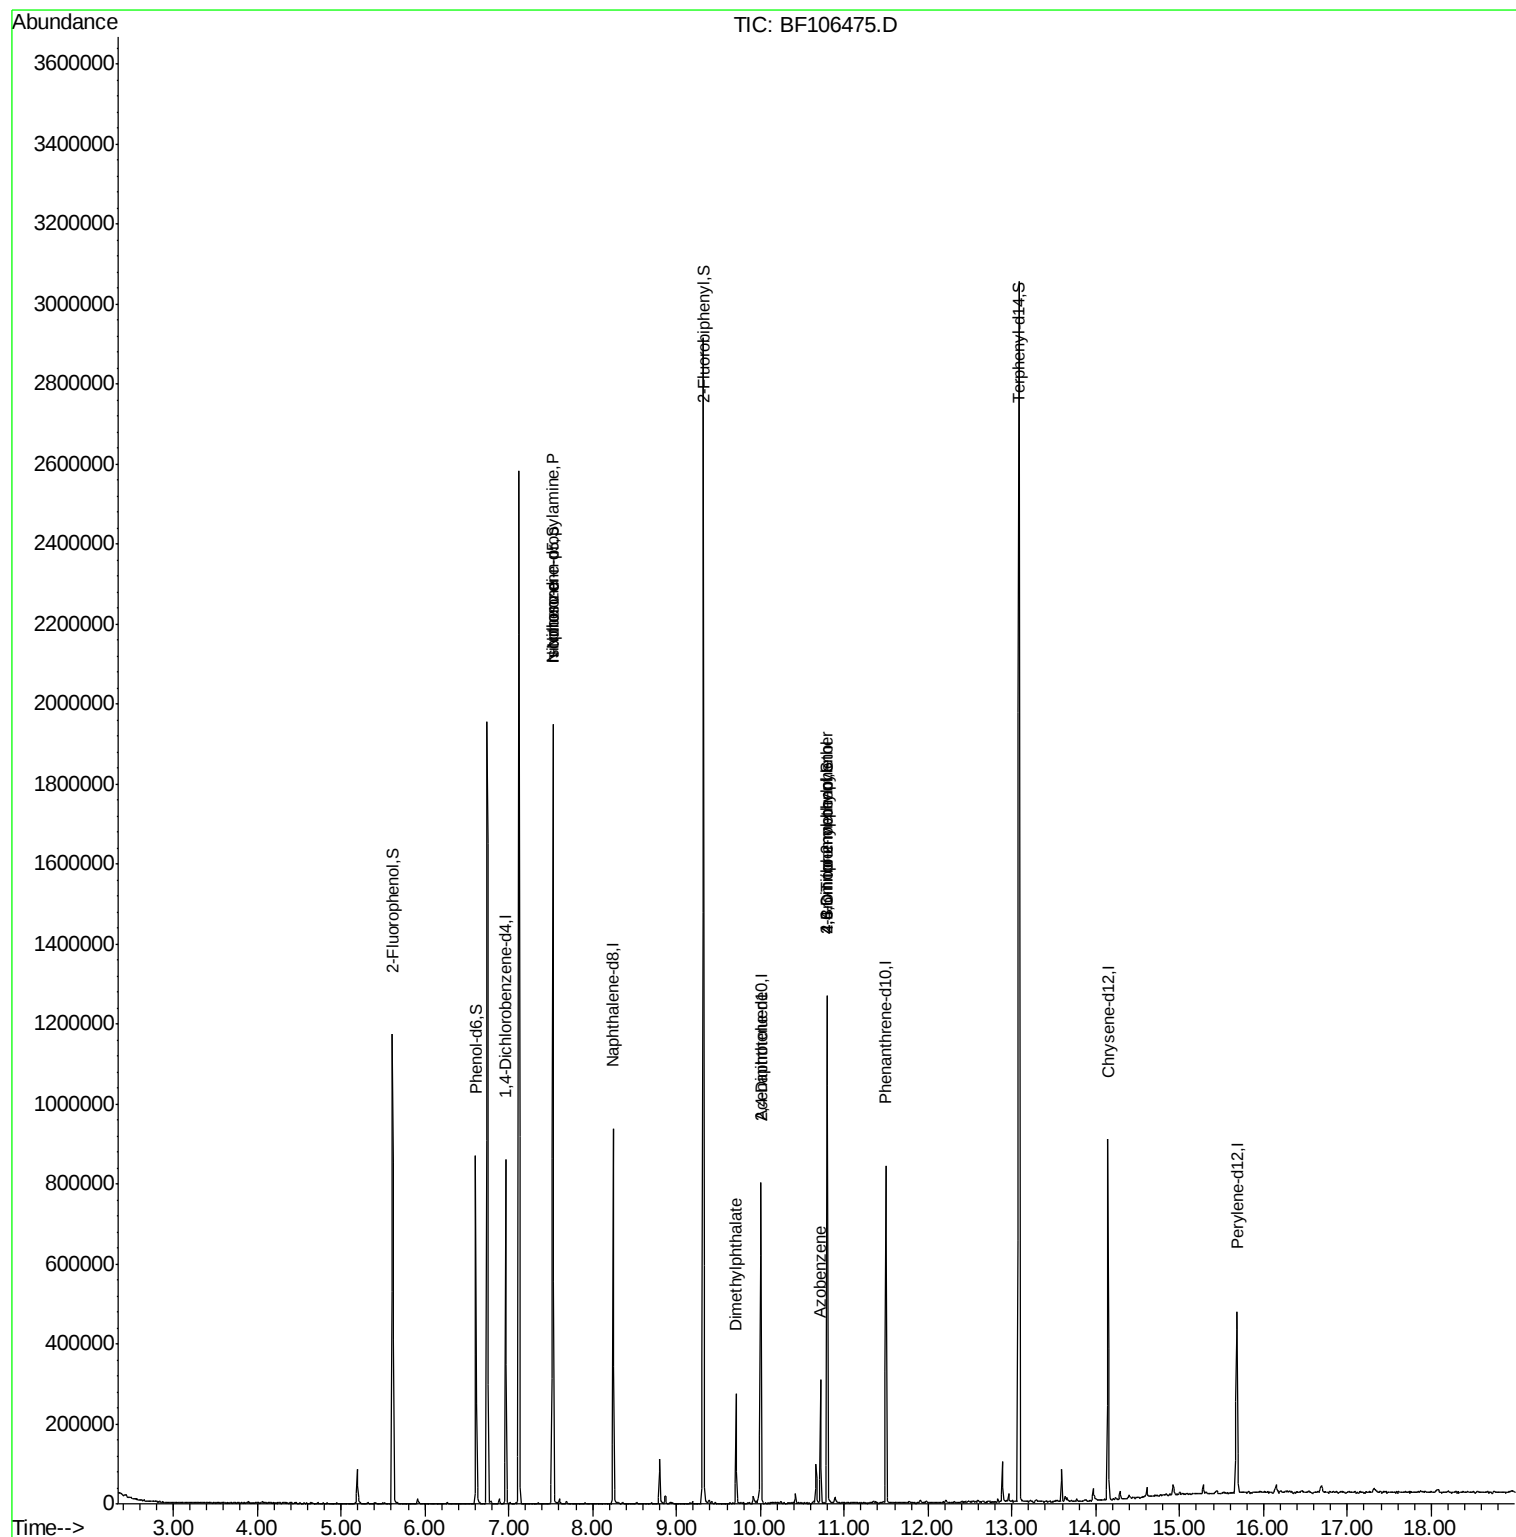




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.97 min Scan# 787
 Delta R.T. -0.00 min
 Lab File: BF106475.D
 Acq: 15 Jun 2018 6:23




Instrument :
 BNA_F
 ClientSampleId :
 061218-DBRI-F-D-M



Tgt Ion:152 Resp: 111778
 Ion Ratio Lower Upper
 152 100
 150 157.5 124.6 186.8
 115 61.4 50.1 75.1

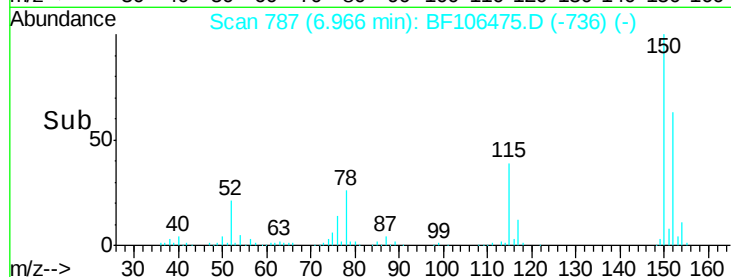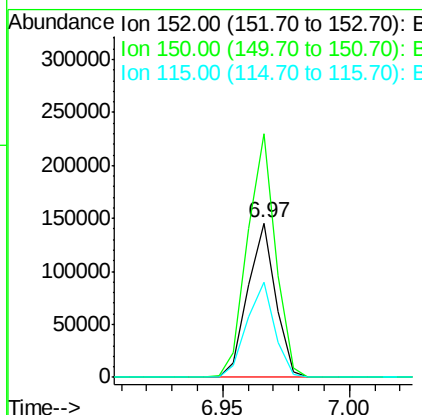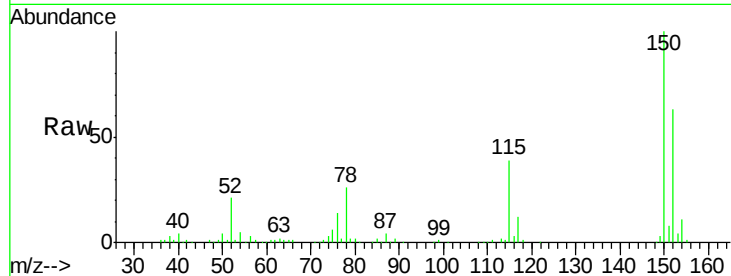

#5
 2-Fluorophenol
 Concen: 50.145 ng
 RT: 5.61 min Scan# 557
 Delta R.T. -0.00 min
 Lab File: BF106475.D
 Acq: 15 Jun 2018 6:23

Tgt Ion:112 Resp: 331173
 Ion Ratio Lower Upper
 112 100
 64 59.9 47.9 71.9
 63 30.4 23.7 35.5

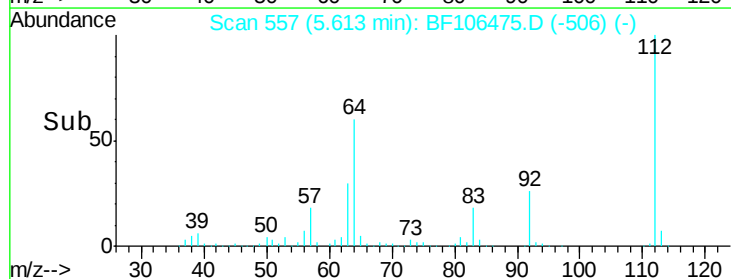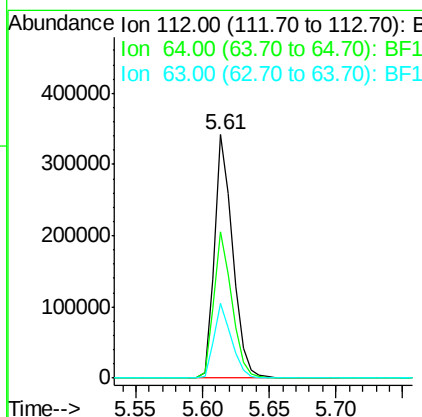

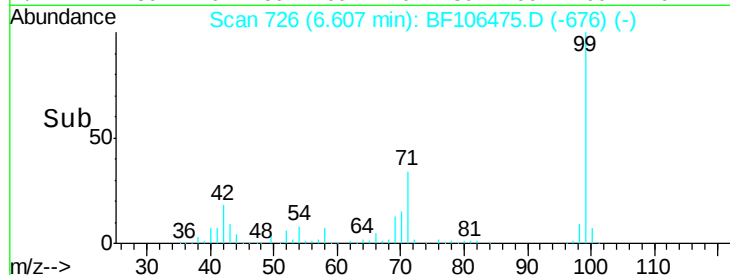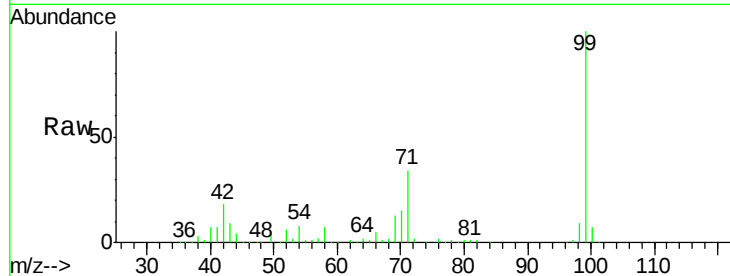

#7

Phenol-d6

Concen: 32.176 ng

RT: 6.61 min Scan# 726

Delta R.T. -0.01 min

Lab File: BF106475.D

Acq: 15 Jun 2018 6:23

Instrument :

BNA_F

ClientSampleId :

061218-DBRI-F-D-M





Tgt Ion: 99 Resp: 268472

Ion Ratio Lower Upper

99 100

42 18.3 14.5 21.7

71 34.5 25.4 38.0

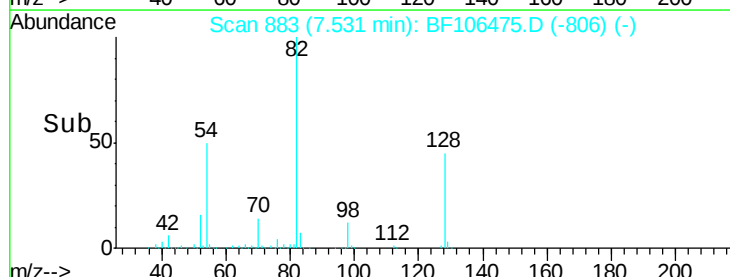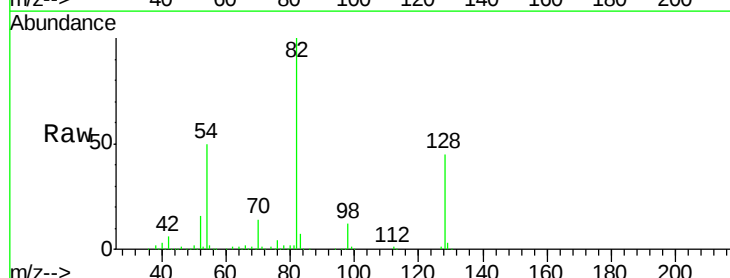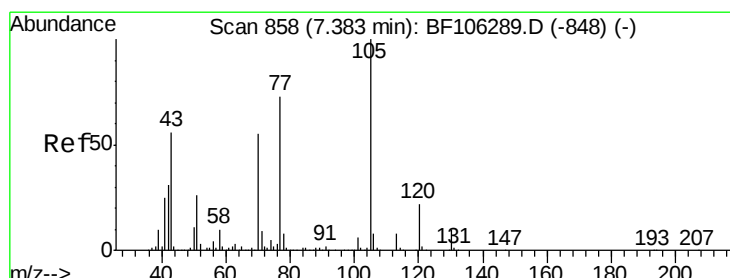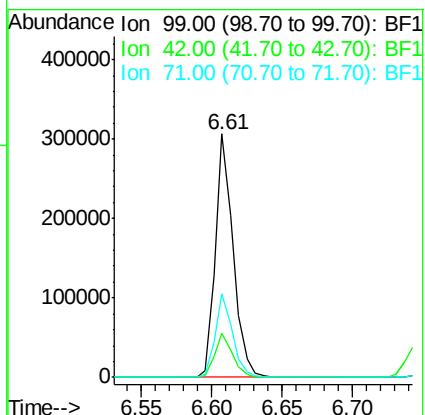

#19

n-Nitroso-di-n-propylamine

Concen: 14.173 ng

RT: 7.53 min Scan# 883

Delta R.T. 0.15 min

Lab File: BF106475.D

Acq: 15 Jun 2018 6:23

Tgt Ion: 70 Resp: 88719


Ion Ratio Lower Upper


70 100

42 43.1 47.5 71.3#

101 0.0 7.4 11.2#

130 2.0 16.6 25.0#

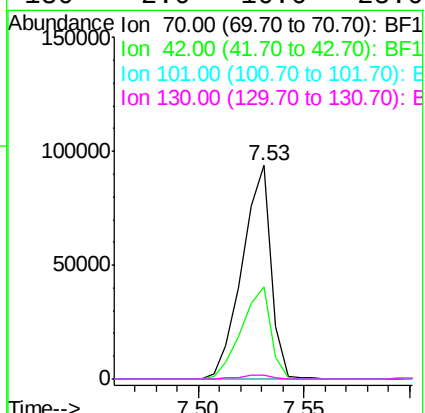


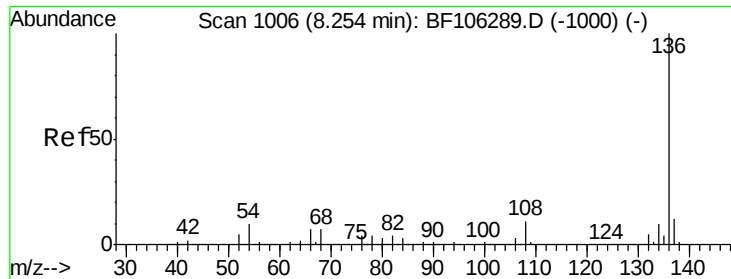




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.25 min Scan# 1005
Delta R.T. -0.01 min
Lab File: BF106475.D
Acq: 15 Jun 2018 6:23

Instrument :
BNA_F
ClientSampleId :
061218-DBRI-F-D-M

Tgt Ion:	136	Resp:	377286
Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.9	13.3
54	8.0	6.6	9.8
68	6.3	5.0	7.4




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

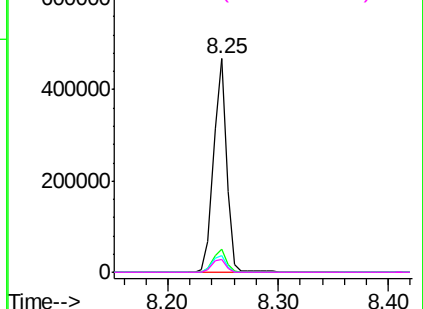
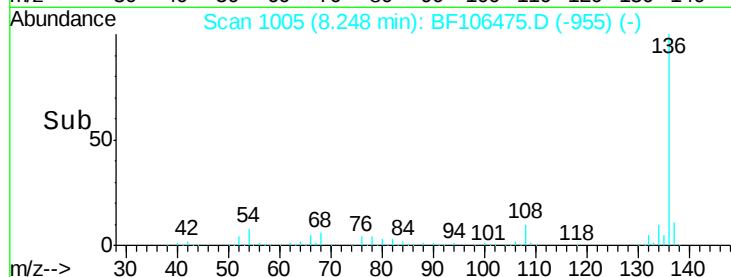



#23
Nitrobenzene-d5
Concen: 102.685 ng
RT: 7.53 min Scan# 883
Delta R.T. -0.01 min
Lab File: BF106475.D
Acq: 15 Jun 2018 6:23

Tgt Ion:	82	Resp:	658553
Ion	Ratio	Lower	Upper
82	100		
128	44.6	36.1	54.1
54	49.9	41.4	62.2



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

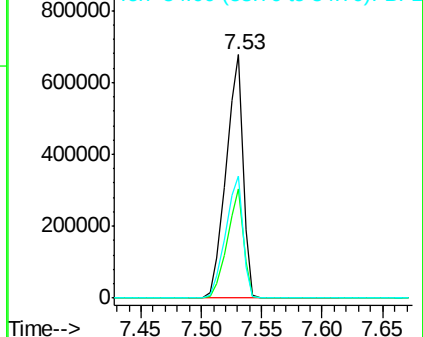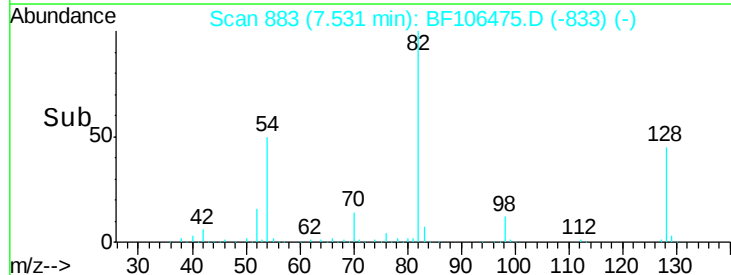

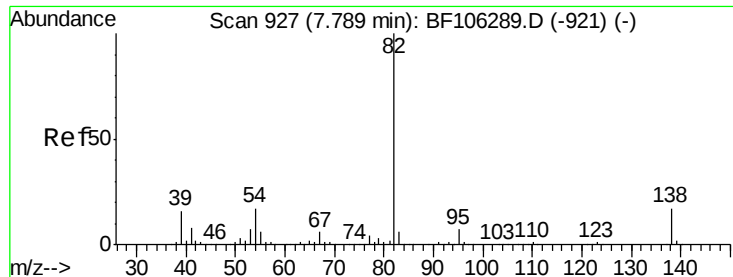

#25

Isophorone

Concen: 52.571 ng

RT: 7.53 min Scan# 883

Delta R.T. -0.26 min

Lab File: BF106475.D

Acq: 15 Jun 2018 6:23

Instrument :

BNA_F

ClientSampleId :

061218-DBRI-F-D-M


Tgt Ion: 82 Resp: 658544

Ion Ratio Lower Upper

82 100

95 0.0 5.2 7.8#




138 0.0 14.9 22.3#

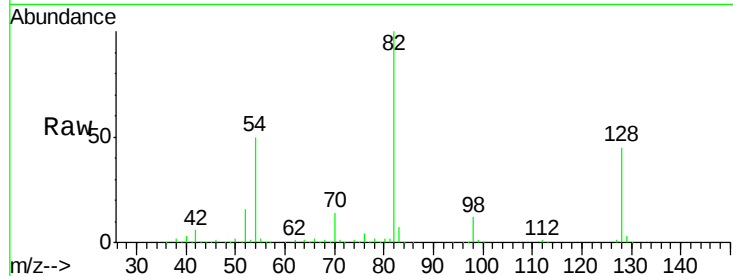

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

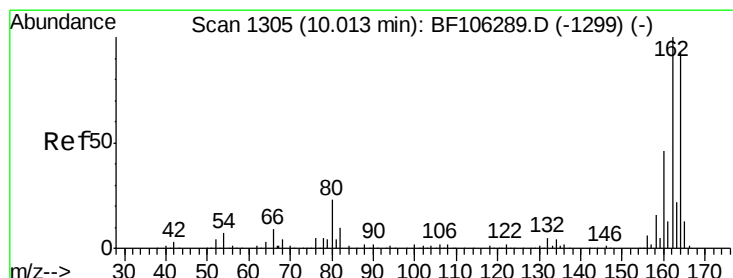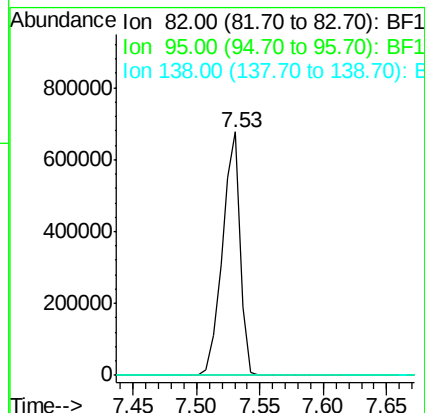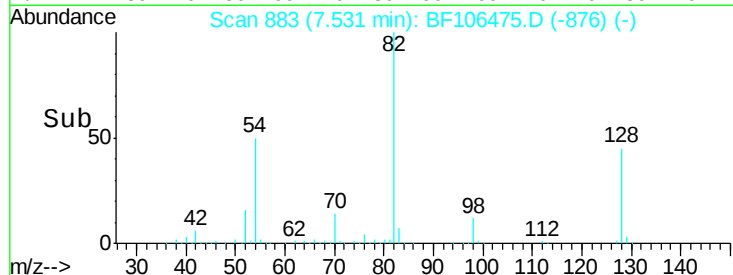

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.01 min Scan# 1304

Delta R.T. -0.01 min

Lab File: BF106475.D

Acq: 15 Jun 2018 6:23


Tgt Ion: 164 Resp: 148731

Ion Ratio Lower Upper

164 100

162 105.5 86.1 129.1



160 47.8 38.3 57.5

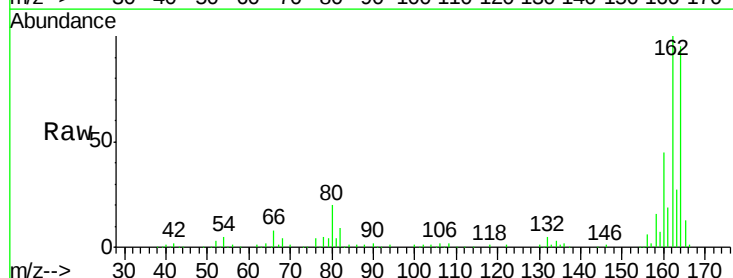


Abundance Ion 164.00 (163.70 to 164.70): BF1

Ion 162.00 (161.70 to 162.70): BF1

Ion 160.00 (159.70 to 160.70): BF1



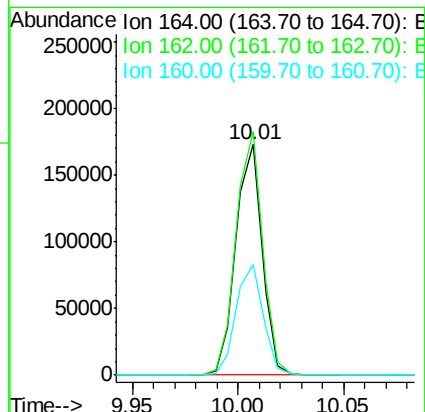
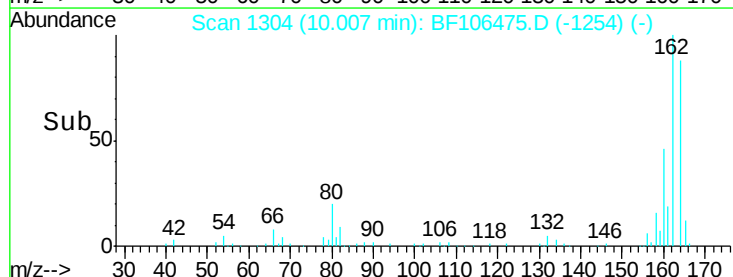


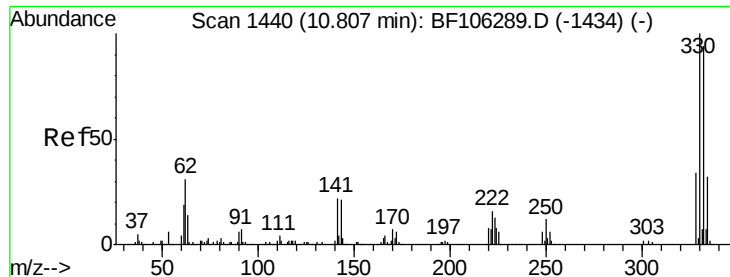

#41
 2,4,6-Tribromophenol
 Concen: 109.940 ng
 RT: 10.80 min Scan# 1439
 Delta R.T. -0.01 min
 Lab File: BF106475.D
 Acq: 15 Jun 2018 6:23




Instrument :
 BNA_F
 ClientSampleId :
 061218-DBRI-F-D-M


Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.7	77.0	115.6
141	28.7	29.9	44.9#

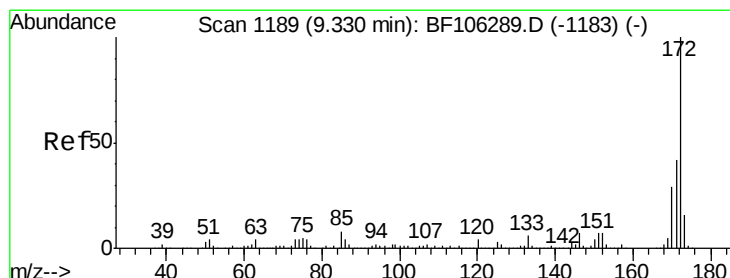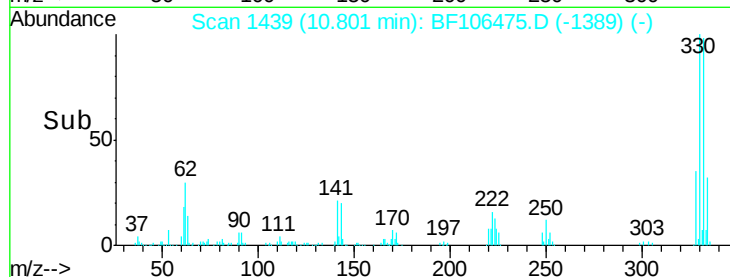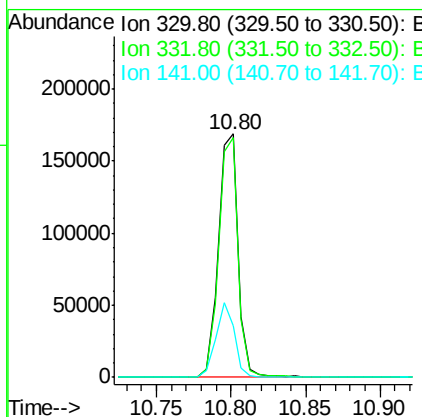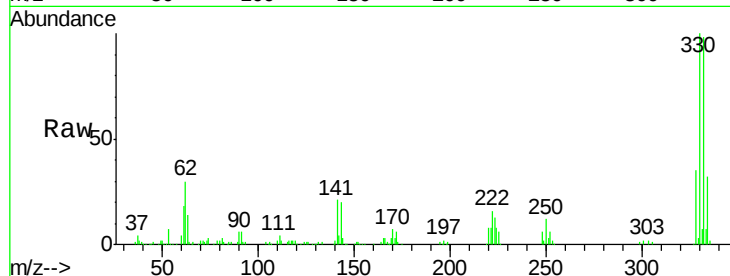

#44
 2-Fluorobiphenyl
 Concen: 153.336 ng
 RT: 9.32 min Scan# 1188
 Delta R.T. 0.00 min
 Lab File: BF106475.D
 Acq: 15 Jun 2018 6:23

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.8	29.7	44.5
170	25.7	19.6	29.4

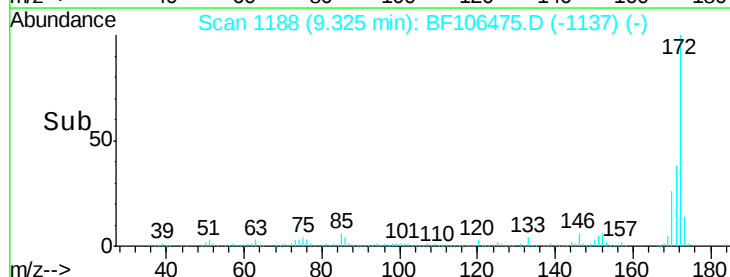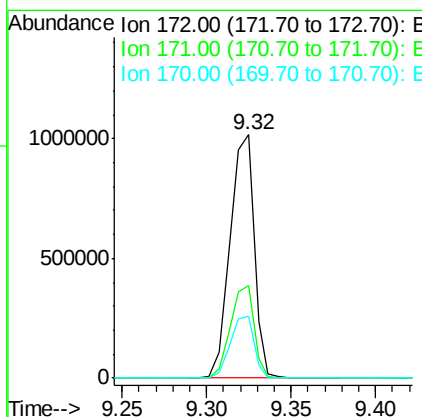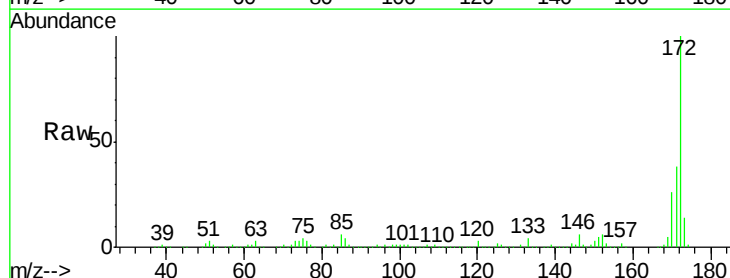

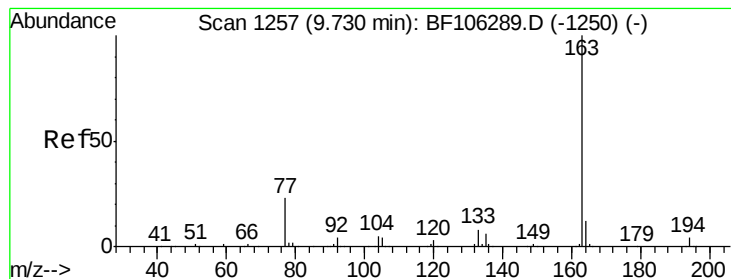

#49

Dimethylphthalate

Concen: 10.127 ng

RT: 9.71 min Scan# 1254

Delta R.T. -0.01 min

Lab File: BF106475.D

Acq: 15 Jun 2018 6:23

Instrument :

BNA_F

ClientSampleId :

061218-DBRI-F-D-M


Tgt Ion:163 Resp: 107608

Ion Ratio Lower Upper

163 100

194 3.9 2.7 4.1




164 10.2 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

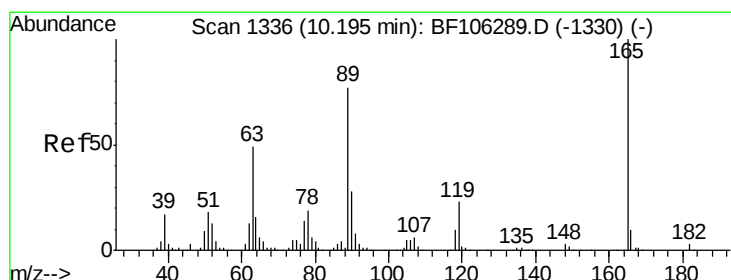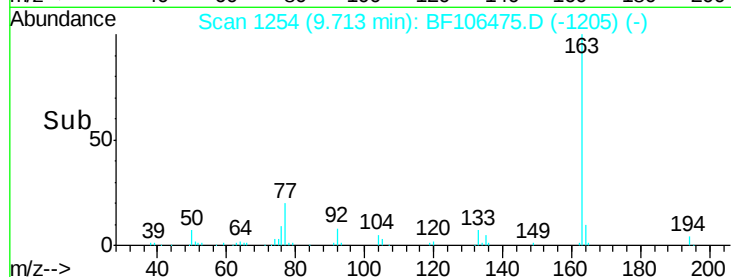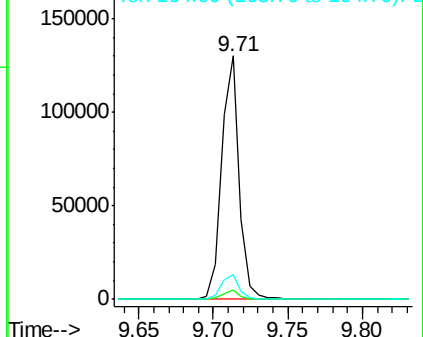

#56

2,4-Dinitrotoluene

Concen: 7.112 ng

RT: 10.01 min Scan# 1304

Delta R.T. -0.19 min

Lab File: BF106475.D

Acq: 15 Jun 2018 6:23

Tgt Ion:165 Resp: 19384


Ion Ratio Lower Upper

165 100

63 1.4 36.4 54.6#

89 0.0 57.8 86.6#

182 0.0 1.6 2.4#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E



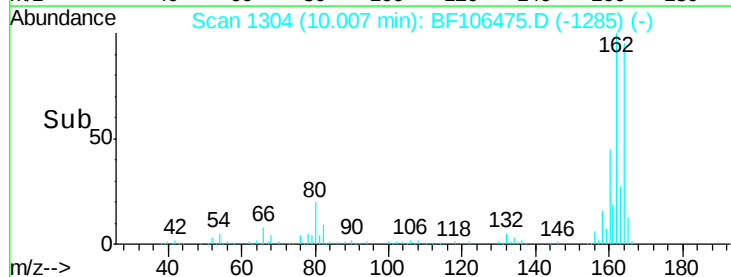
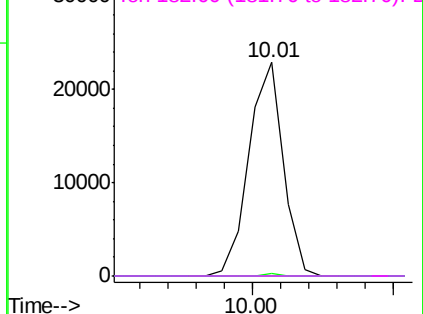


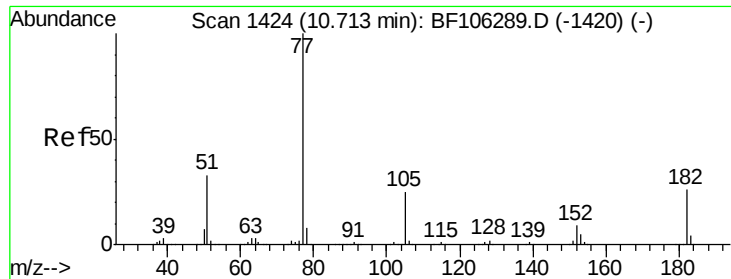

#62
Azobenzene
Concen: 4.749 ng
RT: 10.72 min Scan# 1425
Delta R.T. 0.01 min
Lab File: BF106475.D
Acq: 15 Jun 2018 6:23




Instrument :
BNA_F
ClientSampleId :
061218-DBRI-F-D-M


Tgt Ion: 77 Resp: 52222
Ion Ratio Lower Upper
77 100
182 88.9 1.7 41.7#
105 160.5 3.0 43.0#
51 37.4 9.9 49.9

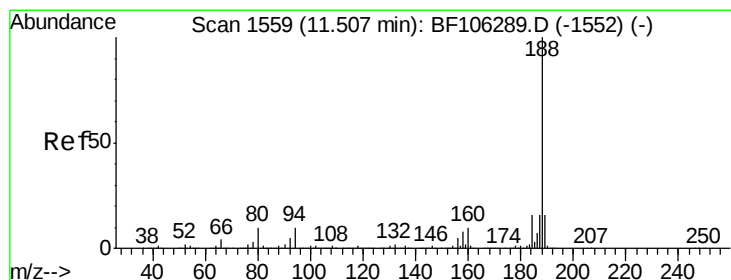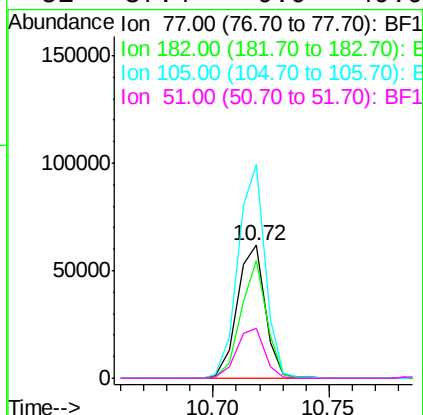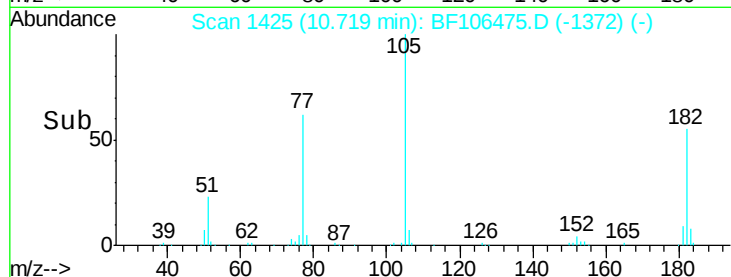

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.50 min Scan# 1557
Delta R.T. -0.01 min
Lab File: BF106475.D
Acq: 15 Jun 2018 6:23

Tgt Ion: 188 Resp: 293679
Ion Ratio Lower Upper
188 100
94 10.7 8.5 12.7
80 11.8 9.2 13.8

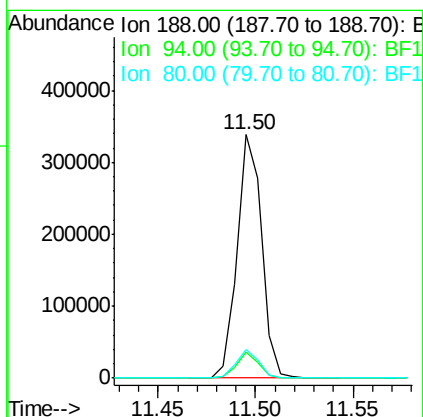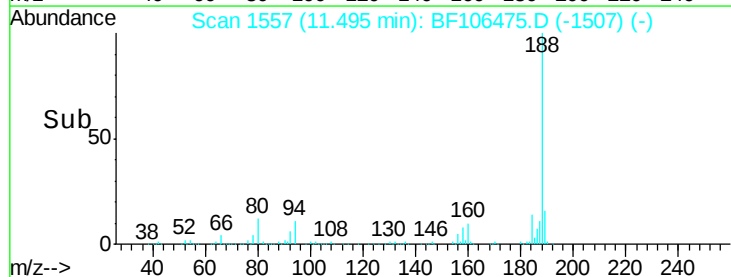


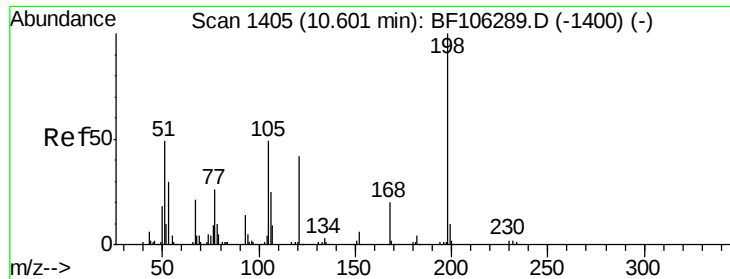




#64
 4,6-Dinitro-2-methylphenol
 Concen: 6.473 ng
 RT: 10.80 min Scan# 1438
 Delta R.T. 0.19 min
 Lab File: BF106475.D
 Acq: 15 Jun 2018 6:23

Instrument :
 BNA_F
 ClientSampleId :
 061218-DBRI-F-D-M

Tgt Ion:198 Resp: 324
 Ion Ratio Lower Upper
 198 100
 51 138.7 37.7 77.7#
 105 180.9 36.3 76.3#

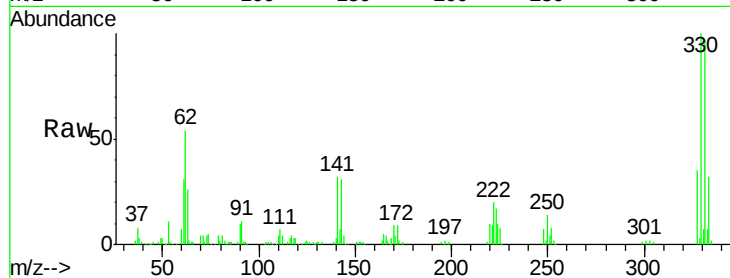


Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BF1
 Ion 105.00 (104.70 to 105.70): E

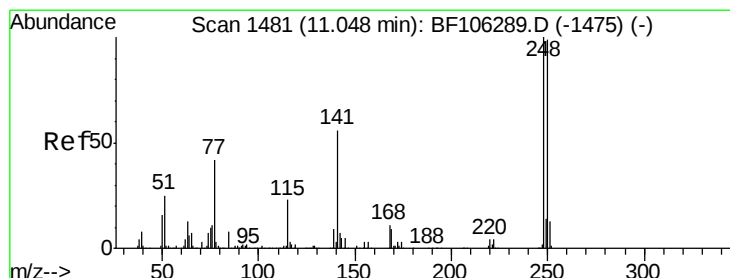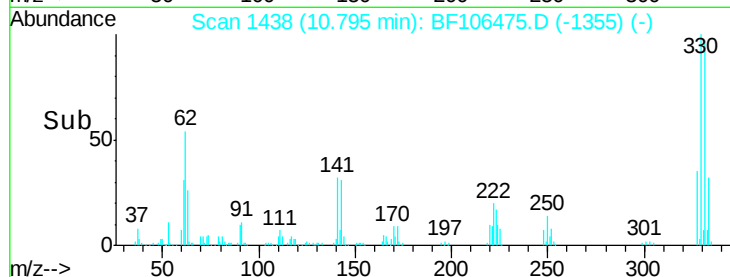
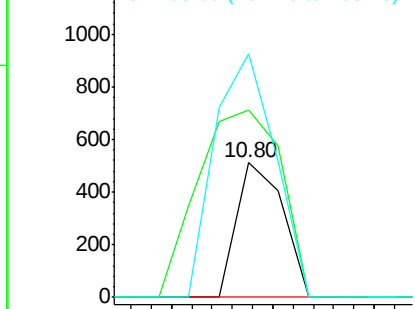



#66
 4-Bromophenyl-phenylether
 Concen: 3.093 ng
 RT: 10.80 min Scan# 1438
 Delta R.T. -0.25 min
 Lab File: BF106475.D
 Acq: 15 Jun 2018 6:23

Tgt Ion:248 Resp: 10331
 Ion Ratio Lower Upper
 248 100
 250 189.8 76.9 115.3#
 141 437.1 74.4 111.6#

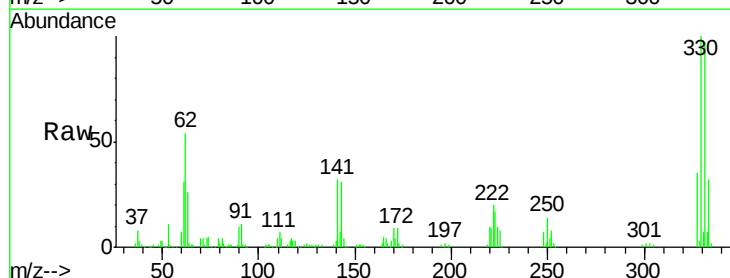

Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

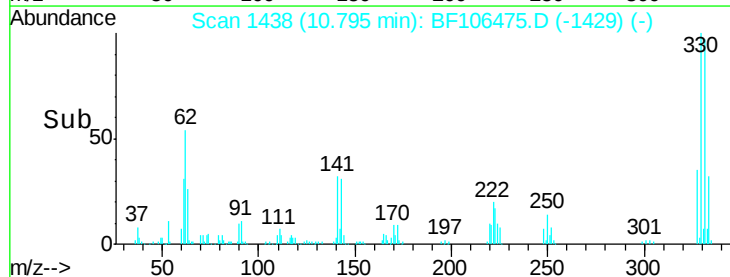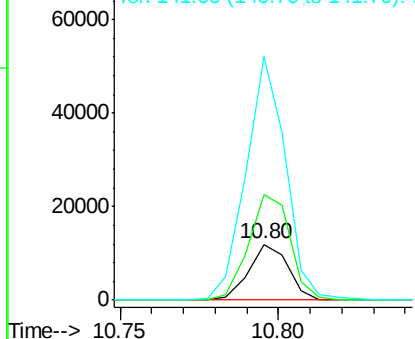

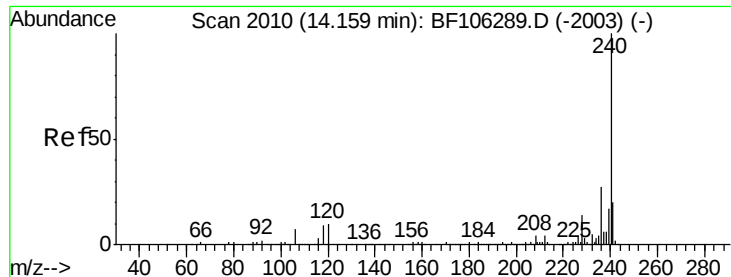

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.15 min Scan# 2008

Delta R.T. -0.01 min

Lab File: BF106475.D

Acq: 15 Jun 2018 6:23

Instrument :

BNA_F

ClientSampleId :

061218-DBRI-F-D-M


Tgt Ion:240 Resp: 309627

Ion Ratio Lower Upper

240 100

120 10.1 9.5 14.3




236 26.5 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

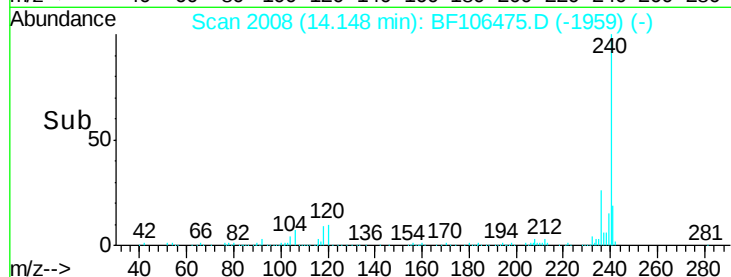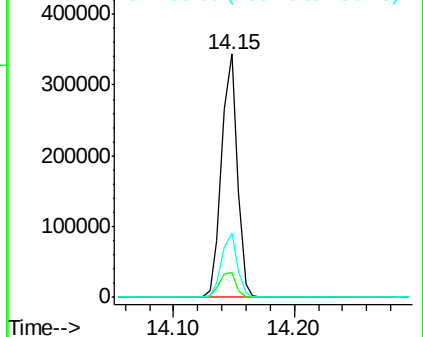

#78

Terphenyl-d14

Concen: 93.625 ng

RT: 13.08 min Scan# 1827

Delta R.T. -0.01 min

Lab File: BF106475.D

Acq: 15 Jun 2018 6:23


Tgt Ion:244 Resp: 1167121

Ion Ratio Lower Upper

244 100

212 7.3 5.4 8.0



122 11.2 11.0 16.4






Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

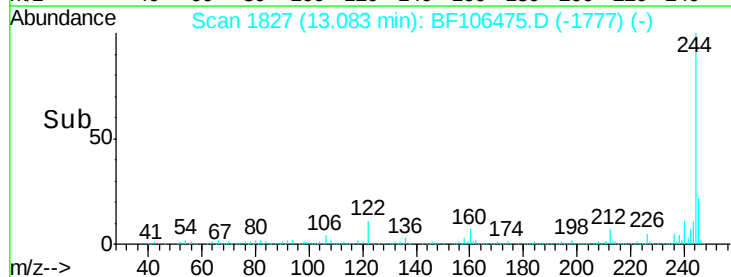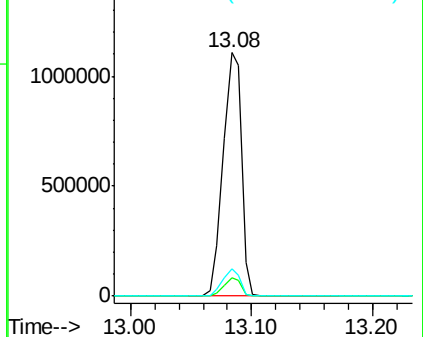

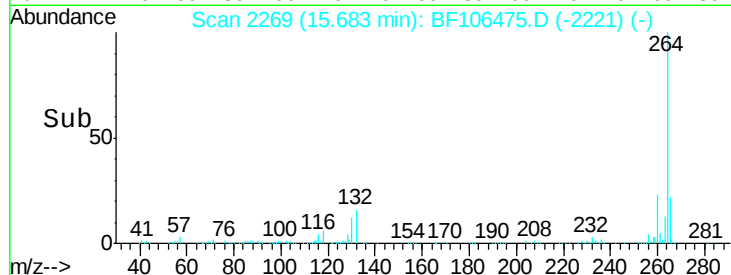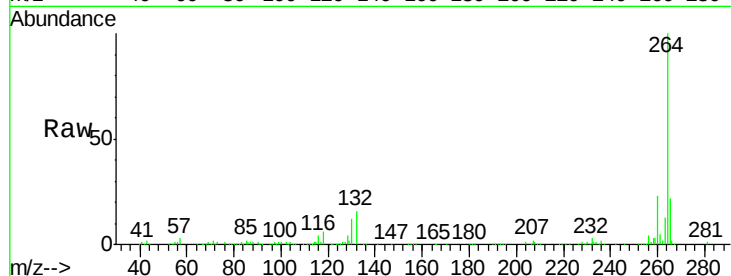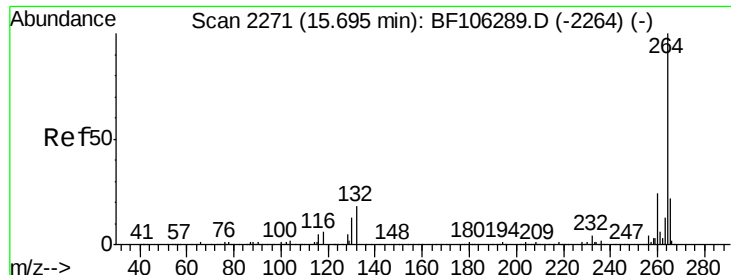

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.68 min Scan# 2269
Delta R.T. -0.02 min
Lab File: BF106475.D
Acq: 15 Jun 2018 6:23

Instrument :
BNA_F
ClientSampleId :
061218-DBRI-F-D-M

Tgt Ion:	264	Resp:	210884
Ion	Ratio	Lower	Upper
264	100		
260	23.3	19.2	28.8
265	22.0	17.5	26.3

