
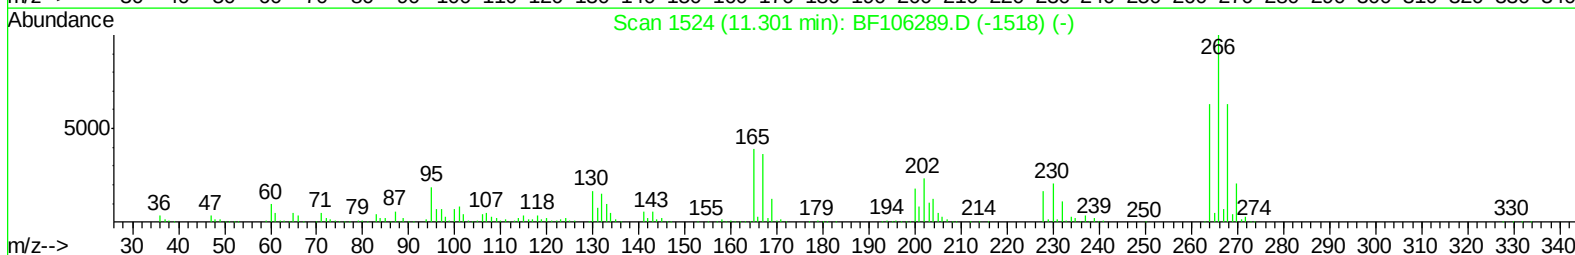
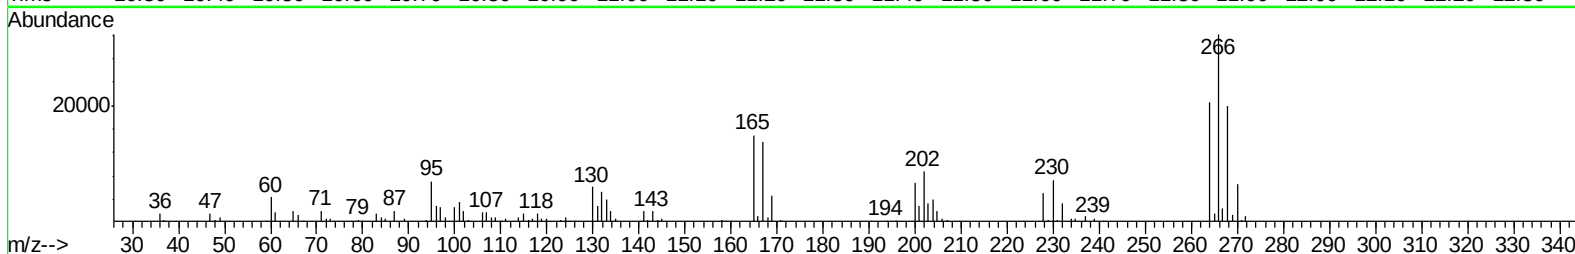


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061418\
Data File : BF106463.D
Acq On : 15 Jun 2018 1:05
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 05:32:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 14 18:39:24 2018
Response via : Initial Calibration

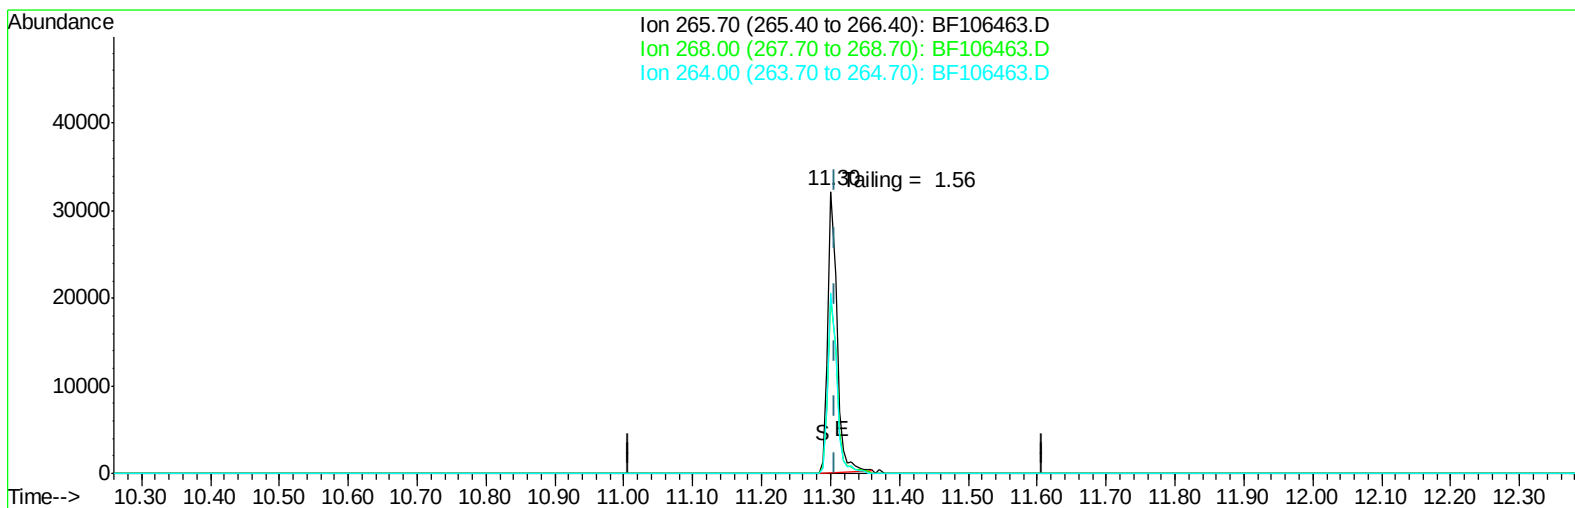

TIC: BF106463.D

(69) Pentachlorophenol (C)




11.301min (-0.006) 35388.00ng

response 29635

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.17
264.00	61.90	64.01
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061418\
Data File : BF106463.D
Acq On : 15 Jun 2018 1:05
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 05:32:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 14 18:39:24 2018
Response via : Initial Calibration

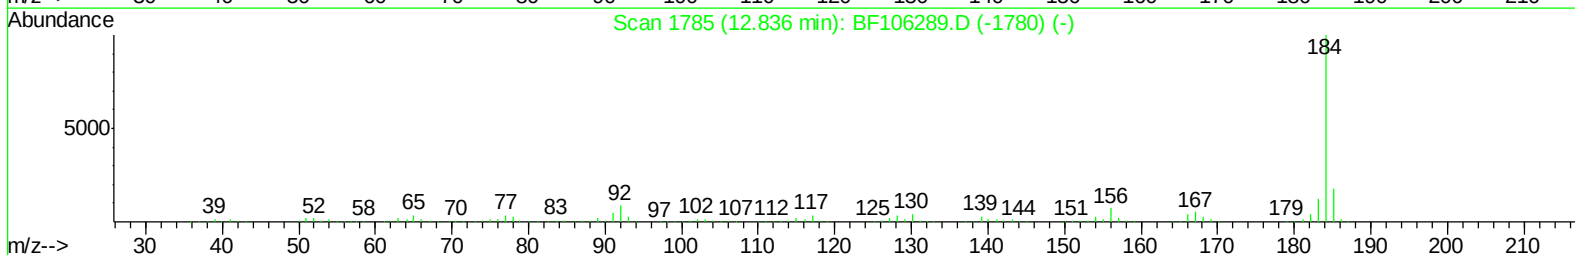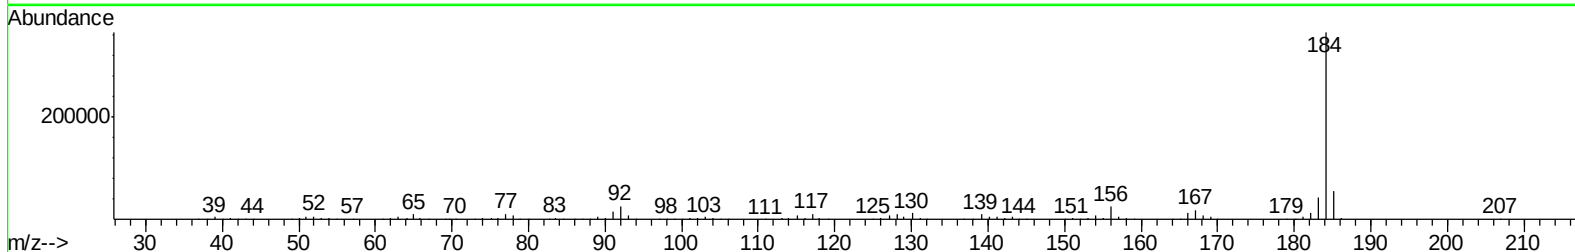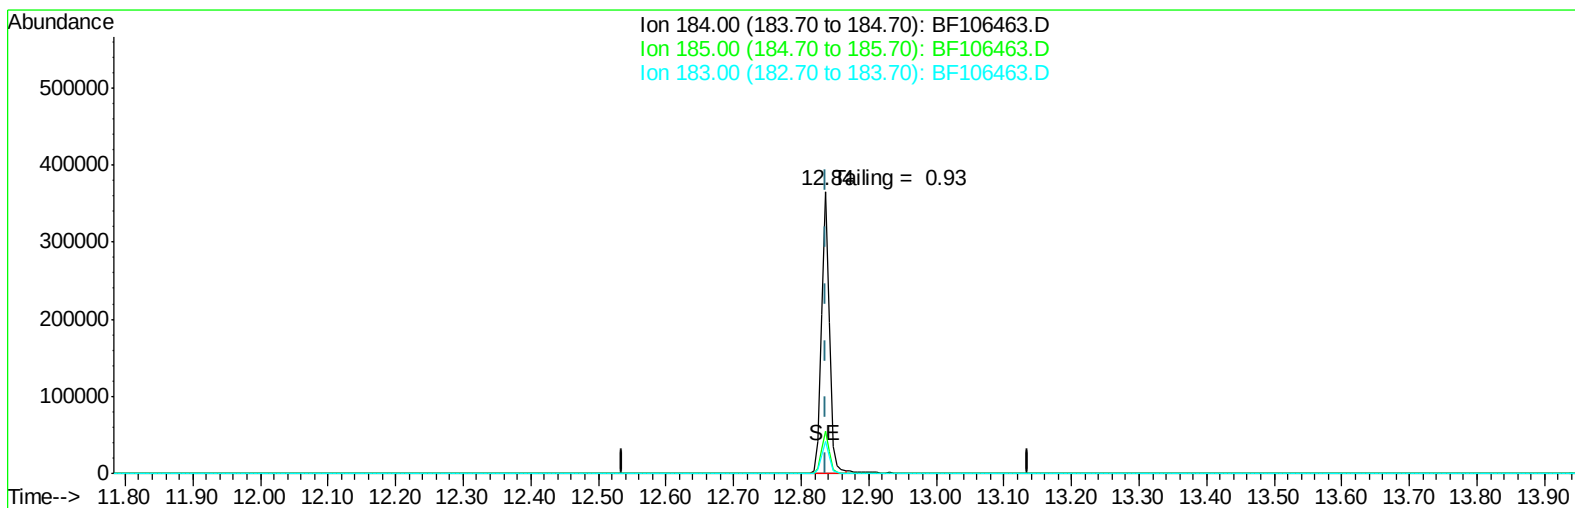

TIC: BF106463.D

(76) Benzidine

12.836min (-0.000) 0.00ng

response 312317

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.13
183.00	11.60	11.44
0.00	0.00	0.00