

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061418\
 Data File : BF106475.D
 Acq On : 15 Jun 2018 6:23
 Operator : JU/SJ
 Sample : J3475-02
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 061218-DBRI-F-D-M

Quant Time: Jun 15 08:48:20 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 14 18:39:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	111778	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	377286	20.00	ng	0.00
38) Acenaphthene-d10	10.01	164	148731	20.00	ng	0.00
63) Phenanthrene-d10	11.50	188	293679	20.00	ng	0.00
75) Chrysene-d12	14.15	240	309627	20.00	ng	-0.01
86) Perylene-d12	15.68	264	210884	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	331173	50.14	ng	0.00
7) Phenol-d6	6.61	99	268472	32.18	ng	0.00
23) Nitrobenzene-d5	7.53	82	658553	102.69	ng	0.00
41) 2,4,6-Tribromophenol	10.80	330	157329	109.94	ng	0.00
44) 2-Fluorobiphenyl	9.32	172	1006301	153.34	ng	0.00
78) Terphenyl-d14	13.08	244	1167121	93.62	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.71	163	107608	10.127	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061418\
Data File : BF106475.D
Acq On : 15 Jun 2018 6:23
Operator : JU/SJ
Sample : J3475-02
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
061218-DBRI-F-D-M

Quant Time: Jun 15 08:48:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 14 18:39:24 2018
Response via : Initial Calibration

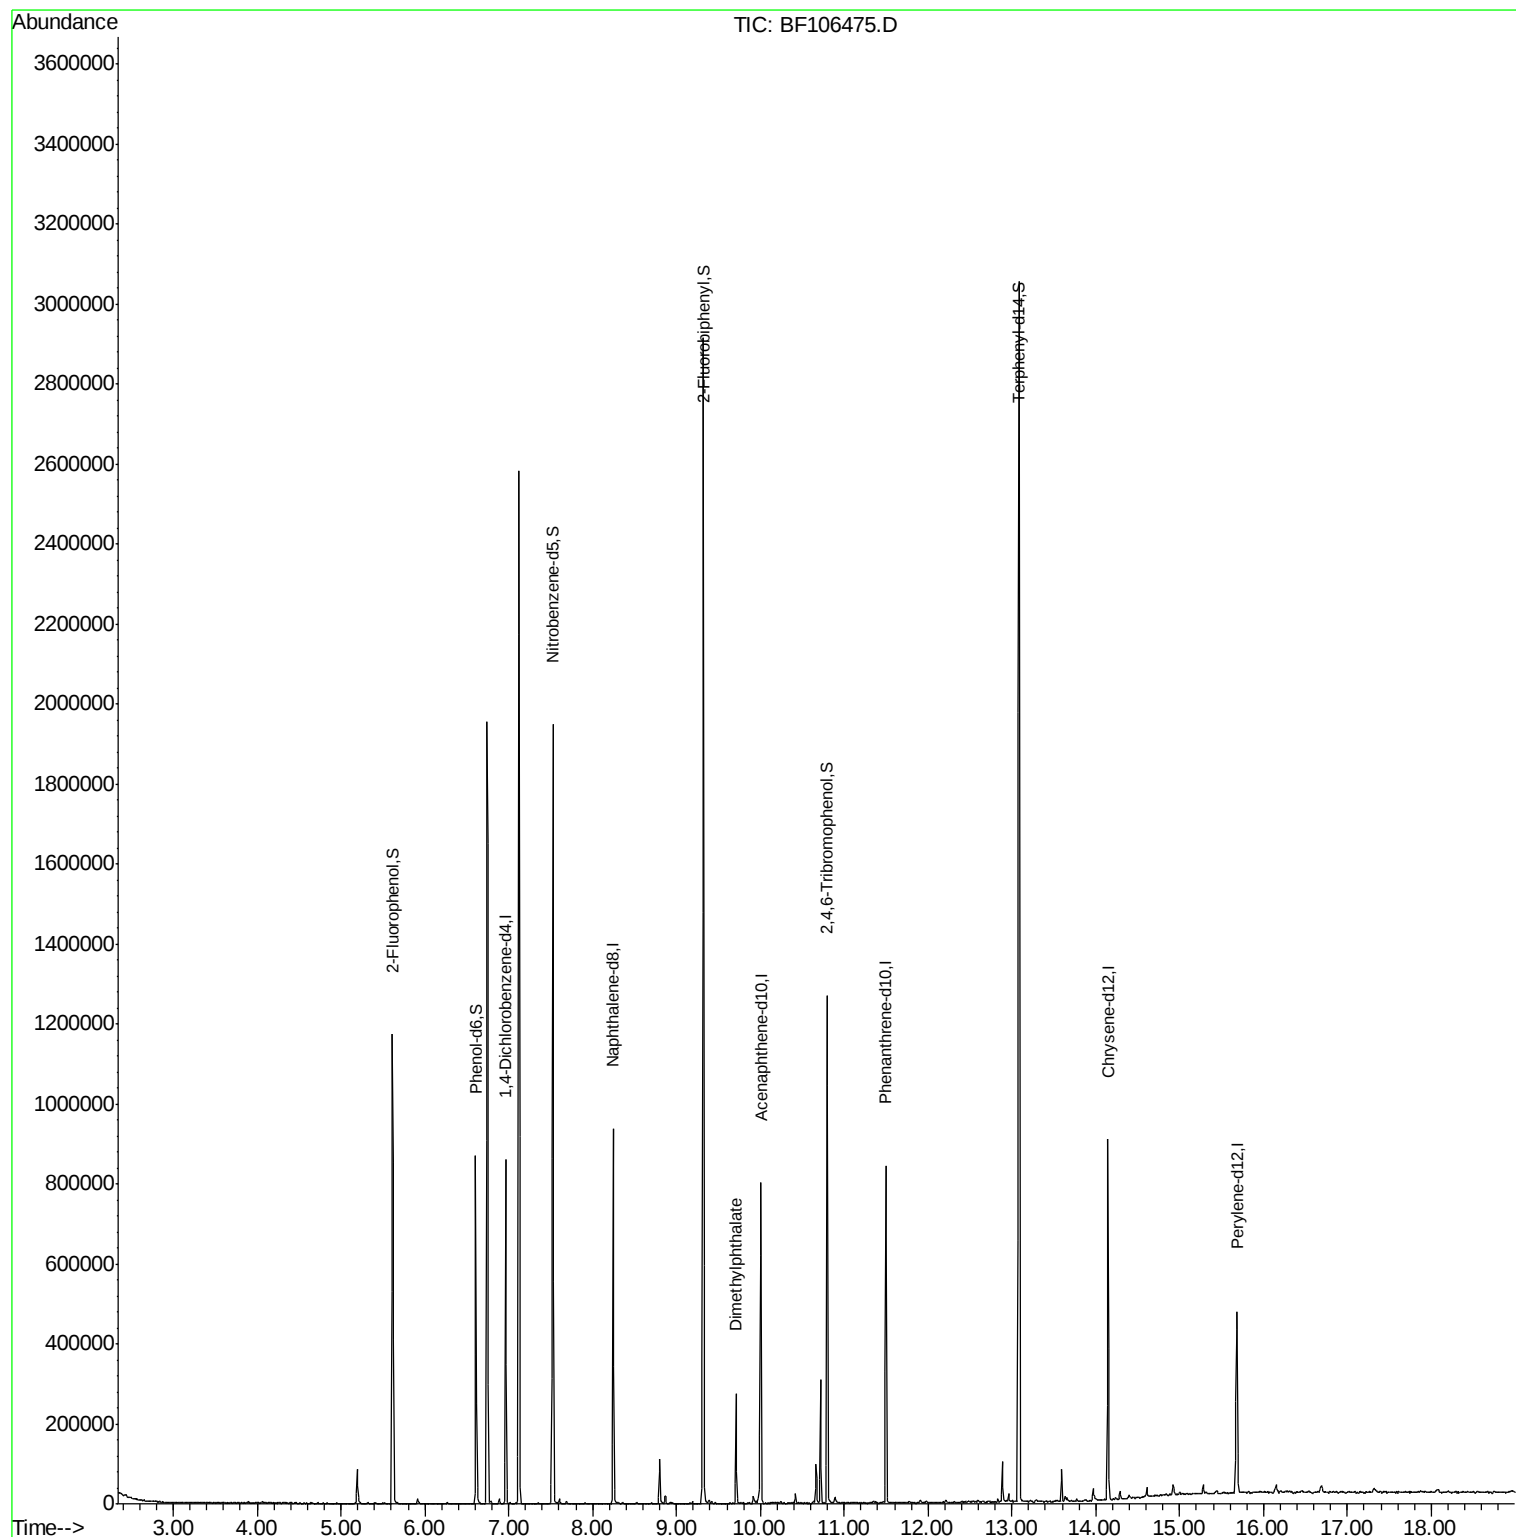

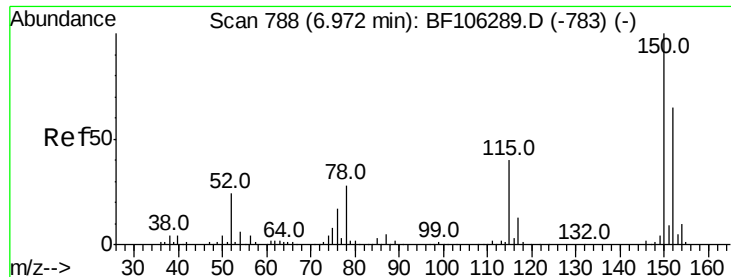


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 787
Delta R.T. -0.00 min
Lab File: BF106475.D
Acq: 15 Jun 2018 6:23

Instrument :
BNA_F
ClientSampleId :
061218-DBRI-F-D-M

Tot Ion:152 Resp: 111778
Ion Ratio Lower Upper
152 100
150 157.5 124.6 186.8
115 61.4 50.1 75.1

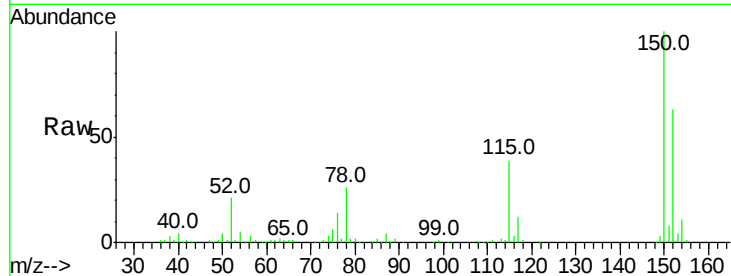


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

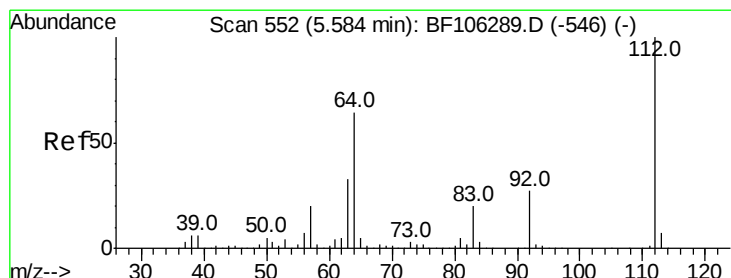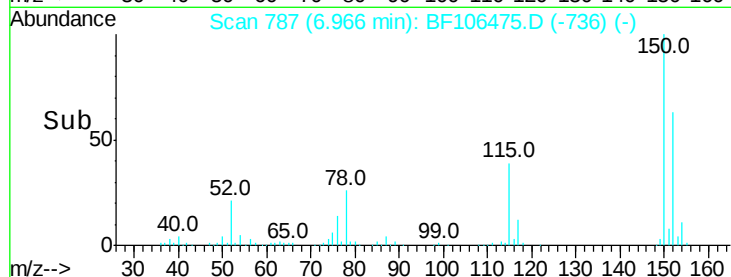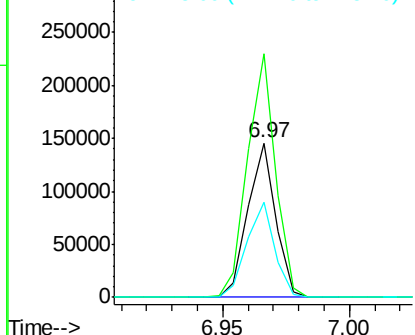



#5

2-Fluorophenol
Concen: 50.145 ng
RT: 5.61 min Scan# 557
Delta R.T. -0.00 min
Lab File: BF106475.D
Acq: 15 Jun 2018 6:23

Tgt Ion:112 Resp: 331173
Ion Ratio Lower Upper
112 100
64 59.9 47.9 71.9
63 30.4 23.7 35.5

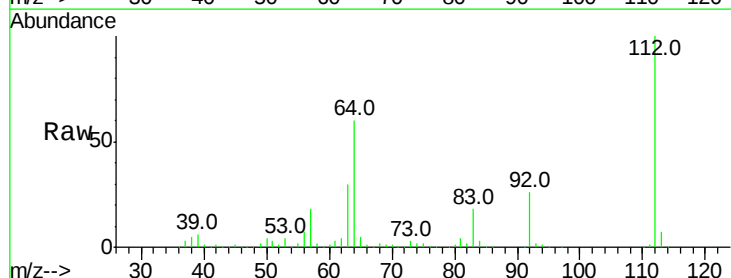

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

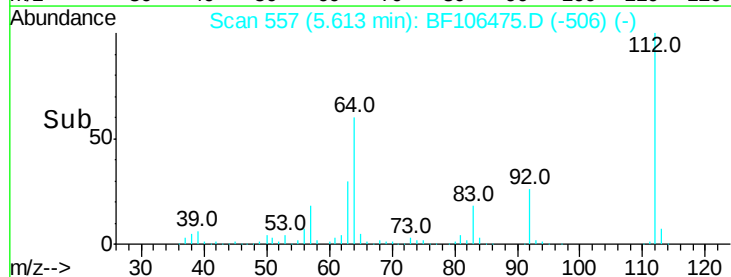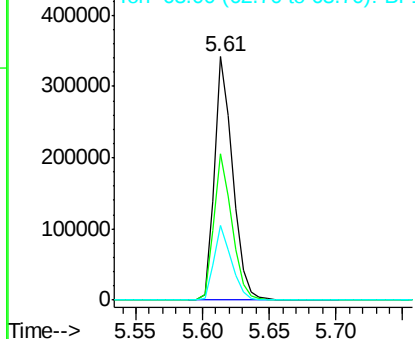



#7

Phenol-d6

Concen: 32.176 ng

RT: 6.61 min Scan# 726

Delta R.T. -0.01 min

Lab File: BF106475.D

Acq: 15 Jun 2018 6:23

Instrument :

BNA_F

ClientSampleId :

061218-DBRI-F-D-M


Tot Ion: 99 Resp: 268472

Ion Ratio Lower Upper




99 100

42 18.3 14.5 21.7

71 34.5 25.4 38.0

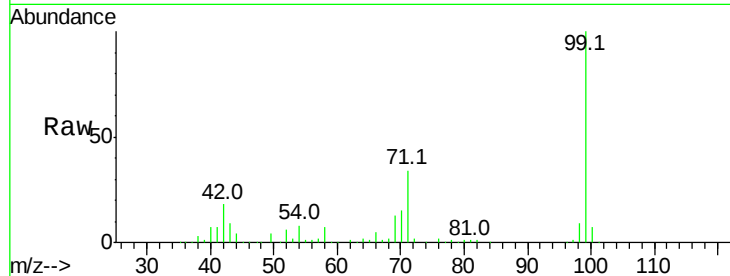

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

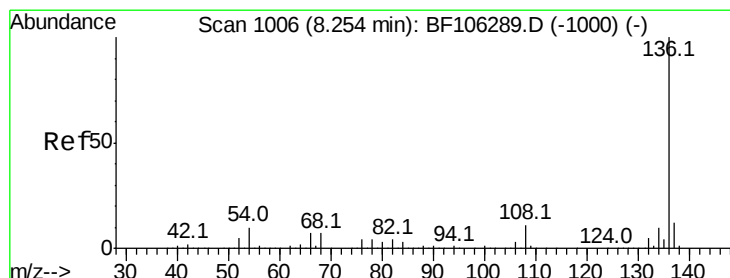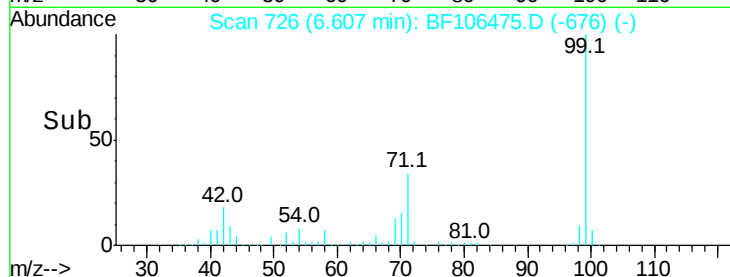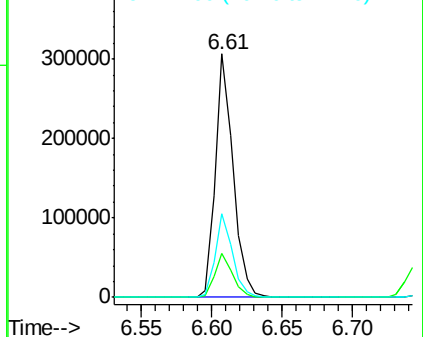

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.25 min Scan# 1005

Delta R.T. -0.01 min

Lab File: BF106475.D

Acq: 15 Jun 2018 6:23

Tgt Ion: 136 Resp: 377286


Ion Ratio Lower Upper

136 100



137 11.1 8.9 13.3


54 8.0 6.6 9.8

68 6.3 5.0 7.4

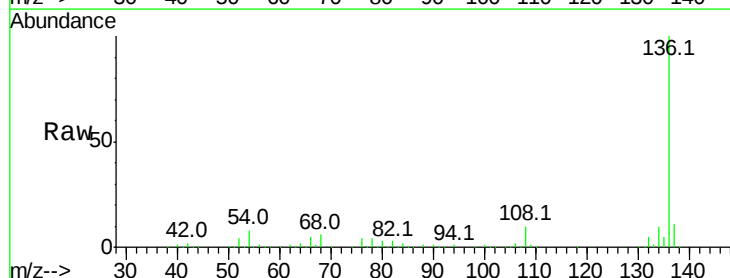

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

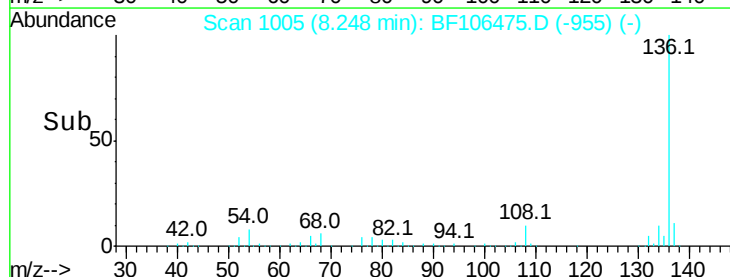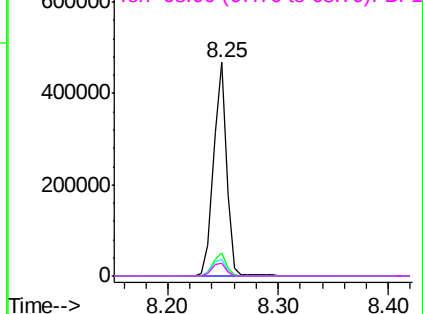

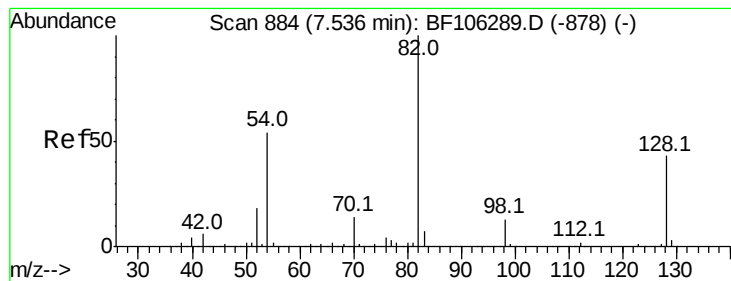

#23

Nitrobenzene-d5

Concen: 102.685 ng

RT: 7.53 min Scan# 883

Delta R.T. -0.01 min

Lab File: BF106475.D

Acq: 15 Jun 2018 6:23

Instrument :

BNA_F

ClientSampleId :

061218-DBRI-F-D-M


Tot Ion: 82 Resp: 658553

Ion Ratio Lower Upper

82 100

128 44.6 36.1 54.1




54 49.9 41.4 62.2

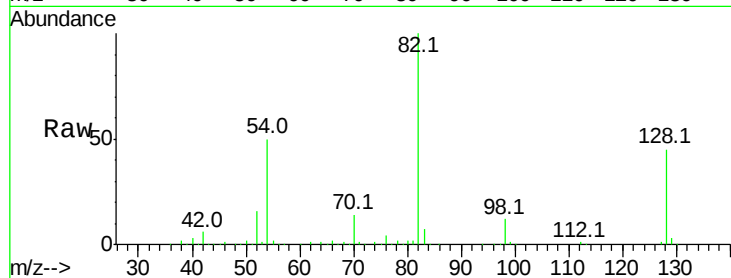

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): BF1

Ion 54.00 (53.70 to 54.70): BF1

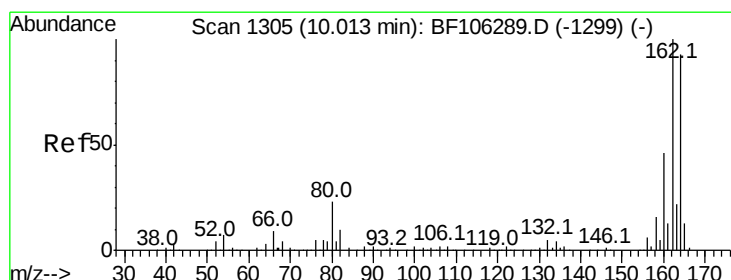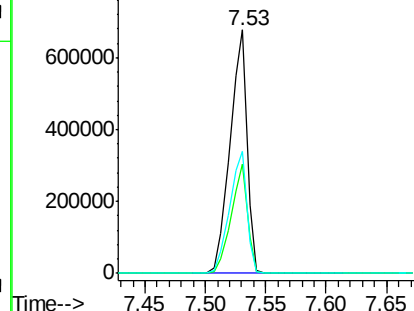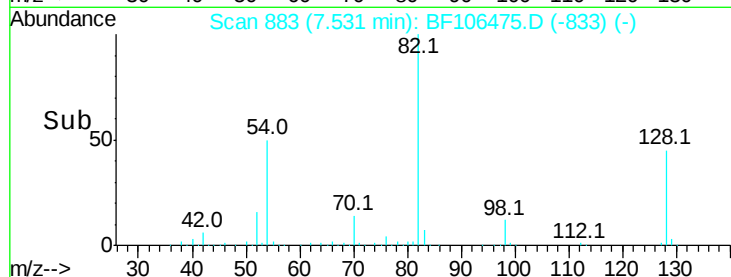

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.01 min Scan# 1304

Delta R.T. -0.01 min

Lab File: BF106475.D

Acq: 15 Jun 2018 6:23


Tgt Ion:164 Resp: 148731

Ion Ratio Lower Upper

164 100

162 105.5 86.1 129.1



160 47.8 38.3 57.5

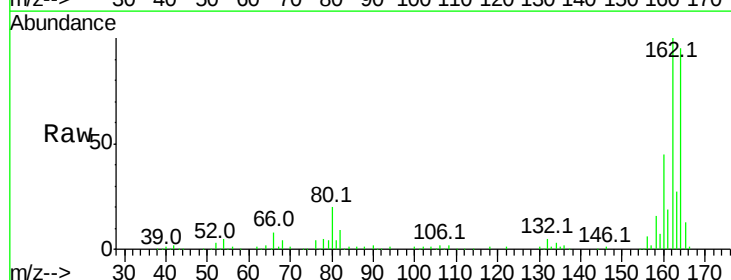


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

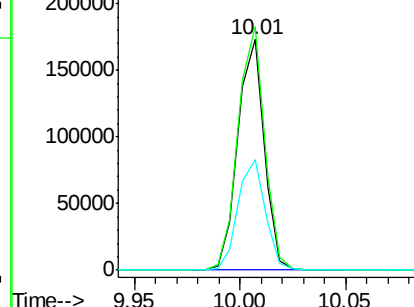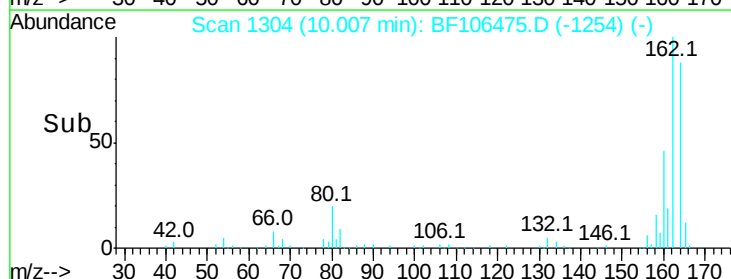

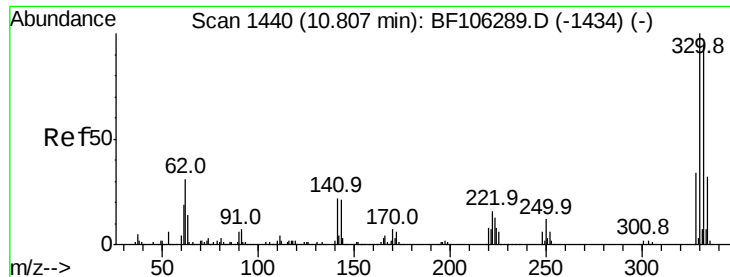

#41

2,4,6-Tribromophenol

Concen: 109.940 ng

RT: 10.80 min Scan# 1439

Delta R.T. -0.01 min

Lab File: BF106475.D

Acq: 15 Jun 2018 6:23

Instrument :

BNA_F

ClientSampleId :

061218-DBRI-F-D-M


Tot Ion:330 Resp: 157329

Ion Ratio Lower Upper

330 100

332 96.7 77.0 115.6




141 28.7 29.9 44.9#

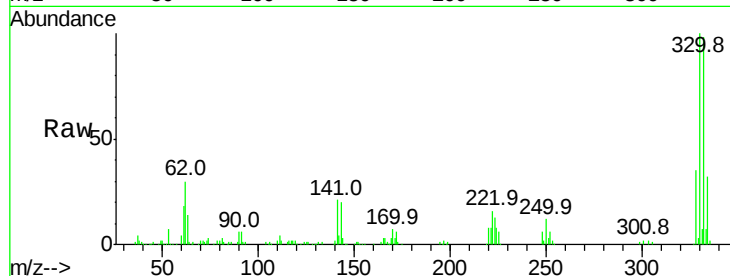

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

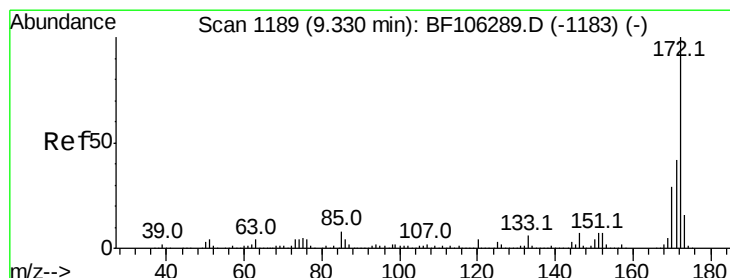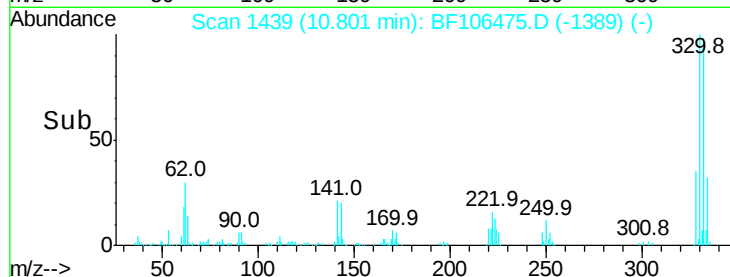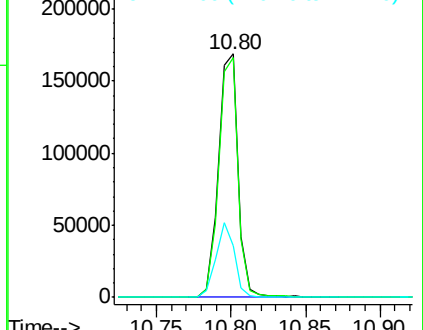

#44

2-Fluorobiphenyl

Concen: 153.336 ng

RT: 9.32 min Scan# 1188

Delta R.T. 0.00 min

Lab File: BF106475.D

Acq: 15 Jun 2018 6:23


Tgt Ion:172 Resp: 1006301

Ion Ratio Lower Upper

172 100

171 37.8 29.7 44.5



170 25.7 19.6 29.4

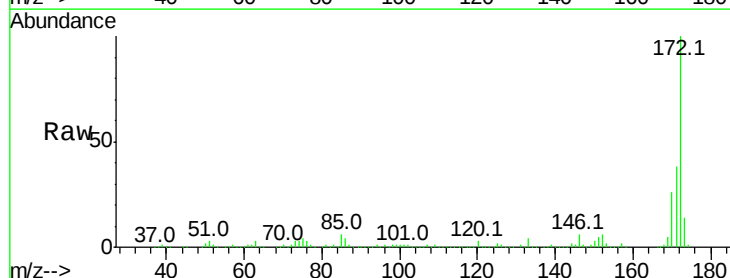


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

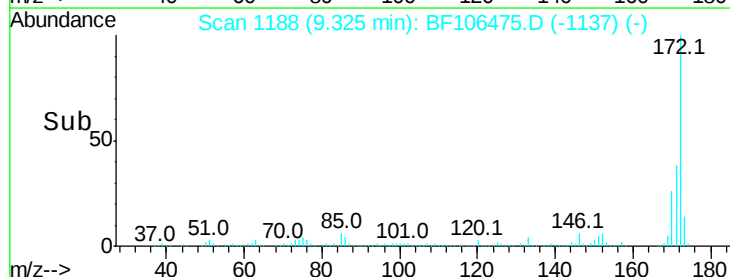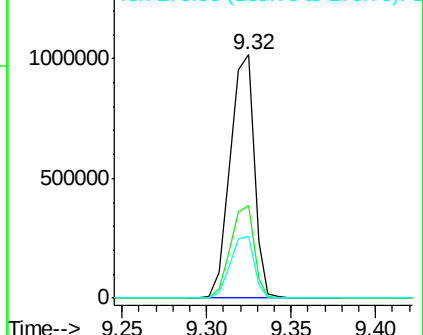

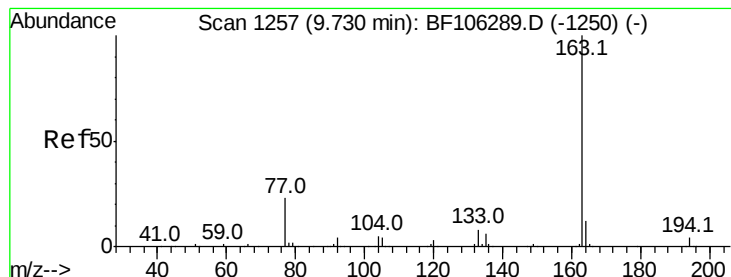

#49

Dimethylphthalate

Concen: 10.127 ng

RT: 9.71 min Scan# 1254

Delta R.T. -0.01 min

Lab File: BF106475.D

Acq: 15 Jun 2018 6:23

Instrument :

BNA_F

ClientSampleId :

061218-DBRI-F-D-M


Tot Ion:163 Resp: 107608

Ion Ratio Lower Upper

163 100

194 3.9 2.7 4.1




164 10.2 8.2 12.2

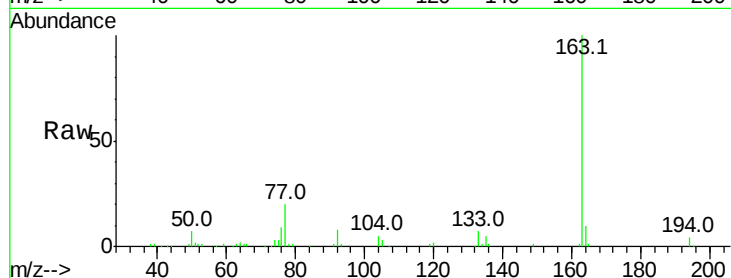

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

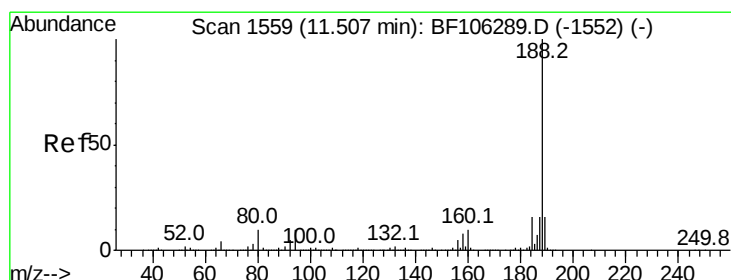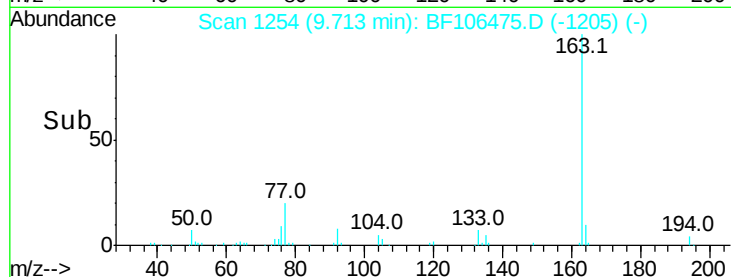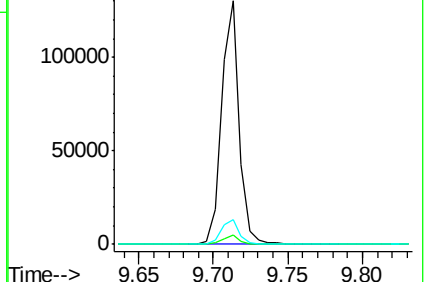

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.50 min Scan# 1557

Delta R.T. -0.01 min

Lab File: BF106475.D

Acq: 15 Jun 2018 6:23


Tgt Ion:188 Resp: 293679

Ion Ratio Lower Upper

188 100

94 10.7 8.5 12.7



80 11.8 9.2 13.8

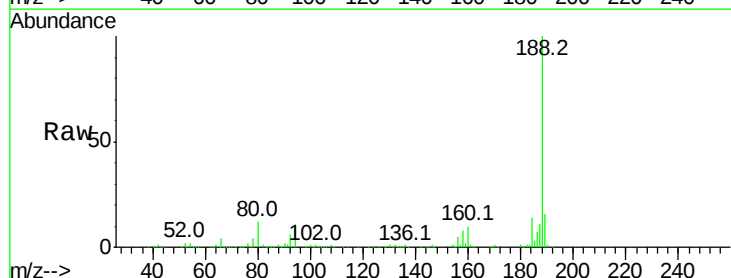


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

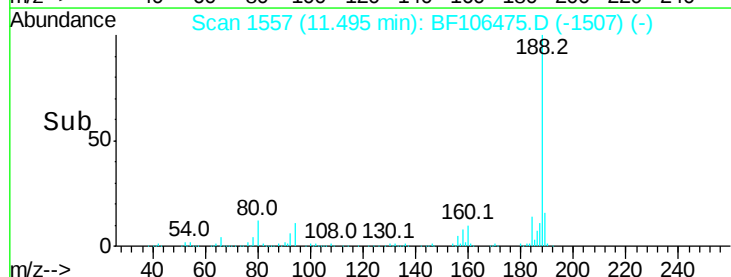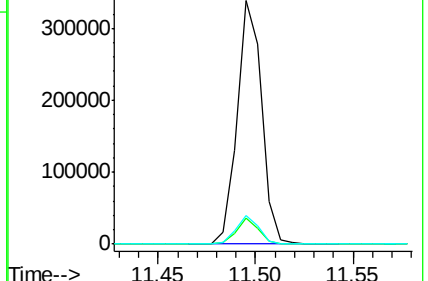

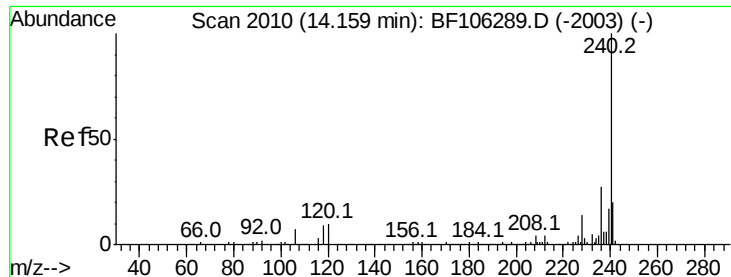

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.15 min Scan# 2008

Delta R.T. -0.01 min

Lab File: BF106475.D

Acq: 15 Jun 2018 6:23

Instrument :

BNA_F

ClientSampleId :

061218-DBRI-F-D-M


Tot Ion:240 Resp: 309627

Ion Ratio Lower Upper

240 100

120 10.1 9.5 14.3




236 26.5 20.7 31.1

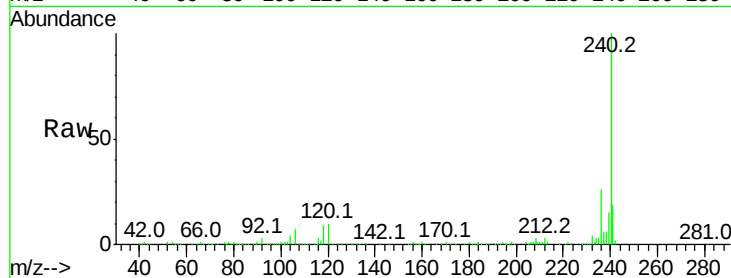

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

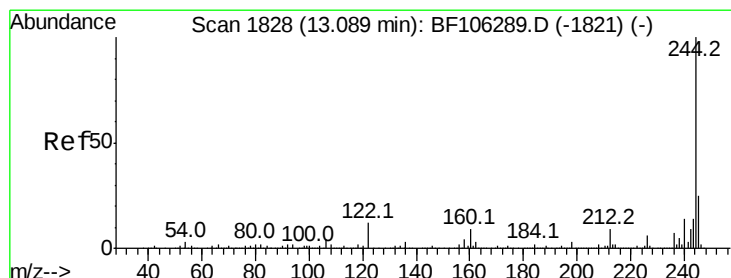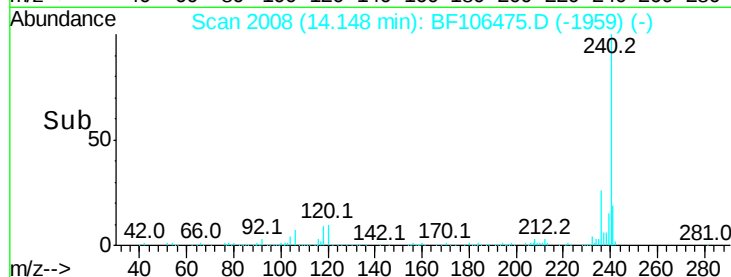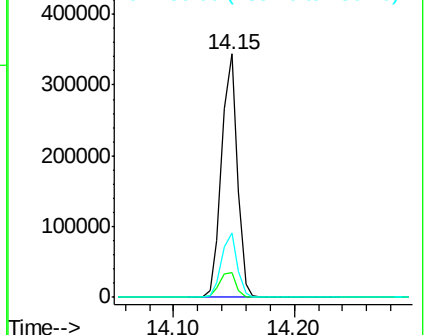

#78

Terphenyl-d14

Concen: 93.625 ng

RT: 13.08 min Scan# 1827

Delta R.T. -0.01 min

Lab File: BF106475.D

Acq: 15 Jun 2018 6:23


Tgt Ion:244 Resp: 1167121

Ion Ratio Lower Upper

244 100

212 7.3 5.4 8.0



122 11.2 11.0 16.4

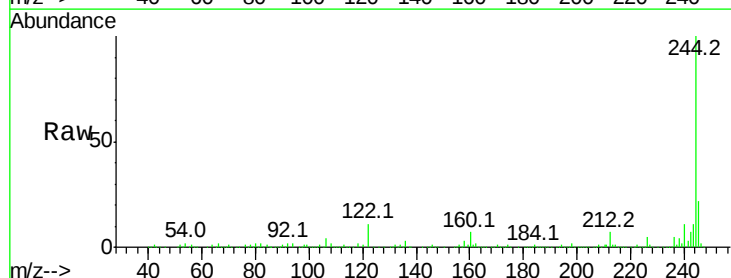


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

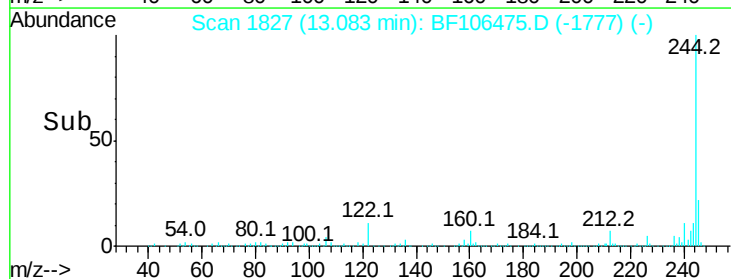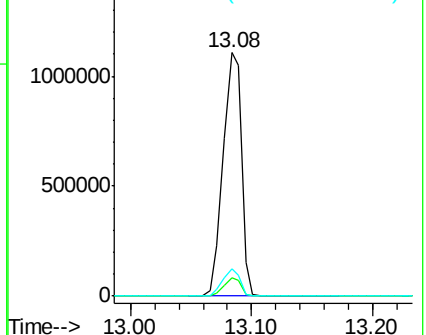


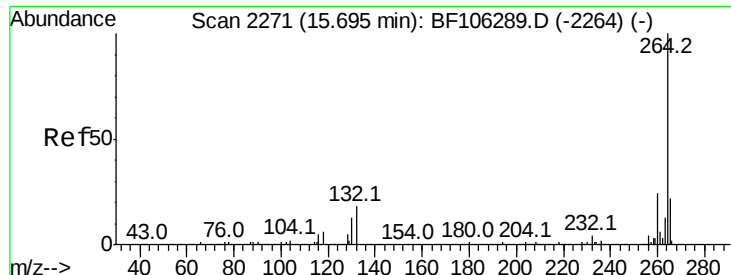

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.68 min Scan# 2269
 Delta R.T. -0.02 min
 Lab File: BF106475.D
 Acq: 15 Jun 2018 6:23

Instrument :
 BNA_F
 ClientSampleId :
 061218-DBRI-F-D-M

Tot Ion:264	Resp:	210884
Ion	Ratio	Lower Upper
264	100	
260	23.3	19.2 28.8
265	22.0	17.5 26.3

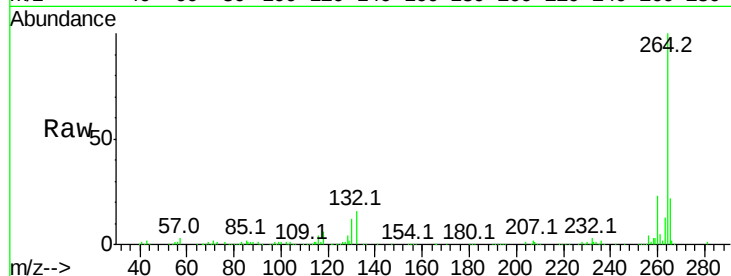

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

