


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061418\
 Data File : BF106435.D
 Acq On : 14 Jun 2018 12:05
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 15 11:11:47 2018

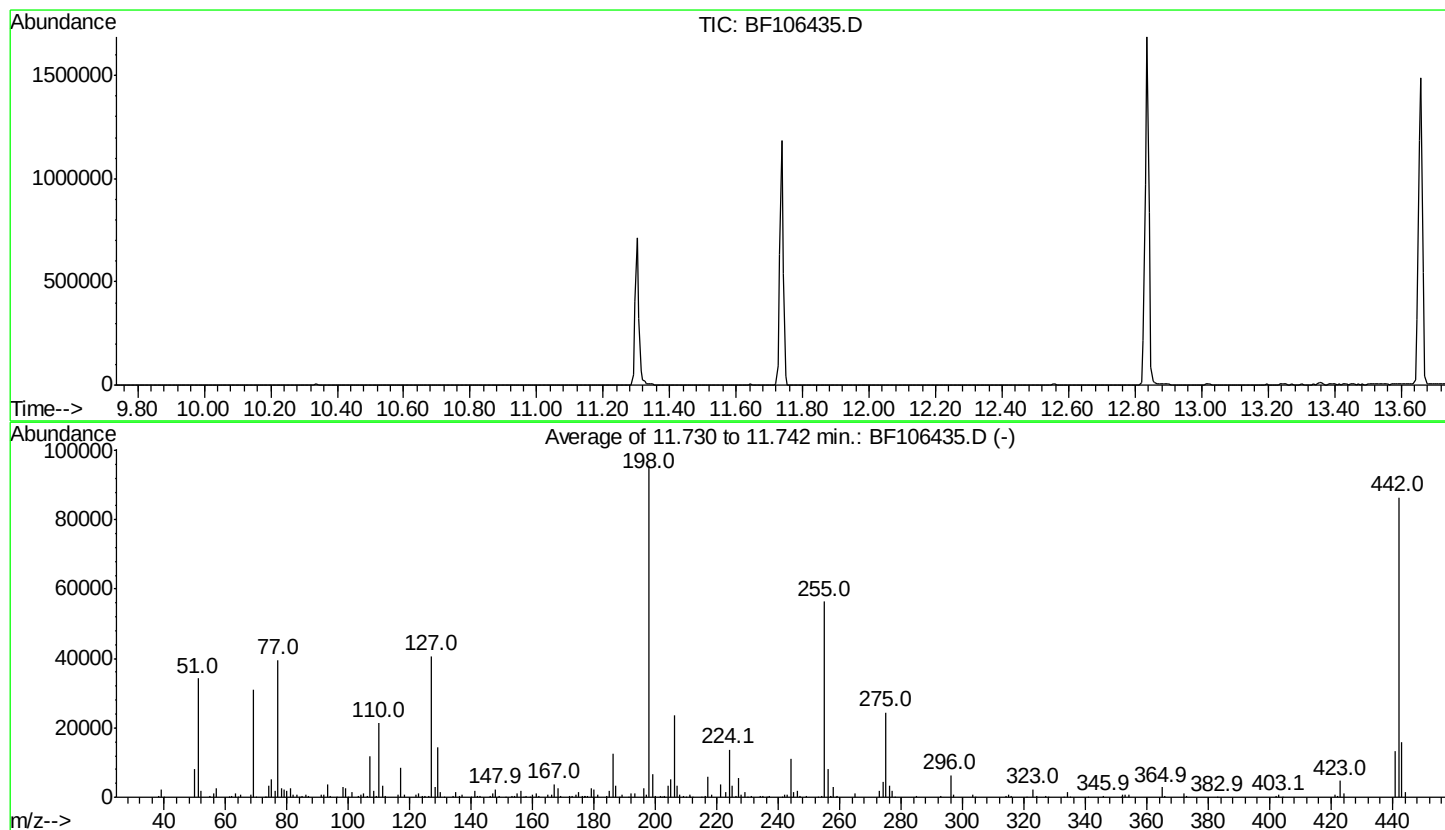

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	34157	PASS
68	69	0.00	2	2.0	616	PASS
69	198	0.00	100	32.6	31189	PASS
70	69	0.00	2	0.3	102	PASS
127	198	10	80	42.6	40696	PASS
197	198	0.00	2	0.6	611	PASS
198	198	100	100	100.0	95602	PASS
199	198	5	9	6.8	6545	PASS
275	198	10	60	25.6	24512	PASS
365	198	1	100	3.1	2934	PASS
441	443	0.01	100	84.2	13305	PASS
442	198	50	100	90.5	86477	PASS
443	442	15	24	18.3	15794	PASS