


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061418\
 Data File : BF106463.D
 Acq On : 15 Jun 2018 1:05
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 15 11:11:47 2018

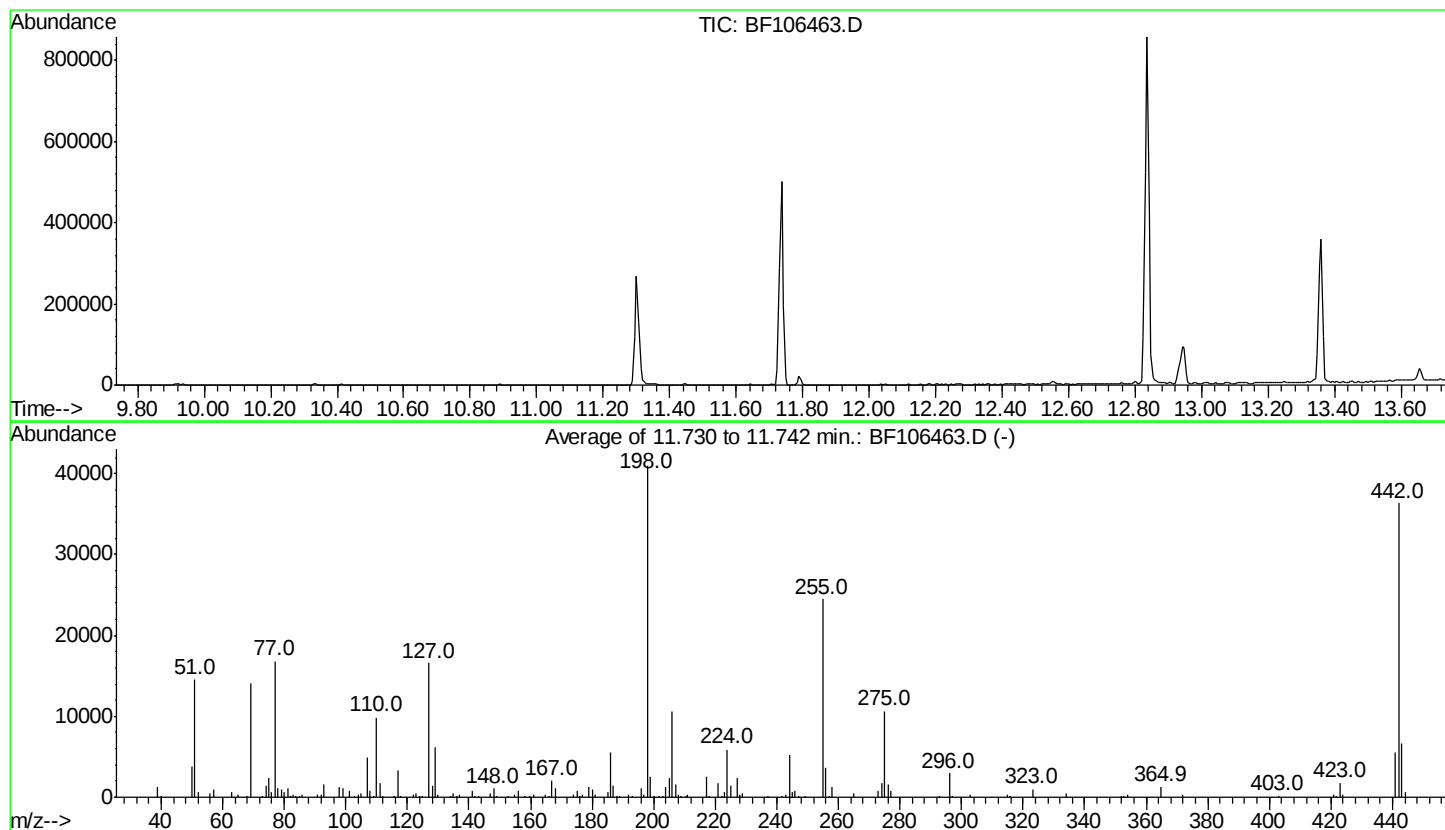

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	14514	PASS
68	69	0.00	2	1.5	217	PASS
69	198	0.00	100	34.5	14127	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.4	16572	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40997	PASS
199	198	5	9	6.3	2573	PASS
275	198	10	60	26.0	10639	PASS
365	198	1	100	3.3	1350	PASS
441	443	0.01	100	83.3	5560	PASS
442	198	50	100	88.8	36392	PASS
443	442	15	24	18.3	6676	PASS