

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061419\
 Data File : BF115035.D
 Acq On : 14 Jun 2019 13:10
 Operator : HP/JU
 Sample : PB120572BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jun 14 15:41:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 12 15:42:37 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.65	152	255065	20.00	ng	0.00
21) Naphthalene-d8	7.93	136	1014324	20.00	ng	0.00
39) Acenaphthene-d10	9.67	164	492054	20.00	ng	0.00
64) Phenanthrene-d10	11.15	188	984944	20.00	ng	-0.01
76) Chrysene-d12	13.77	240	778515	20.00	ng	-0.01
87) Perylene-d12	15.14	264	748674	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.26	112	1626949	106.51	ng	0.00
7) Phenol-d6	6.29	99	1984822	107.72	ng	0.00
23) Nitrobenzene-d5	7.21	82	1231092	73.06	ng	0.00
42) 2,4,6-Tribromophenol	10.46	330	549802	104.34	ng	-0.01
45) 2-Fluorobiphenyl	9.00	172	2389881	82.32	ng	0.00
79) Terphenyl-d14	12.73	244	2531675	61.16	ng	0.00
Target Compounds						
9) Benzaldehyde	6.29	77	2855	Below Cal	#	1
19) n-Nitroso-di-n-propylamine	7.21	70	160574	14.343 ng	#	75
25) Isophorone	7.21	82	1188844	37.667 ng	#	62
50) Dimethylphthalate	9.67	163	138610	3.746 ng	#	1
51) 2,6-Dinitrotoluene	9.67	165	62317	7.424 ng	#	37
57) 2,4-Dinitrotoluene	9.67	165	62317	5.833 ng	#	29
58) Fluorene	10.46	166	24230	Below Cal	#	84
67) 4-Bromophenyl-phenylether	10.46	248	35535	3.360 ng	#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061419\
Data File : BF115035.D
Acq On : 14 Jun 2019 13:10
Operator : HP/JU
Sample : PB120572BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jun 14 15:41:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 12 15:42:37 2019
Response via : Initial Calibration

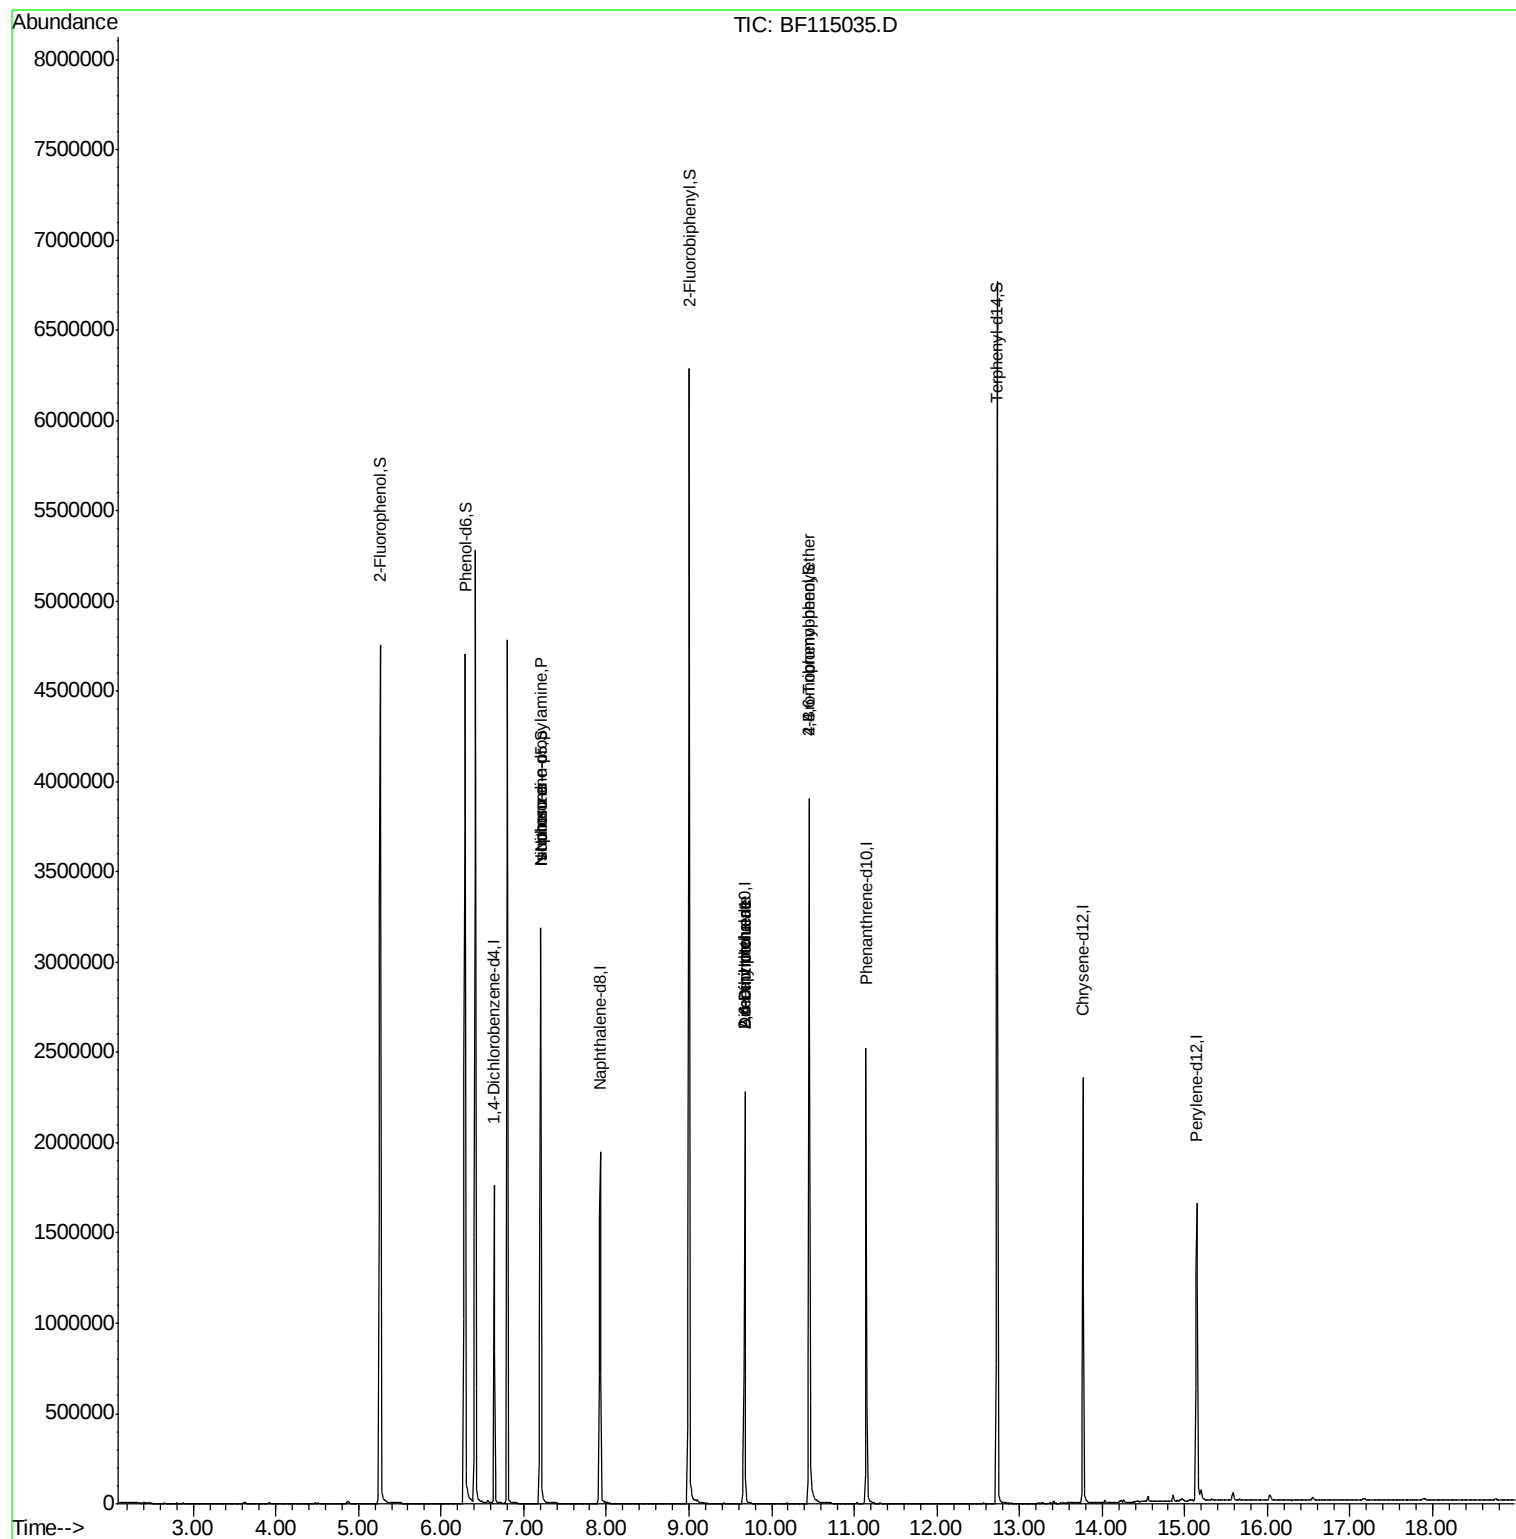

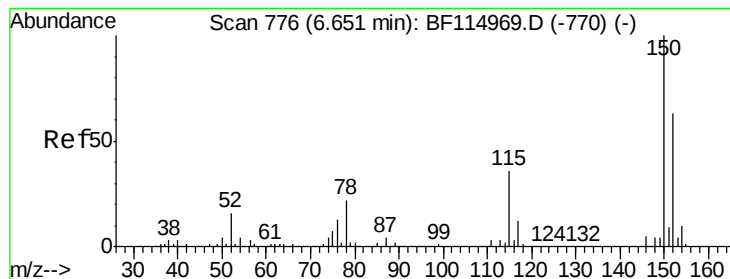


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.65 min Scan# 775
Delta R.T. -0.01 min
Lab File: BF115035.D
Acq: 14 Jun 2019 13:10

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 255065
Ion Ratio Lower Upper
152 100
150 156.4 127.4 191.0
115 58.7 46.0 69.0

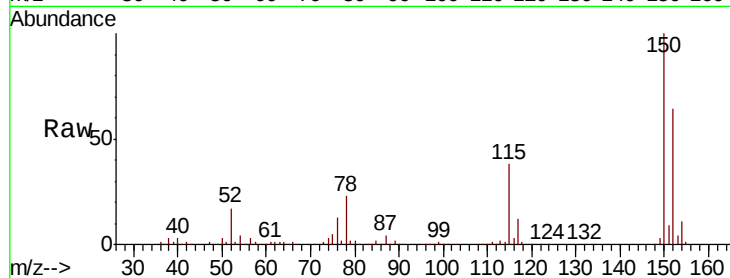


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

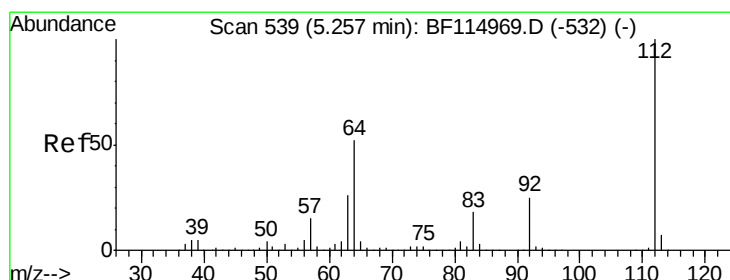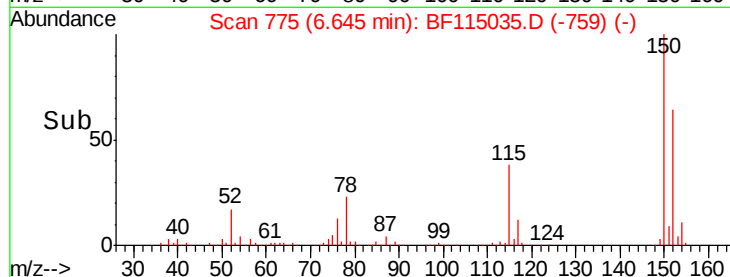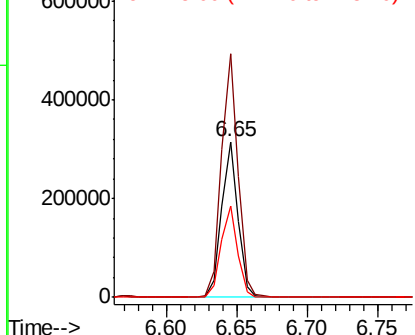



#5


2-Fluorophenol
Concen: 106.508 ng
RT: 5.26 min Scan# 540
Delta R.T. 0.01 min
Lab File: BF115035.D
Acq: 14 Jun 2019 13:10

Tgt Ion:112 Resp: 1626949
Ion Ratio Lower Upper
112 100
64 55.1 41.6 62.4
63 28.3 20.9 31.3

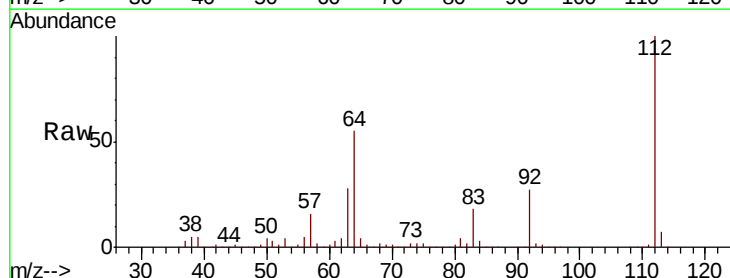

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

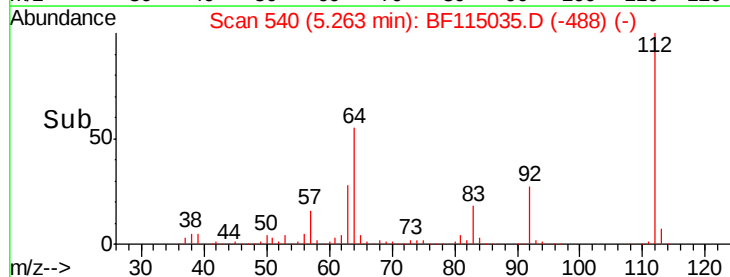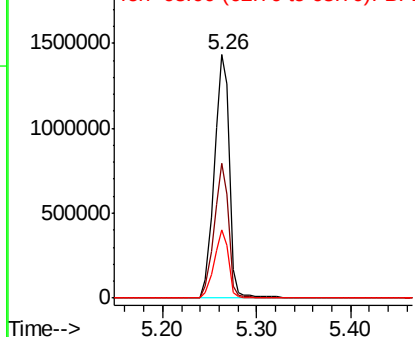

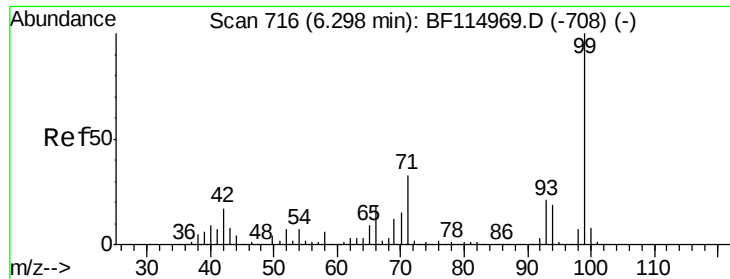

#7

Phenol-d6

Concen: 107.716 ng

RT: 6.29 min Scan# 715

Delta R.T. -0.01 min

Lab File: BF115035.D

Acq: 14 Jun 2019 13:10

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 1984822

Ion Ratio Lower Upper

99 100

42 16.0 13.4 20.2

71 33.7 26.4 39.6

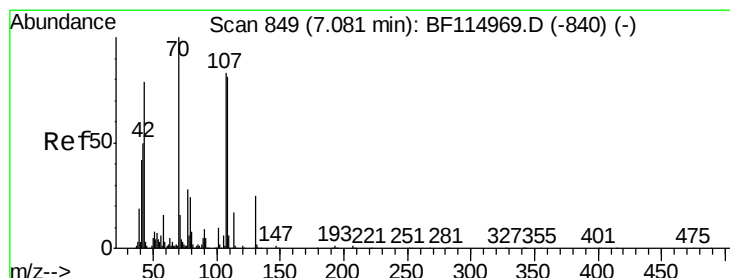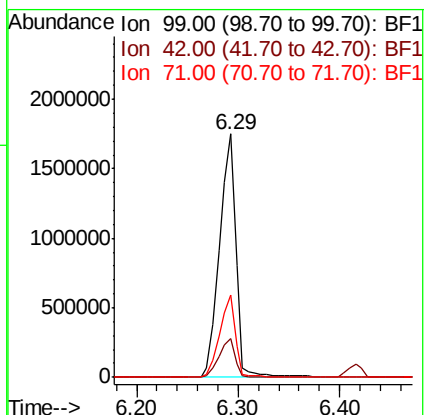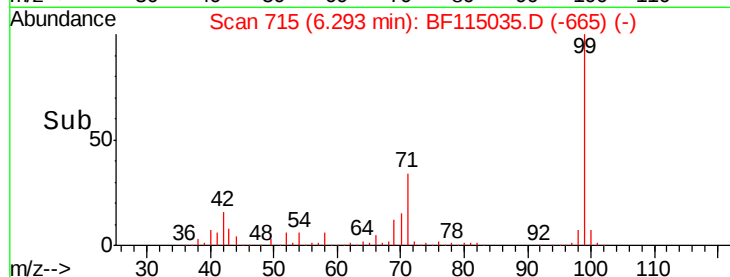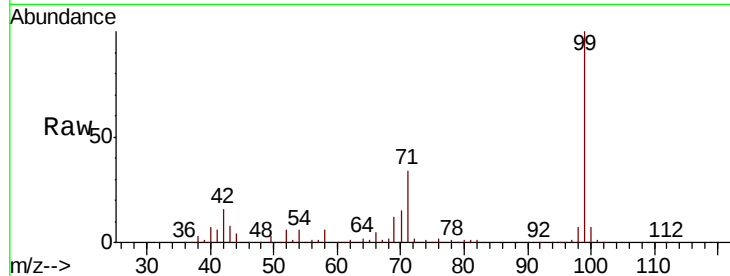

#19

n-Nitroso-di-n-propylamine

Concen: 14.343 ng

RT: 7.21 min Scan# 871

Delta R.T. 0.13 min

Lab File: BF115035.D

Acq: 14 Jun 2019 13:10

Tgt Ion: 70 Resp: 160574




Ion Ratio Lower Upper


70 100

42 40.8 40.3 60.5

101 0.0 8.2 12.4#

130 2.7 20.3 30.5#

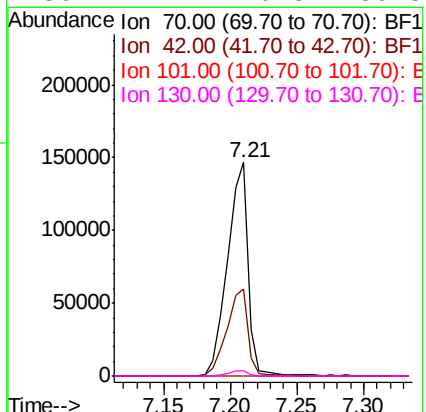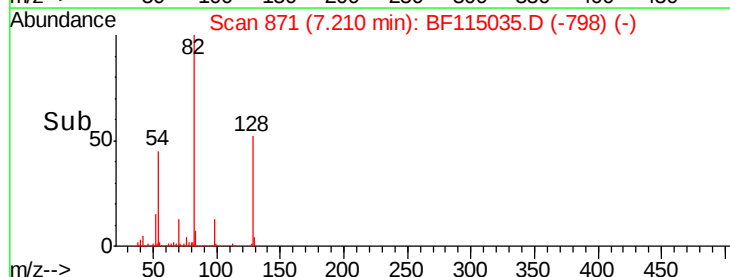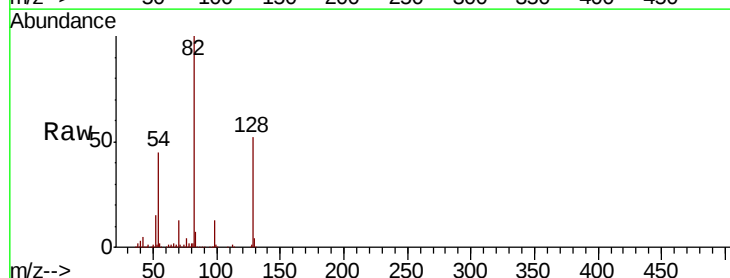


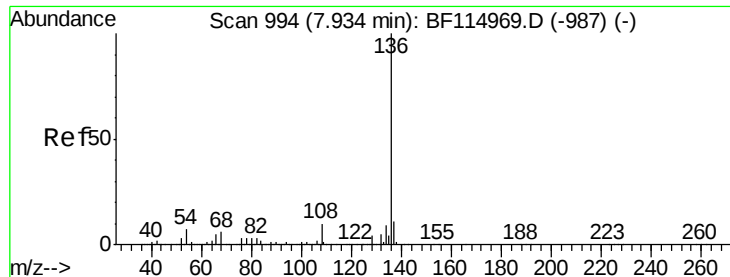




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.93 min Scan# 993
Delta R.T. -0.01 min
Lab File: BF115035.D
Acq: 14 Jun 2019 13:10

Instrument :
BNA_F
ClientSampleId :

Tot Ion:136	Resp: 1014324
Ion Ratio	Lower Upper
136 100	
137 11.0	9.0 13.4
54 6.2	5.4 8.0
68 5.4	4.6 7.0

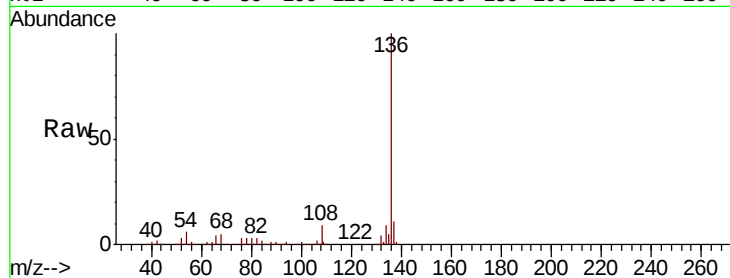


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

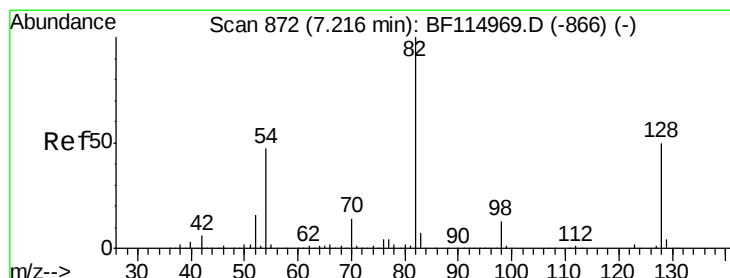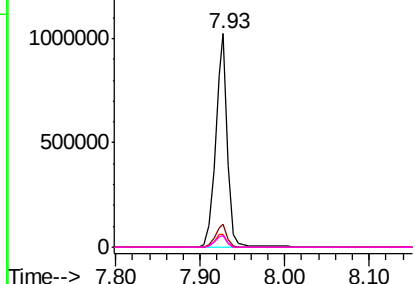
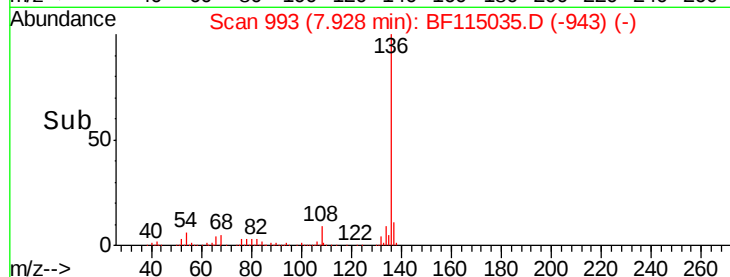



#23
Nitrobenzene-d5
Concen: 73.056 ng
RT: 7.21 min Scan# 871
Delta R.T. -0.01 min
Lab File: BF115035.D
Acq: 14 Jun 2019 13:10

Tgt	Ion: 82	Resp: 1231092	
Ion	Ratio	Lower	Upper
82	100		
128	51.9	39.9	59.9
54	44.8	37.3	55.9

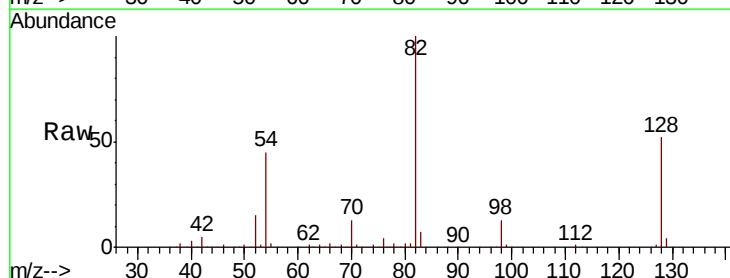

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

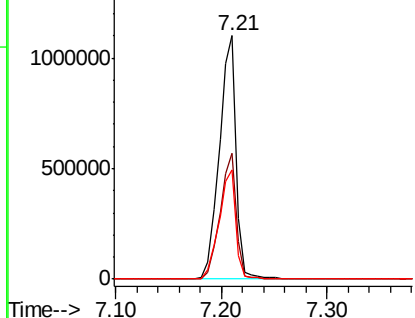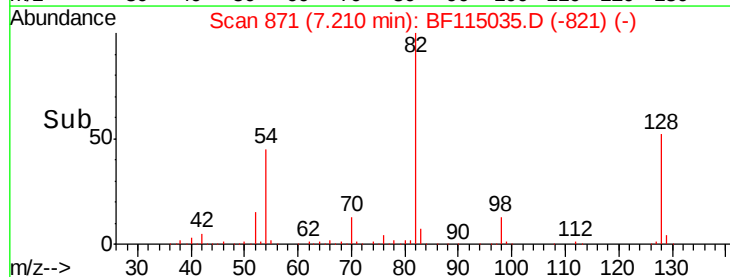

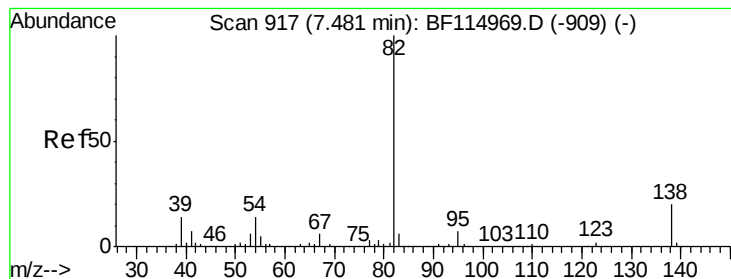

#25

Isophorone

Concen: 37.667 ng

RT: 7.21 min Scan# 871

Delta R.T. -0.27 min

Lab File: BF115035.D

Acq: 14 Jun 2019 13:10

Instrument :

BNA_F

ClientSampled :


Tot Ion: 82 Resp: 1188844

Ion Ratio Lower Upper




82 100

95 0.0 5.6 8.4#

138 0.0 16.1 24.1#



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

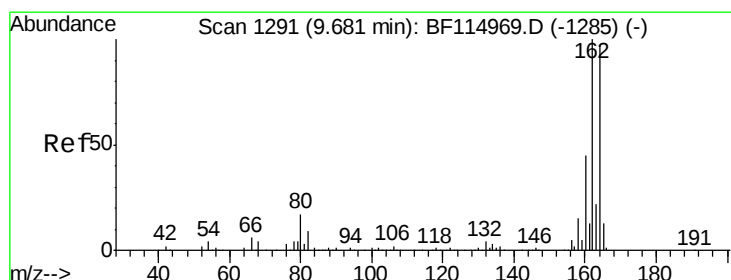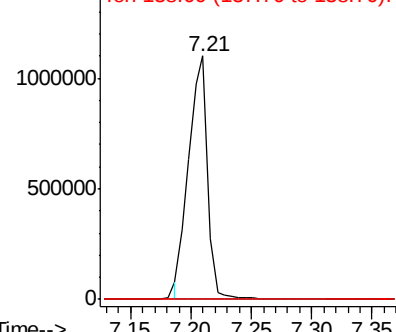

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.67 min Scan# 1290

Delta R.T. -0.01 min

Lab File: BF115035.D

Acq: 14 Jun 2019 13:10


Tgt Ion: 164 Resp: 492054

Ion Ratio Lower Upper



164 100


162 102.8 82.6 124.0

160 46.2 36.9 55.3



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

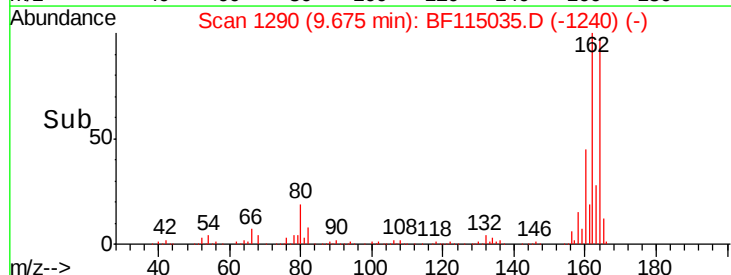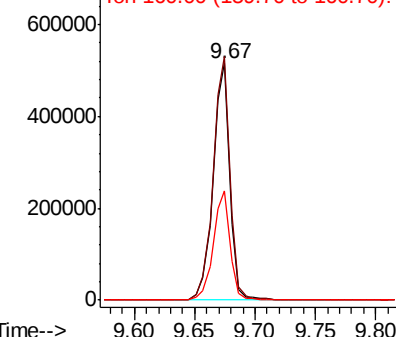




#42
 2,4,6-Tribromophenol
 Concen: 104.342 ng
 RT: 10.46 min Scan# 1423
 Delta R.T. -0.01 min
 Lab File: BF115035.D
 Acq: 14 Jun 2019 13:10

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.3	77.6	116.4
141	33.7	27.2	40.8



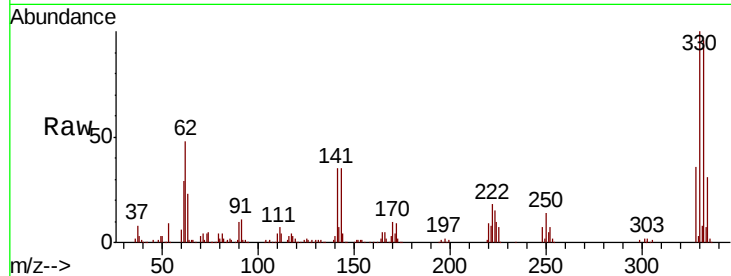


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

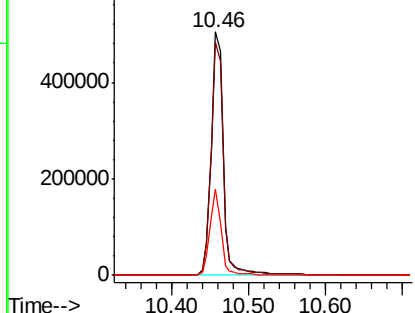

#45
 2-Fluorobiphenyl
 Concen: 82.317 ng
 RT: 9.00 min Scan# 1176
 Delta R.T. -0.01 min
 Lab File: BF115035.D
 Acq: 14 Jun 2019 13:10

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.9	29.8	44.6
170	25.3	20.6	31.0






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

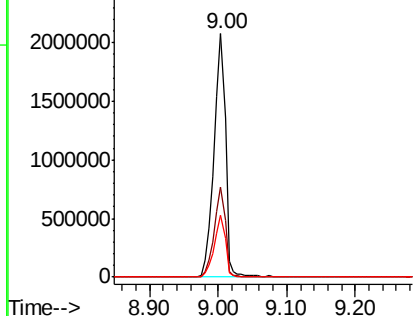



#50

Dimethylphthalate

Concen: 3.746 ng

RT: 9.67 min Scan# 1290

Delta R.T. 0.26 min

Lab File: BF115035.D

Acq: 14 Jun 2019 13:10

Instrument :

BNA_F

ClientSampleId :


Tot Ion:163 Resp: 138610

Ion Ratio Lower Upper

163 100

194 0.0 3.3 4.9#




164 348.0 8.6 12.8#



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

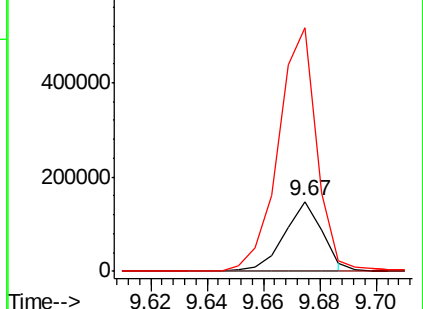

#51

2,6-Dinitrotoluene

Concen: 7.424 ng

RT: 9.67 min Scan# 1290

Delta R.T. 0.20 min

Lab File: BF115035.D

Acq: 14 Jun 2019 13:10


Tgt Ion:165 Resp: 62317

Ion Ratio Lower Upper

165 100

63 1.5 30.6 46.0#



89 1.2 34.4 51.6#




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

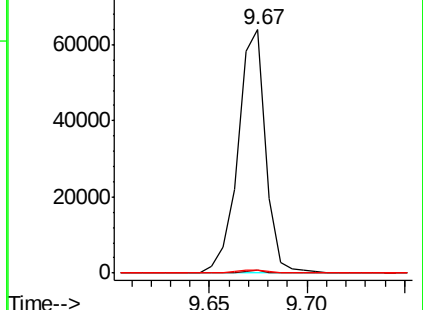


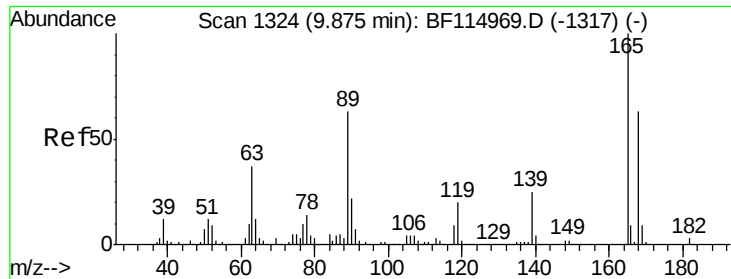




#57
 2,4-Dinitrotoluene
 Concen: 5.833 ng
 RT: 9.67 min Scan# 1290
 Delta R.T. -0.20 min
 Lab File: BF115035.D
 Acq: 14 Jun 2019 13:10

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:165	Resp:	62317
Ion Ratio	Lower	Upper
165	100	
63	1.5	29.4 44.2#
89	1.2	50.6 75.8#
182	0.0	2.2 3.2#




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1
 Ion 182.00 (181.70 to 182.70): E

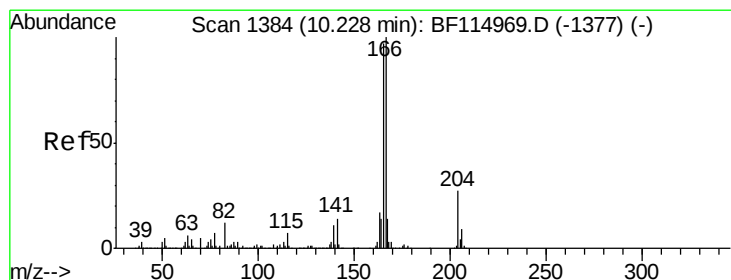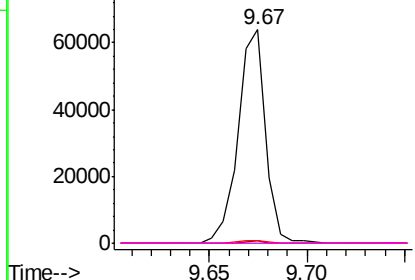




#58
 Fluorene
 Concen: Below Cal
 RT: 10.46 min Scan# 1423
 Delta R.T. 0.23 min
 Lab File: BF115035.D
 Acq: 14 Jun 2019 13:10

Tgt Ion:166	Resp:	24230
Ion Ratio	Lower	Upper
166	100	
165	107.9	77.6 116.4
167	34.9	11.0 16.4#



Abundance Ion 166.00 (165.70 to 166.70): E
 Ion 165.00 (164.70 to 165.70): E
 Ion 167.00 (166.70 to 167.70): E



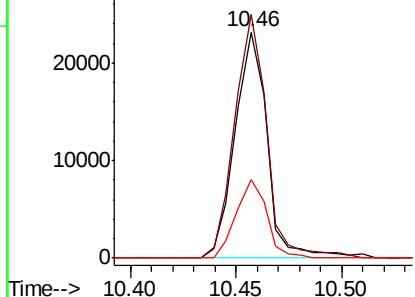



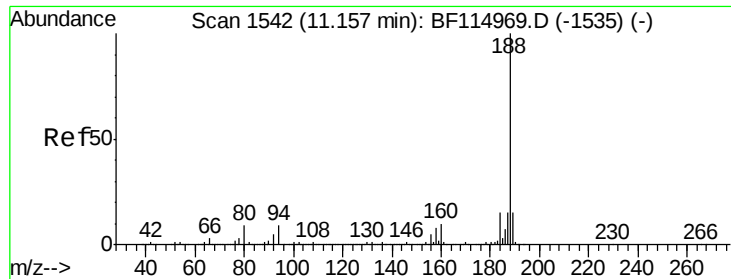

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.15 min Scan# 1540
Delta R.T. -0.01 min
Lab File: BF115035.D
Acq: 14 Jun 2019 13:10




Instrument :
BNA_F
ClientSampleId :


Tot Ion:188 Resp: 984944
Ion Ratio Lower Upper
188 100
94 10.3 7.2 10.8
80 11.0 7.4 11.2

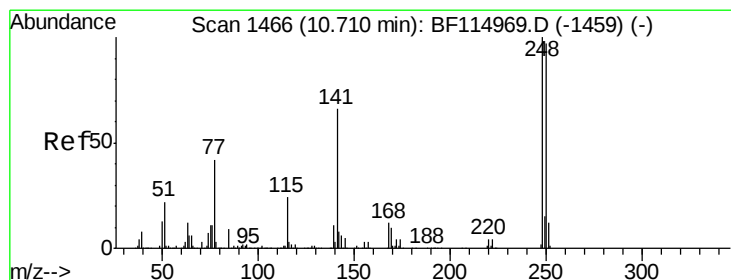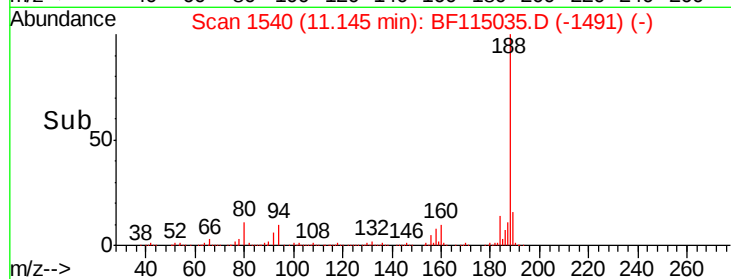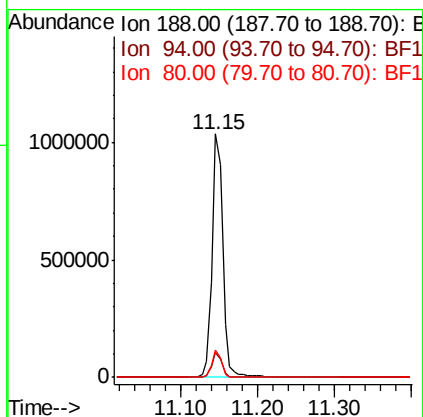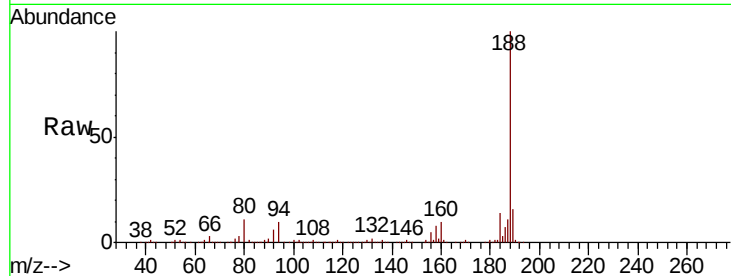

#67
4-Bromophenyl-phenylether
Concen: 3.360 ng
RT: 10.46 min Scan# 1423
Delta R.T. -0.25 min
Lab File: BF115035.D
Acq: 14 Jun 2019 13:10

Tgt Ion:248 Resp: 35535
Ion Ratio Lower Upper
248 100
250 200.6 77.8 116.8#
141 510.2 53.1 79.7#



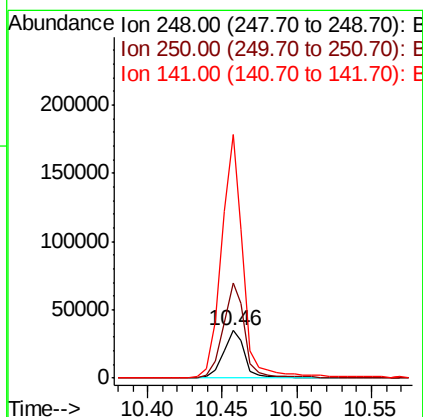



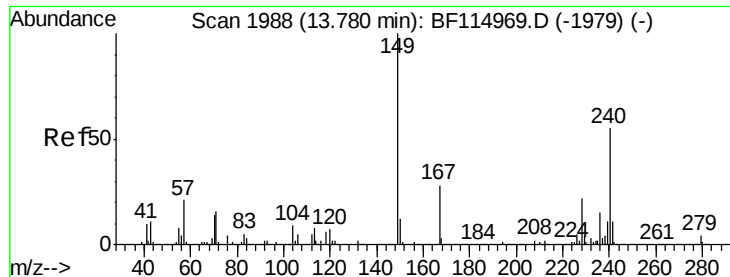

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.77 min Scan# 1986
Delta R.T. -0.01 min
Lab File: BF115035.D
Acq: 14 Jun 2019 13:10




Instrument :
BNA_F
ClientSampled :


Tot Ion:240 Resp: 778515
Ion Ratio Lower Upper
240 100
120 12.6 10.0 15.0
236 26.8 21.6 32.4

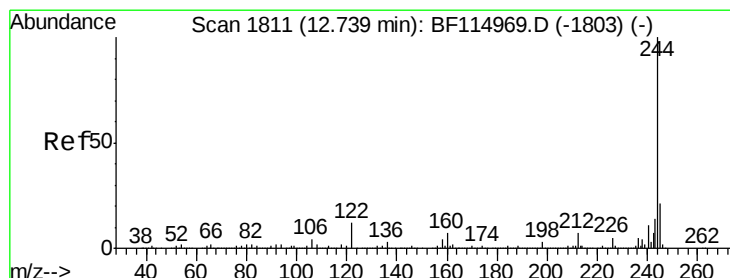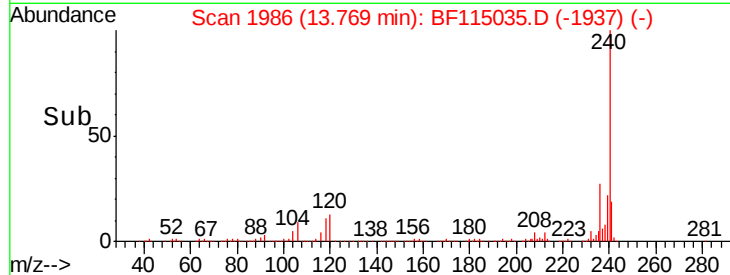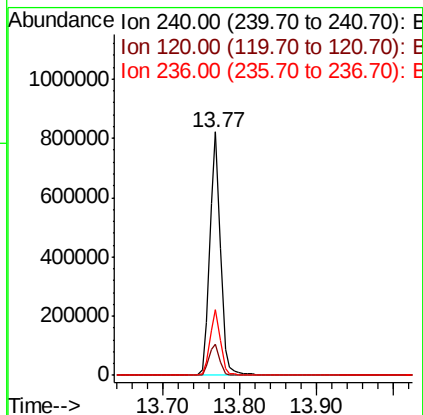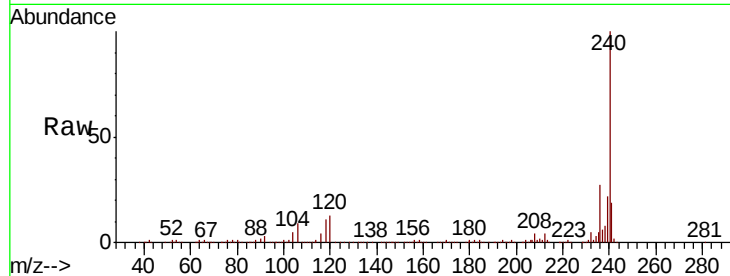

#79
Terphenyl-d14
Concen: 61.165 ng
RT: 12.73 min Scan# 1810
Delta R.T. -0.01 min
Lab File: BF115035.D
Acq: 14 Jun 2019 13:10

Tgt Ion:244 Resp: 2531675
Ion Ratio Lower Upper
244 100
212 7.4 5.8 8.8
122 12.5 9.4 14.0

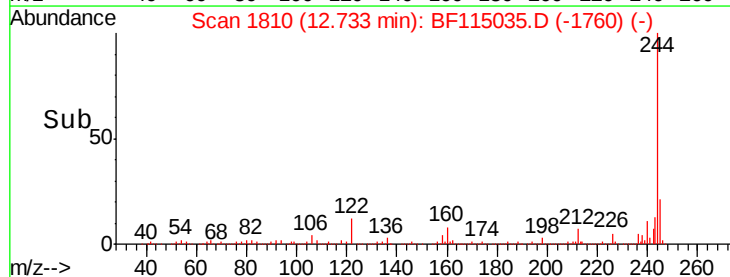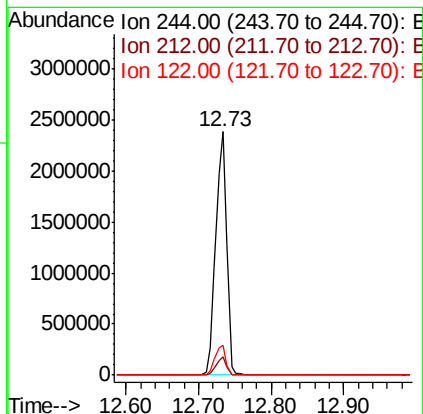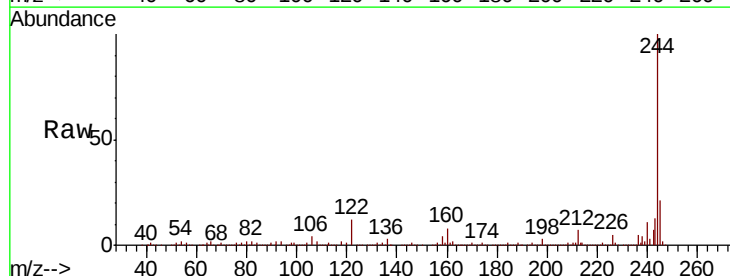

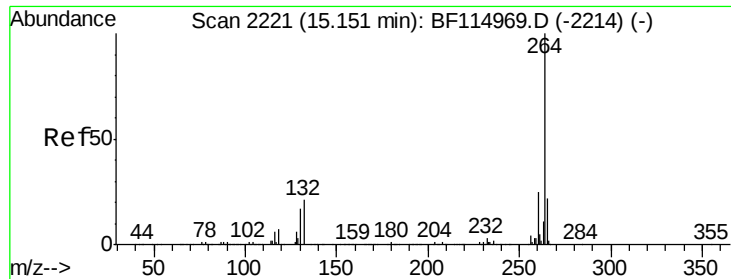

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.14 min Scan# 2220
Delta R.T. -0.01 min
Lab File: BF115035.D
Acq: 14 Jun 2019 13:10

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.9	19.9	29.9
265	21.7	17.6	26.4

