

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061419\
 Data File : BF115030.D
 Acq On : 14 Jun 2019 10:57
 Operator : HP/JU
 Sample : PB120585BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120585BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.263	535	540	543	rBV	4943566	5556725	70.73%	9.243%
2	6.292	709	715	718	rBV	4693276	5665395	72.11%	9.424%
3	6.416	731	736	740	rBV	5385325	5987355	76.21%	9.959%
4	6.645	771	775	779	rBV	1943374	1597509	20.33%	2.657%
5	6.804	797	802	805	rBV	5252597	4891593	62.26%	8.137%
6	7.210	865	871	874	rBV	3580652	3771259	48.00%	6.273%
7	7.928	988	993	996	rBV	2218250	2109926	26.86%	3.510%
8	9.004	1170	1176	1179	rBV	6748727	7346142	93.51%	12.220%
9	9.675	1284	1290	1302	rBV	2700257	2509367	31.94%	4.174%
10	10.457	1418	1423	1454	rBV	4083436	4674898	59.51%	7.776%
11	11.145	1535	1540	1544	rBV	2765478	2726563	34.71%	4.535%
12	12.733	1803	1810	1813	rBV2	7133401	7856237	100.00%	13.068%
13	13.768	1982	1986	1999	rBV	2807389	2602901	33.13%	4.330%
14	15.145	2215	2220	2226	rBV	2069075	2509513	31.94%	4.174%
15	15.198	2226	2229	2234	rVB	90617	116524	1.48%	0.194%
16	15.586	2290	2295	2304	rVB	74214	109129	1.39%	0.182%
17	16.033	2365	2371	2380	rVB2	52077	87057	1.11%	0.145%


Sum of corrected areas: 60118093

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061419\
Data File : BF115030.D
Acq On : 14 Jun 2019 10:57
Operator : HP/JU
Sample : PB120585BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120585BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

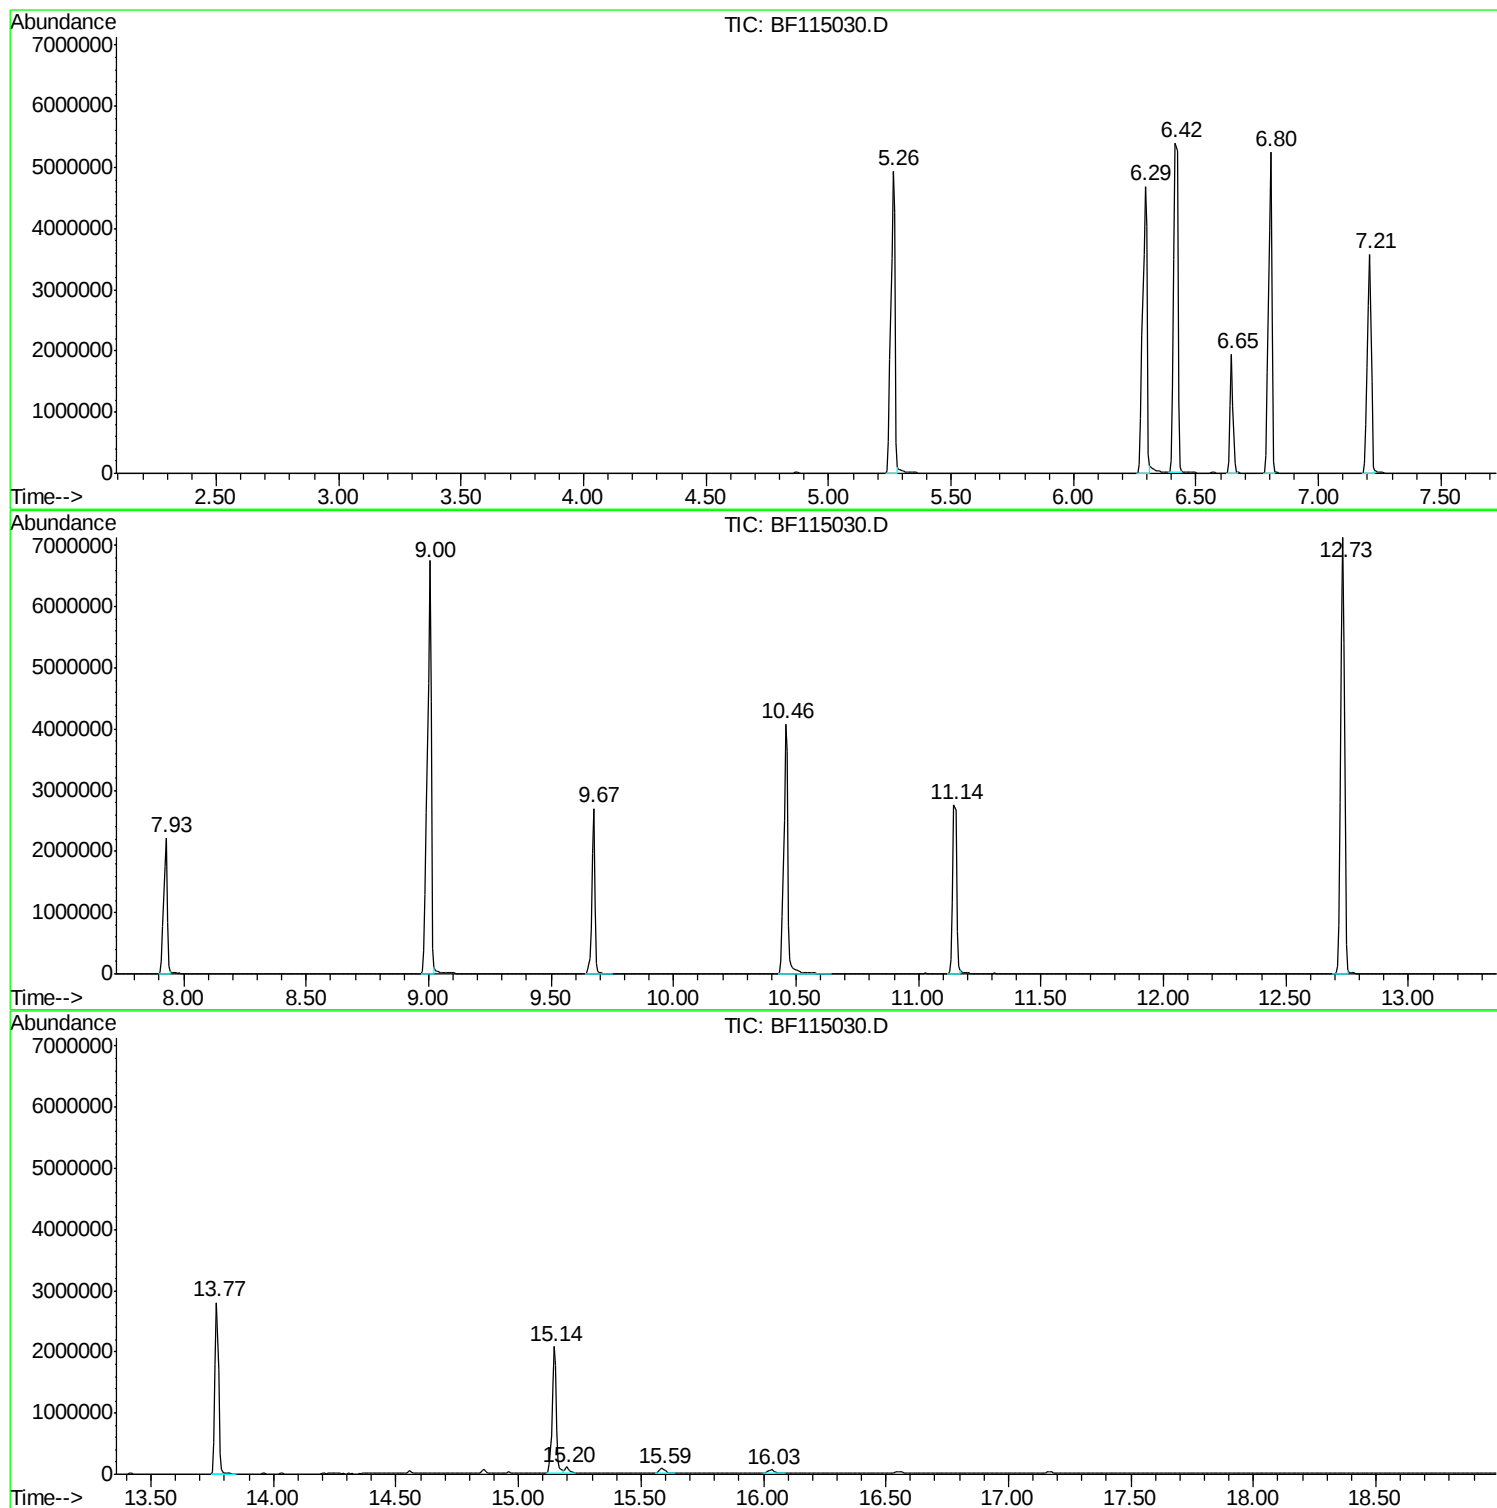

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061419\
Data File : BF115030.D
Acq On : 14 Jun 2019 10:57
Operator : HP/JU
Sample : PB120585BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120585BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.42 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.42	74.96 ng	5987360	1,4-Dichlorobenzene-d4	6.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

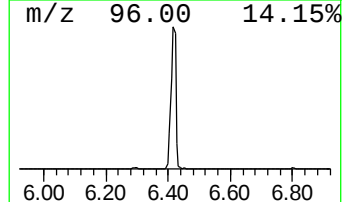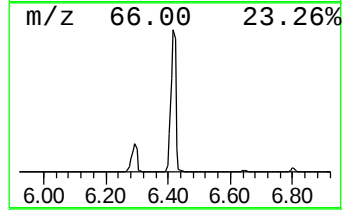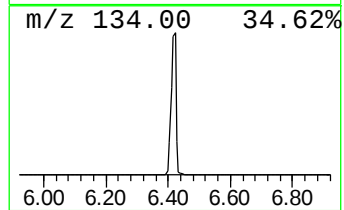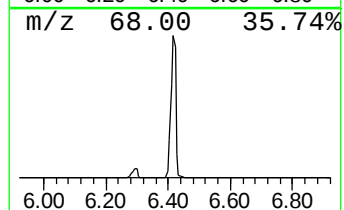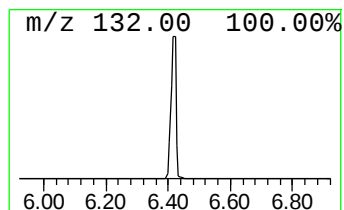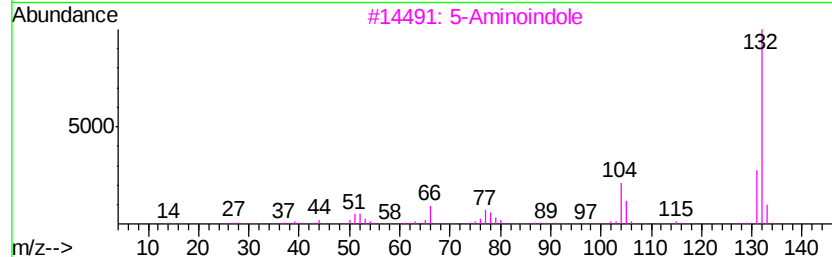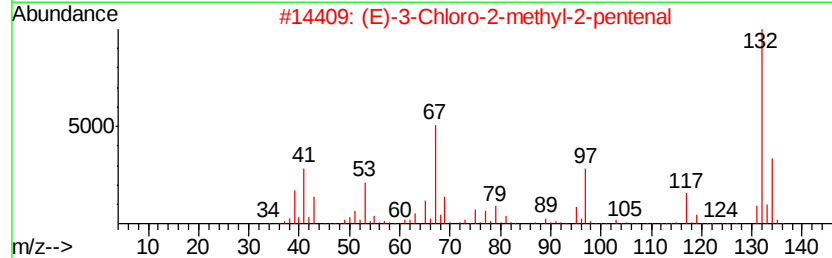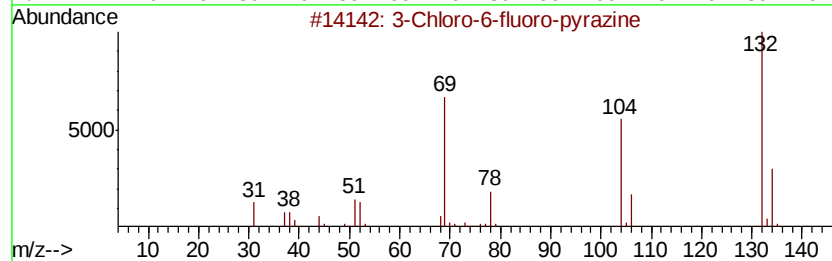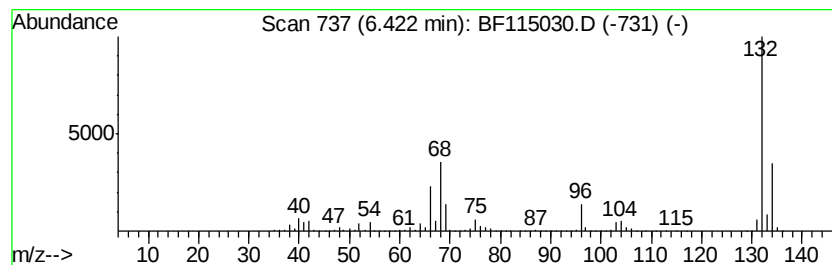

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061419\
Data File : BF115030.D
Acq On : 14 Jun 2019 10:57
Operator : HP/JU
Sample : PB120585BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120585BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.42	6.42	75.0	ng	5987360	1	6.65	1597510	20.0