

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061419\
 Data File : BF115033.D
 Acq On : 14 Jun 2019 12:17
 Operator : HP/JU
 Sample : PB120556BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120556BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.269	535	541	544	rBV	4933256	5731472	74.43%	9.711%
2	6.298	710	716	718	rBV	4696124	5796676	75.27%	9.821%
3	6.422	731	737	740	rBV	5727508	6099668	79.21%	10.335%
4	6.645	771	775	779	rBV	1795587	1478564	19.20%	2.505%
5	6.804	797	802	805	rBV	5520252	5018981	65.17%	8.504%
6	7.210	865	871	874	rBV	3681080	3857670	50.09%	6.536%
7	7.928	988	993	996	rBV	1985510	1925182	25.00%	3.262%
8	9.004	1170	1176	1179	rBV	6909702	7400931	96.11%	12.539%
9	9.675	1284	1290	1299	rBV	2383158	2243775	29.14%	3.802%
10	10.457	1418	1423	1444	rBV	4047266	4620447	60.00%	7.828%
11	11.145	1536	1540	1548	rBV	2476727	2409133	31.28%	4.082%
12	12.733	1805	1810	1813	rBV2	7105696	7700799	100.00%	13.047%
13	13.768	1982	1986	2002	rBV	2404548	2282110	29.63%	3.867%
14	14.857	2165	2171	2176	rBV	69141	79023	1.03%	0.134%
15	15.145	2215	2220	2226	rBV	1759967	2060281	26.75%	3.491%
16	15.198	2226	2229	2234	rVB	99518	121649	1.58%	0.206%
17	15.586	2290	2295	2302	rVB2	74842	106373	1.38%	0.180%
18	16.033	2366	2371	2377	rVB	55460	88758	1.15%	0.150%


Sum of corrected areas: 59021492

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061419\
Data File : BF115033.D
Acq On : 14 Jun 2019 12:17
Operator : HP/JU
Sample : PB120556BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120556BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

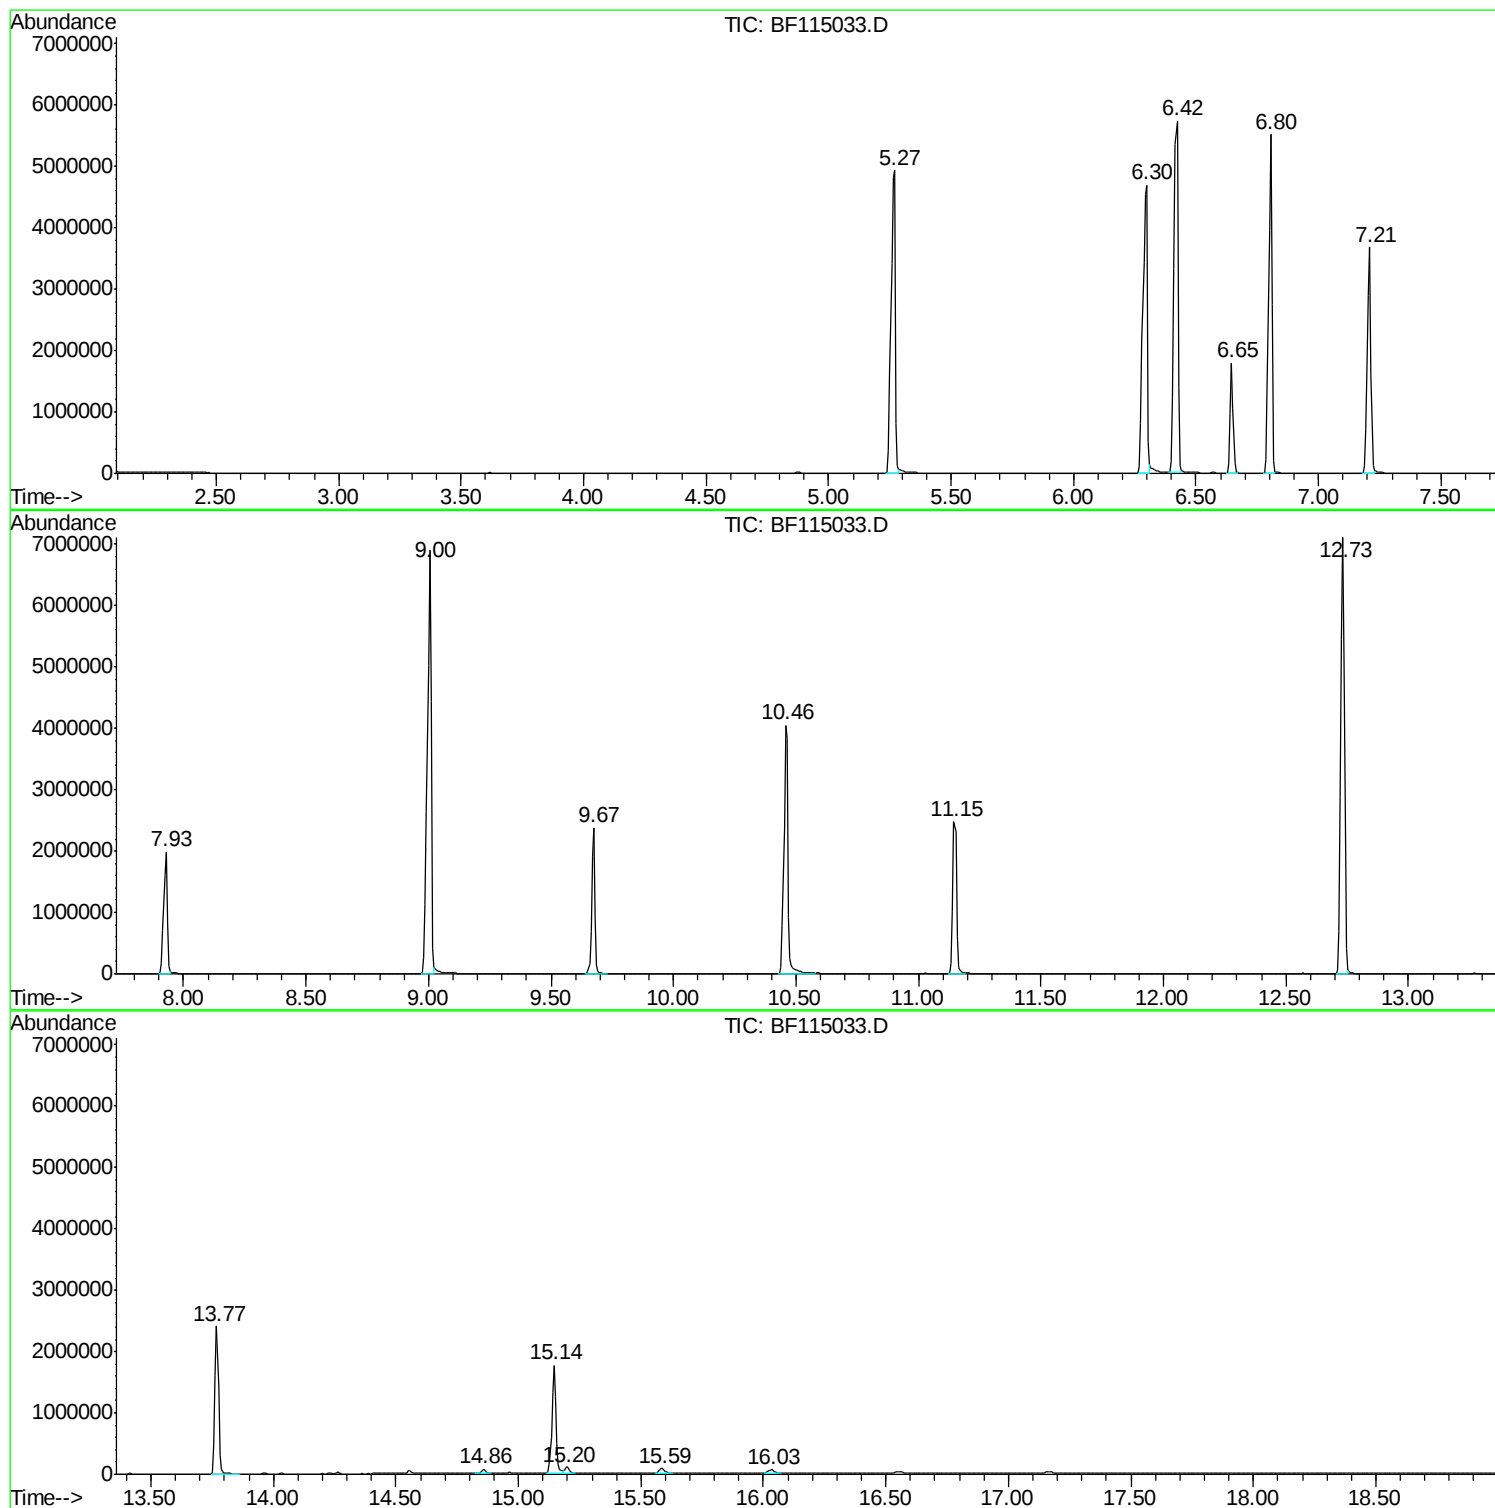

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061419\
Data File : BF115033.D
Acq On : 14 Jun 2019 12:17
Operator : HP/JU
Sample : PB120556BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120556BL









Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.42 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.42	82.51 ng	6099670	1,4-Dichlorobenzene-d4	6.65

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	37
2			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
3			Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	16
4			Cyclopropanamine, 1-phenyl-	133	C9H11N	1000351-26-2	9
5			2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

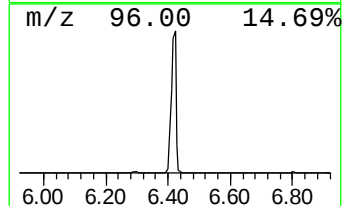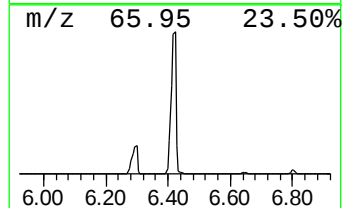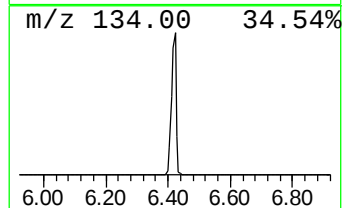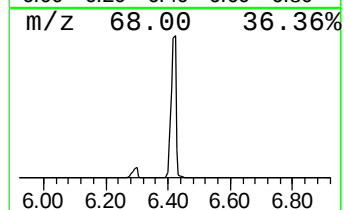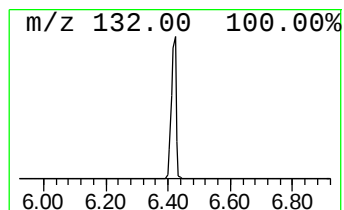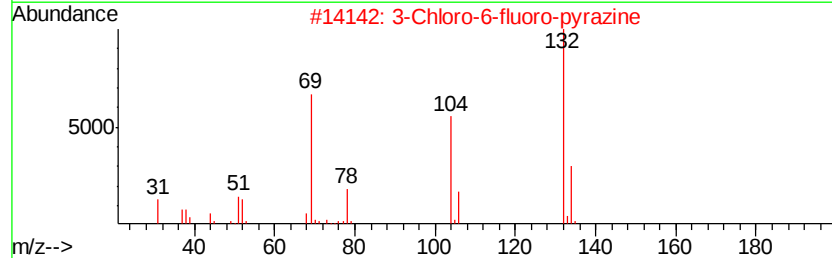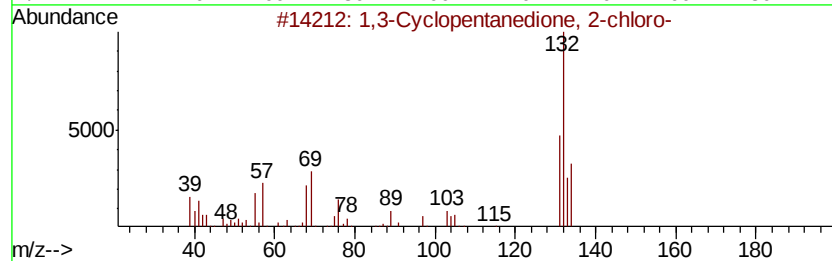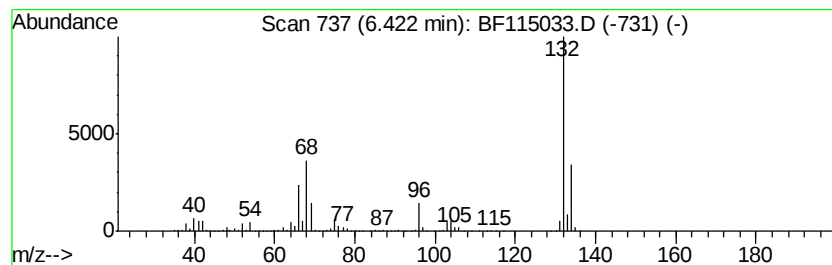

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061419\
Data File : BF115033.D
Acq On : 14 Jun 2019 12:17
Operator : HP/JU
Sample : PB120556BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120556BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.42	6.42	82.5	ng	6099670	1	6.65	1478560	20.0