

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061419\
 Data File : BF115035.D
 Acq On : 14 Jun 2019 13:10
 Operator : HP/JU
 Sample : PB120572BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120572BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.263	535	540	543	rBV	4756879	5104743	74.44%	9.520%
2	6.293	709	715	718	rBV	4704196	5085812	74.17%	9.485%
3	6.416	731	736	740	rBV	5271580	5532284	80.68%	10.317%
4	6.645	771	775	779	rBV	1759284	1437803	20.97%	2.681%
5	6.804	797	802	805	rBV	4783319	4540554	66.21%	8.468%
6	7.210	865	871	874	rBV	3185979	3464623	50.52%	6.461%
7	7.928	988	993	1001	rBV	1945279	1906939	27.81%	3.556%
8	9.004	1170	1176	1179	rBV	6285009	6762718	98.62%	12.612%
9	9.675	1284	1290	1299	rBV	2283640	2202482	32.12%	4.107%
10	10.457	1418	1423	1446	rBV	3907452	4049031	59.05%	7.551%
11	11.145	1535	1540	1555	rBV	2524966	2375191	34.64%	4.430%
12	12.733	1805	1810	1813	rBV	6763094	6857318	100.00%	12.788%
13	13.769	1982	1986	2003	rBV	2355819	2225789	32.46%	4.151%
14	15.145	2214	2220	2226	rBV	1645527	2001133	29.18%	3.732%
15	15.198	2226	2229	2234	rVB	56348	74580	1.09%	0.139%




Sum of corrected areas: 53621000

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061419\
Data File : BF115035.D
Acq On : 14 Jun 2019 13:10
Operator : HP/JU
Sample : PB120572BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120572BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

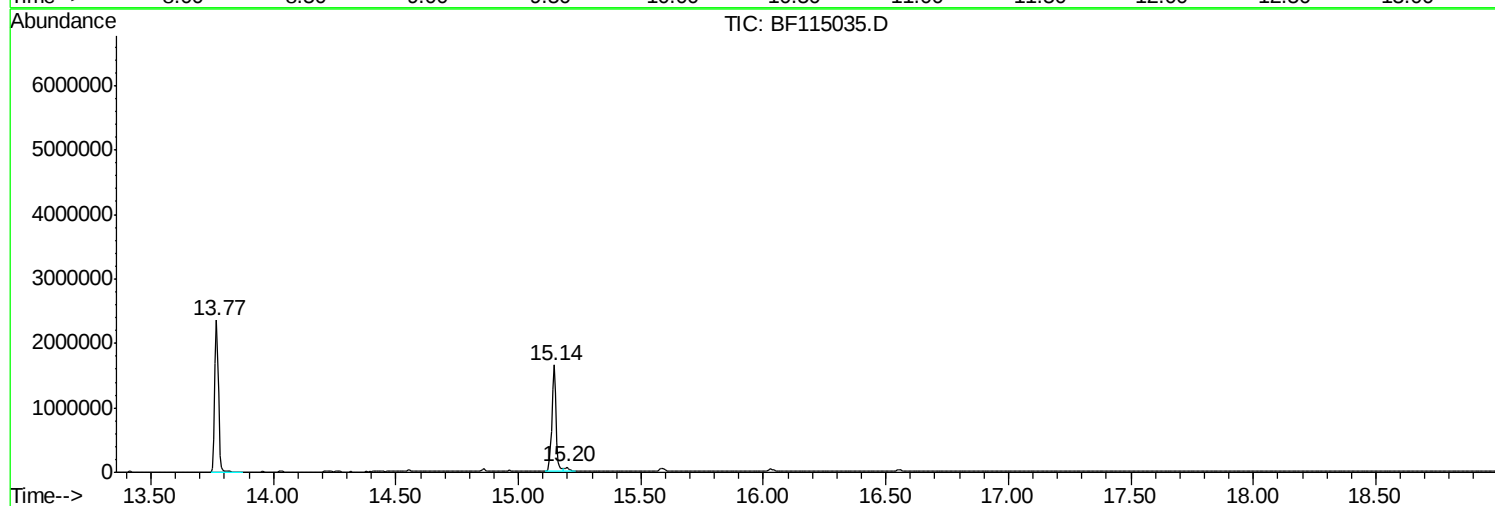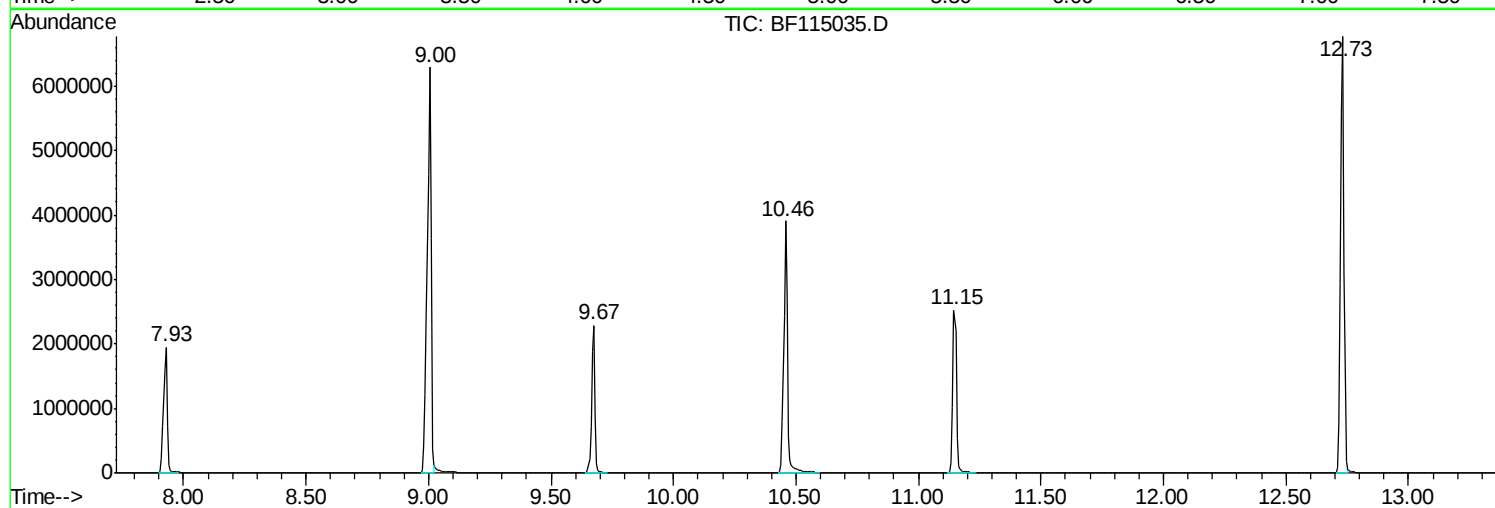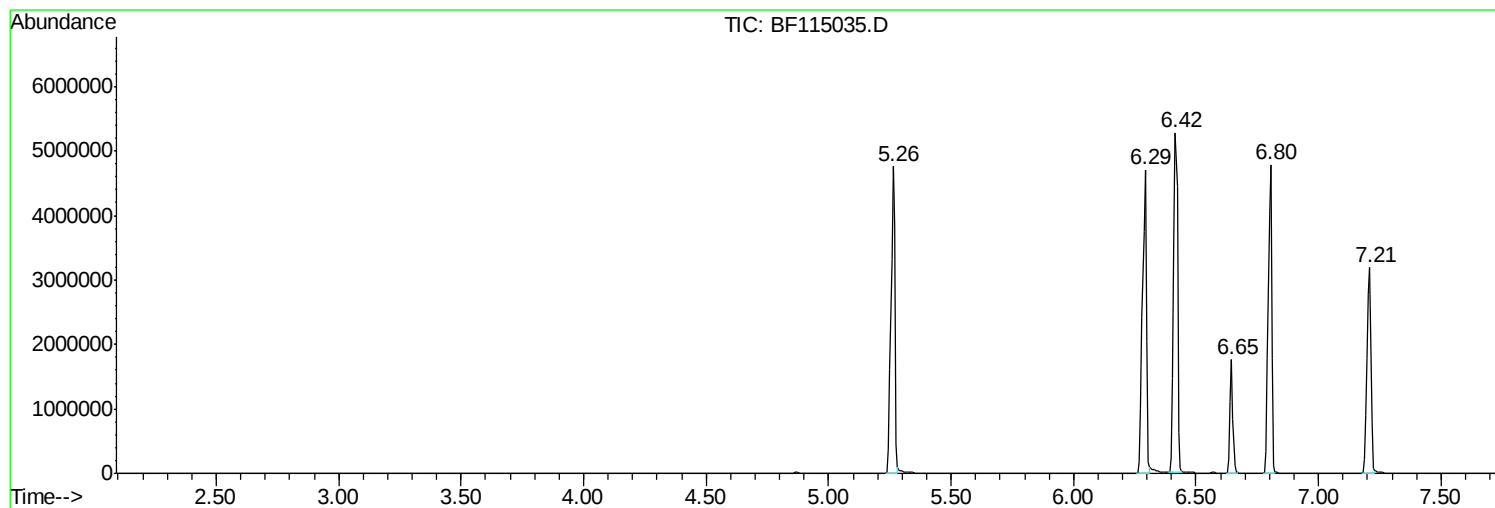

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061419\
Data File : BF115035.D
Acq On : 14 Jun 2019 13:10
Operator : HP/JU
Sample : PB120572BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120572BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.42 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.42	76.95 ng	5532280	1,4-Dichlorobenzene-d4	6.65

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
2			5-Aminoindole	132	C8H8N2	005192-03-0	12
3			Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

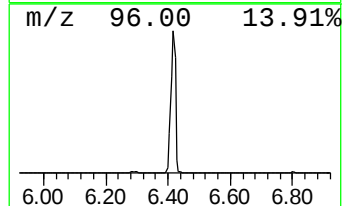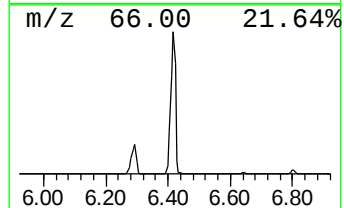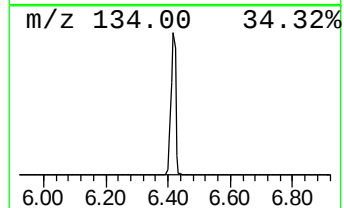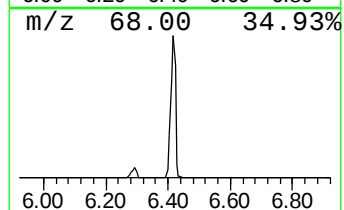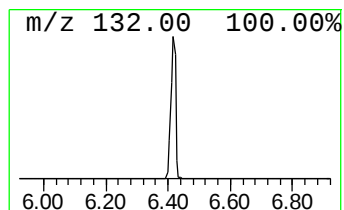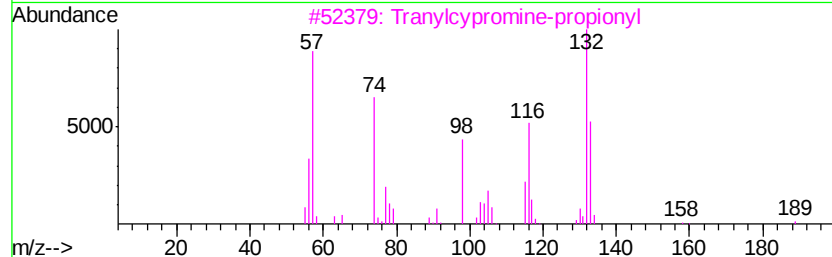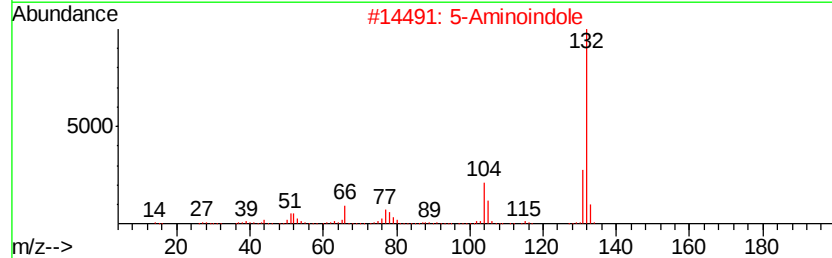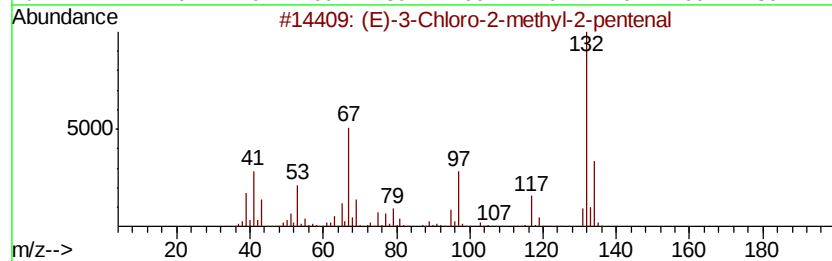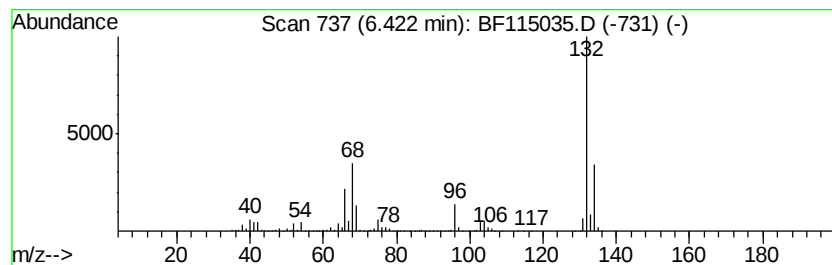

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061419\
Data File : BF115035.D
Acq On : 14 Jun 2019 13:10
Operator : HP/JU
Sample : PB120572BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120572BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.42	6.42	77.0	ng	5532280	1	6.65	1437800	20.0