

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061419\
 Data File : BF115058.D
 Acq On : 14 Jun 2019 23:29
 Operator : HP/JU
 Sample : K3369-12
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 Z-3-SOIL-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.263	534	540	543	rBV	5609845	5974448	84.45%	10.454%
2	6.298	709	716	731	rBV	4945708	6374039	90.10%	11.154%
3	6.416	731	736	740	rBV	5758825	6438810	91.01%	11.267%
4	6.645	771	775	779	rBV	1984495	1546046	21.85%	2.705%
5	6.804	797	802	805	rBV	5724063	5197727	73.47%	9.095%
6	7.210	865	871	874	rBV	3868011	4061102	57.40%	7.106%
7	7.928	988	993	996	rBV	2157542	1887152	26.67%	3.302%
8	9.004	1170	1176	1179	rBV	7277071	7074721	100.00%	12.380%
9	9.398	1239	1243	1255	rVB	550785	503874	7.12%	0.882%
10	9.675	1284	1290	1294	rBV	2244342	2070325	29.26%	3.623%
11	10.457	1419	1423	1438	rBV	3947378	3744399	52.93%	6.552%
12	11.145	1536	1540	1543	rBV	2205532	1940073	27.42%	3.395%
13	11.169	1543	1544	1548	rVB	167086	99405	1.41%	0.174%
14	11.692	1628	1633	1637	rBV2	151141	175650	2.48%	0.307%
15	12.351	1741	1745	1749	rBV	218955	204115	2.89%	0.357%
16	12.574	1778	1783	1788	rBV	211362	208523	2.95%	0.365%
17	12.727	1805	1809	1813	rBV	5470594	5637735	79.69%	9.865%
18	13.769	1980	1986	1989	rBV	1561477	1689426	23.88%	2.956%
19	14.557	2117	2120	2124	rVB	89666	93050	1.32%	0.163%
20	14.621	2127	2131	2134	rVV	90112	90104	1.27%	0.158%
21	14.763	2151	2155	2162	rBV	98804	167441	2.37%	0.293%
22	14.857	2168	2171	2176	rBV	119136	120313	1.70%	0.211%
23	15.086	2207	2210	2213	rVB	74958	75804	1.07%	0.133%
24	15.145	2215	2220	2226	rVV	1203134	1431030	20.23%	2.504%
25	15.198	2226	2229	2234	rVB	97529	122997	1.74%	0.215%
26	15.586	2291	2295	2300	rBV	77764	106524	1.51%	0.186%
27	16.033	2367	2371	2382	rVB3	49641	112448	1.59%	0.197%


Sum of corrected areas: 57147281

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061419\
Data File : BF115058.D
Acq On : 14 Jun 2019 23:29
Operator : HP/JU
Sample : K3369-12
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
Z-3-SOIL-3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

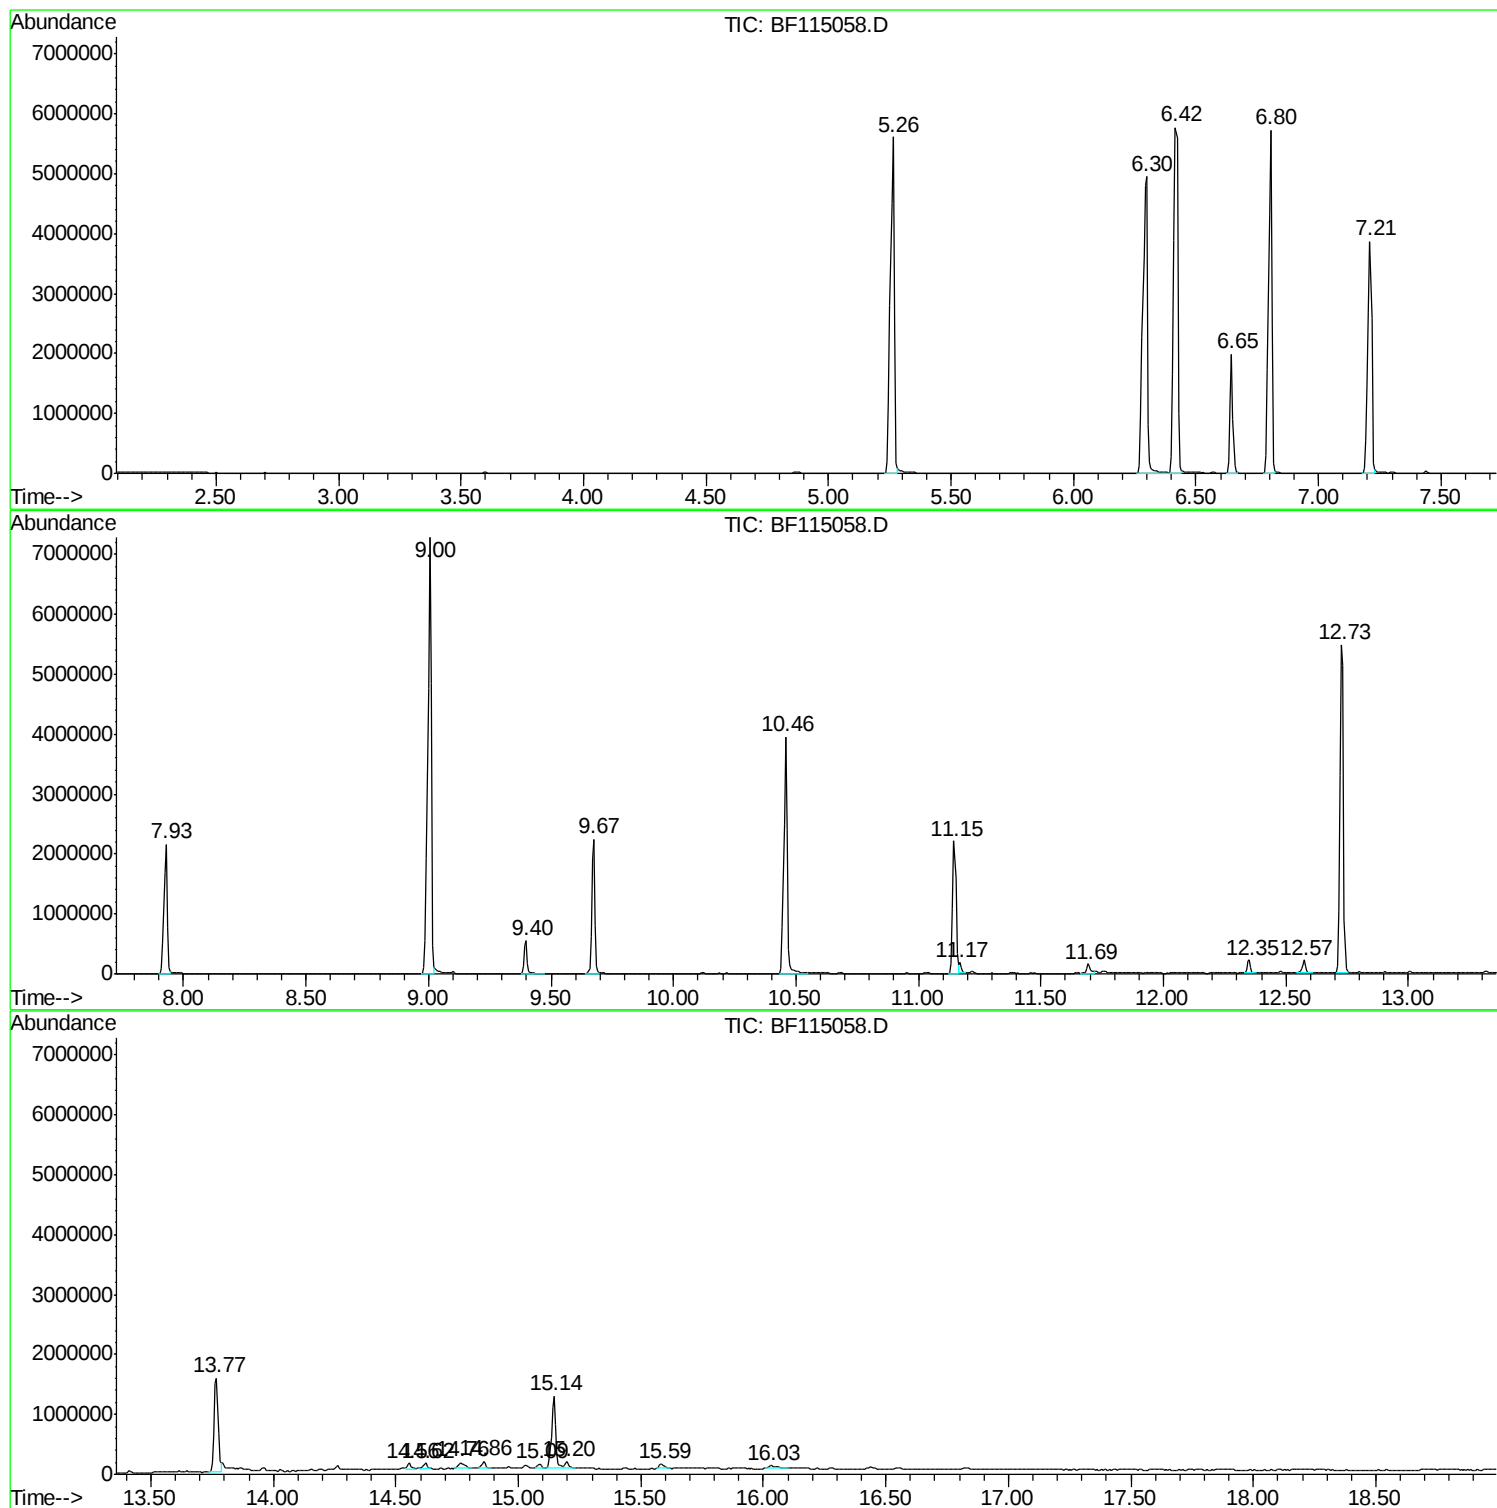

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF061419\
Data File : BF115058.D
Acq On : 14 Jun 2019 23:29
Operator : HP/JU
Sample : K3369-12
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
Z-3-SOIL-3










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.42 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.42	83.29 ng	6438810	1,4-Dichlorobenzene-d4	6.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
2		5-Aminoindole	132	C8H8N2	005192-03-0	12
3		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9
5		(5-Methyl-2-pyridyl)acetonitrile	132	C8H8N2	1000241-93-9	9

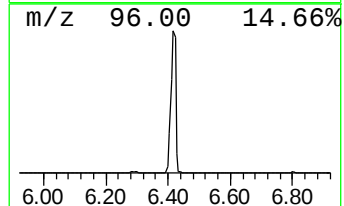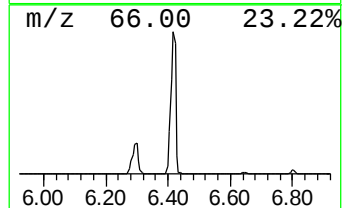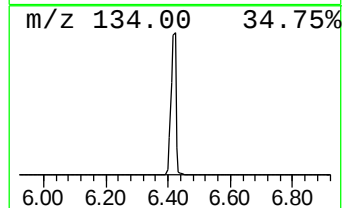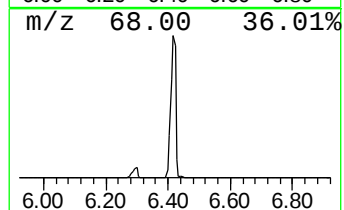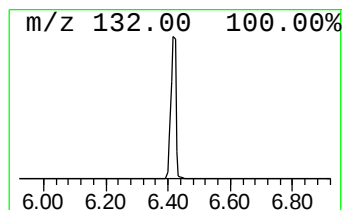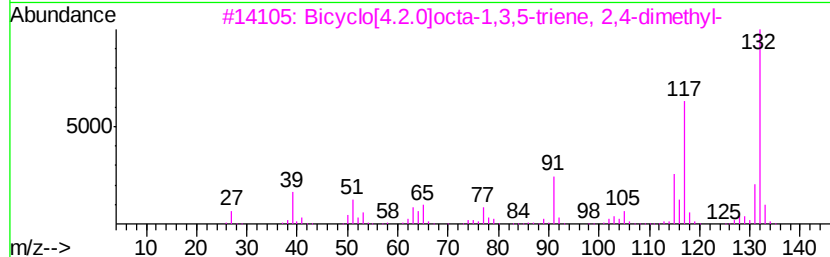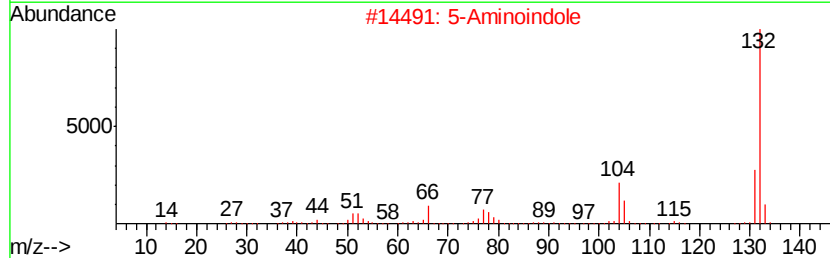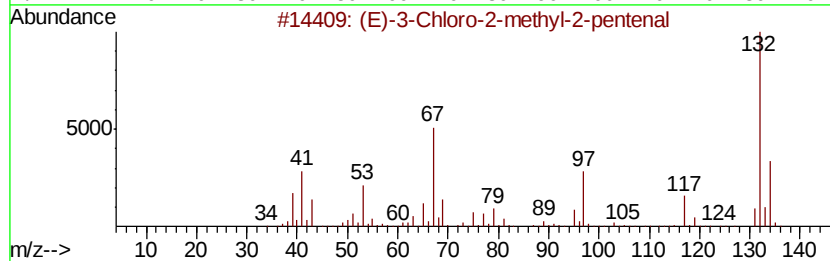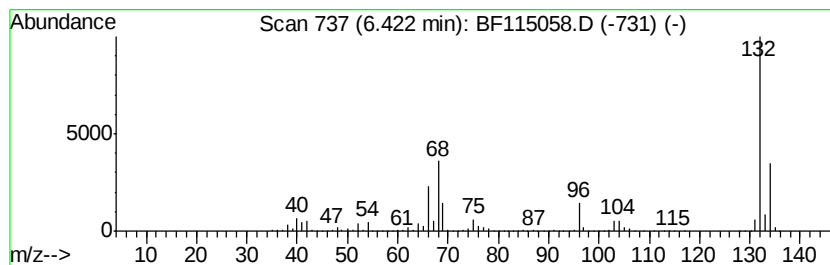

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061419\
Data File : BF115058.D
Acq On : 14 Jun 2019 23:29
Operator : HP/JU
Sample : K3369-12
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
Z-3-SOIL-3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.42	6.42	83.3	ng	6438810	1	6.65	1546050	20.0