


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061419\
Data File : BF115027.D
Acq On : 14 Jun 2019 9:11
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061219.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 12 15:42:37 2019

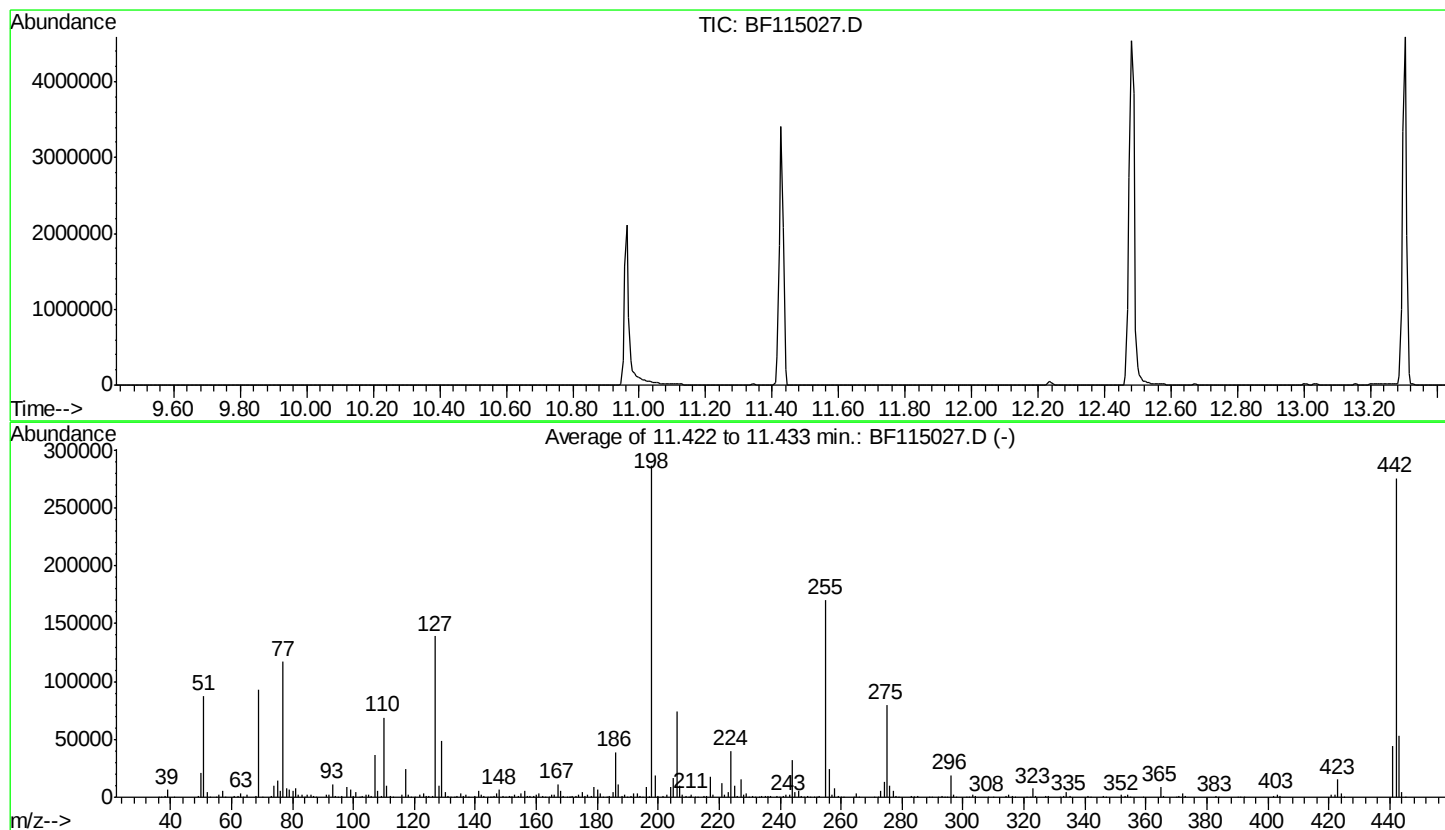

AutoFind: Scans 1587, 1588, 1589; Background Corrected with Scan 1582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	87410	PASS
68	69	0.00	2	1.7	1583	PASS
69	198	0.00	100	32.4	92840	PASS
70	69	0.00	2	0.6	549	PASS
127	198	10	80	48.6	139245	PASS
197	198	0.00	2	0.2	458	PASS
198	198	100	100	100.0	286613	PASS
199	198	5	9	6.8	19358	PASS
275	198	10	60	27.8	79816	PASS
365	198	1	100	3.2	9043	PASS
441	198	0.01	100	15.4	44093	PASS
442	198	50	100	96.2	275821	PASS
443	442	15	24	19.3	53117	PASS