


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF061419\
 Data File : BF115042.D
 Acq On : 14 Jun 2019 16:15
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 12 15:42:37 2019

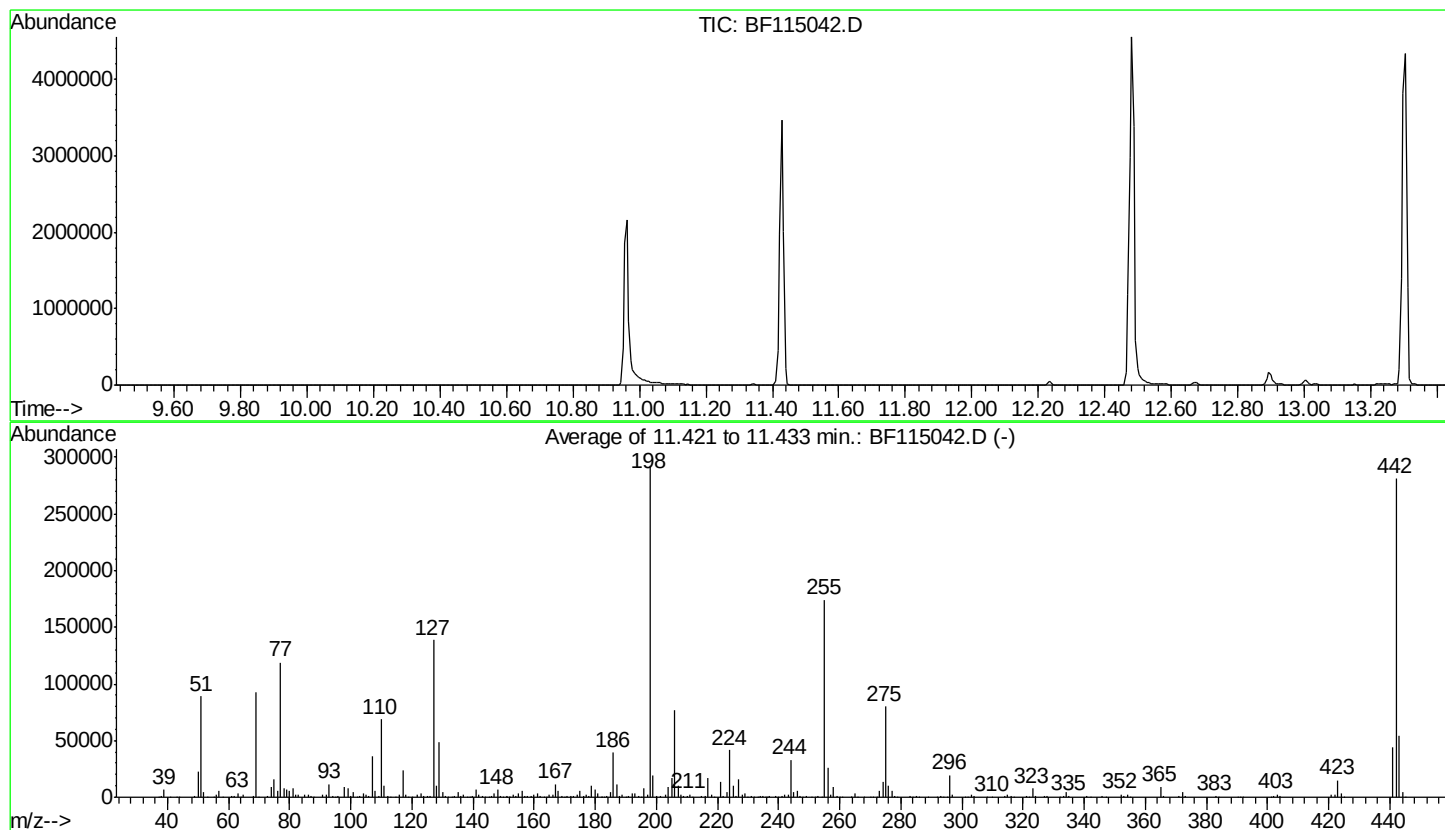

AutoFind: Scans 1587, 1588, 1589; Background Corrected with Scan 1581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	89194	PASS
68	69	0.00	2	1.8	1697	PASS
69	198	0.00	100	31.5	92173	PASS
70	69	0.00	2	0.4	353	PASS
127	198	10	80	47.3	138456	PASS
197	198	0.00	2	0.6	1787	PASS
198	198	100	100	100.0	292672	PASS
199	198	5	9	6.7	19575	PASS
275	198	10	60	27.4	80064	PASS
365	198	1	100	3.3	9615	PASS
441	198	0.01	100	15.0	43802	PASS
442	198	50	100	96.0	281093	PASS
443	442	15	24	19.5	54762	PASS