
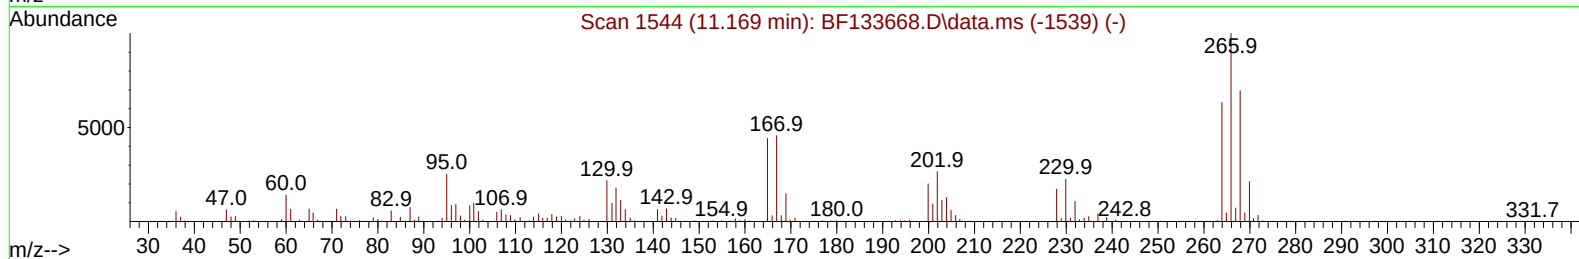
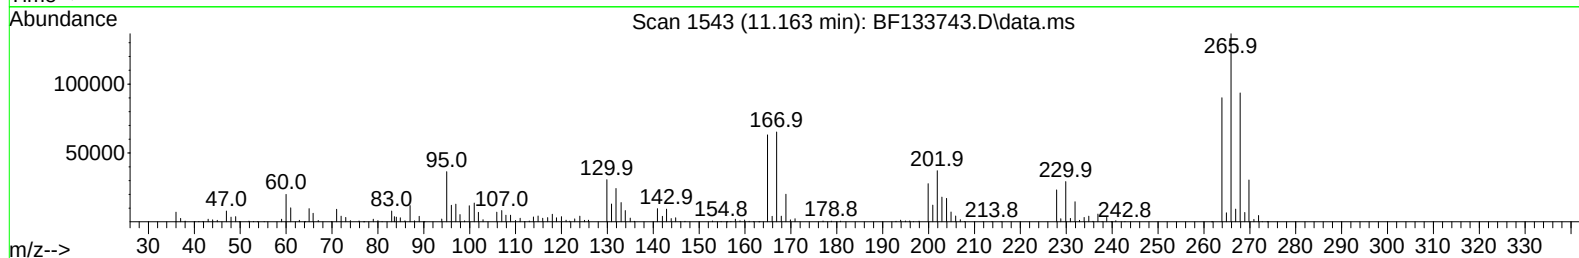


Quant Time: Jun 14 10:23:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 13 11:26:55 2023
Response via : Initial Calibration

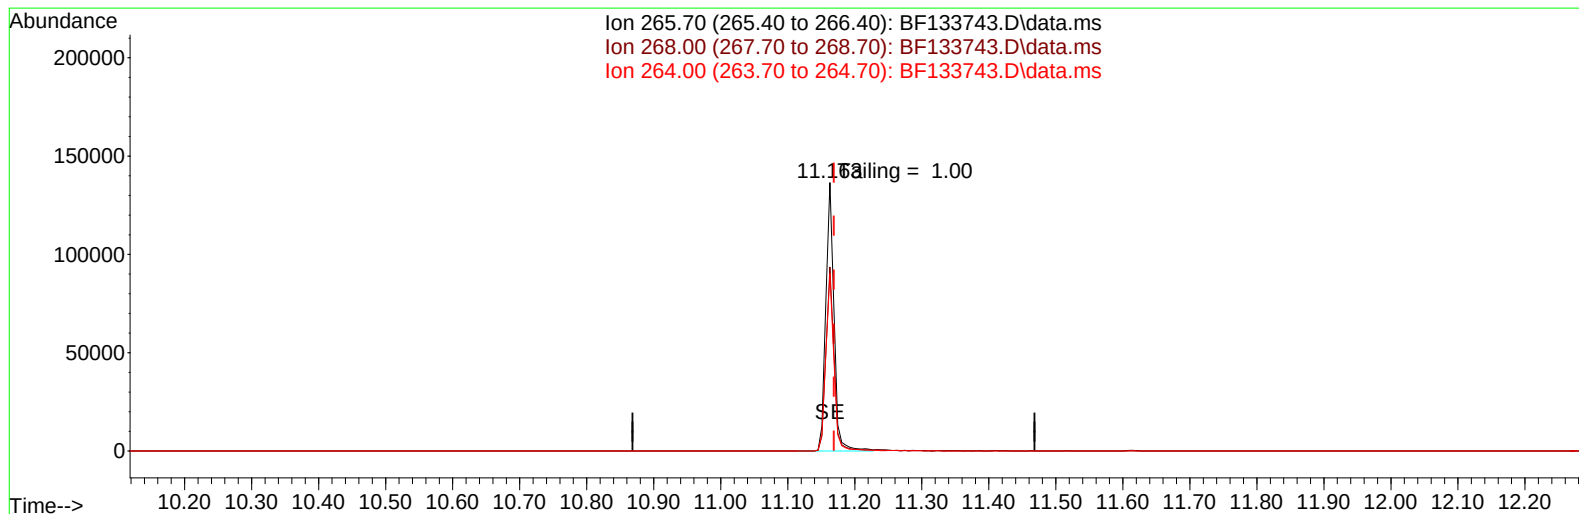

TIC: BF133743.D\data.ms

(70) Pentachlorophenol (C)




11.163min (-0.006) 26512.57 ng

response **117764**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.60	68.53
264.00	63.40	66.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061423\
Data File : BF133743.D
Acq On : 14 Jun 2023 09:58
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 10:23:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 13 11:26:55 2023
Response via : Initial Calibration

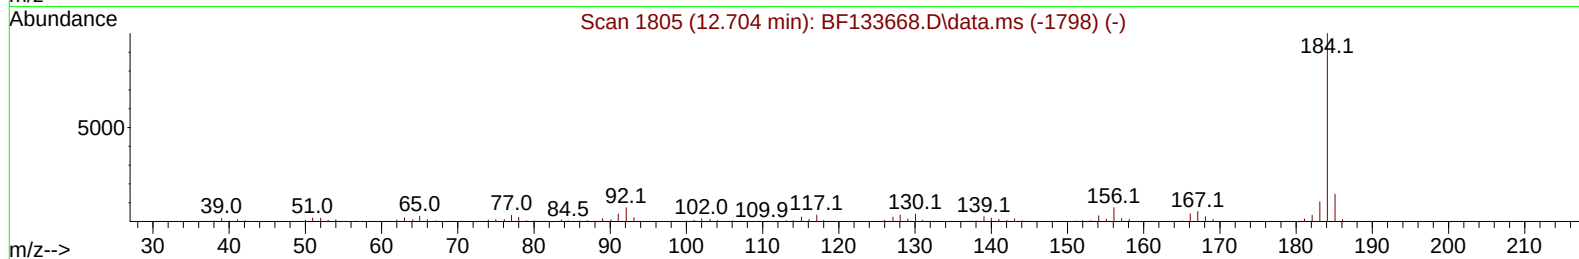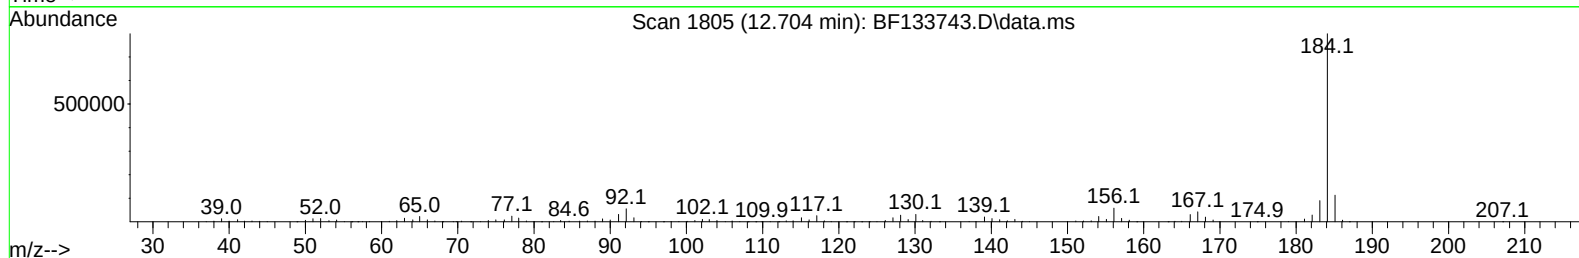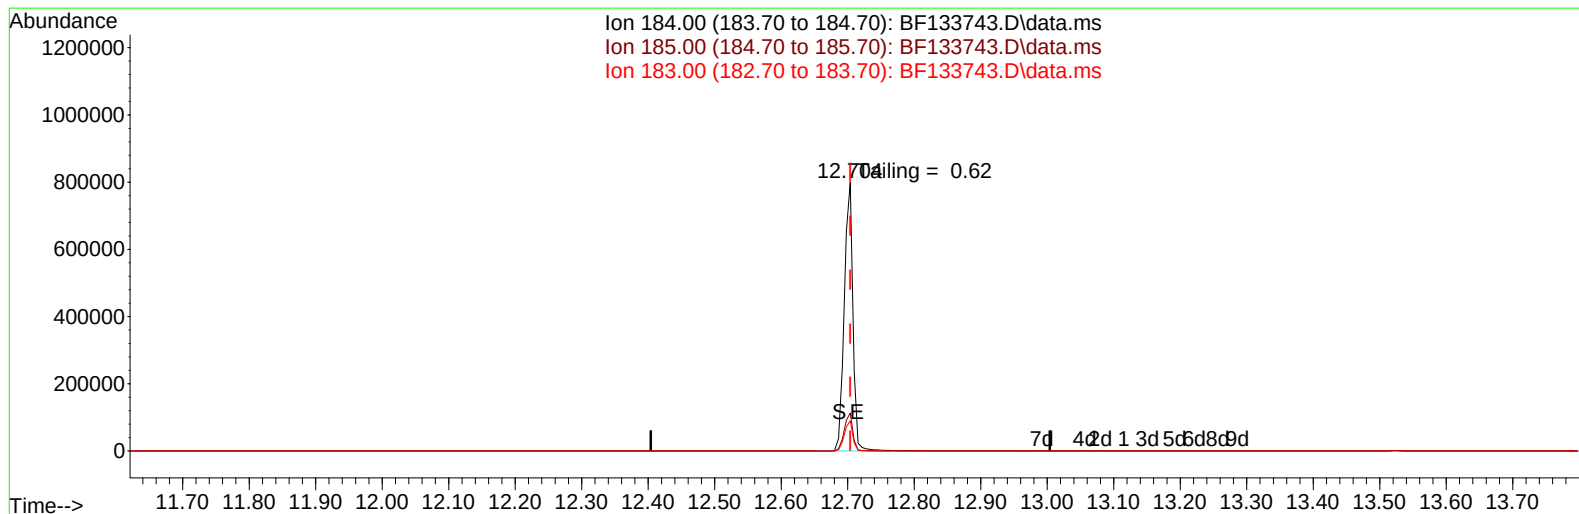

TIC: BF133743.D\data.ms

(77) Benzidine

12.704min (+ 0.000) 391202.01 ng m

response 721994

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.14
183.00	10.50	11.24
0.00	0.00	0.00