

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061423\
 Data File : BF133745.D
 Acq On : 14 Jun 2023 11:01
 Operator : CG\JU
 Sample : PB153266BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB153266BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133745.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.140	6	9	18	rVB	58250	83577	2.26%	0.355%
2	5.075	504	508	517	rVB	38199	52863	1.43%	0.225%
3	5.457	567	573	576	rBV	3242287	3245831	87.74%	13.788%
4	6.469	738	745	747	rBV	2756496	3297595	89.14%	14.008%
5	6.828	803	806	810	rBV	774968	694957	18.79%	2.952%
6	7.398	897	903	906	rBV	2305115	2175792	58.82%	9.242%
7	8.116	1021	1025	1028	rBV	1113862	892071	24.11%	3.789%
8	9.192	1204	1208	1211	rBV	4203728	3699255	100.00%	15.714%
9	9.869	1320	1323	1327	rBV	1208888	986477	26.67%	4.190%
10	10.663	1453	1458	1461	rBV	2723242	2508060	67.80%	10.654%
11	11.357	1572	1576	1580	rBV	1231354	1081541	29.24%	4.594%
12	12.951	1842	1847	1850	rBV	3589506	3534080	95.53%	15.012%
13	14.004	2022	2026	2030	rBV	848242	744208	20.12%	3.161%
14	15.463	2269	2274	2283	rVB	418912	545232	14.74%	2.316%




Sum of corrected areas: 23541539

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061423\
Data File : BF133745.D
Acq On : 14 Jun 2023 11:01
Operator : CG\JU
Sample : PB153266BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153266BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

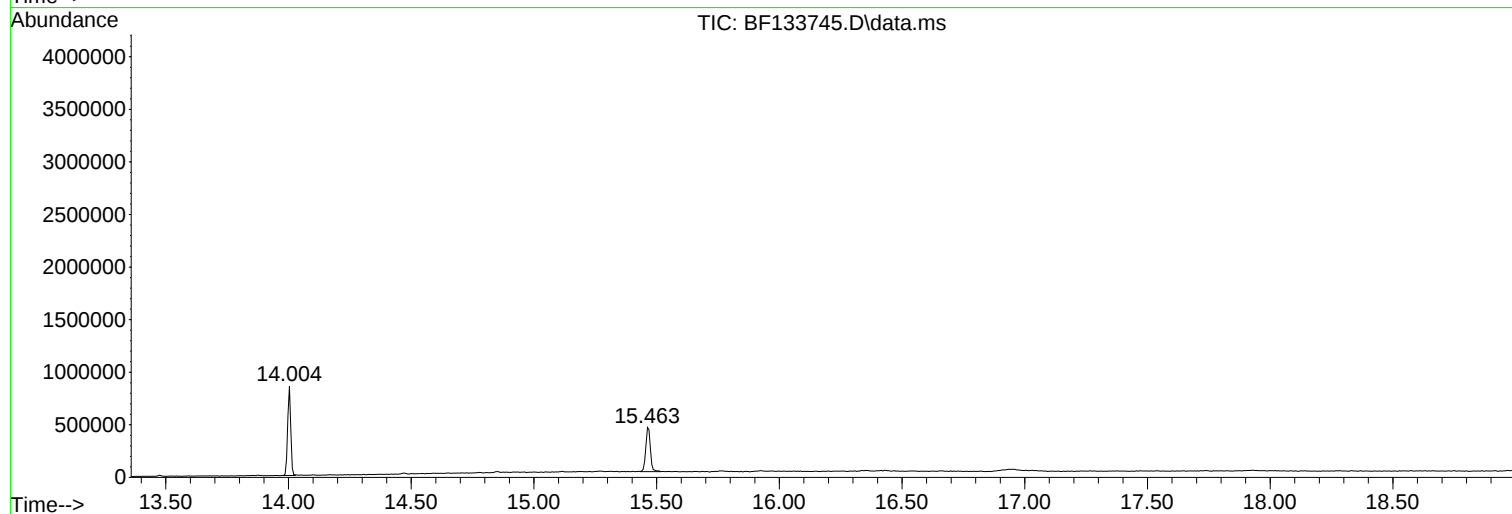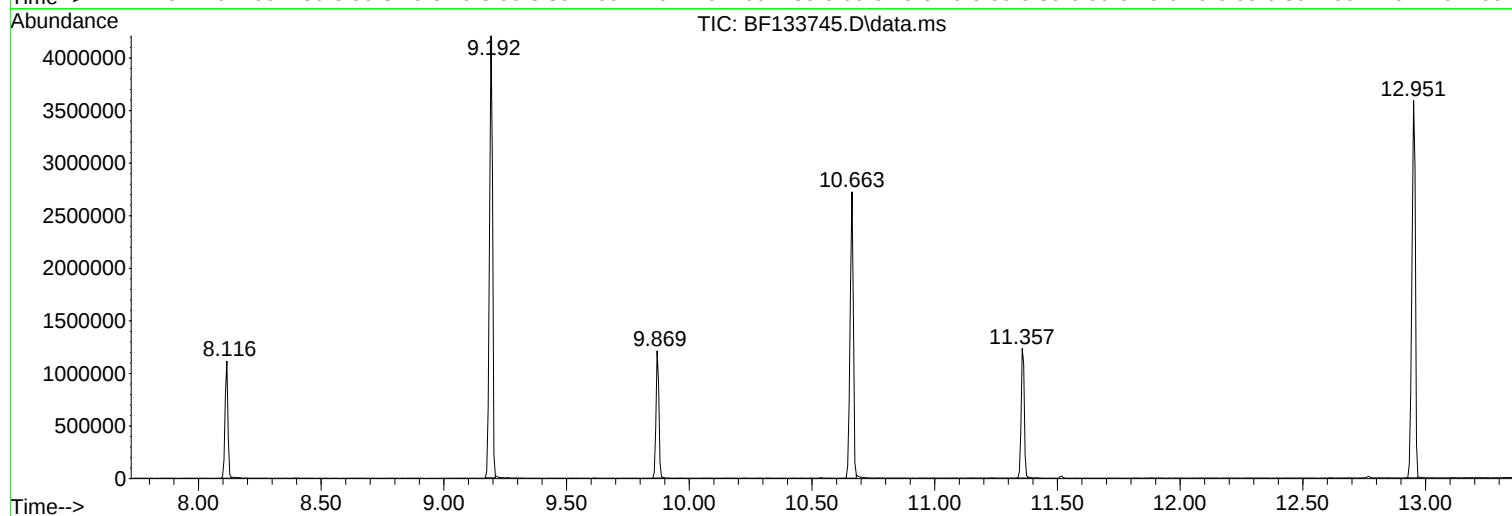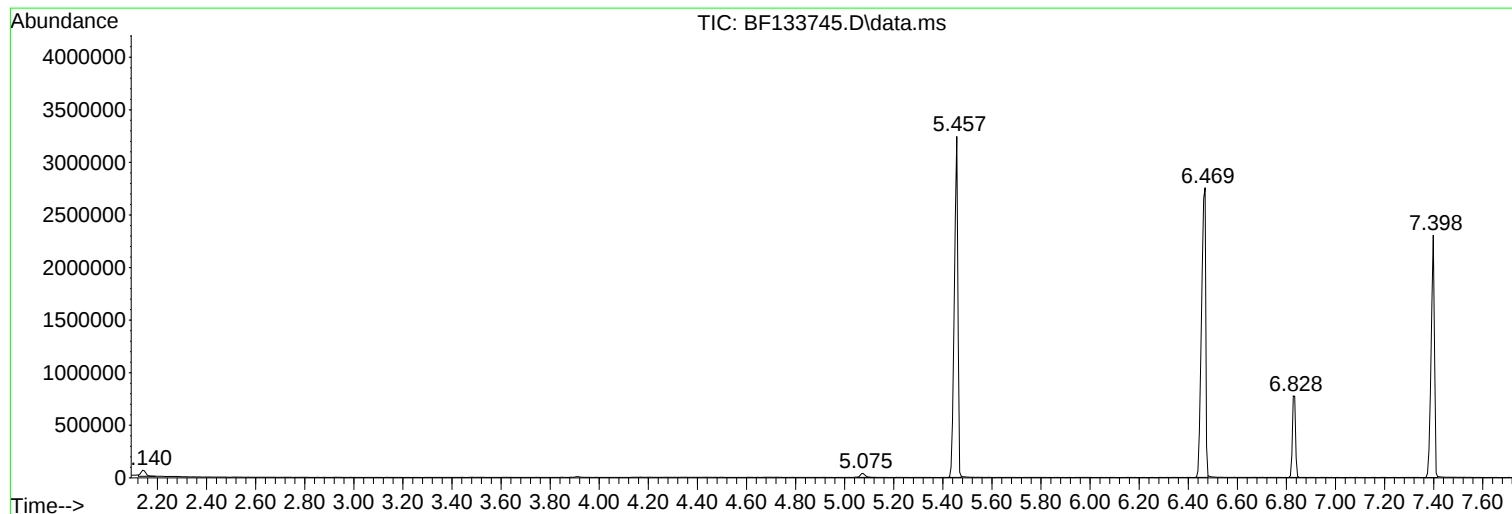

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061423\
Data File : BF133745.D
Acq On : 14 Jun 2023 11:01
Operator : CG\JU
Sample : PB153266BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153266BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.140	2.41 ng	83577	1,4-Dichlorobenzene-d4	6.834

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
2			2,5-Dimethyl-4-hydroxy-3-hexanone	144	C8H16O2	000815-77-0	50
3			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	37
4			Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	36
5			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	17

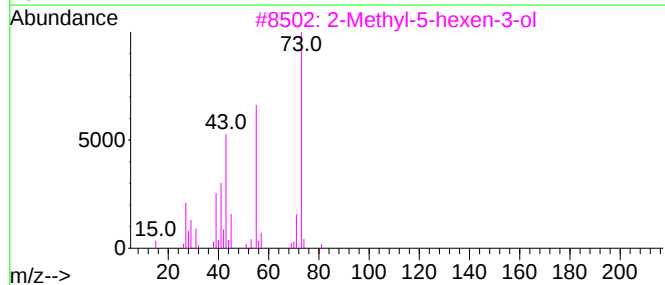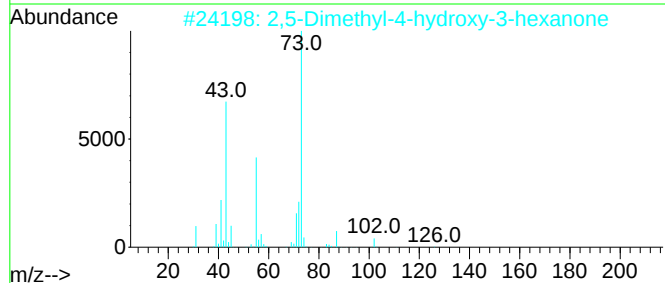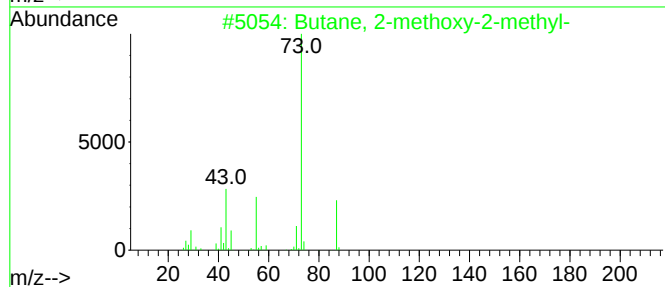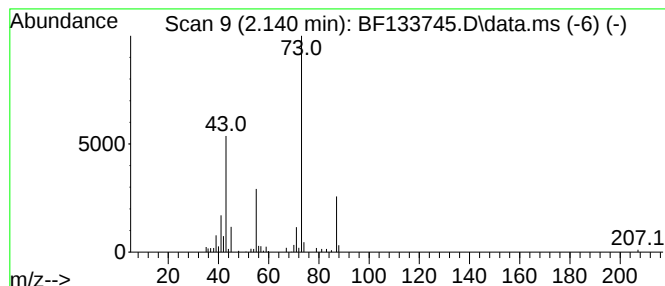

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061423\
Data File : BF133745.D
Acq On : 14 Jun 2023 11:01
Operator : CG\JU
Sample : PB153266BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153266BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.140	2.4	ng	83577	1	6.834	694957	20.0